

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
 Data File : PL092047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 17:21
 Operator : AR\AJ
 Sample : P3879-03RE
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DCVY6RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/26/2024
 Supervised By : Ankita Jodhani 09/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 02:11:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.530	2.794	151.8E6	384.1E6	86.891m	180.453m#
2) SA Decachlor...	9.058	7.919	24475033	48584613	18.215	22.834m#
Target Compounds						
2) A alpha-BHC	3.997	3.284	456.7E6	492.2E6	179.746	164.477
5) MB Aldrin	5.275	4.243	104.6E6	58428772	46.591m	22.318m#
7) B delta-BHC	4.773	4.142	578.8E6	594.4E6	237.135m	206.147

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
Data File : PL092047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 17:21
Operator : AR\AJ
Sample : P3879-03RE
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 02:11:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

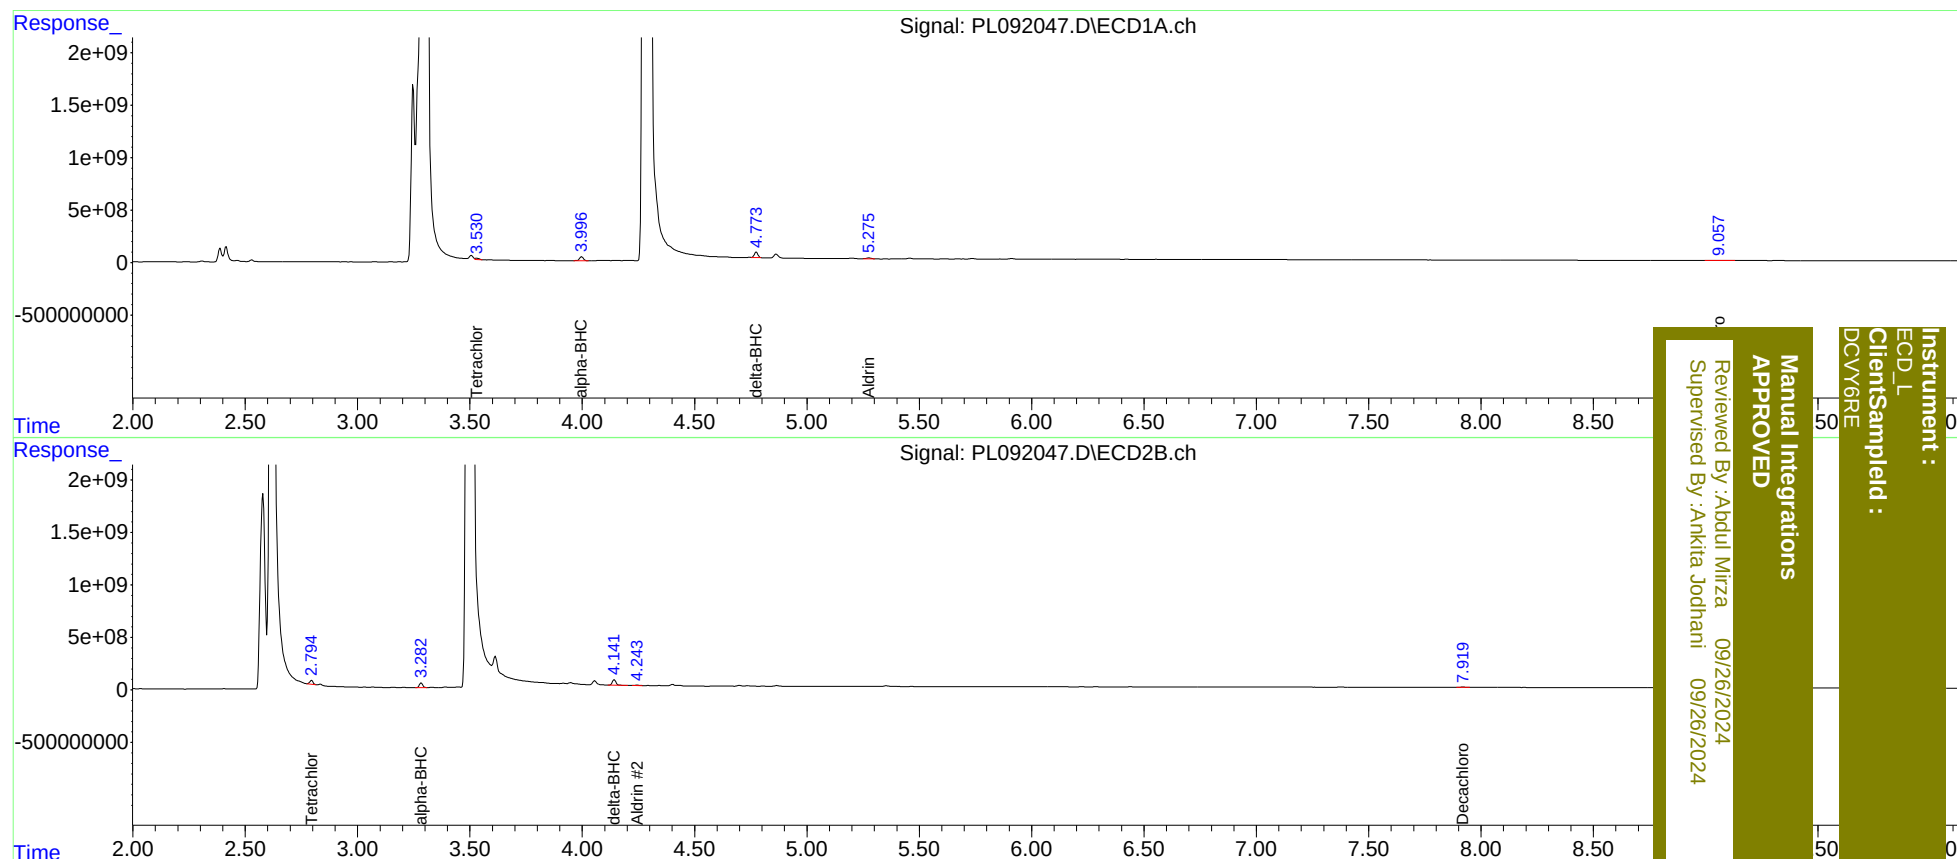

Reviewed By: Abdul Mirza 09/26/2024
Supervised By: Ankita Jodhani 09/26/2024

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
DCVY6RE