

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
 Data File : PL092050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 18:01
 Operator : AR\AJ
 Sample : P3879-06MSRE
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DDC59MSRE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/26/2024
 Supervised By :Ankita Jodhani 09/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 02:11:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.529	2.795	410.4E6	14849.4E6	234.952m	6976.457m#
27) SA Decachlor...	9.057	7.921	26635619	44063003	19.822	20.709
Target Compounds						
2) A alpha-BHC	3.998	3.284	720.9E6	893.2E6	283.705	298.497
3) MA gamma-BHC...	4.268f	3.613	84380.4E6	1470.2E6	34317.886m	526.504m#
4) MA Heptachlor	4.915	3.950	84985711	138.0E6	37.373m	49.274m#
5) MB Aldrin	5.260	4.233	132.2E6	174.5E6	58.875m	66.672m
6) B beta-BHC	4.526	3.914	69291138	132.9E6	59.852m	102.585m#
7) B delta-BHC	4.773	4.143	830.0E6	965.2E6	340.053m	334.737
8) B Heptachlo...	5.685	4.736	146.2E6	227.2E6	71.771	92.699m#
9) A Endosulfan I	6.071	5.115	77281670	420.8E6	42.637m	193.858 #
10) B trans-Chl...	5.949	4.986	384.2E6	105.8E6	197.283	43.929 #
11) B cis-Chlor...	6.019	5.049	132.2E6	117.2E6	65.084m	48.880
12) B 4,4'-DDE	6.195	5.238	277.2E6	242.9E6	154.745	103.359 #
13) MA Dieldrin	6.347	5.370	251.1E6	394.1E6	129.367	165.001 #
14) MA Endrin	6.576	5.645	179.7E6	237.8E6	112.882	110.572
15) B Endosulfa...	6.796	5.940	173.5E6	198.0E6	97.911	93.436
16) A 4,4'-DDD	6.711	5.794	162.1E6	215.3E6	113.705	117.808
17) MA 4,4'-DDT	7.026	6.043	158.9E6	228.0E6	108.115	117.488
18) B Endrin al...	6.927	6.119	141.7E6	172.5E6	111.279	111.659
19) B Endosulfa...	7.160	6.342	161.2E6	213.8E6	97.857	103.692
20) A Methoxychlor	7.502	6.619	396.9E6	516.5E6	511.056	493.835
21) B Endrin ke...	7.645	6.847	199.9E6	244.8E6	110.191	105.581

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
Data File : PL092050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 18:01
Operator : AR\AJ
Sample : P3879-06MSRE
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 02:11:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

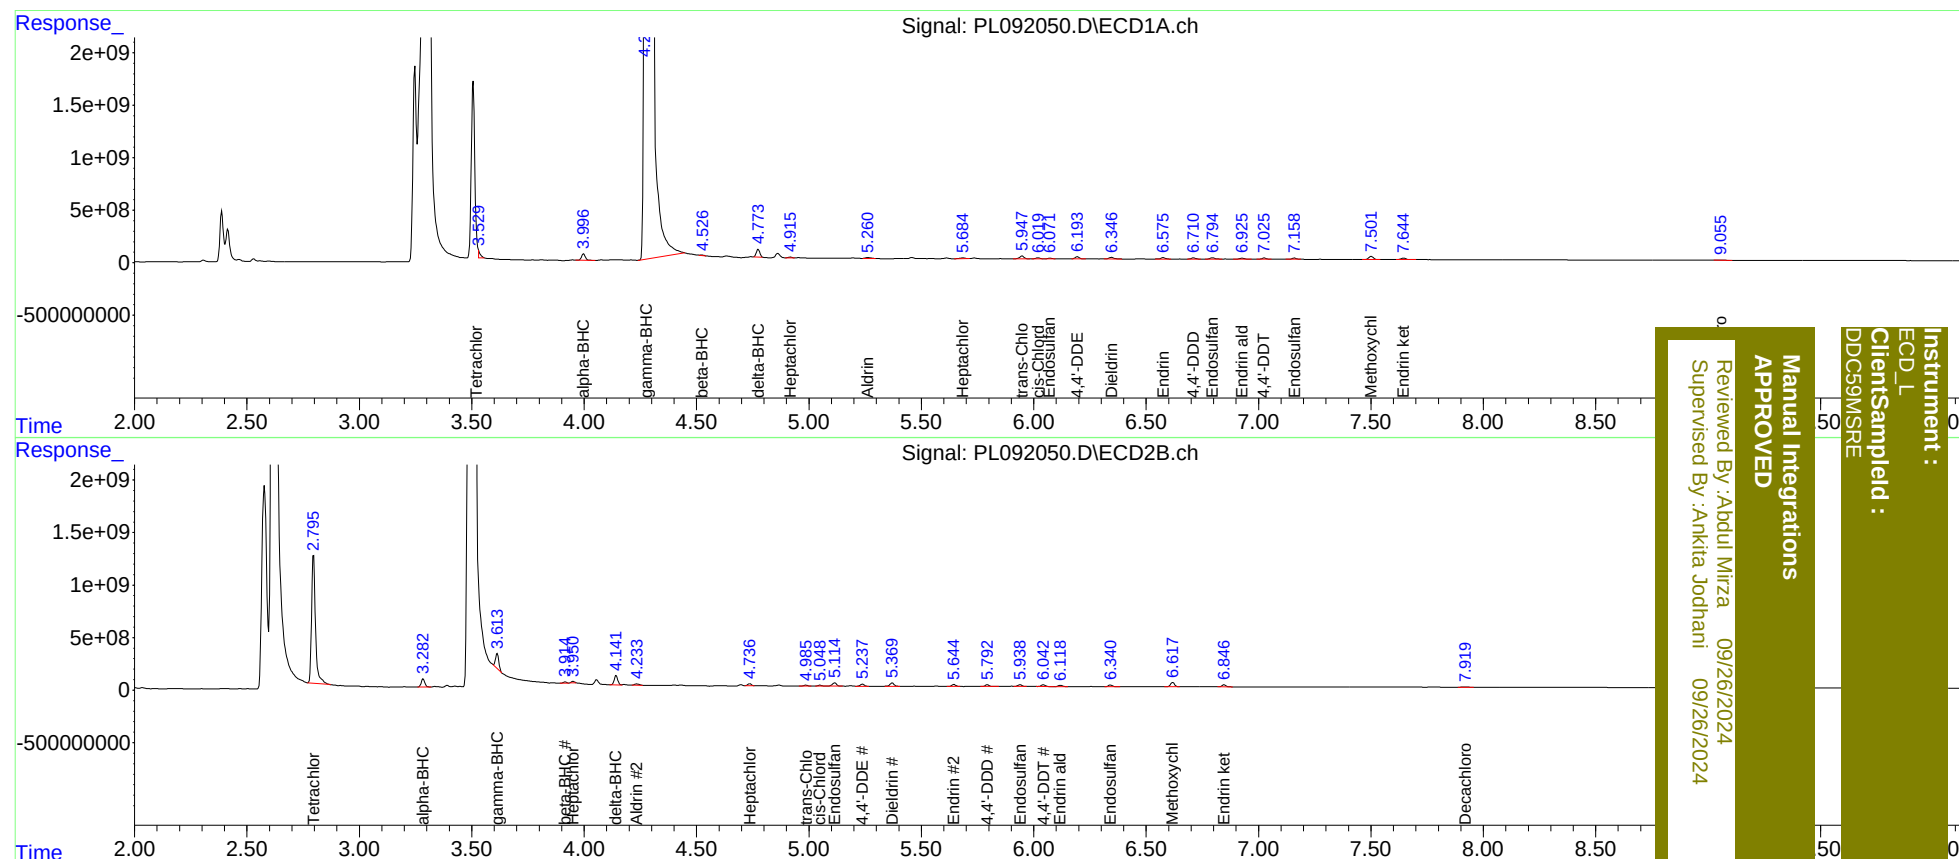

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/26/2024
Supervised By: Ankita Jodhani 09/26/2024

Instrument :
ECD_L
ClientSampled :
DDC59MSRE