

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092618\
 Data File : PL040382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2018 16:21
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 01:08:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:06:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.215	3.807	725.2E6	303.8E6	98.700	99.047
28)	SA Decachlor...	7.821	8.733	886.0E6	294.3E6	96.651	95.604
Target Compounds							
23)	Chlordane-1	4.038	4.768	334.2E6	153.5E6	990.757	996.265
24)	Chlordane-2	4.520	5.223	323.9E6	159.7E6	956.364	975.950
25)	Chlordane-3	5.065	5.854	1268.5E6	552.2E6	986.281	985.911
26)	Chlordane-4	5.118	5.929	1160.3E6	645.4E6	984.993	981.024
27)	Chlordane-5	5.929	6.712	382.6E6	122.0E6	982.071	982.668



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092618\
Data File : PL040382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2018 16:21
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 01:08:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:06:02 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

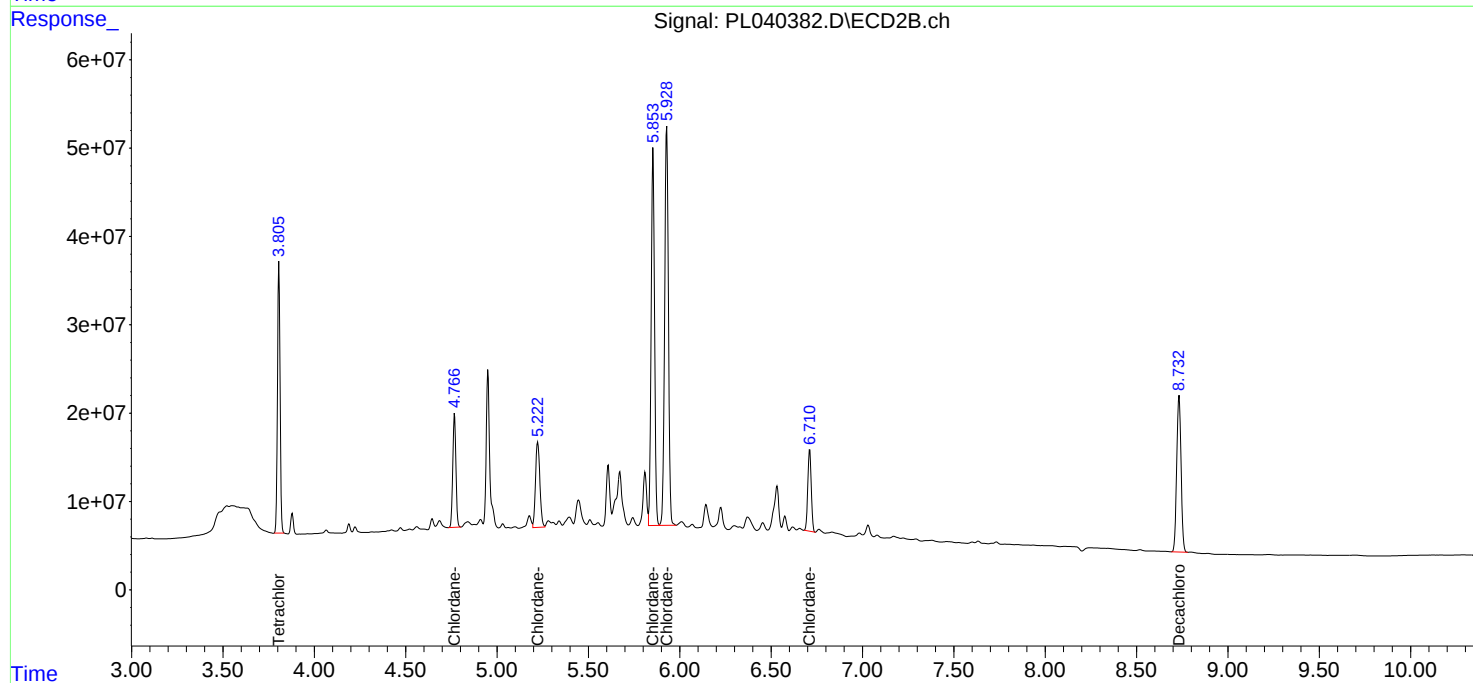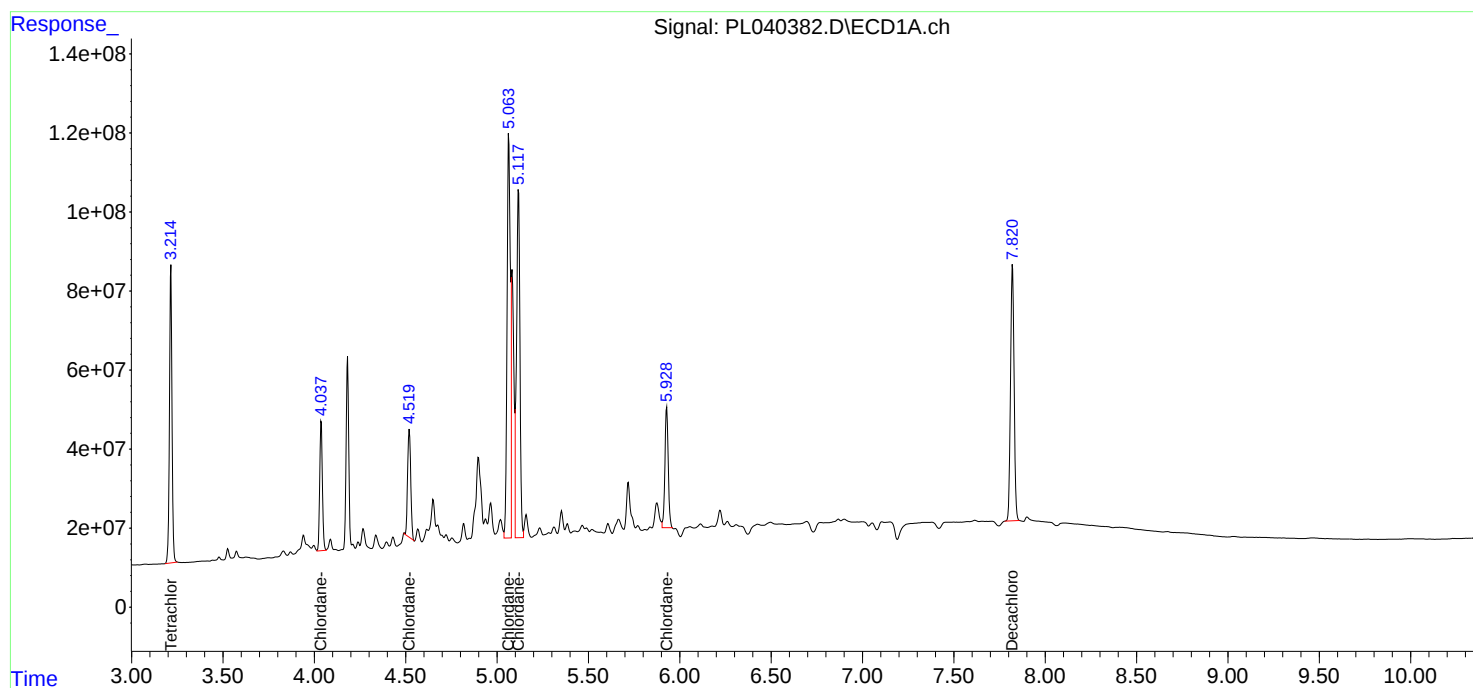


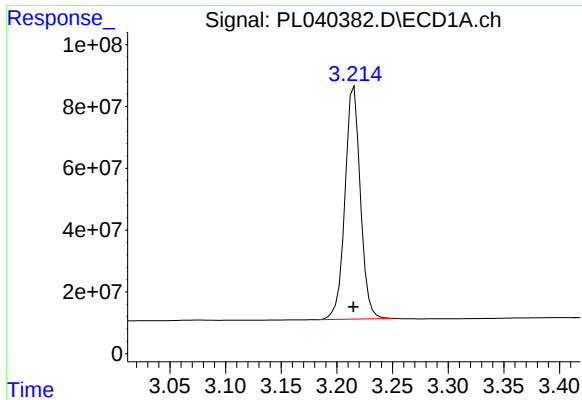

#1 Tetrachloro-m-xylene


R.T.: 3.215 min
Delta R.T.: 0.000 min
Response: 725244964
Conc: 98.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

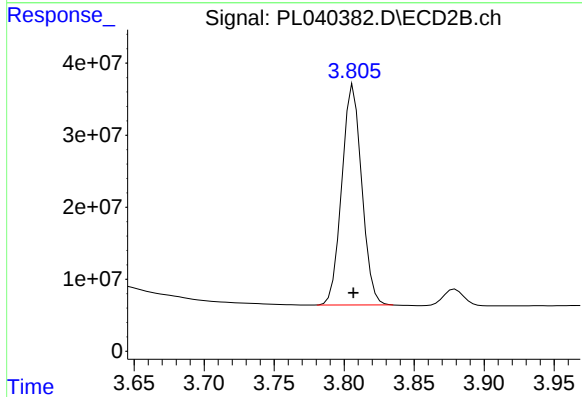


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 303780243
Conc: 99.05 ng/ml

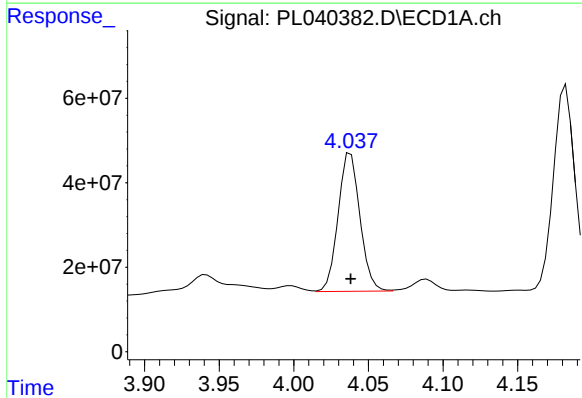


#23 Chlordane-1

R.T.: 4.038 min
Delta R.T.: 0.000 min
Response: 334207794
Conc: 990.76 ng/ml

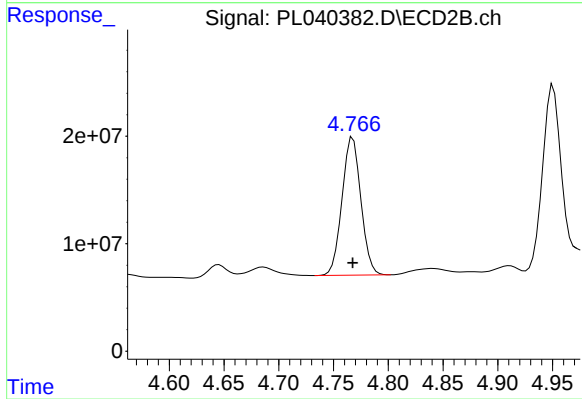

#23 Chlordane-1


R.T.: 4.768 min
Delta R.T.: 0.000 min
Response: 153476999
Conc: 996.27 ng/ml

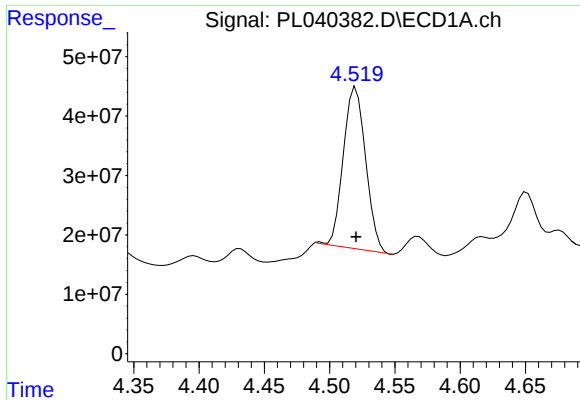

#24 Chlordane-2


R.T.: 4.520 min
Delta R.T.: 0.000 min
Response: 323859018
Conc: 956.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

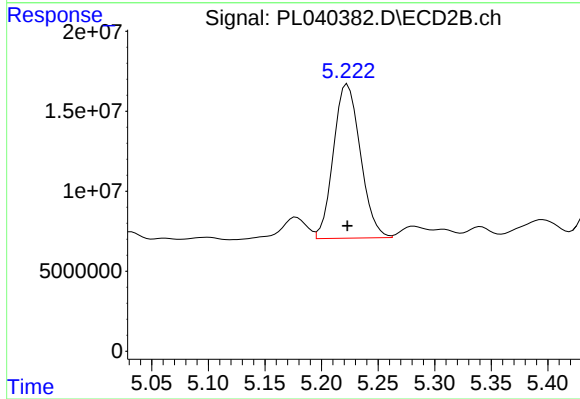


#24 Chlordane-2

R.T.: 5.223 min
Delta R.T.: 0.000 min
Response: 159718641
Conc: 975.95 ng/ml

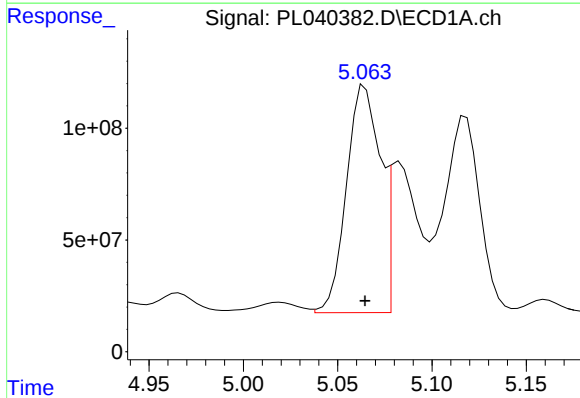


#25 Chlordane-3

R.T.: 5.065 min
Delta R.T.: 0.000 min
Response: 1268519218
Conc: 986.28 ng/ml

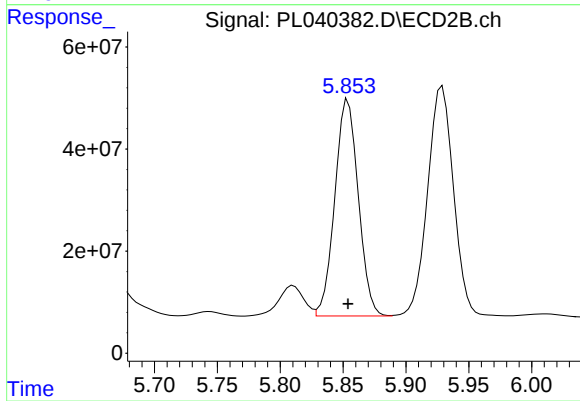

#25 Chlordane-3


R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 552171249
Conc: 985.91 ng/ml

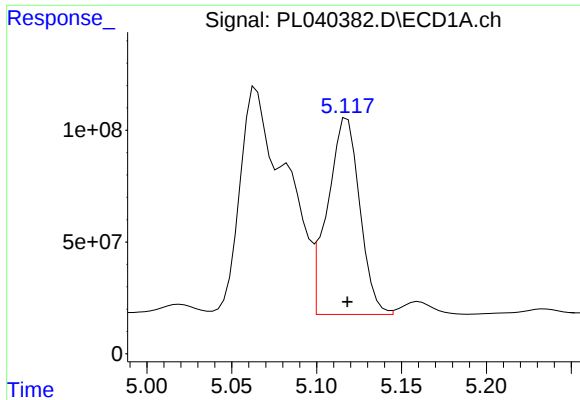

#26 Chlordane-4


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 1160343346
Conc: 984.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

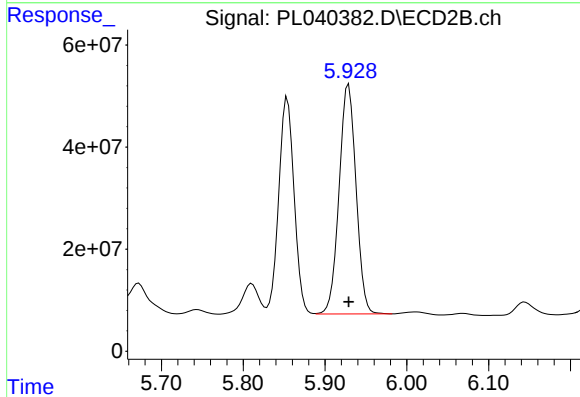


#26 Chlordane-4

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 645379260
Conc: 981.02 ng/ml

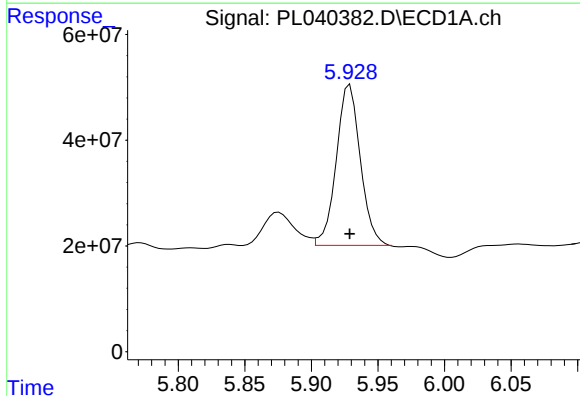


#27 Chlordane-5

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 382617806
Conc: 982.07 ng/ml

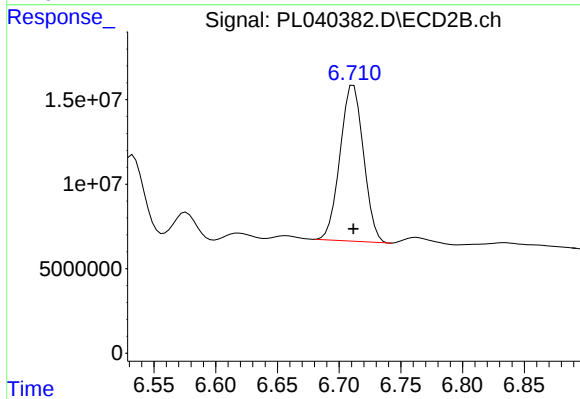

#27 Chlordane-5


R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 121997545
Conc: 982.67 ng/ml

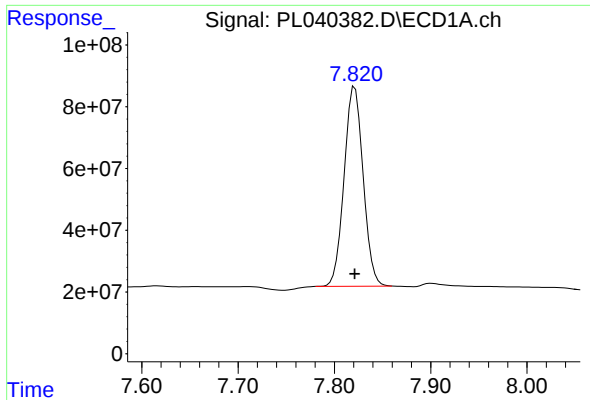

#28 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: 0.000 min
Response: 886037949
Conc: 96.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

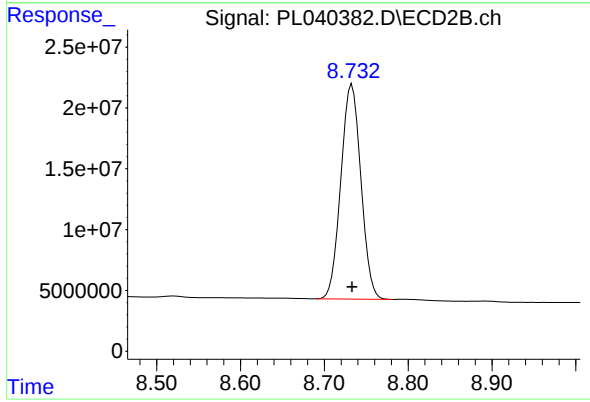

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: 0.000 min
Response: 294272463
Conc: 95.60 ng/ml