

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092618\
 Data File : PL040383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2018 16:35
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Manual Integrations
 APPROVED

Sohil
 9/28/2018 9:52:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 01:10:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:06:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.213	3.808	568.8E6	237.3E6	76.591	76.569
28)	SA Decachlor...	7.818	8.731	680.6E6	228.6E6	74.490	74.502
Target Compounds							
23)	Chlordane-1	4.035	4.768	265.8E6	118.9E6	774.880	764.489
24)	Chlordane-2	4.517	5.224	259.4E6	125.0E6	760.580	759.301
25)	Chlordane-3	5.060	5.854	984.1E6	428.4E6	754.180m	759.856
26)	Chlordane-4	5.115	5.929	899.0E6	500.3E6	758.701	756.927
27)	Chlordane-5	5.926	6.711	299.1E6	93869803	761.753	754.058

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092618\
Data File : PL040383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2018 16:35
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
9/28/2018 9:52:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 01:10:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:06:02 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

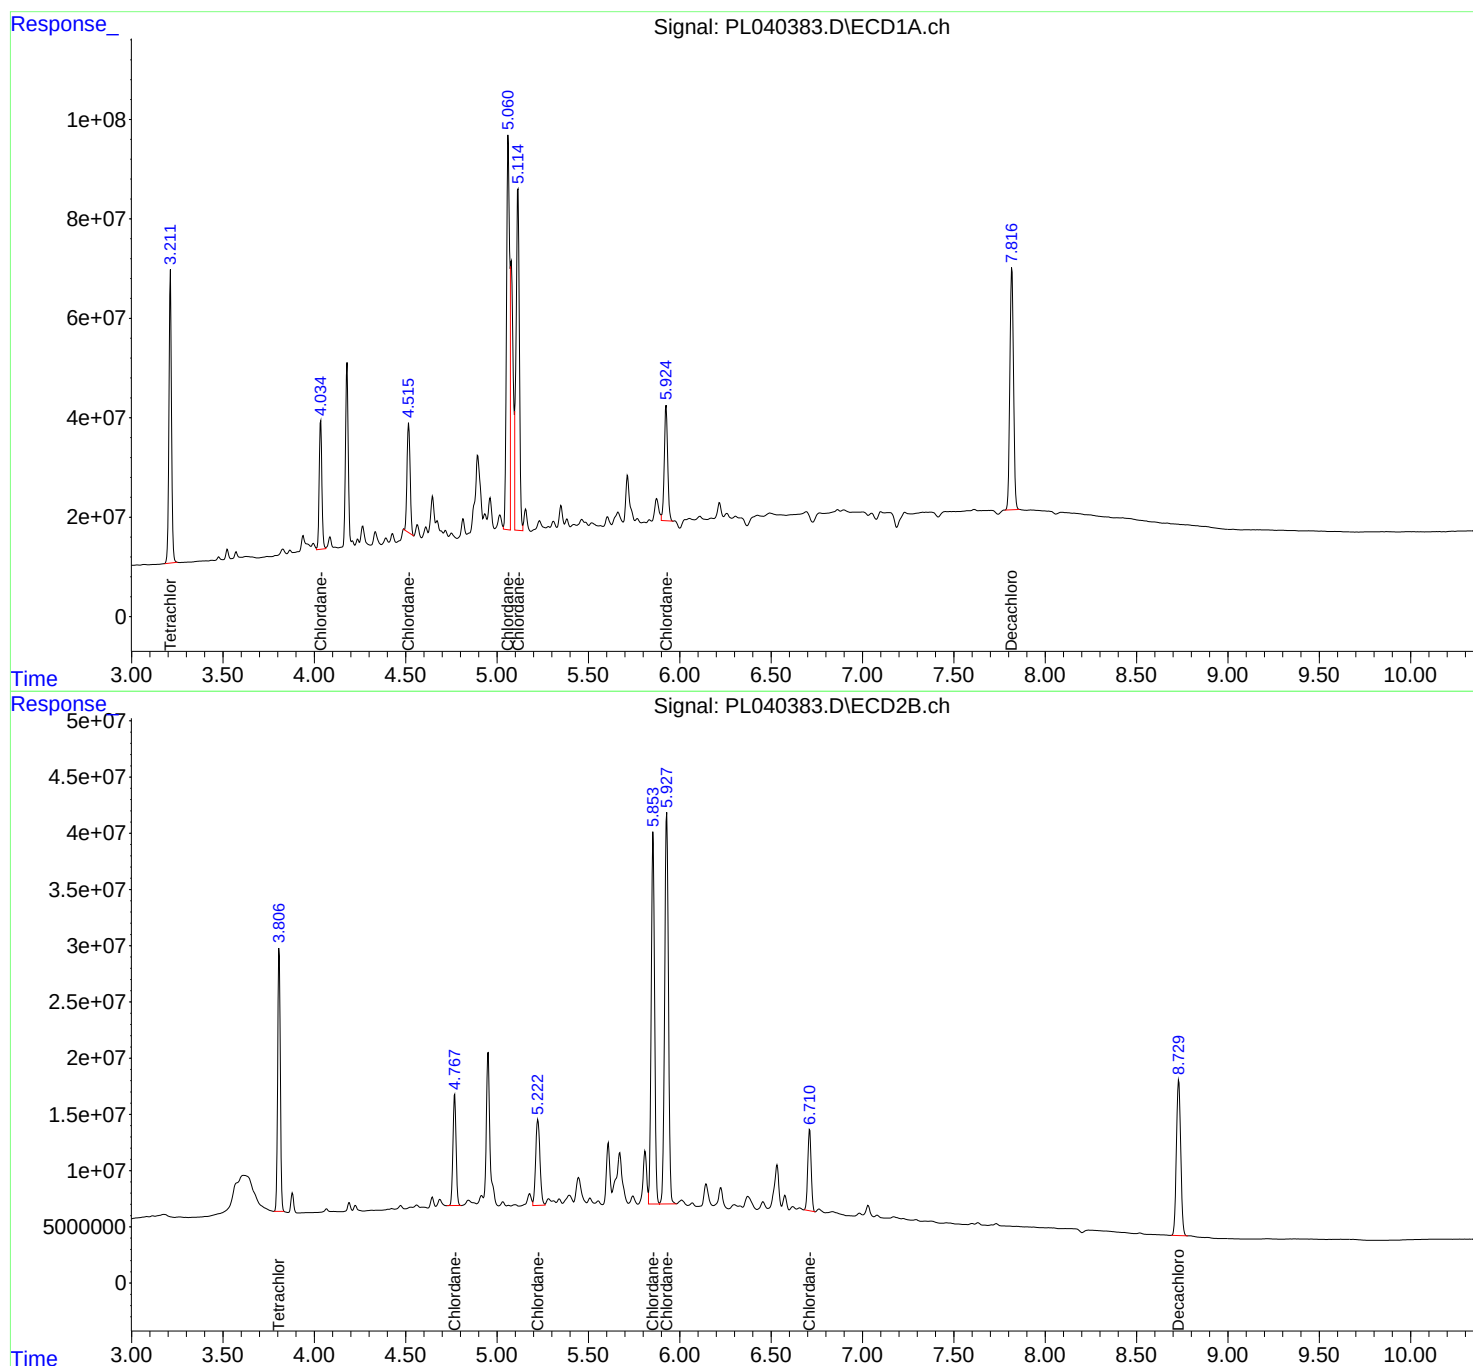

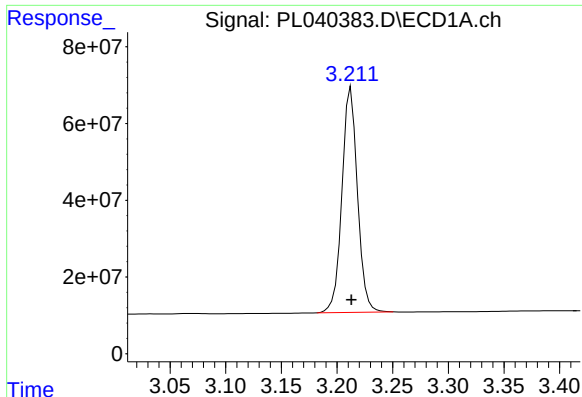


#1 Tetrachloro-m-xylene

R.T.: 3.213 min
Delta R.T.: 0.000 min
Response: 568820351
Conc: 76.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
9/28/2018 9:52:17 AM

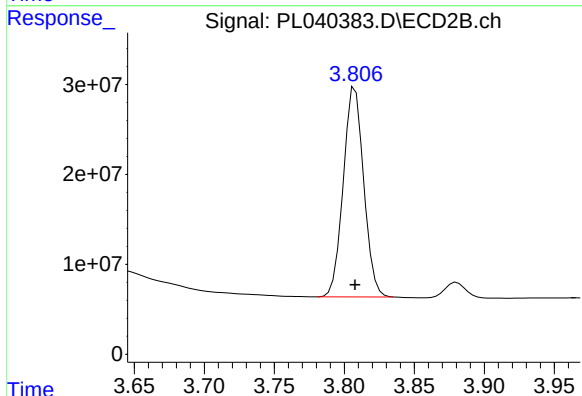


#1 Tetrachloro-m-xylene

R.T.: 3.808 min
Delta R.T.: 0.000 min
Response: 237322124
Conc: 76.57 ng/ml

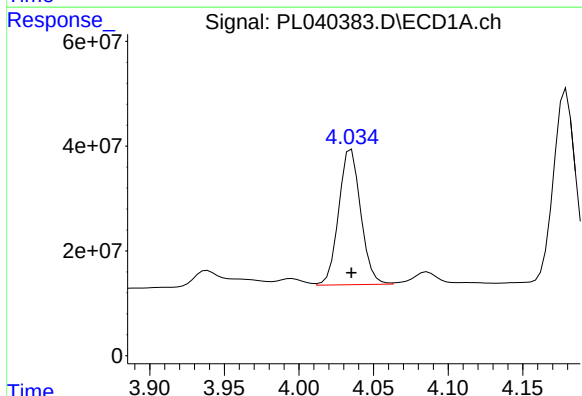


#23 Chlordane-1

R.T.: 4.035 min
Delta R.T.: 0.000 min
Response: 265795448
Conc: 774.88 ng/ml

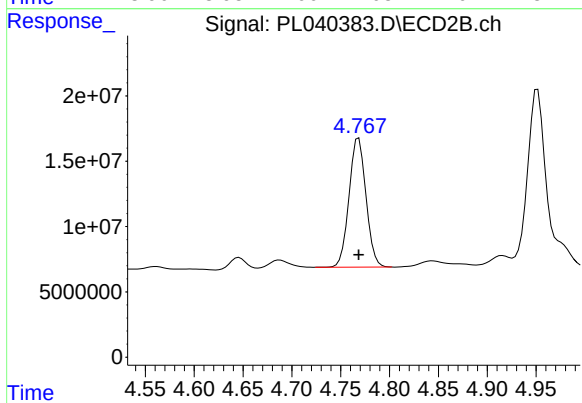

#23 Chlordane-1

R.T.: 4.768 min
Delta R.T.: 0.000 min
Response: 118919891
Conc: 764.49 ng/ml

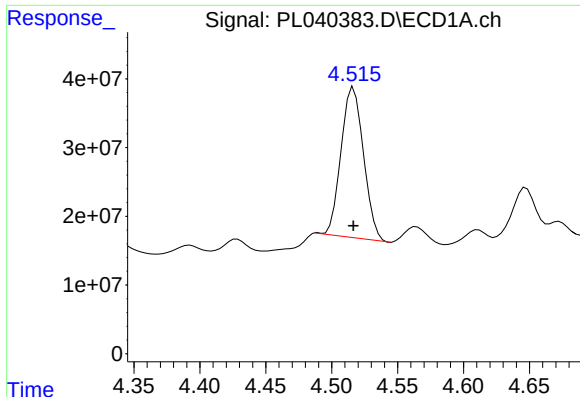


#24 Chlordane-2

R.T.: 4.517 min
Delta R.T.: 0.000 min
Response: 259389151
Conc: 760.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
9/28/2018 9:52:17 AM

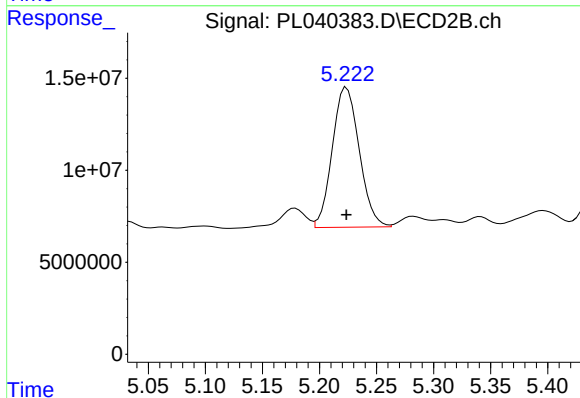


#24 Chlordane-2

R.T.: 5.224 min
Delta R.T.: 0.000 min
Response: 125038345
Conc: 759.30 ng/ml

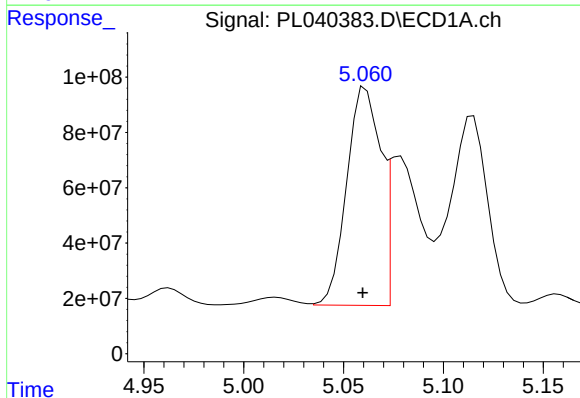


#25 Chlordane-3

R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 984112576
Conc: 754.18 ng/ml m

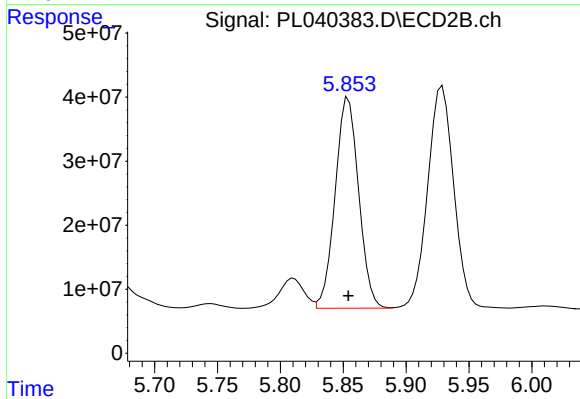

#25 Chlordane-3

R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 428381460
Conc: 759.86 ng/ml

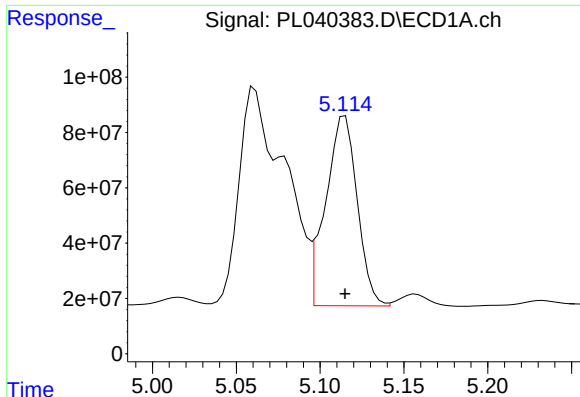


#26 Chlordane-4

R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 898981952
Conc: 758.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
9/28/2018 9:52:17 AM

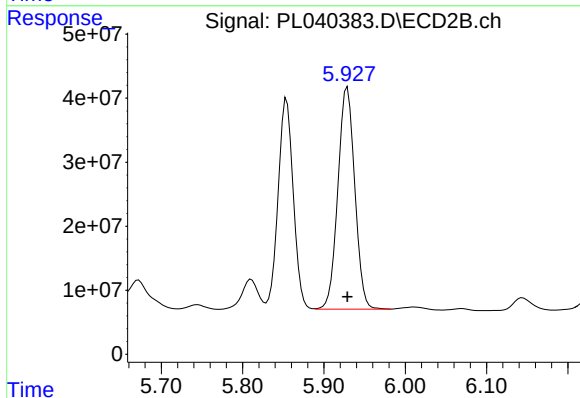


#26 Chlordane-4

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 500264337
Conc: 756.93 ng/ml

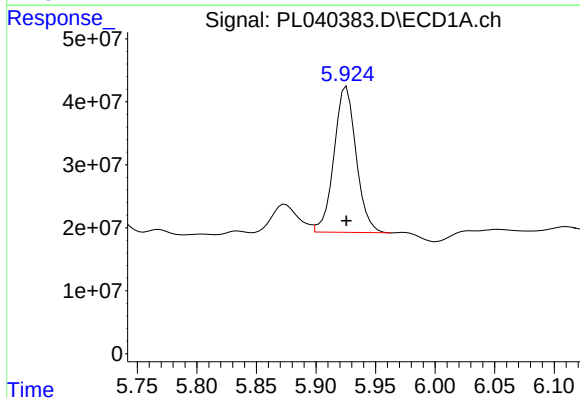


#27 Chlordane-5

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 299125068
Conc: 761.75 ng/ml

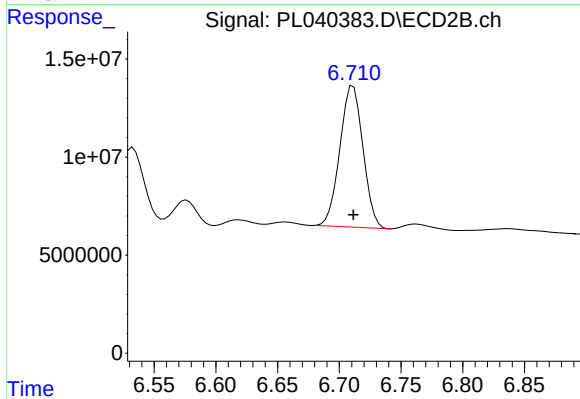

#27 Chlordane-5

R.T.: 6.711 min
Delta R.T.: 0.000 min
Response: 93869803
Conc: 754.06 ng/ml

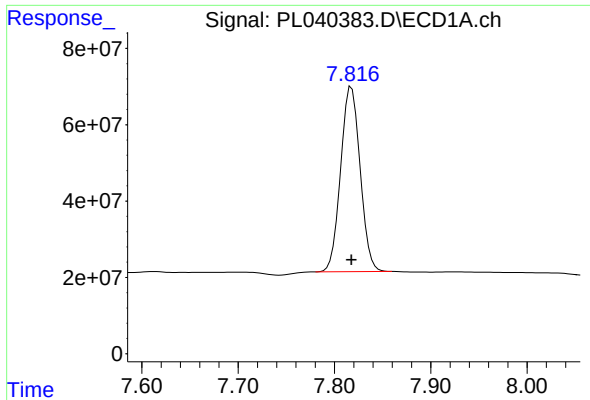


#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 680565988
Conc: 74.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Manual Integrations
APPROVED

Sohil
9/28/2018 9:52:17 AM

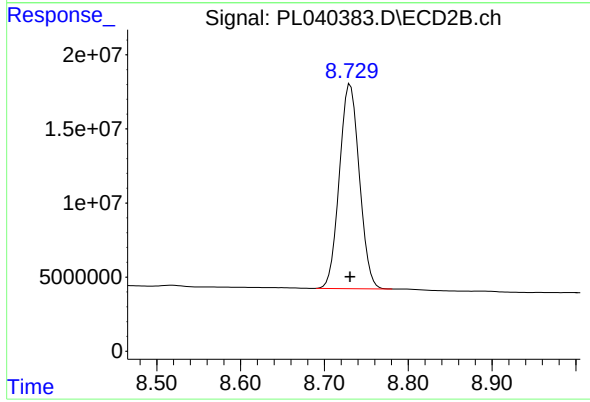

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 228561608
Conc: 74.50 ng/ml