

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092618\
 Data File : PL040384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2018 16:49
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 01:06:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:06:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.212	3.807	372.2E6	154.8E6	50.000	50.000
28)	SA Decachlor...	7.817	8.731	473.7E6	160.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.035	4.768	170.2E6	77313839	500.000	500.000
24)	Chlordane-2	4.516	5.223	176.7E6	83795187	500.000	500.000
25)	Chlordane-3	5.061	5.854	651.9E6	284.0E6	500.000	500.000
26)	Chlordane-4	5.114	5.928	597.9E6	335.2E6	500.000	500.000
27)	Chlordane-5	5.925	6.710	198.3E6	63150561	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092618\
Data File : PL040384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2018 16:49
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 01:06:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:06:02 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

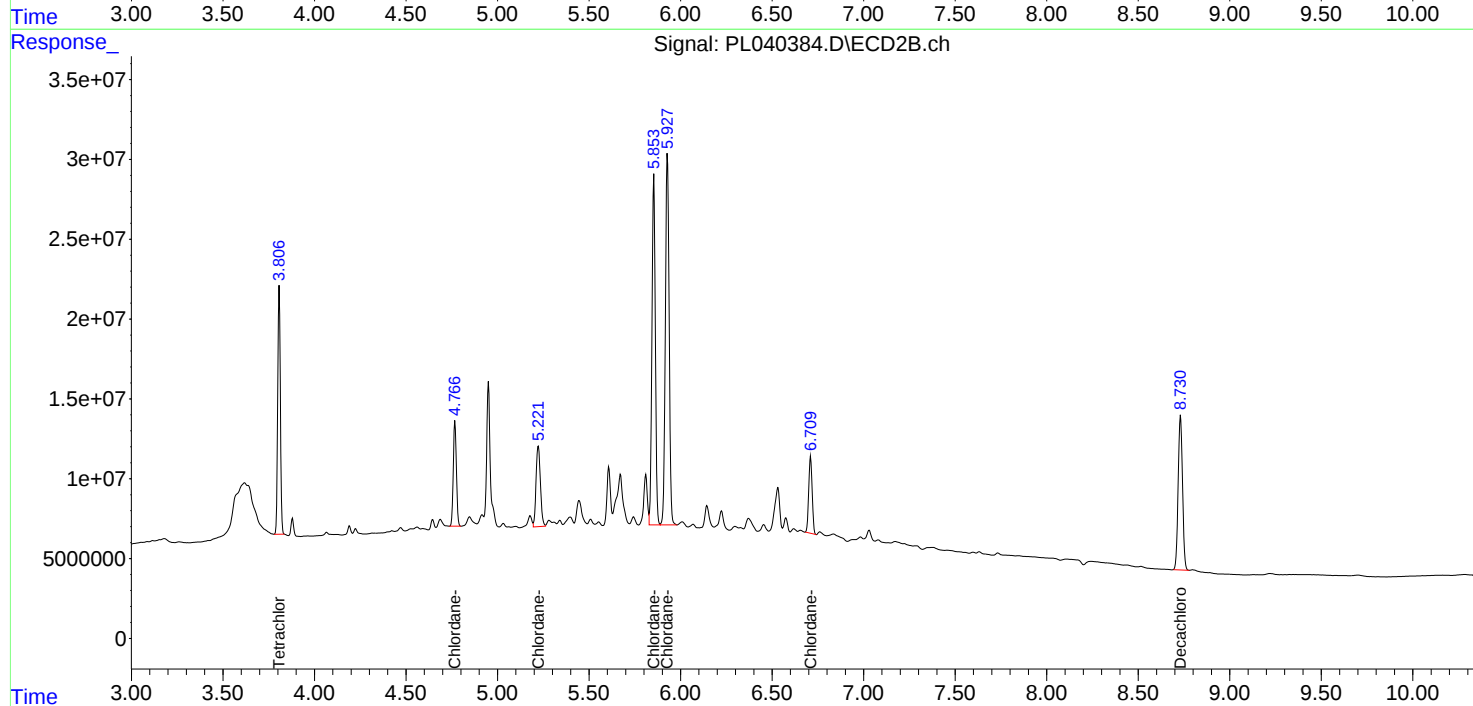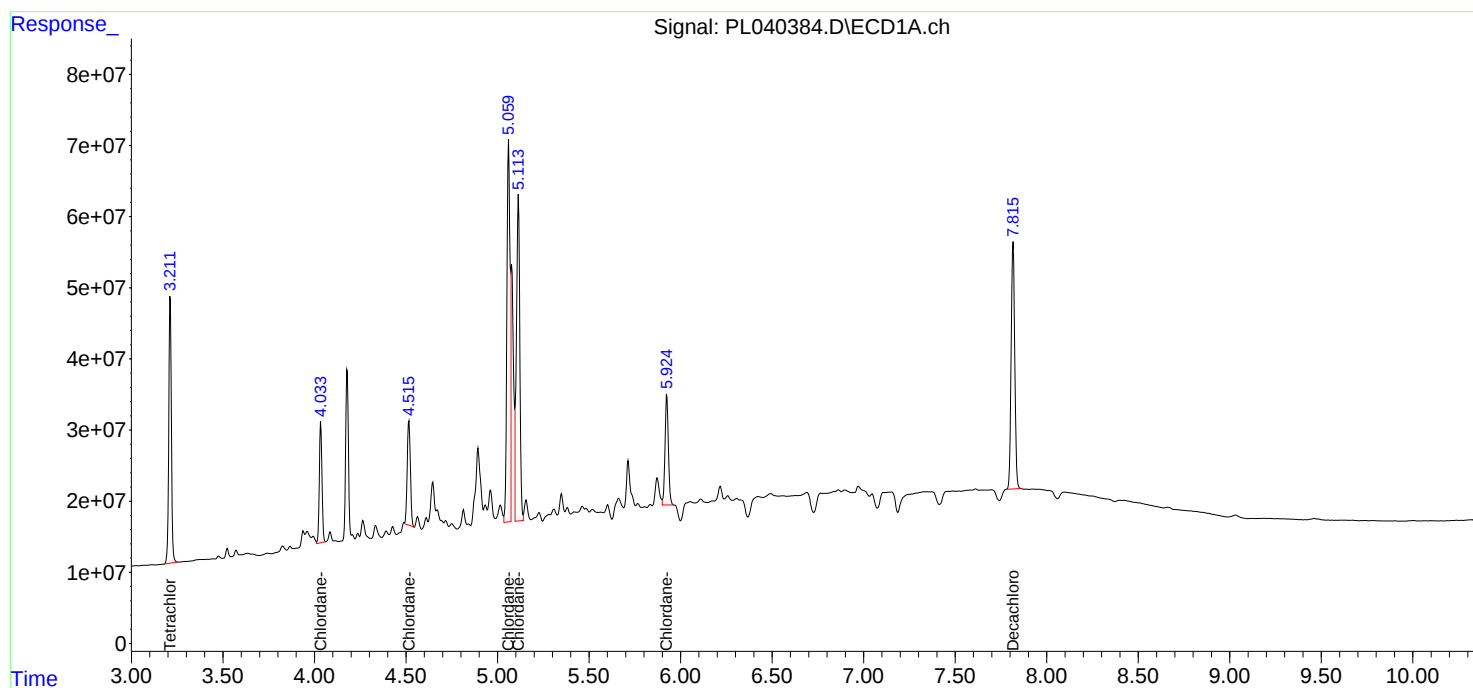


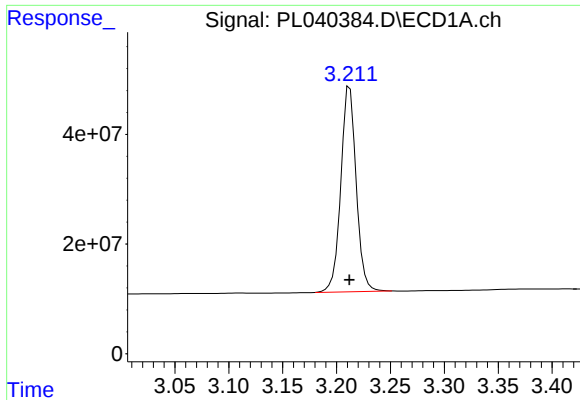

#1 Tetrachloro-m-xylene


R.T.: 3.212 min
Delta R.T.: 0.000 min
Response: 372177752
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

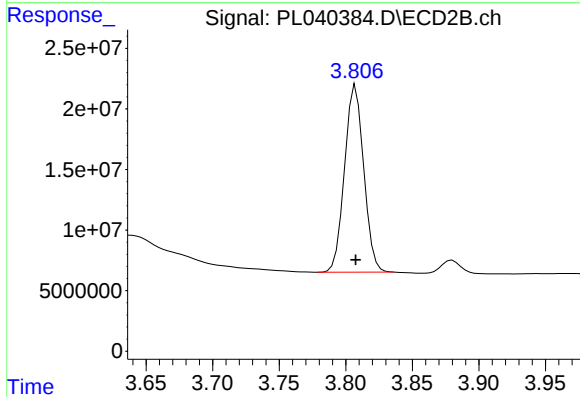


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 154811790
Conc: 50.00 ng/ml

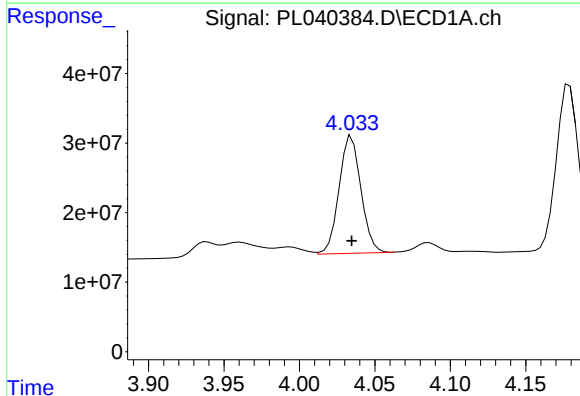


#23 Chlordane-1

R.T.: 4.035 min
Delta R.T.: 0.000 min
Response: 170221917
Conc: 500.00 ng/ml

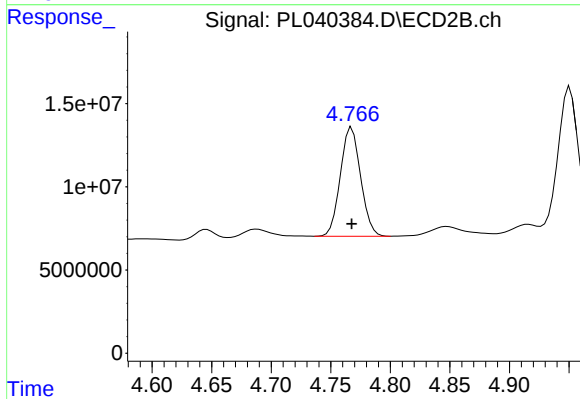

#23 Chlordane-1


R.T.: 4.768 min
Delta R.T.: 0.000 min
Response: 77313839
Conc: 500.00 ng/ml

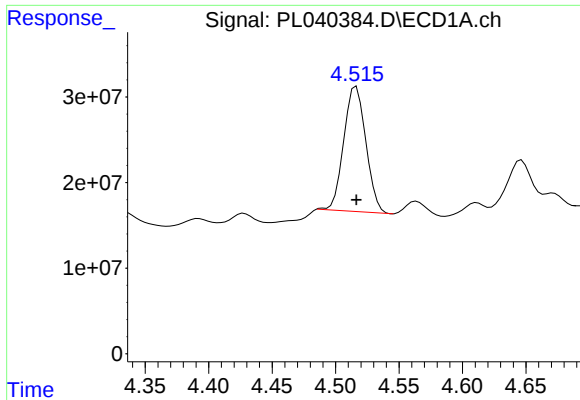

#24 Chlordane-2


R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 176706090
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

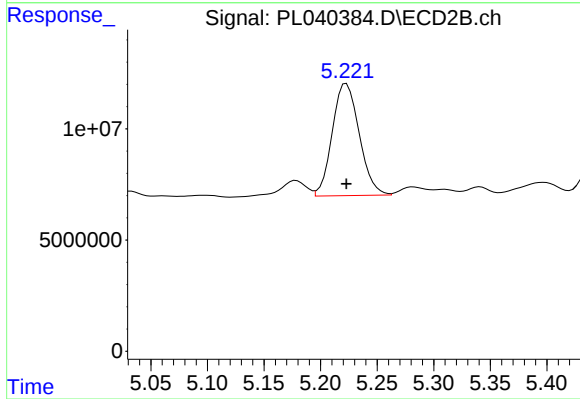


#24 Chlordane-2

R.T.: 5.223 min
Delta R.T.: 0.000 min
Response: 83795187
Conc: 500.00 ng/ml

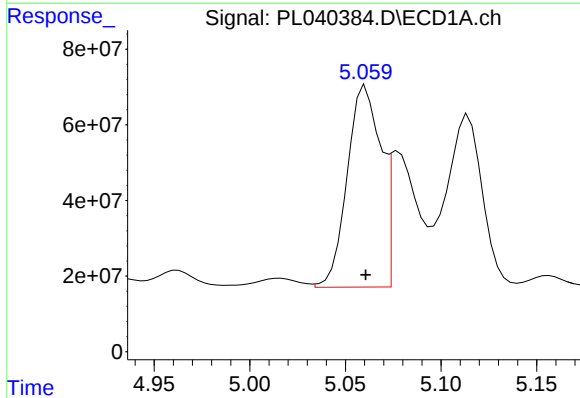


#25 Chlordane-3

R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 651904082
Conc: 500.00 ng/ml

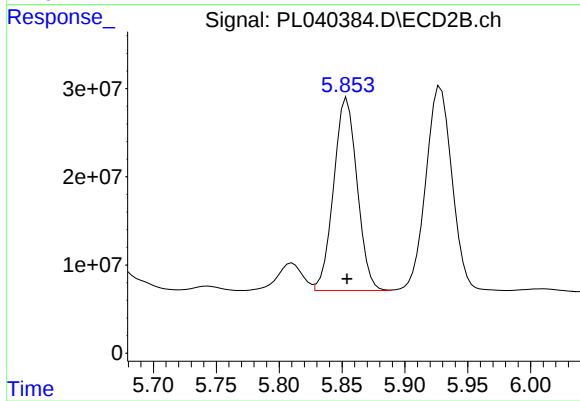

#25 Chlordane-3


R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 283976158
Conc: 500.00 ng/ml

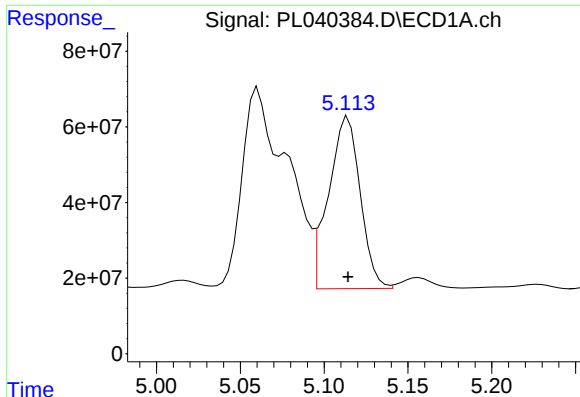

#26 Chlordane-4


R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 597850253
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

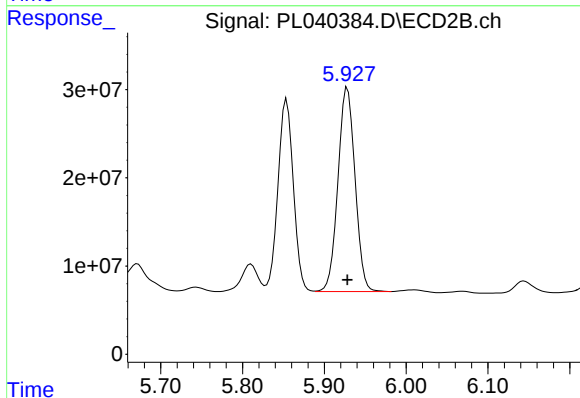


#26 Chlordane-4

R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 335173257
Conc: 500.00 ng/ml

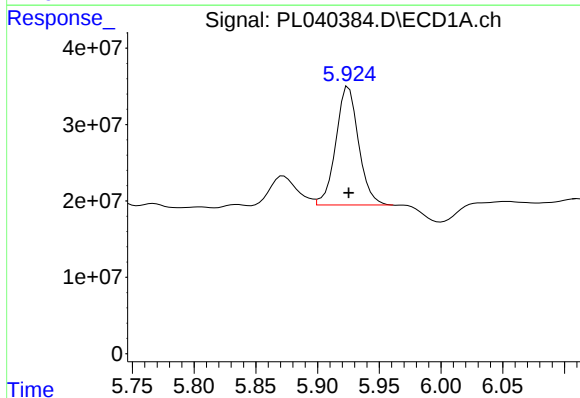


#27 Chlordane-5

R.T.: 5.925 min
Delta R.T.: 0.000 min
Response: 198294146
Conc: 500.00 ng/ml

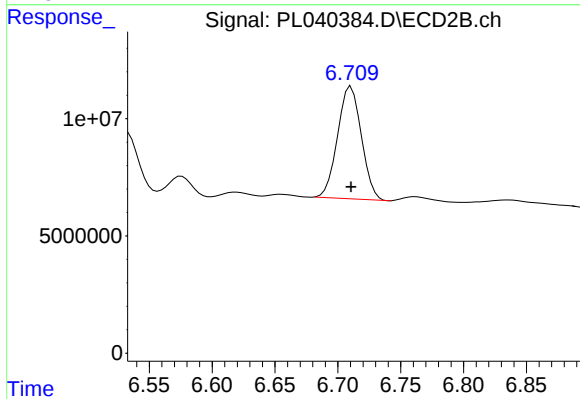

#27 Chlordane-5


R.T.: 6.710 min
Delta R.T.: 0.000 min
Response: 63150561
Conc: 500.00 ng/ml

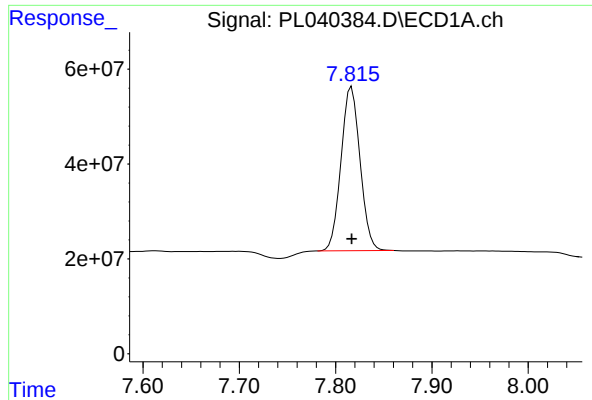

#28 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: 0.000 min
Response: 473723523
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

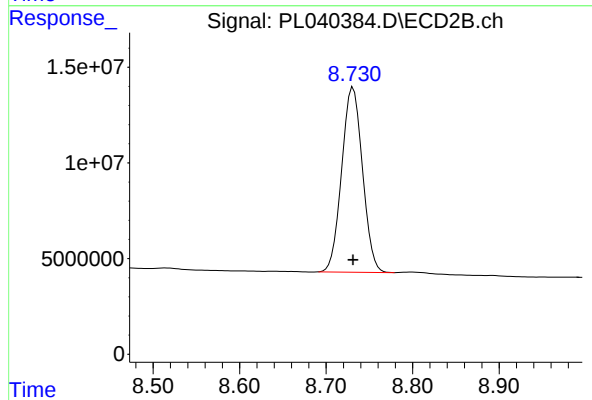

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 160666612
Conc: 50.00 ng/ml