

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092618\
 Data File : PL040393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2018 18:56
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL092618CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 01:16:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:06:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.807	374.8E6	153.4E6	50.325	49.877
28)	SA Decachlor...	7.817	8.732	474.3E6	159.2E6	50.447	50.091
Target Compounds							
23)	Chlordane-1	4.034	4.768	170.4E6	76560889	483.373	496.094
24)	Chlordane-2	4.516	5.223	176.0E6	83028399	469.289	493.430
25)	Chlordane-3	5.060	5.854	644.8E6	279.3E6	501.972	500.726
26)	Chlordane-4	5.114	5.928	606.7E6	327.4E6	512.054	496.139
27)	Chlordane-5	5.924	6.711	204.2E6	61821385	505.929	507.698



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092618\
Data File : PL040393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2018 18:56
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL092618CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 01:16:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:06:02 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

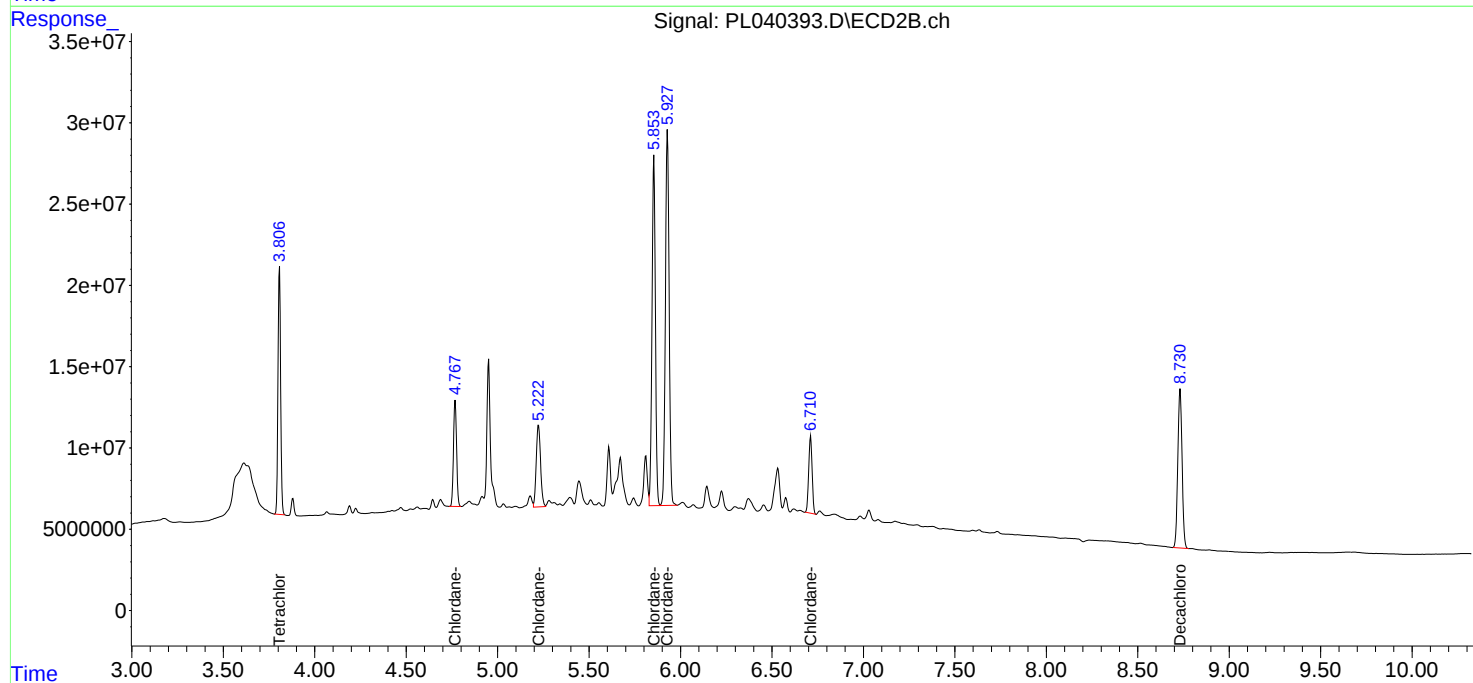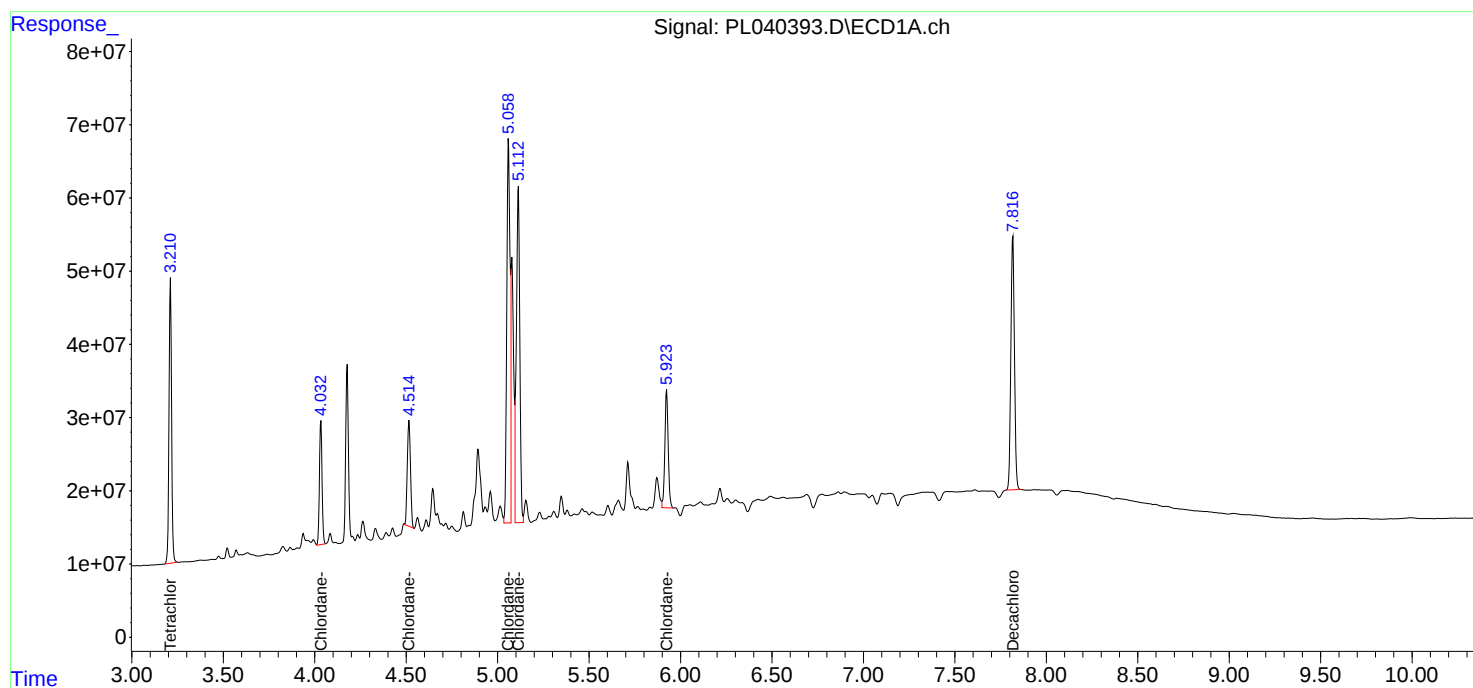


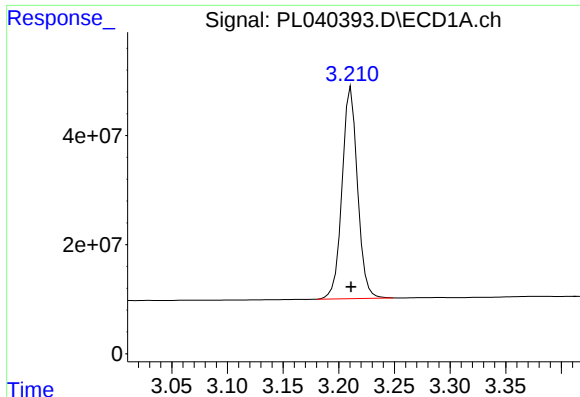

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: 0.000 min
Response: 374843813
Conc: 50.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092618CHLOR

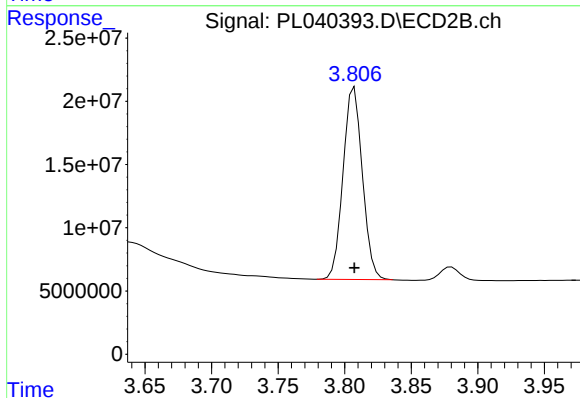


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 153391932
Conc: 49.88 ng/ml

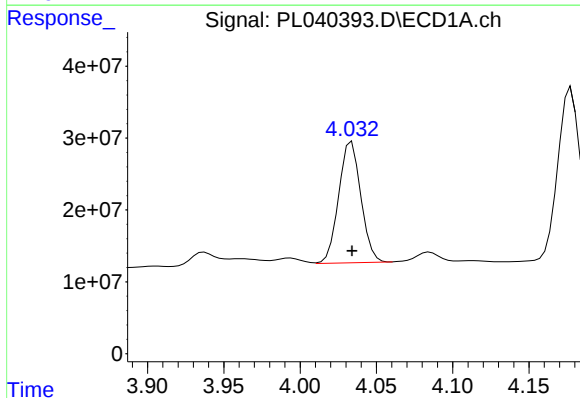


#23 Chlordane-1

R.T.: 4.034 min
Delta R.T.: 0.000 min
Response: 170394599
Conc: 483.37 ng/ml

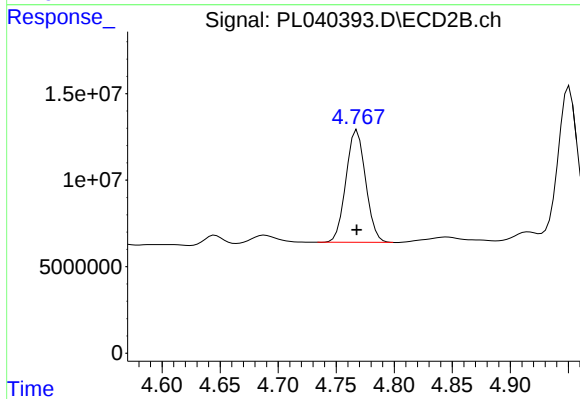

#23 Chlordane-1


R.T.: 4.768 min
Delta R.T.: 0.000 min
Response: 76560889
Conc: 496.09 ng/ml

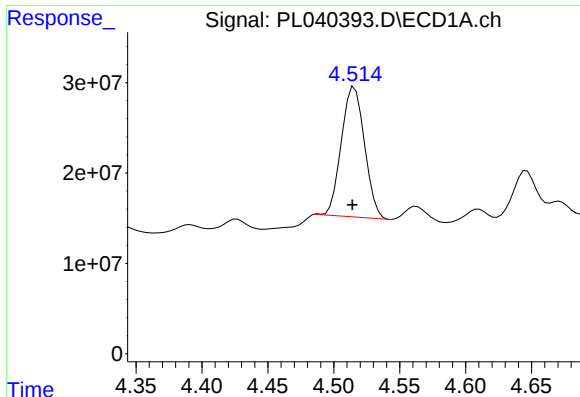

#24 Chlordane-2


R.T.: 4.516 min
Delta R.T.: 0.002 min
Response: 176027436
Conc: 469.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092618CHLOR

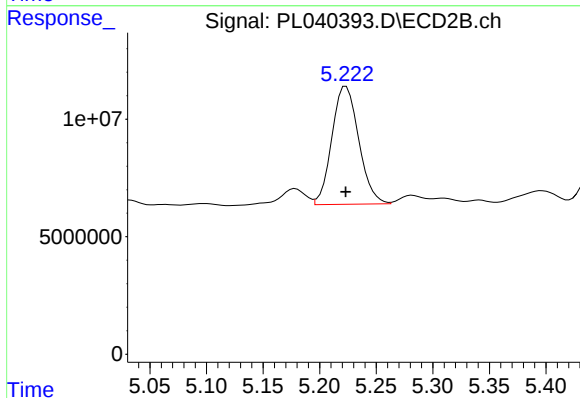


#24 Chlordane-2

R.T.: 5.223 min
Delta R.T.: 0.000 min
Response: 83028399
Conc: 493.43 ng/ml

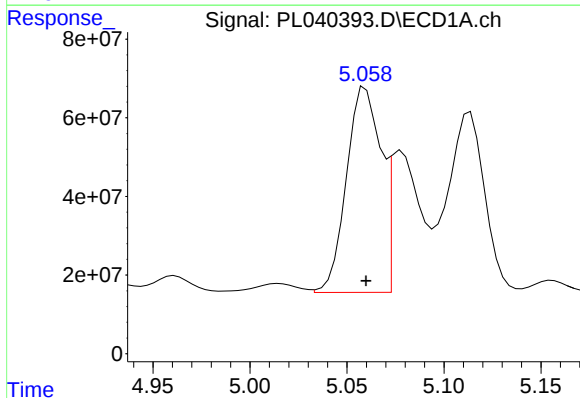


#25 Chlordane-3

R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 644804370
Conc: 501.97 ng/ml

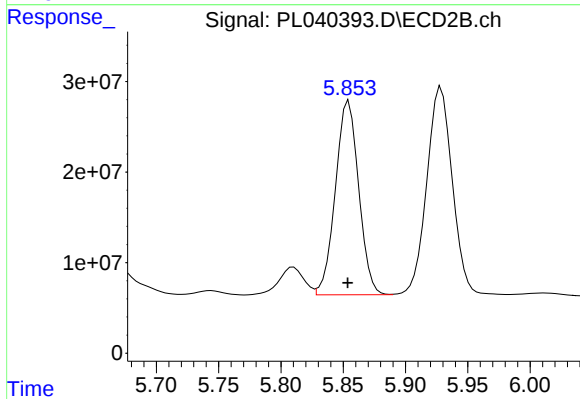

#25 Chlordane-3


R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 279261873
Conc: 500.73 ng/ml

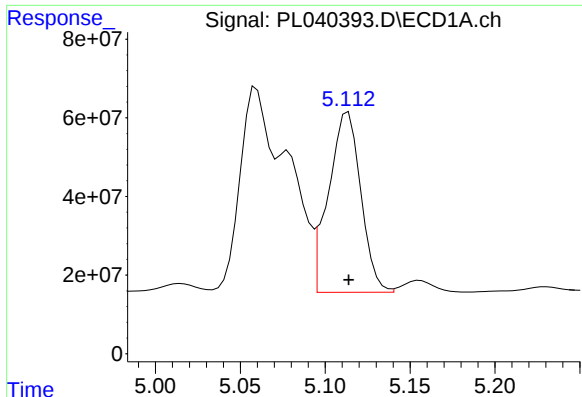

#26 Chlordane-4


R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 606735193
Conc: 512.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092618CHLOR

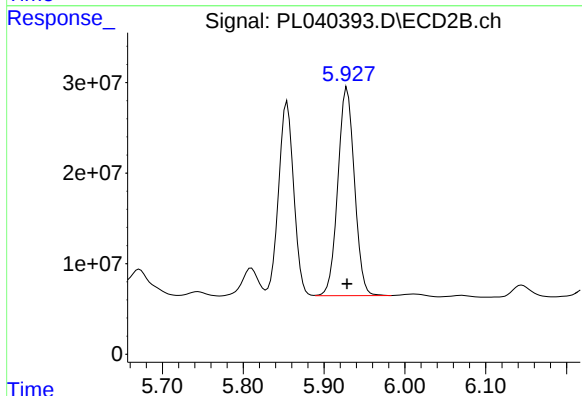


#26 Chlordane-4

R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 327433099
Conc: 496.14 ng/ml

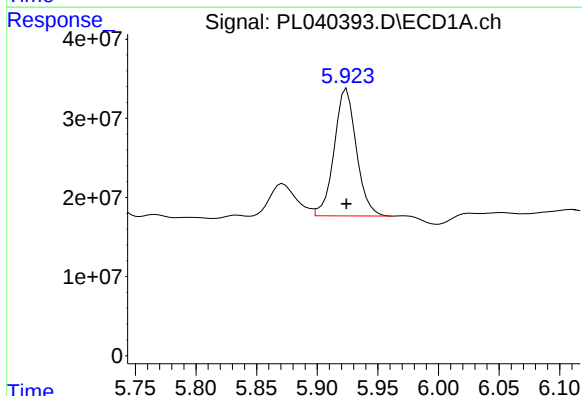


#27 Chlordane-5

R.T.: 5.924 min
Delta R.T.: 0.000 min
Response: 204220204
Conc: 505.93 ng/ml

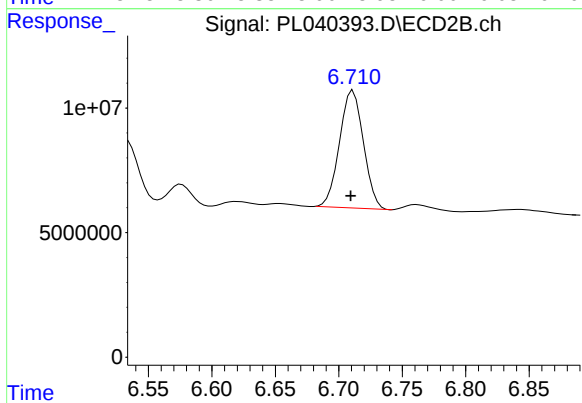

#27 Chlordane-5


R.T.: 6.711 min
Delta R.T.: 0.002 min
Response: 61821385
Conc: 507.70 ng/ml

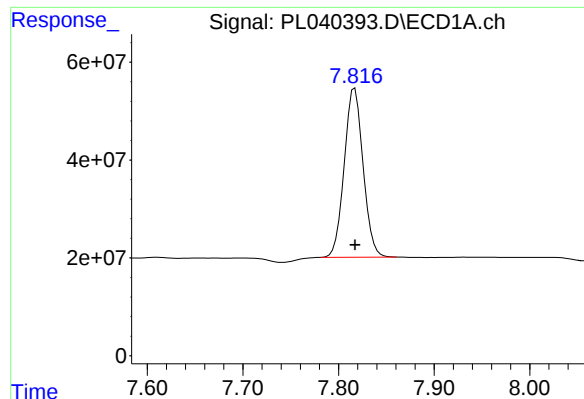

#28 Decachlorobiphenyl

R.T.: 7.817 min
Delta R.T.: 0.000 min
Response: 474251615
Conc: 50.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092618CHLOR

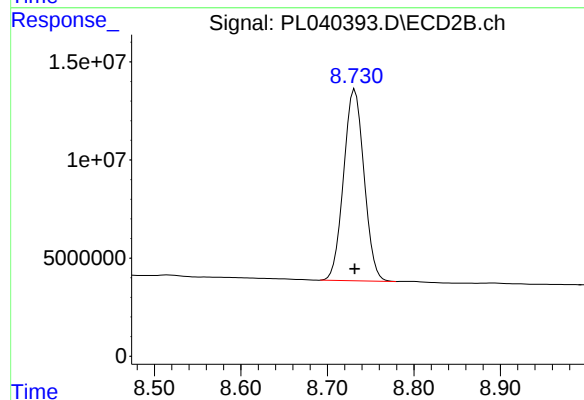

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: 0.000 min
Response: 159234124
Conc: 50.09 ng/ml