

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092619\
 Data File : PL052742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2019 09:01
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 00:45:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	0.000	4.734	0	239669	N.D.	0.083 #
6) B	beta-BHC	0.000	4.907f	0	2341921	N.D.	1.756 #
8) B	Heptachlo...	5.279	0.000	400.4E6	0	39.190	N.D. #
10) B	gamma-Chl...	0.000	6.152	0	1627262	N.D.	0.640 #
11) B	alpha-Chl...	5.585	0.000	1883.8E6	0	182.235	N.D. #
13) MA	Dieldrin	0.000	6.536	0	3209957	N.D.	1.314 #
22)	Mirex	7.476	0.000	298.4E6	0	39.017	N.D. #
25)	Chlordane-3	0.000	6.152	0	1627262	N.D.	5.318 #
26)	Chlordane-4	5.585	0.000	1883.8E6	0	2393.832	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092619\
Data File : PL052742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2019 09:01
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 00:45:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

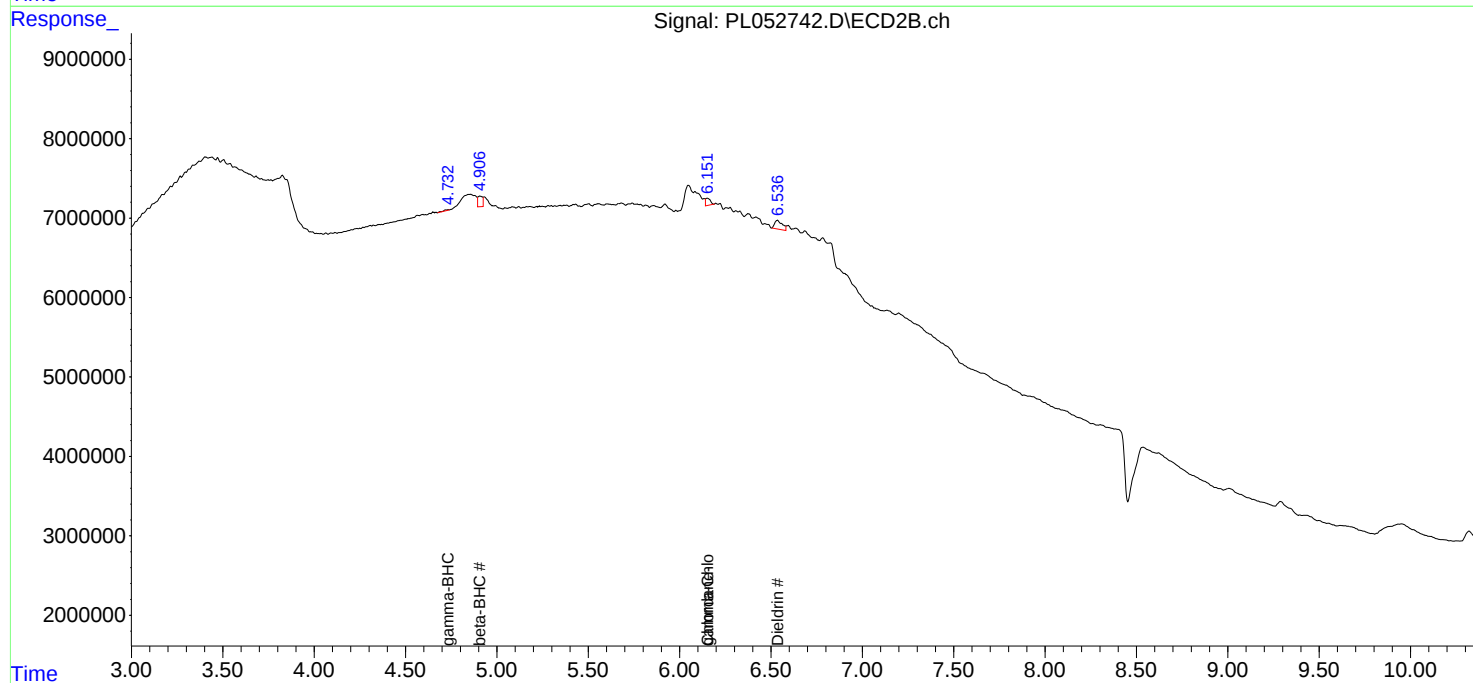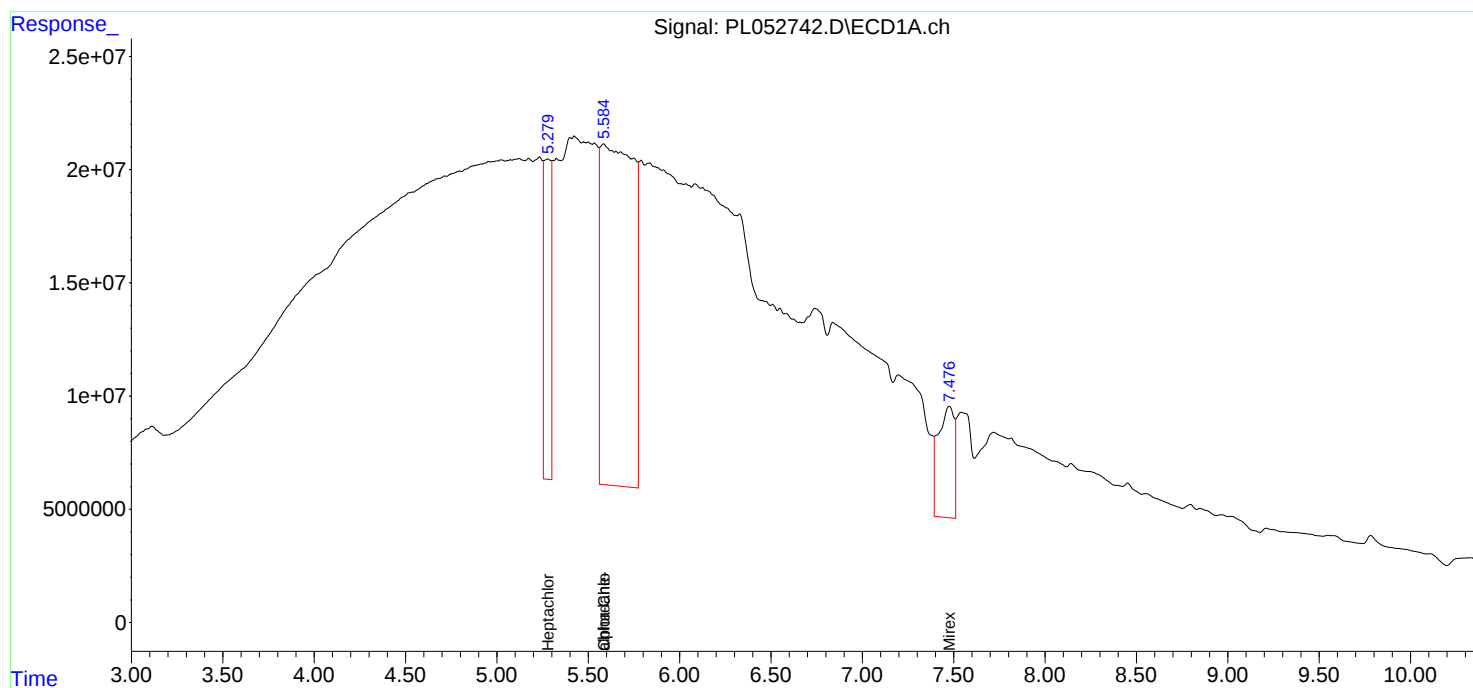


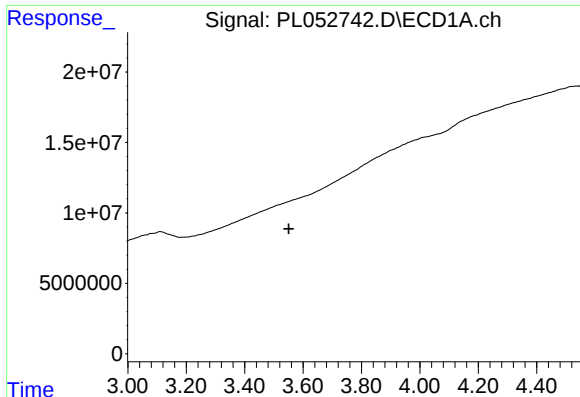

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

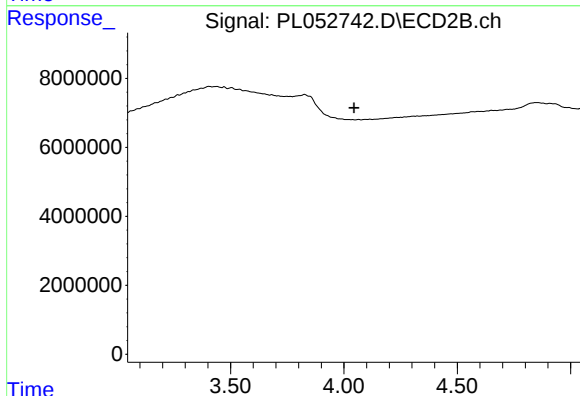


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.045 min
Response: 0
Conc: N.D.

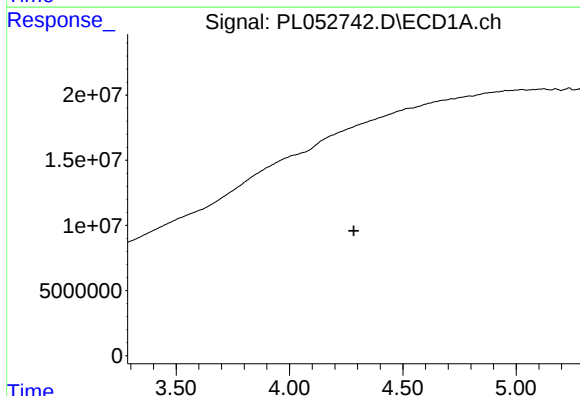


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.284 min
Response: 0
Conc: N.D.

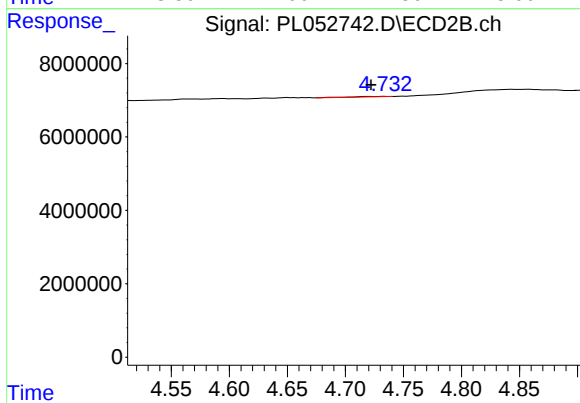

#3 gamma-BHC (Lindane)


R.T.: 4.734 min
Delta R.T.: 0.011 min
Response: 239669
Conc: 0.08 ng/ml

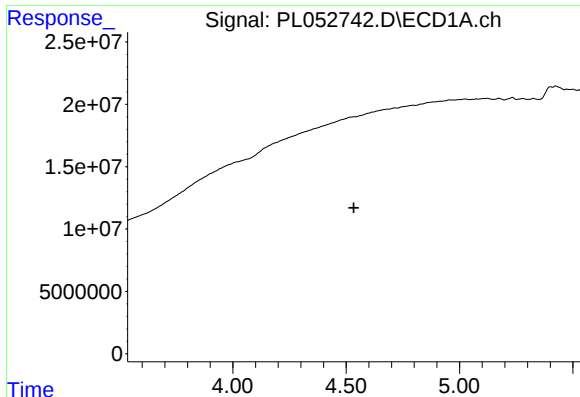

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

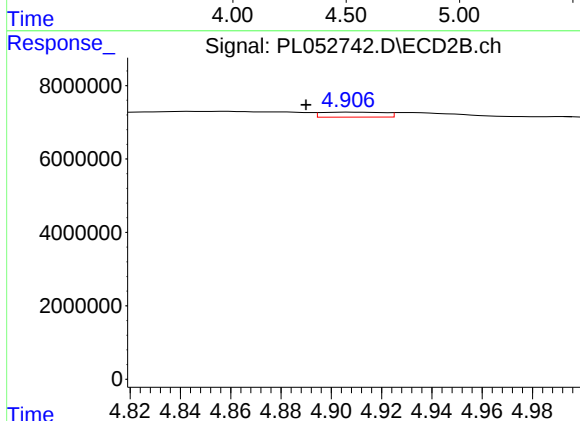


#6 beta-BHC

R.T.: 4.907 min
Delta R.T.: 0.018 min
Response: 2341921
Conc: 1.76 ng/ml

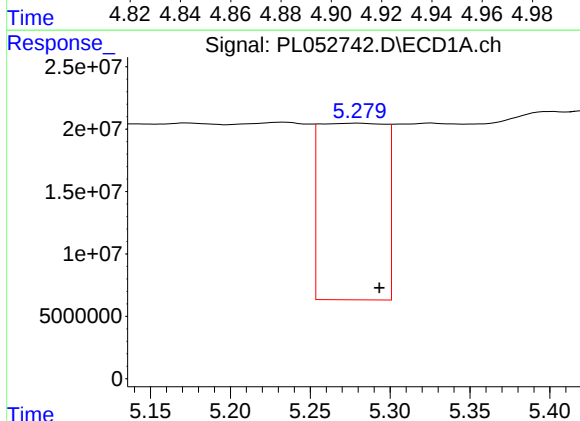


#8 Heptachlor epoxide

R.T.: 5.279 min
Delta R.T.: -0.014 min
Response: 400409780
Conc: 39.19 ng/ml

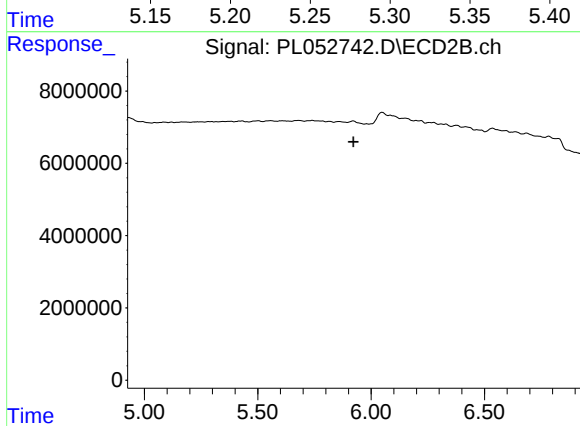

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.922 min
Response: 0
Conc: N.D.

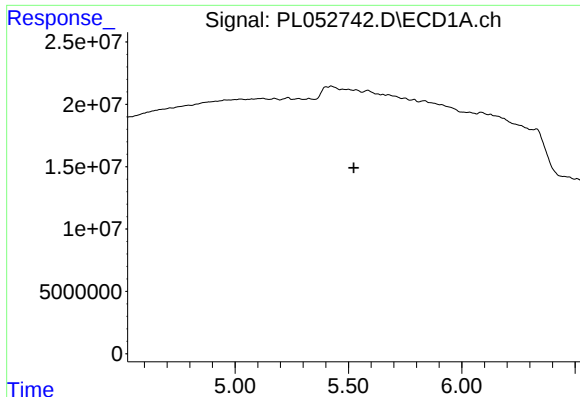

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

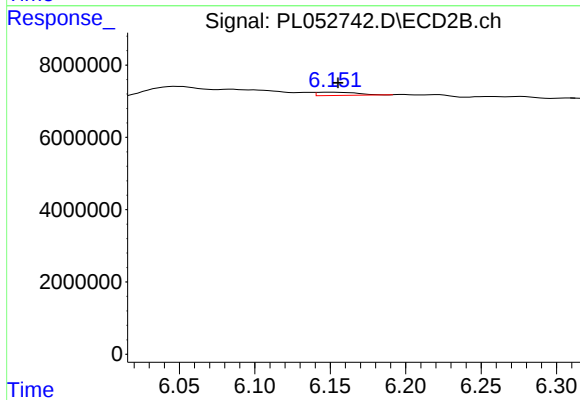


#10 gamma-Chlordane

R.T.: 6.152 min
Delta R.T.: -0.003 min
Response: 1627262
Conc: 0.64 ng/ml

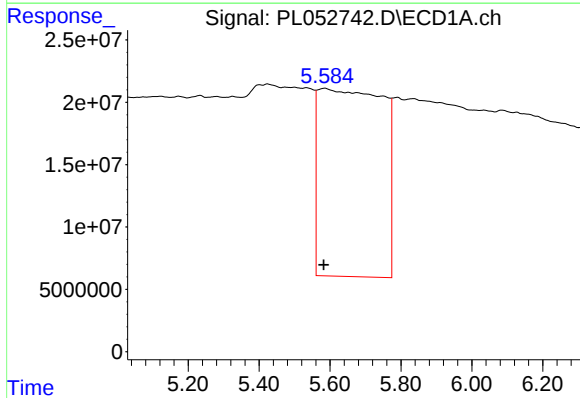


#11 alpha-Chlordane

R.T.: 5.585 min
Delta R.T.: 0.003 min
Response: 1883813651
Conc: 182.23 ng/ml

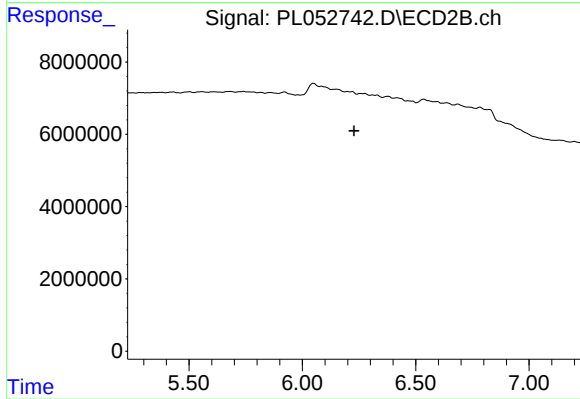

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.229 min
Response: 0
Conc: N.D.

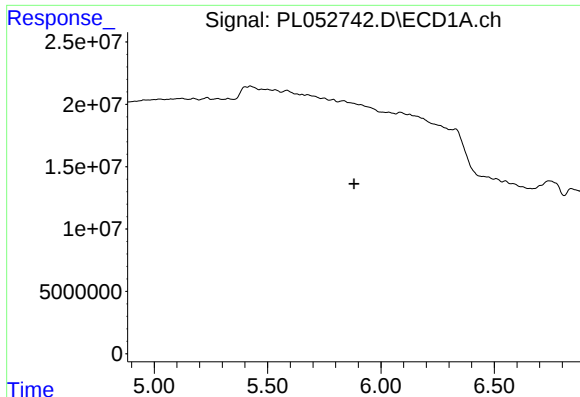

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

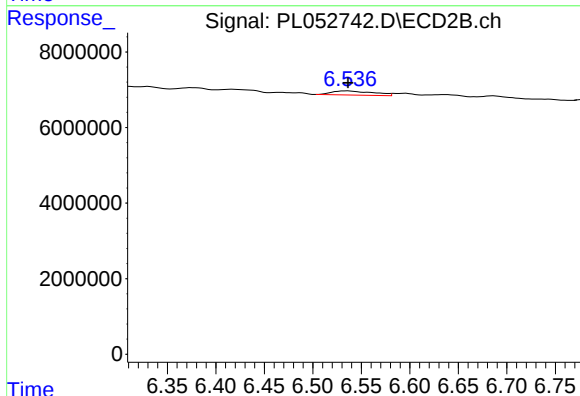


#13 Dieldrin

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 3209957
Conc: 1.31 ng/ml

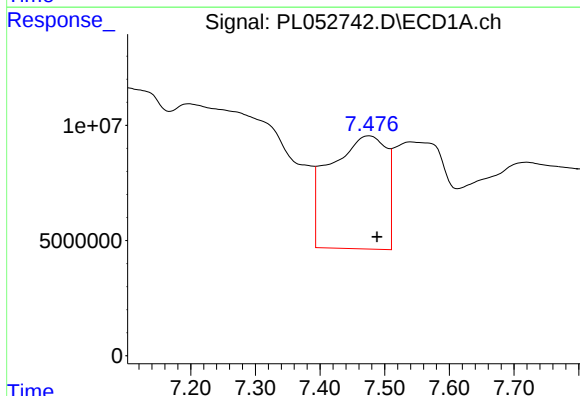


#22 Mirex

R.T.: 7.476 min
Delta R.T.: -0.012 min
Response: 298390614
Conc: 39.02 ng/ml

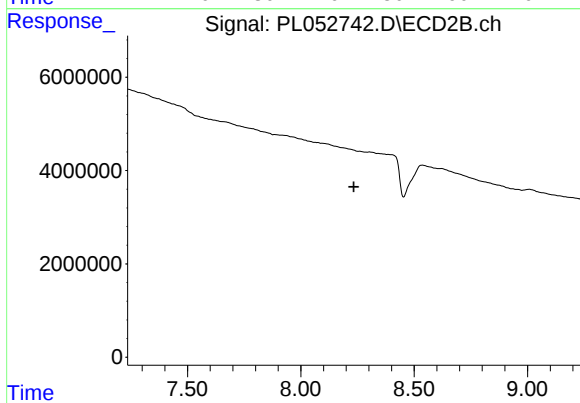

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.234 min
Response: 0
Conc: N.D.

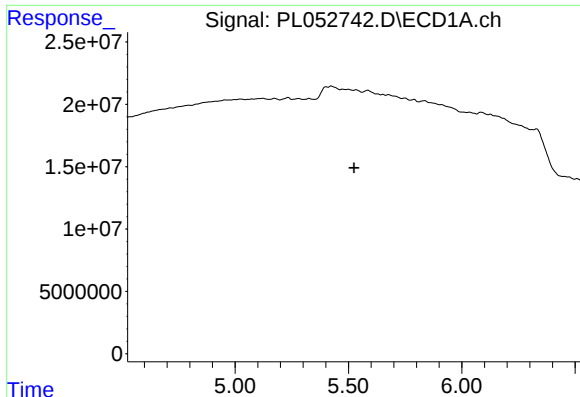

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

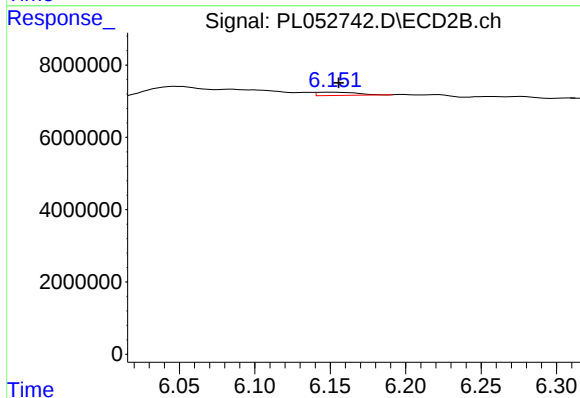


#25 Chlordane-3

R.T.: 6.152 min
Delta R.T.: -0.004 min
Response: 1627262
Conc: 5.32 ng/ml

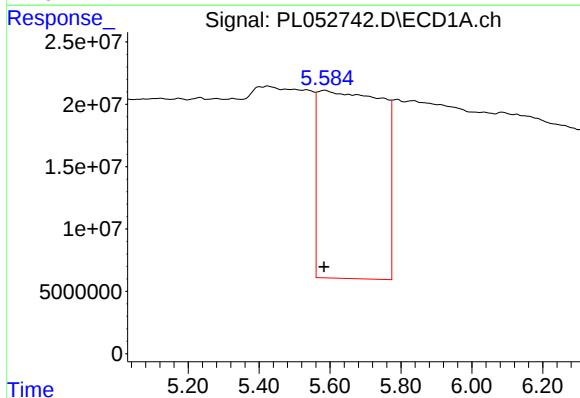


#26 Chlordane-4

R.T.: 5.585 min
Delta R.T.: 0.001 min
Response: 1883813651
Conc: 2393.83 ng/ml

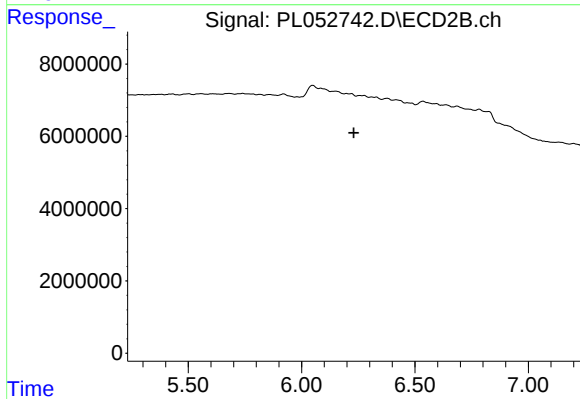

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.230 min
Response: 0
Conc: N.D.

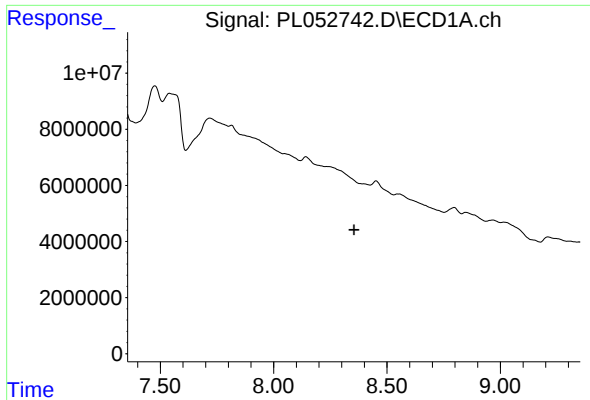

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

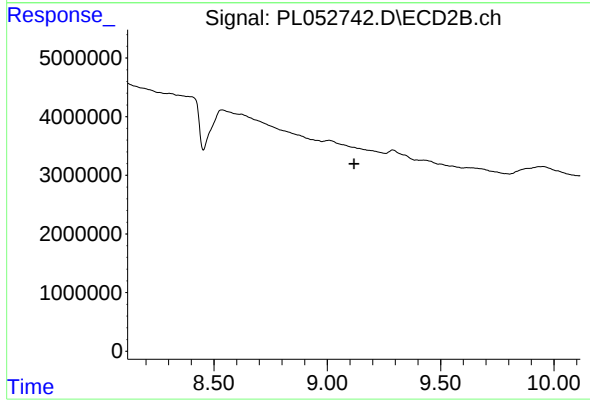

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.