

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092623\
 Data File : PL085515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2023 15:25
 Operator : AR\AJ
 Sample : 04590-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SAMPLE-1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/27/2023
 Supervised By :Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 21:27:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 26 01:26:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	2.650	31230863	17133115	12.143m	15.100
2)	SA Decachlor...	8.942	7.823	30651027	17871778	14.936	15.053

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092623\
Data File : PL085515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2023 15:25
Operator : AR\AJ
Sample : 04590-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SAMPLE-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/27/2023
Supervised By : Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 21:27:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 26 01:26:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

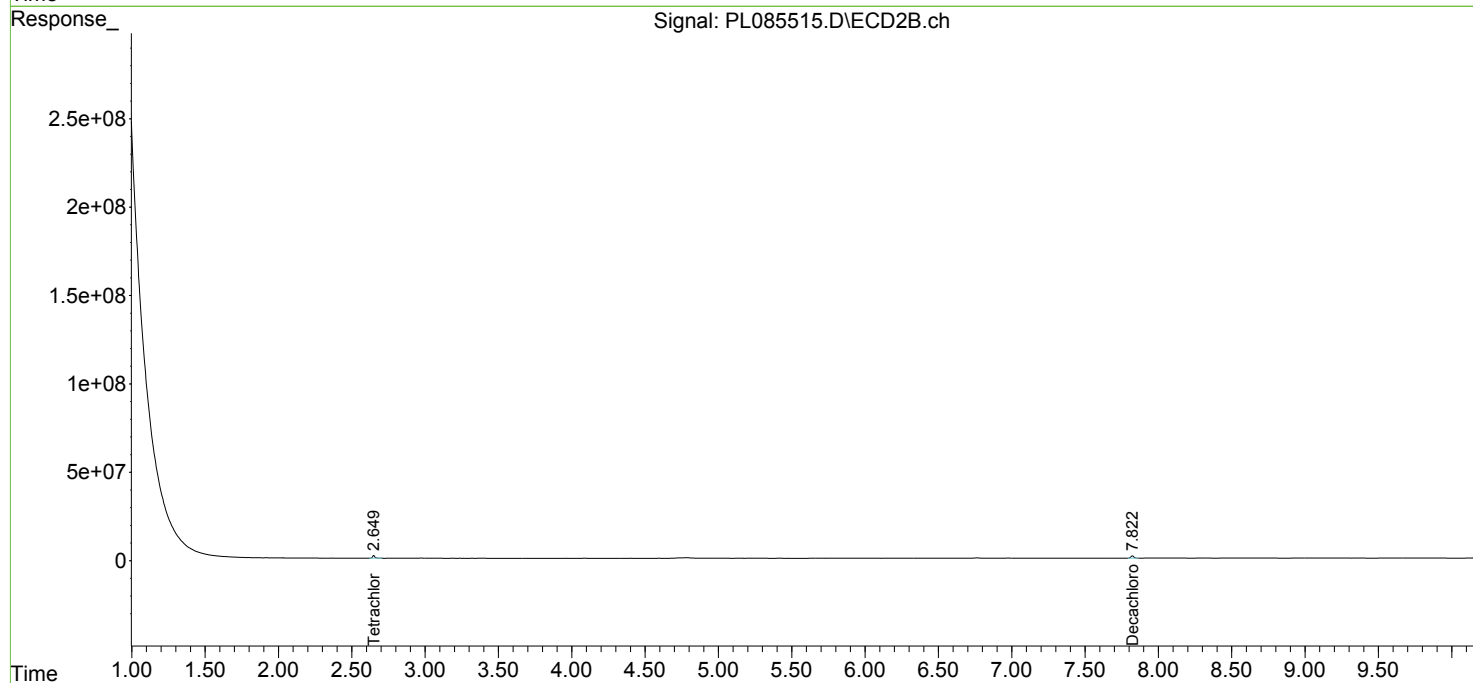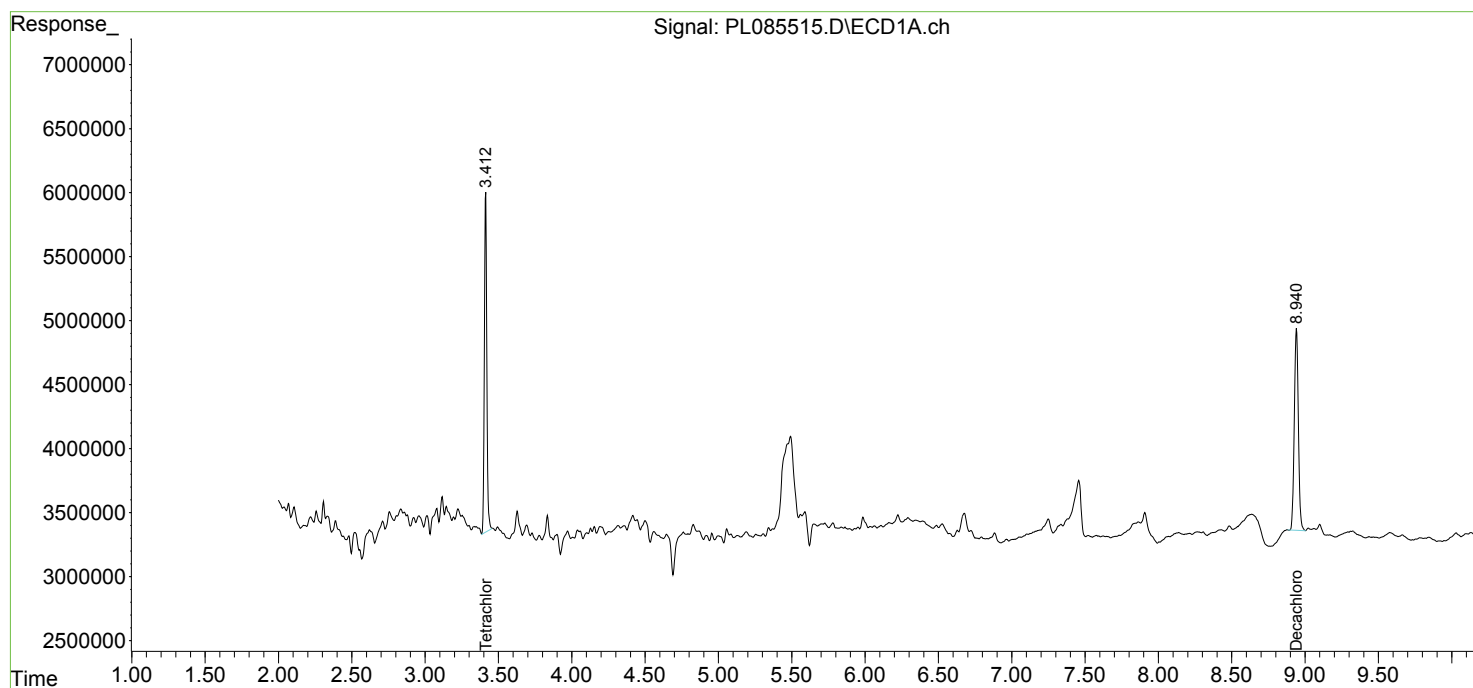

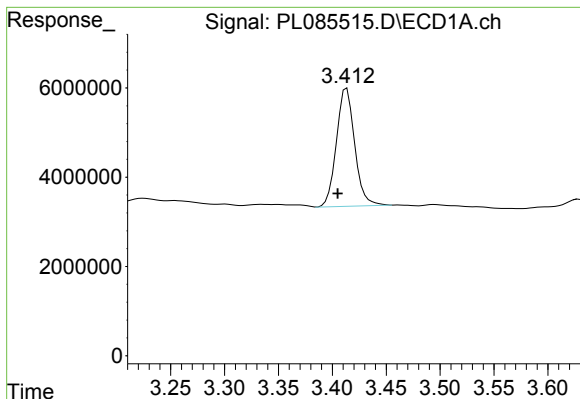


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.007 min
Response: 31230863
Conc: 12.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

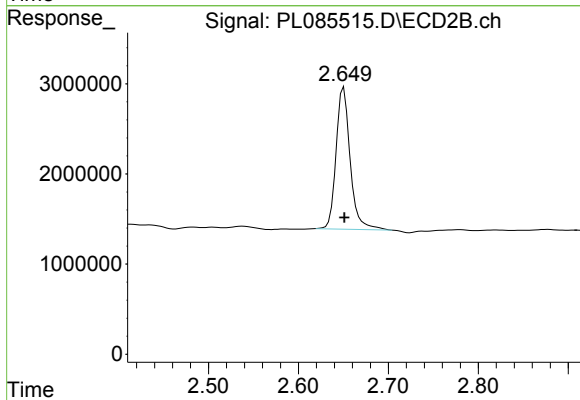


#1 Tetrachloro-m-xylene

R.T.: 2.650 min
Delta R.T.: 0.000 min
Response: 17133115
Conc: 15.10 ng/ml

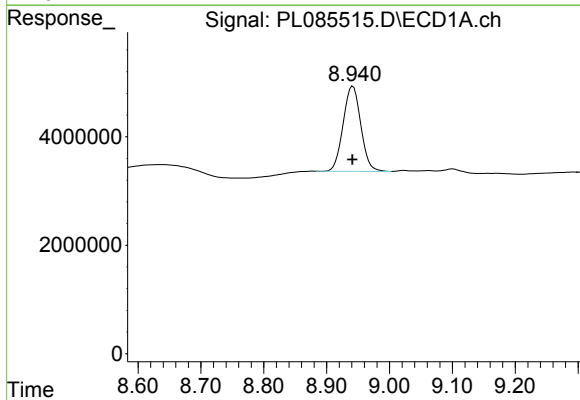

#28 Decachlorobiphenyl

R.T.: 8.942 min
Delta R.T.: 0.000 min
Response: 30651027
Conc: 14.94 ng/ml

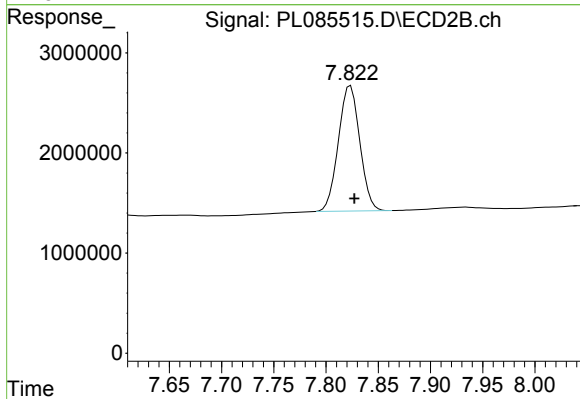

#28 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: -0.004 min
Response: 17871778
Conc: 15.05 ng/ml