

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092623\
 Data File : PL085521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2023 16:49
 Operator : AR\AJ
 Sample : 04601-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/27/2023
 Supervised By :Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 21:29:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 26 01:26:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	2.650	42817206	19179152	16.648m	16.903
2)	SA Decachlor...	8.939	7.822	33360749	20495902	16.256	17.263

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092623\
Data File : PL085521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2023 16:49
Operator : AR\AJ
Sample : 04601-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/27/2023
Supervised By : Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 21:29:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 26 01:26:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

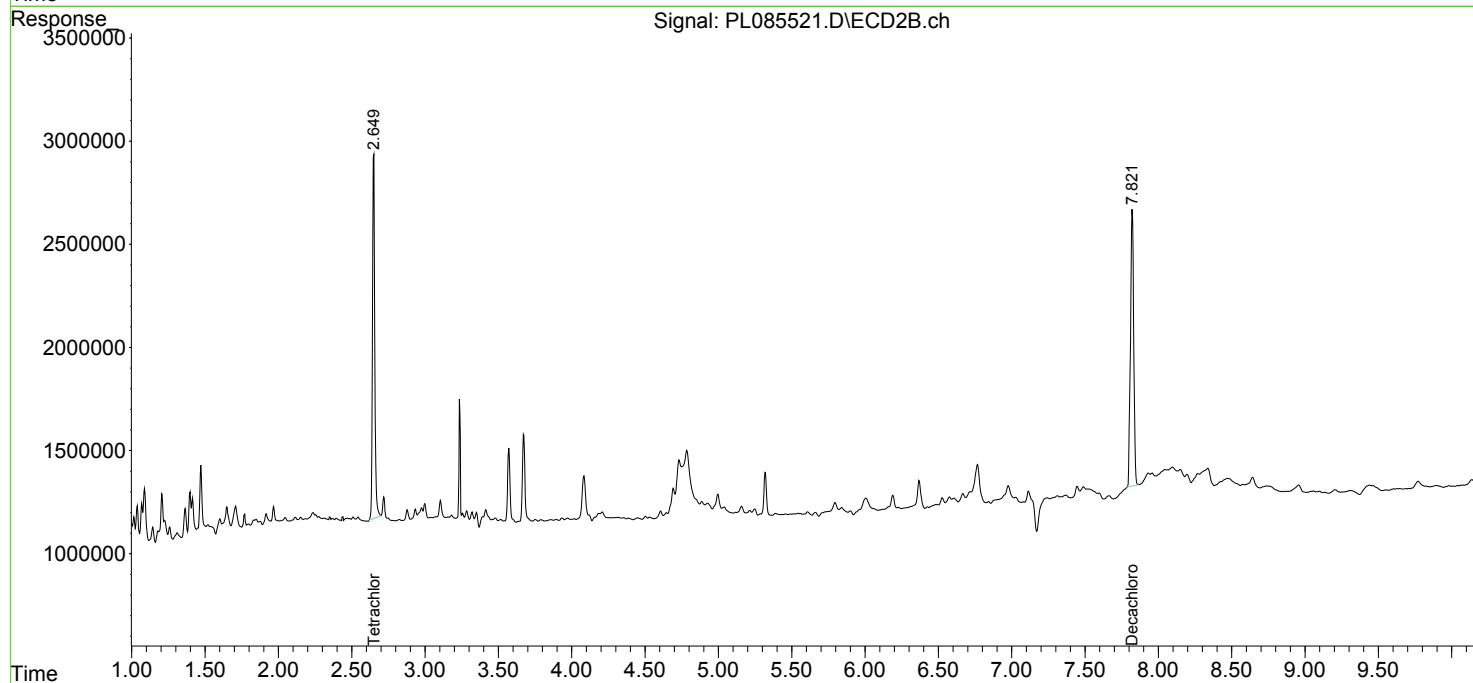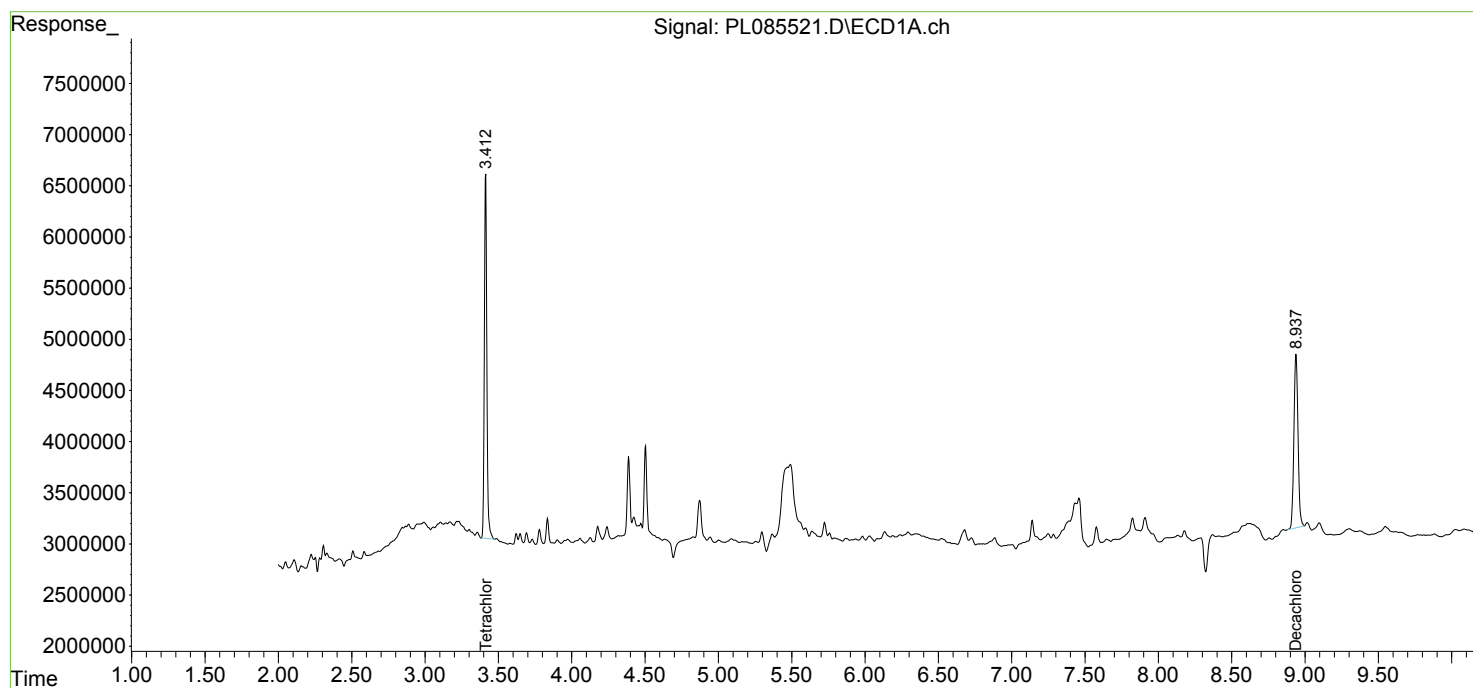

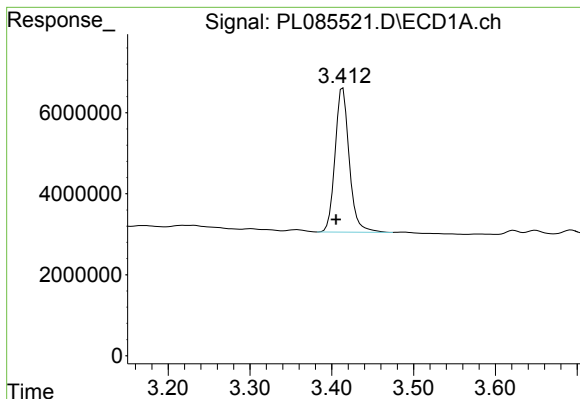


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.007 min
Response: 42817206
Conc: 16.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

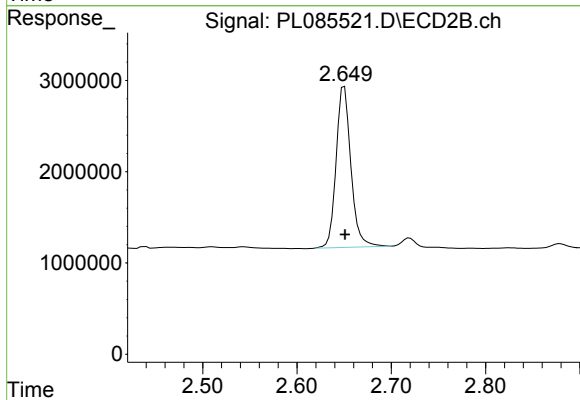


#1 Tetrachloro-m-xylene

R.T.: 2.650 min
Delta R.T.: 0.000 min
Response: 19179152
Conc: 16.90 ng/ml

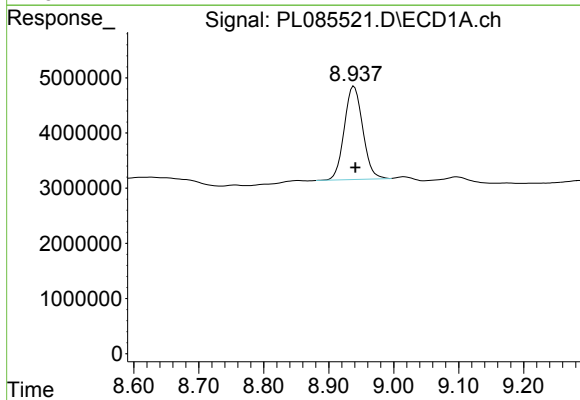

#28 Decachlorobiphenyl

R.T.: 8.939 min
Delta R.T.: -0.002 min
Response: 33360749
Conc: 16.26 ng/ml

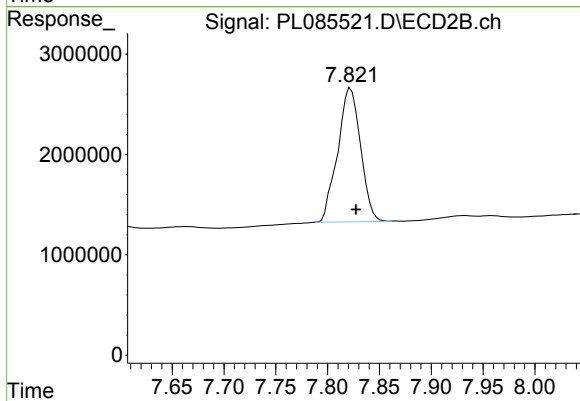

#28 Decachlorobiphenyl

R.T.: 7.822 min
Delta R.T.: -0.005 min
Response: 20495902
Conc: 17.26 ng/ml