

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092624\
 Data File : PL092083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2024 19:52
 Operator : AR\AJ
 Sample : P4172-04MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 04:14:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.780	40843576	34249504	18.359	13.656 #
28)	SA Decachlor...	9.060	7.922	10460157	15500056	6.385	6.195
Target Compounds							
2)	A alpha-BHC	3.997	3.283	119.6E6	151.9E6	38.610	41.692
3)	MA gamma-BHC...	4.330	3.613	135.9E6	142.3E6	43.843	40.293
4)	MA Heptachlor	4.918	3.952	116.1E6	143.6E6	41.978	41.627
5)	MB Aldrin	5.260	4.232	108.0E6	134.8E6	38.899	39.620
6)	B beta-BHC	4.527	3.913	50005822	72273049	37.701	48.083 #
7)	B delta-BHC	4.772	4.141	143.1E6	103.8E6	49.607	29.908 #
8)	B Heptachlo...	5.686	4.735	116.5E6	142.0E6	45.774	46.991
9)	A Endosulfan I	6.072	5.105	88167002	119.9E6	38.111	43.680
10)	B gamma-Chl...	5.943	4.985	209.1E6	218.1E6	84.601	72.478
11)	B alpha-Chl...	6.024	5.048	291.2E6	293.0E6	118.227	97.880
12)	B 4,4'-DDE	6.195	5.238	84900726	130.1E6	39.226	46.821
13)	MA Dieldrin	6.348	5.369	220.5E6	310.9E6	90.412	106.033
14)	MA Endrin	6.578	5.645	71709014	116.7E6	34.798	44.522 #
15)	B Endosulfa...	6.797	5.940	81609705	124.8E6	37.100	49.854 #
16)	A 4,4'-DDD	6.712	5.793	80887941	91730482	45.045	42.941
17)	MA 4,4'-DDT	7.027	6.043	77191605	108.6E6	41.925	46.963
18)	B Endrin al...	6.927	6.119	67139999	82047696	38.525	40.205
19)	B Endosulfa...	7.162	6.342	69272105	93836352	34.946	38.896
20)	A Methoxychlor	7.503	6.619	33081746	56131977	33.698	44.893 #
21)	B Endrin ke...	7.647	6.848	79484017	102.7E6	36.169	37.084
22)	Mirex	8.120	7.029	56403290	84381877	31.318	34.687
24)	Chlordane-2	5.260f	4.359	108.0E6	5556033	1007.453	49.508 #
25)	Chlordane-3	5.943	4.985	209.1E6	218.1E6	558.141	658.321
26)	Chlordane-4	6.024	5.048	291.2E6	293.0E6	643.118	923.493 #
27)	Chlordane-5	6.875	5.940	13211443	124.8E6	151.481	1150.355 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092624\
Data File : PL092083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2024 19:52
Operator : AR\AJ
Sample : P4172-04MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 04:14:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

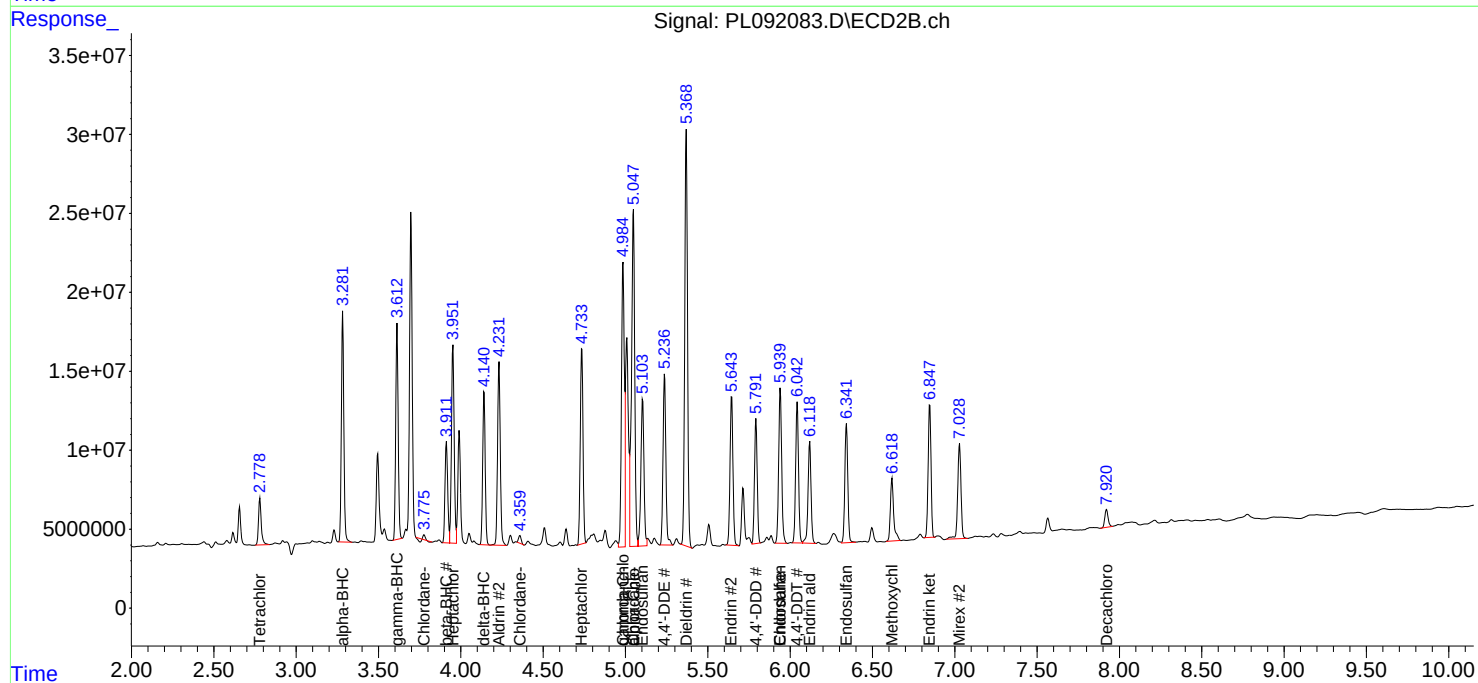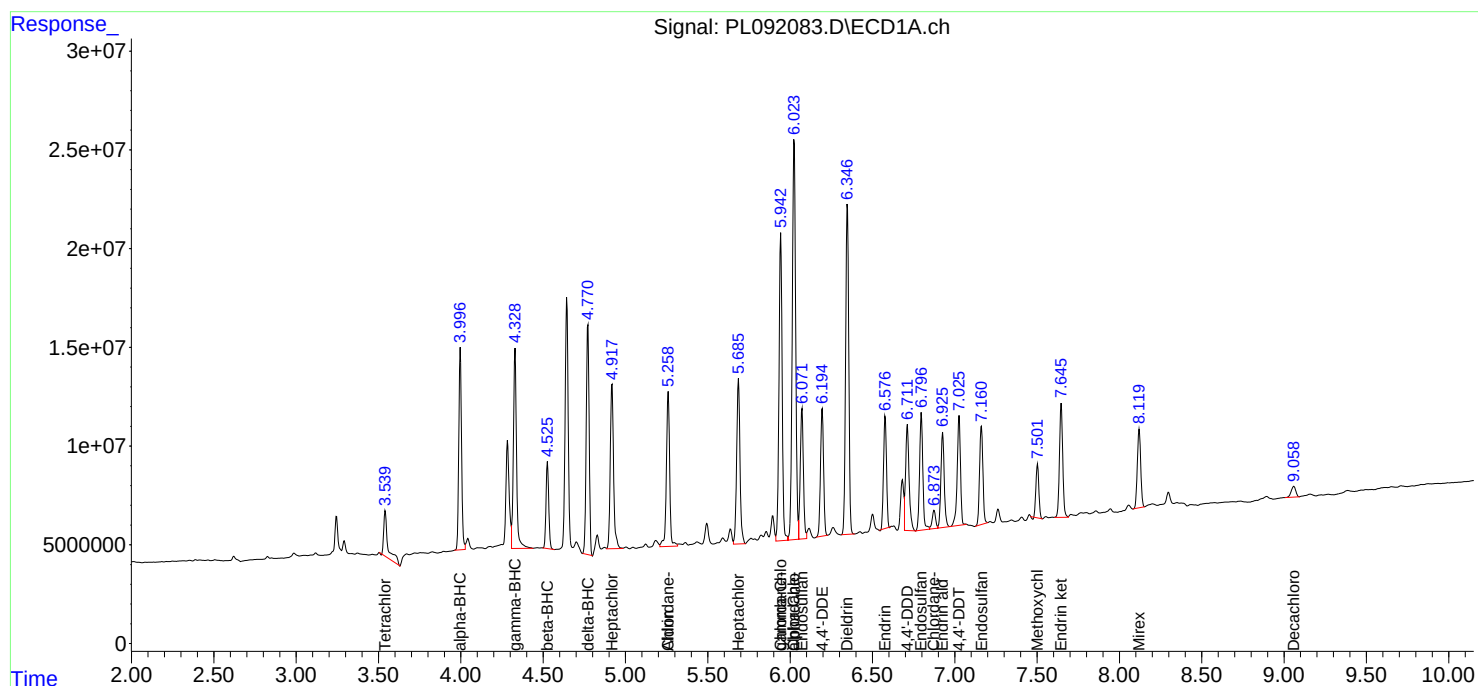


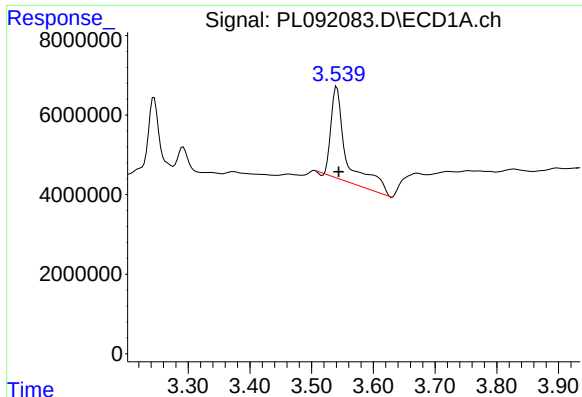

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: -0.003 min
Response: 40843576
Conc: 18.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

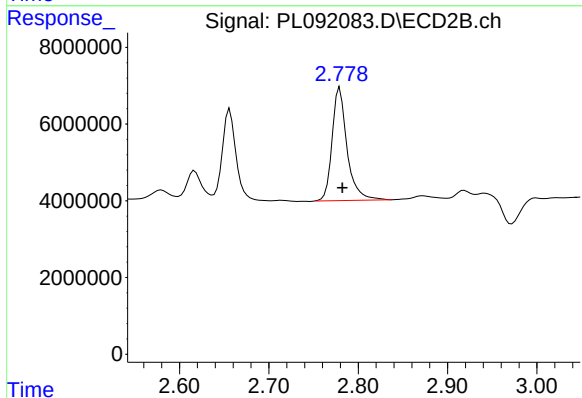


#1 Tetrachloro-m-xylene

R.T.: 2.780 min
Delta R.T.: -0.003 min
Response: 34249504
Conc: 13.66 ng/ml

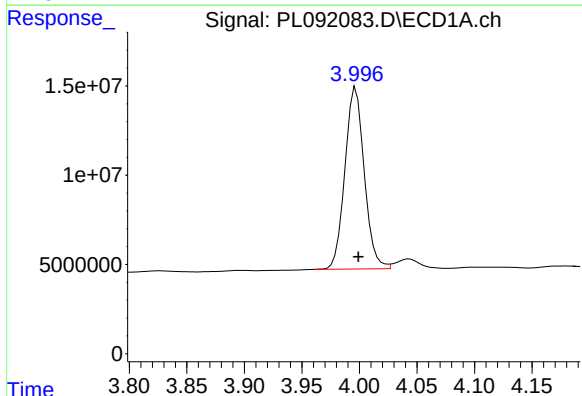


#2 alpha-BHC

R.T.: 3.997 min
Delta R.T.: -0.002 min
Response: 119557644
Conc: 38.61 ng/ml

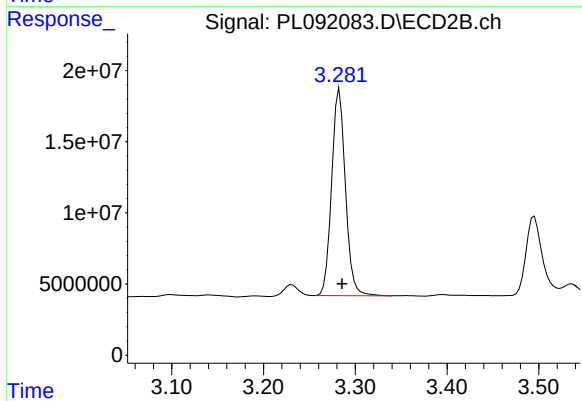

#2 alpha-BHC


R.T.: 3.283 min
Delta R.T.: -0.003 min
Response: 151899122
Conc: 41.69 ng/ml

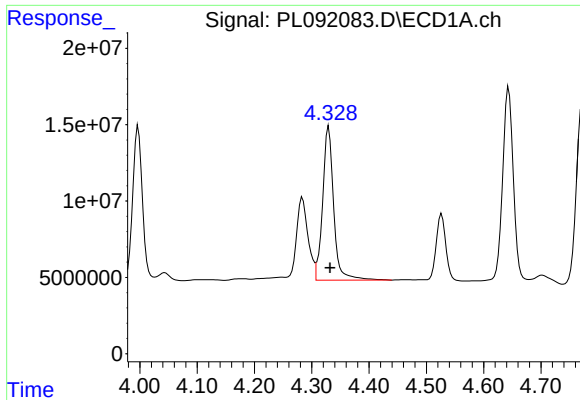

#3 gamma-BHC (Lindane)


R.T.: 4.330 min
Delta R.T.: -0.003 min
Response: 135860396
Conc: 43.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

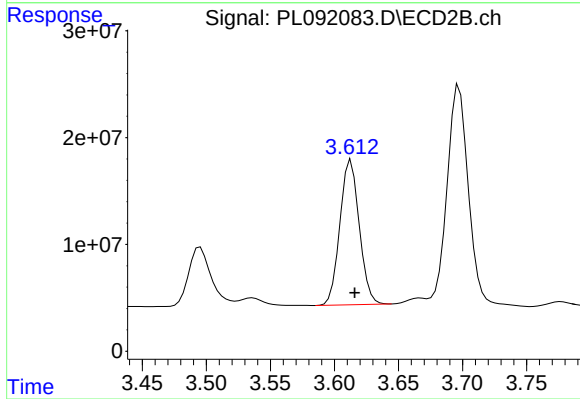


#3 gamma-BHC (Lindane)

R.T.: 3.613 min
Delta R.T.: -0.003 min
Response: 142274419
Conc: 40.29 ng/ml

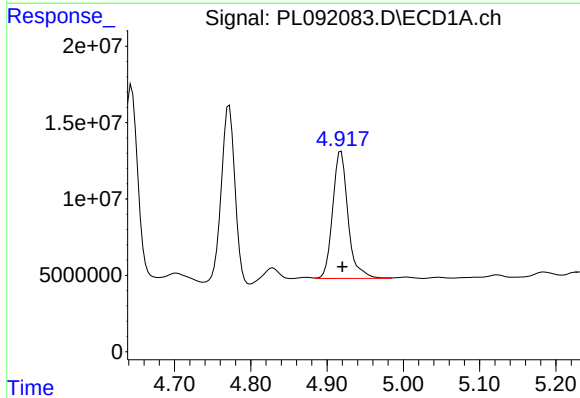


#4 Heptachlor

R.T.: 4.918 min
Delta R.T.: -0.002 min
Response: 116087406
Conc: 41.98 ng/ml

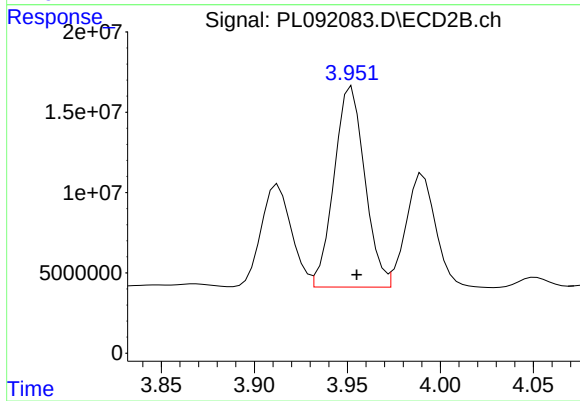

#4 Heptachlor


R.T.: 3.952 min
Delta R.T.: -0.003 min
Response: 143637673
Conc: 41.63 ng/ml

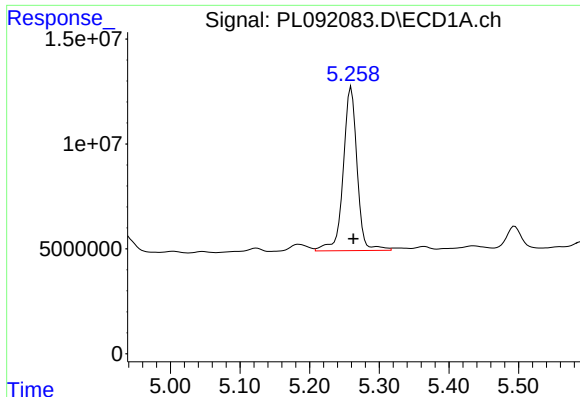

#5 Aldrin


R.T.: 5.260 min
Delta R.T.: -0.003 min
Response: 108045975
Conc: 38.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

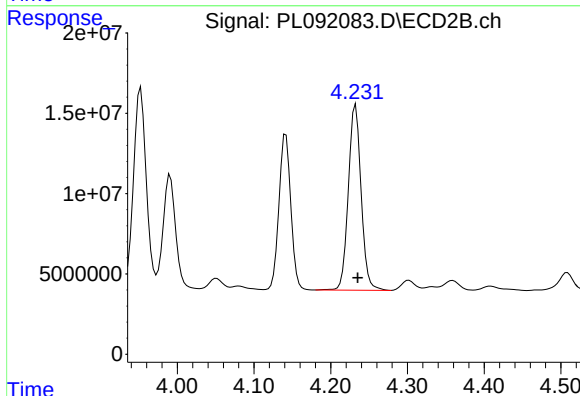


#5 Aldrin

R.T.: 4.232 min
Delta R.T.: -0.003 min
Response: 134750389
Conc: 39.62 ng/ml

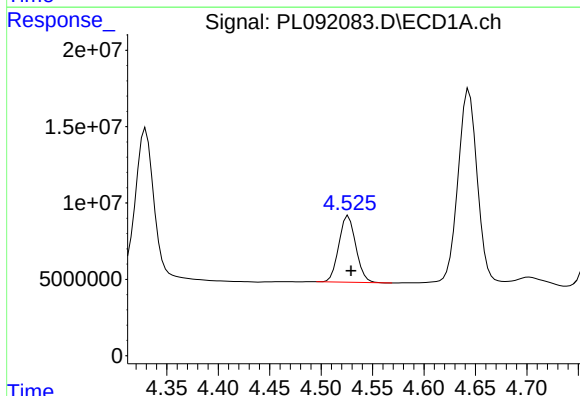


#6 beta-BHC

R.T.: 4.527 min
Delta R.T.: -0.003 min
Response: 50005822
Conc: 37.70 ng/ml

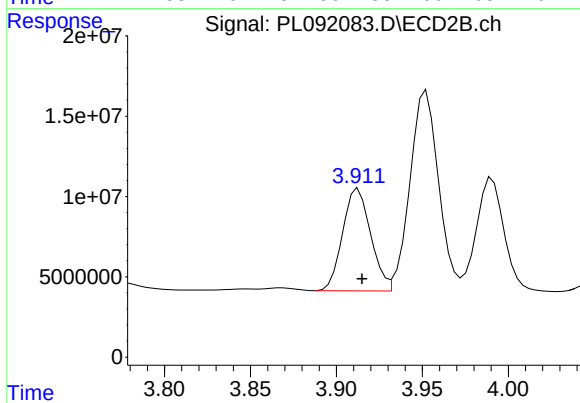

#6 beta-BHC


R.T.: 3.913 min
Delta R.T.: -0.002 min
Response: 72273049
Conc: 48.08 ng/ml

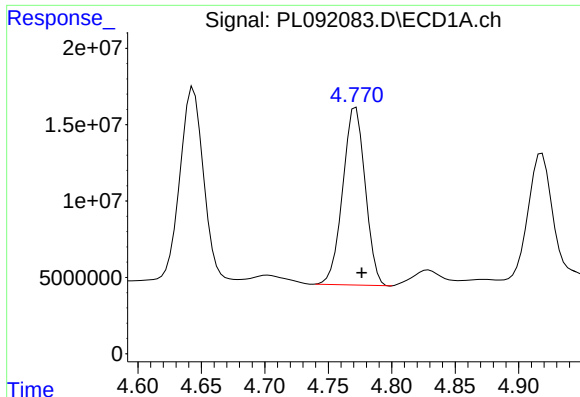

#7 delta-BHC


R.T.: 4.772 min
Delta R.T.: -0.005 min
Response: 143075743
Conc: 49.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

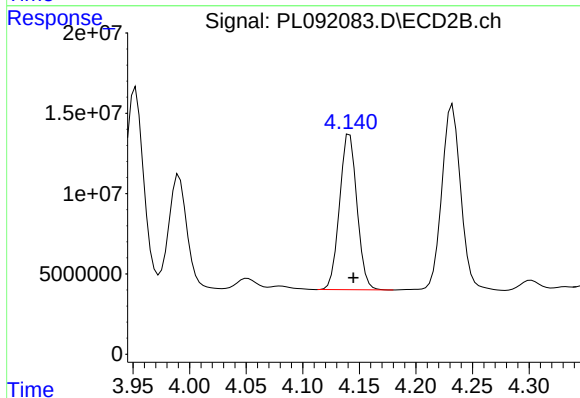


#7 delta-BHC

R.T.: 4.141 min
Delta R.T.: -0.003 min
Response: 103830523
Conc: 29.91 ng/ml

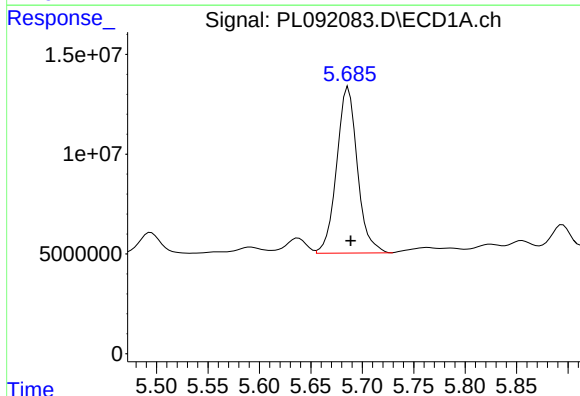


#8 Heptachlor epoxide

R.T.: 5.686 min
Delta R.T.: -0.002 min
Response: 116494641
Conc: 45.77 ng/ml

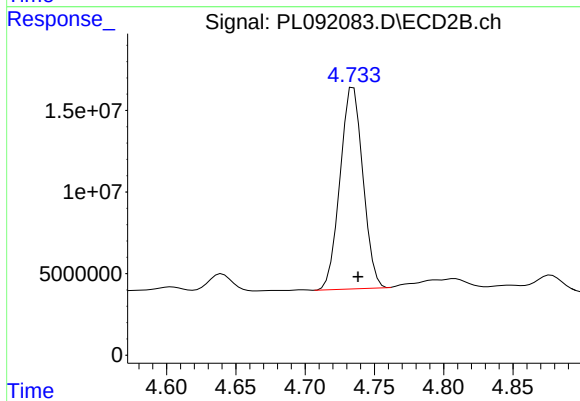

#8 Heptachlor epoxide


R.T.: 4.735 min
Delta R.T.: -0.003 min
Response: 142047946
Conc: 46.99 ng/ml

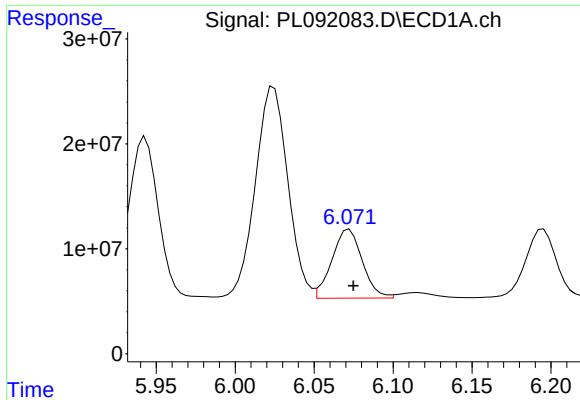

#9 Endosulfan I


R.T.: 6.072 min
Delta R.T.: -0.003 min
Response: 88167002
Conc: 38.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

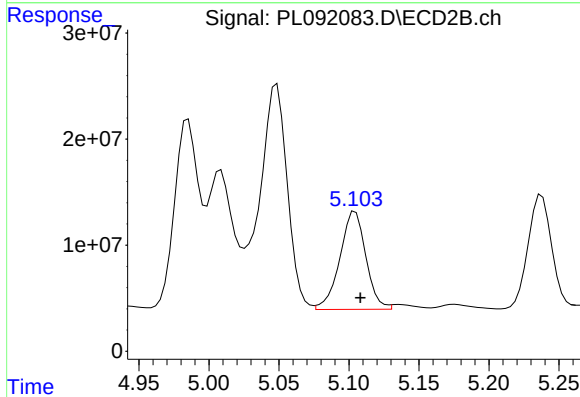


#9 Endosulfan I

R.T.: 5.105 min
Delta R.T.: -0.004 min
Response: 119884480
Conc: 43.68 ng/ml

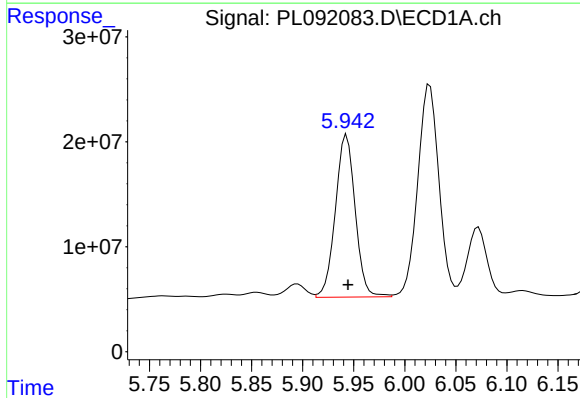


#10 gamma-Chlordane

R.T.: 5.943 min
Delta R.T.: -0.002 min
Response: 209066951
Conc: 84.60 ng/ml

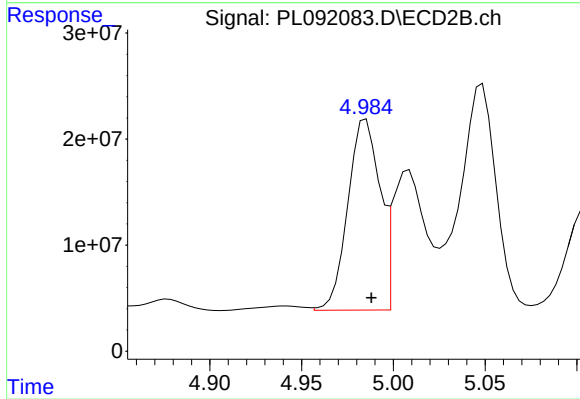

#10 gamma-Chlordane


R.T.: 4.985 min
Delta R.T.: -0.003 min
Response: 218054445
Conc: 72.48 ng/ml

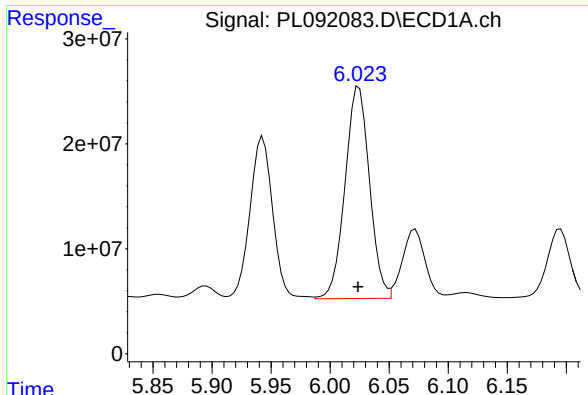

#11 alpha-Chlordane


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 291233722
Conc: 118.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

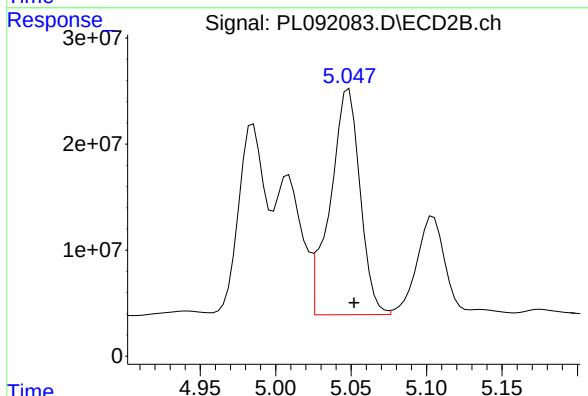


#11 alpha-Chlordane

R.T.: 5.048 min
Delta R.T.: -0.003 min
Response: 293007658
Conc: 97.88 ng/ml

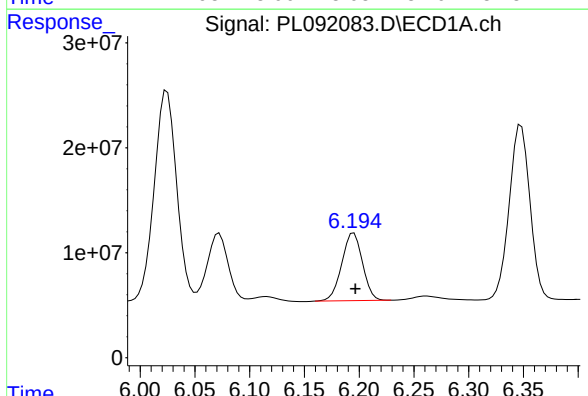


#12 4,4'-DDE

R.T.: 6.195 min
Delta R.T.: -0.002 min
Response: 84900726
Conc: 39.23 ng/ml

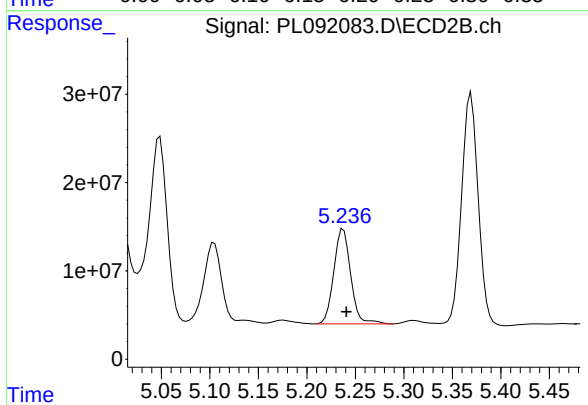

#12 4,4'-DDE


R.T.: 5.238 min
Delta R.T.: -0.003 min
Response: 130109630
Conc: 46.82 ng/ml

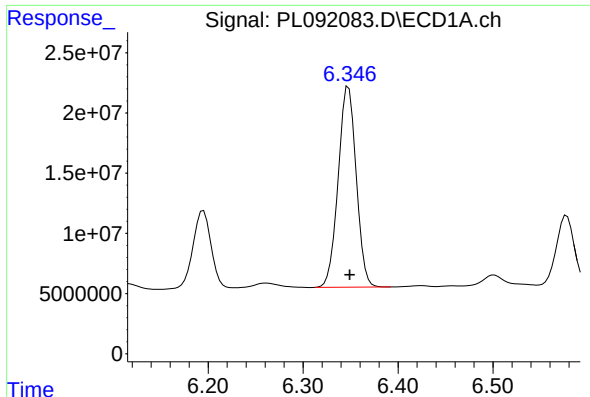

#13 Dieldrin


R.T.: 6.348 min
Delta R.T.: -0.001 min
Response: 220501448
Conc: 90.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

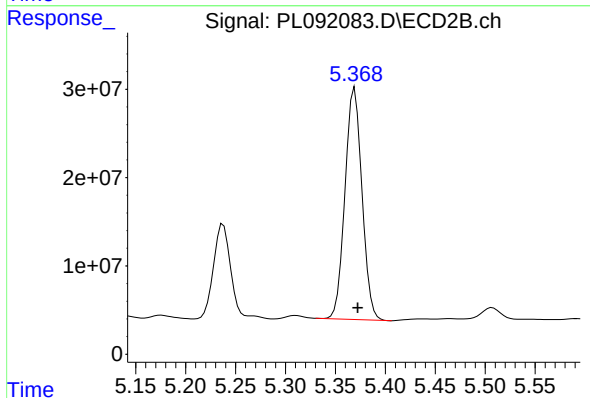


#13 Dieldrin

R.T.: 5.369 min
Delta R.T.: -0.003 min
Response: 310870770
Conc: 106.03 ng/ml

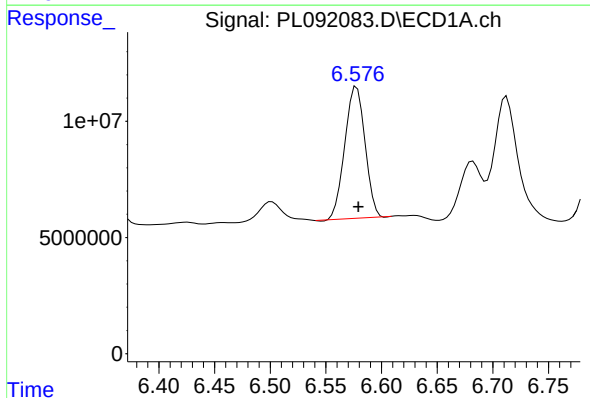


#14 Endrin

R.T.: 6.578 min
Delta R.T.: -0.002 min
Response: 71709014
Conc: 34.80 ng/ml

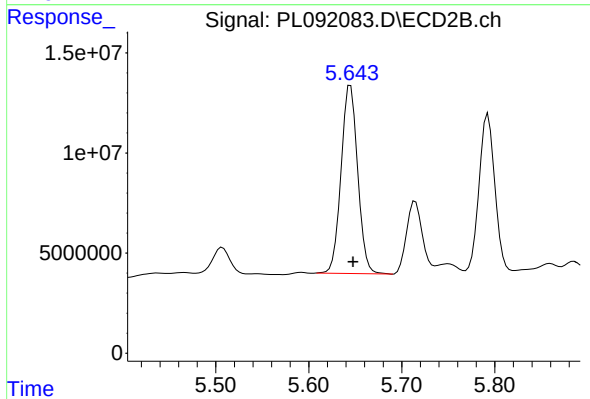

#14 Endrin


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 116745754
Conc: 44.52 ng/ml

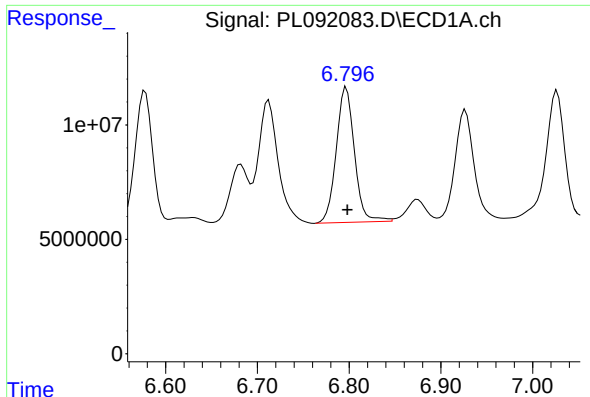

#15 Endosulfan II


R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 81609705
Conc: 37.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

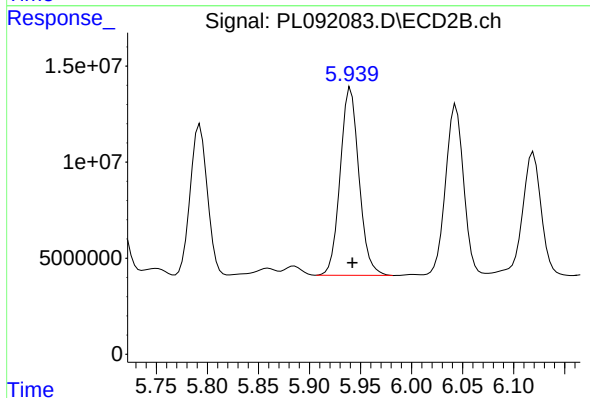


#15 Endosulfan II

R.T.: 5.940 min
Delta R.T.: -0.002 min
Response: 124755321
Conc: 49.85 ng/ml

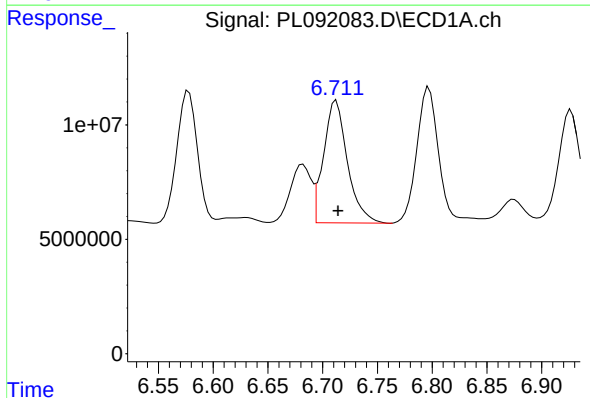


#16 4,4'-DDD

R.T.: 6.712 min
Delta R.T.: -0.002 min
Response: 80887941
Conc: 45.04 ng/ml

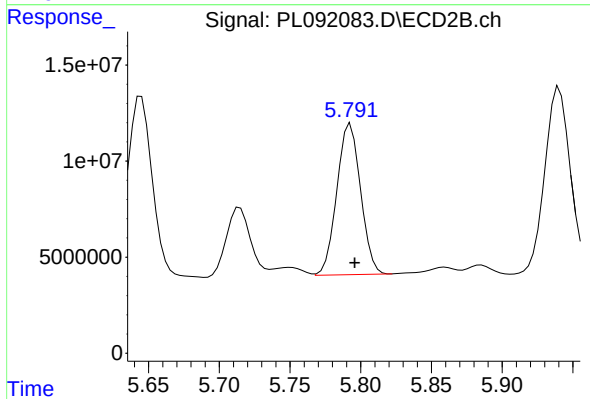

#16 4,4'-DDD


R.T.: 5.793 min
Delta R.T.: -0.003 min
Response: 91730482
Conc: 42.94 ng/ml

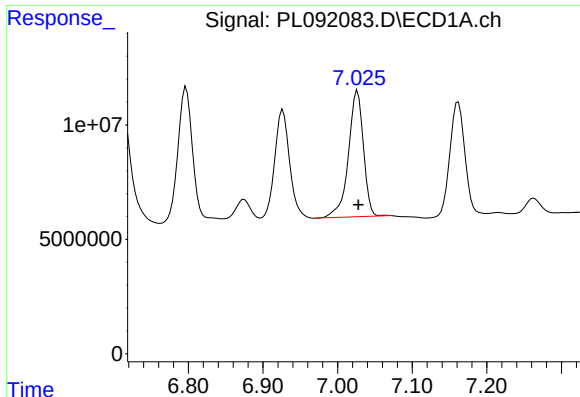

#17 4,4'-DDT


R.T.: 7.027 min
Delta R.T.: -0.001 min
Response: 77191605
Conc: 41.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

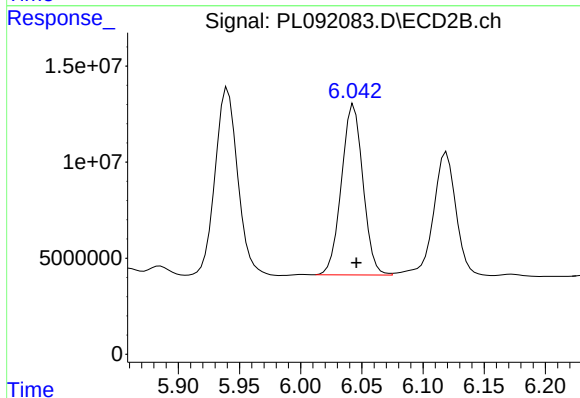


#17 4,4'-DDT

R.T.: 6.043 min
Delta R.T.: -0.002 min
Response: 108633589
Conc: 46.96 ng/ml

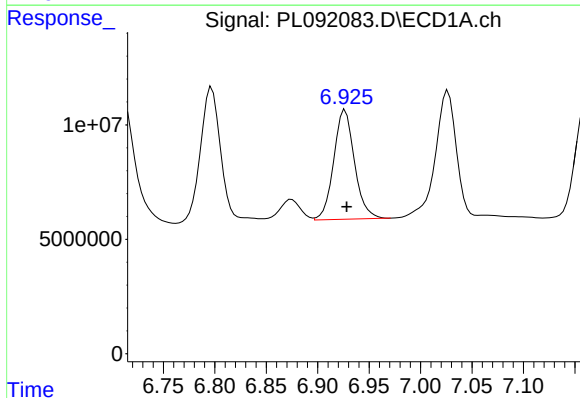


#18 Endrin aldehyde

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 67139999
Conc: 38.52 ng/ml

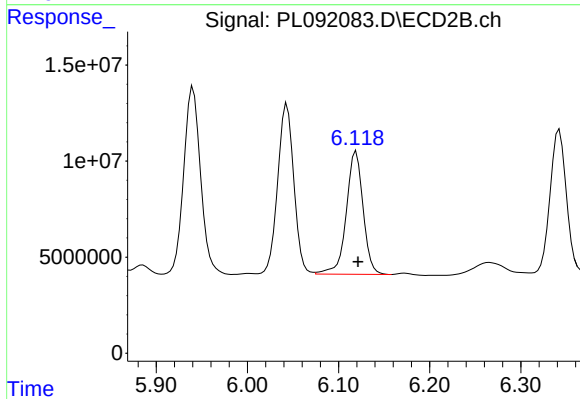

#18 Endrin aldehyde


R.T.: 6.119 min
Delta R.T.: -0.002 min
Response: 82047696
Conc: 40.21 ng/ml

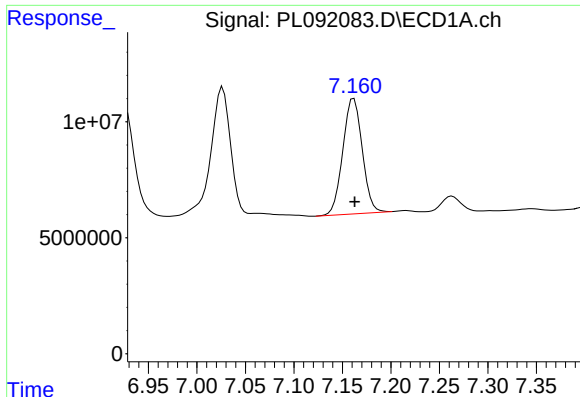

#19 Endosulfan Sulfate


R.T.: 7.162 min
Delta R.T.: -0.001 min
Response: 69272105
Conc: 34.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

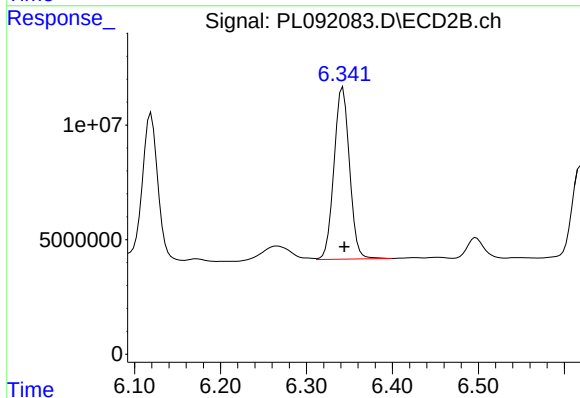


#19 Endosulfan Sulfate

R.T.: 6.342 min
Delta R.T.: -0.002 min
Response: 93836352
Conc: 38.90 ng/ml

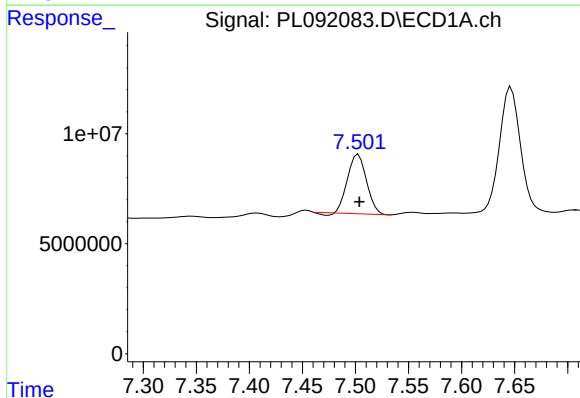


#20 Methoxychlor

R.T.: 7.503 min
Delta R.T.: 0.000 min
Response: 33081746
Conc: 33.70 ng/ml

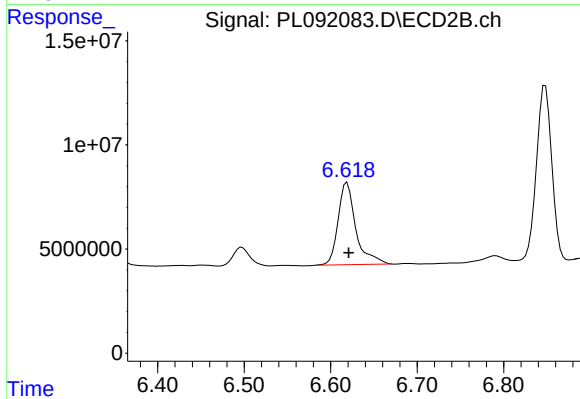

#20 Methoxychlor


R.T.: 6.619 min
Delta R.T.: -0.002 min
Response: 56131977
Conc: 44.89 ng/ml

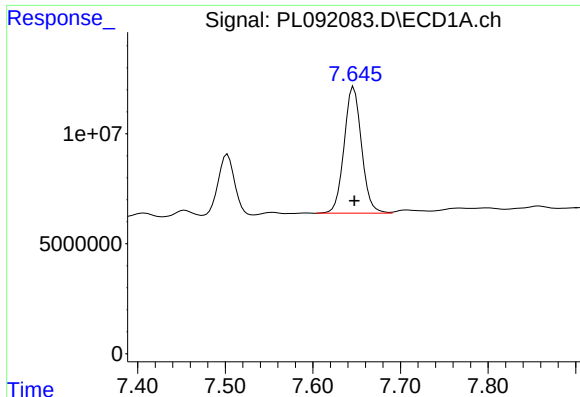

#21 Endrin ketone


R.T.: 7.647 min
Delta R.T.: 0.000 min
Response: 79484017
Conc: 36.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

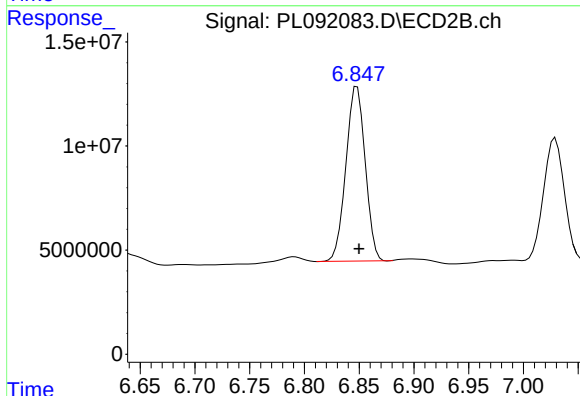


#21 Endrin ketone

R.T.: 6.848 min
Delta R.T.: -0.002 min
Response: 102684148
Conc: 37.08 ng/ml

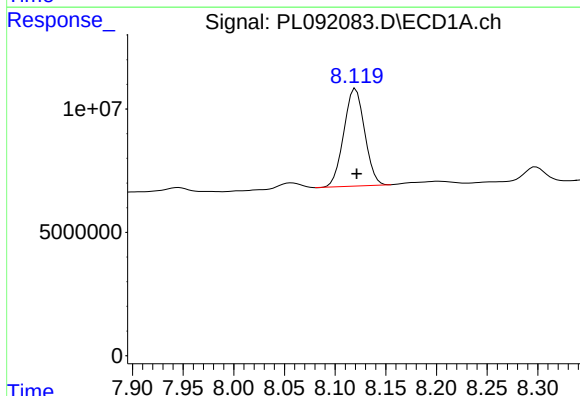


#22 Mirex

R.T.: 8.120 min
Delta R.T.: -0.001 min
Response: 56403290
Conc: 31.32 ng/ml

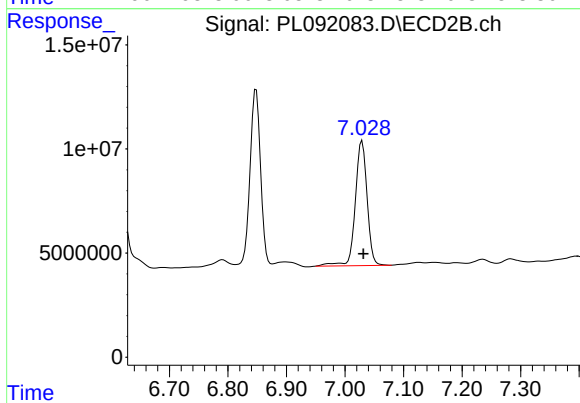

#22 Mirex


R.T.: 7.029 min
Delta R.T.: -0.002 min
Response: 84381877
Conc: 34.69 ng/ml

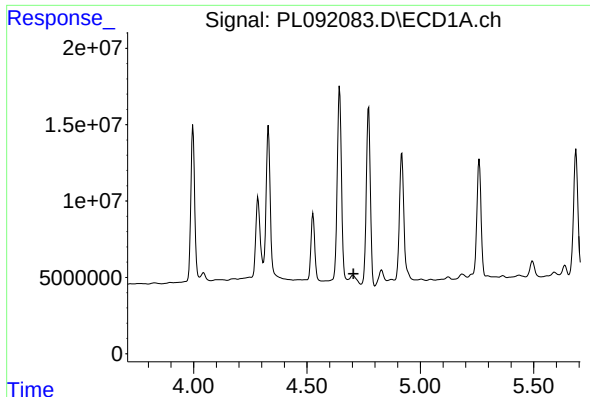

#23 Chlordane-1


R.T.: 4.703 min
Delta R.T.: -0.003 min
Response: -19716008
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

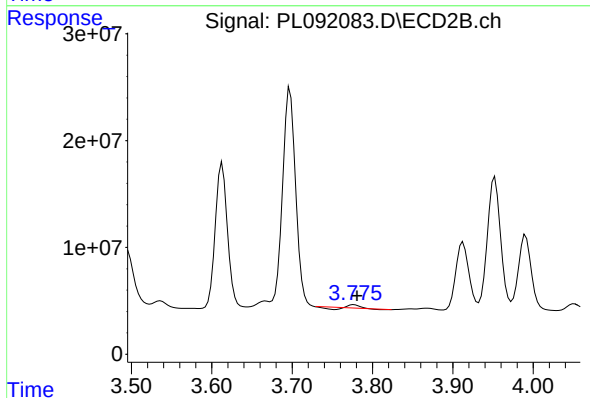


#23 Chlordane-1

R.T.: 3.777 min
Delta R.T.: -0.004 min
Response: 551293
Conc: 5.51 ng/ml

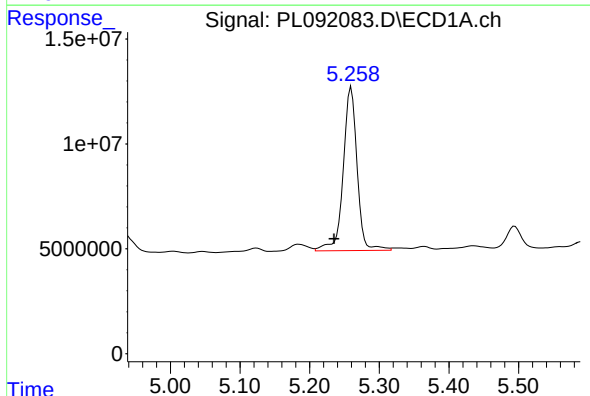


#24 Chlordane-2

R.T.: 5.260 min
Delta R.T.: 0.025 min
Response: 108045975
Conc: 1007.45 ng/ml

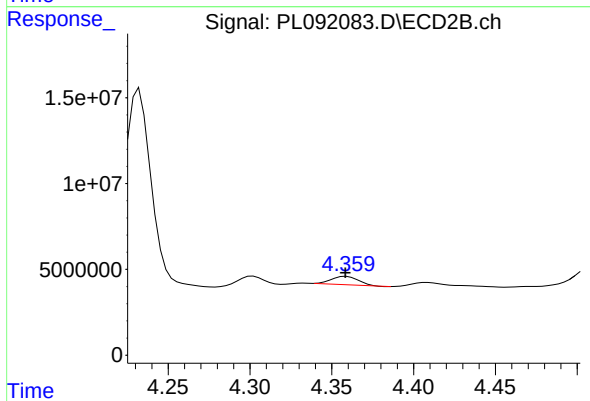

#24 Chlordane-2


R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 5556033
Conc: 49.51 ng/ml

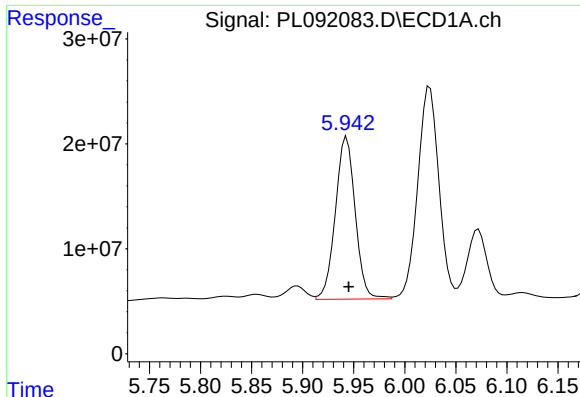

#25 Chlordane-3


R.T.: 5.943 min
Delta R.T.: -0.002 min
Response: 209066951
Conc: 558.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

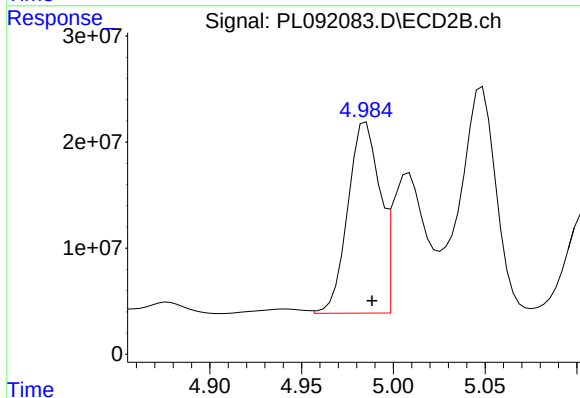


#25 Chlordane-3

R.T.: 4.985 min
Delta R.T.: -0.003 min
Response: 218054445
Conc: 658.32 ng/ml

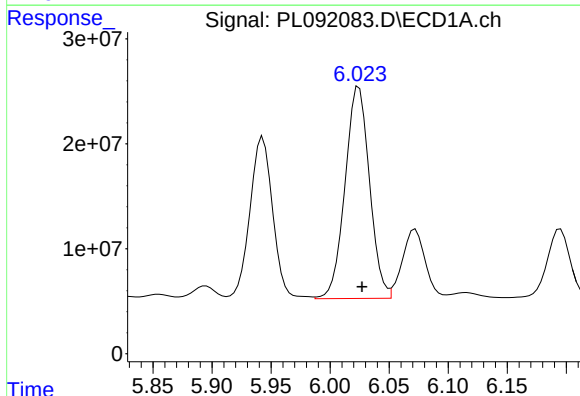


#26 Chlordane-4

R.T.: 6.024 min
Delta R.T.: -0.003 min
Response: 291233722
Conc: 643.12 ng/ml

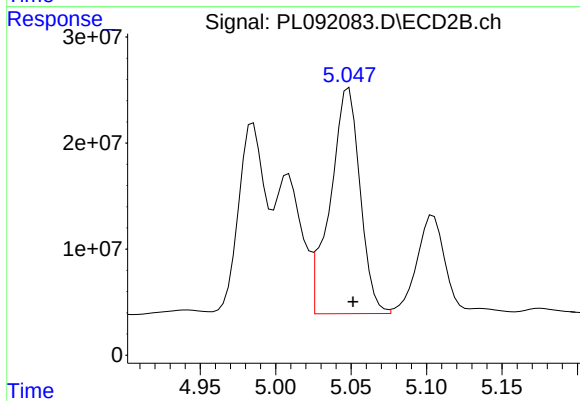

#26 Chlordane-4


R.T.: 5.048 min
Delta R.T.: -0.003 min
Response: 293007658
Conc: 923.49 ng/ml

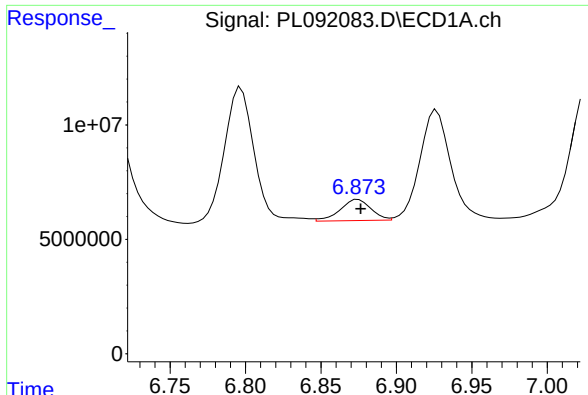

#27 Chlordane-5


R.T.: 6.875 min
Delta R.T.: -0.002 min
Response: 13211443
Conc: 151.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

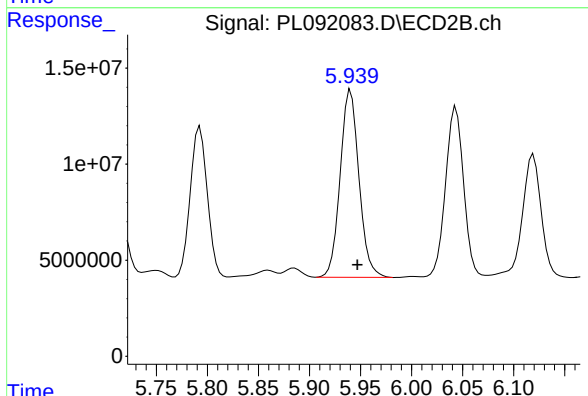


#27 Chlordane-5

R.T.: 5.940 min
Delta R.T.: -0.007 min
Response: 124755321
Conc: 1150.35 ng/ml

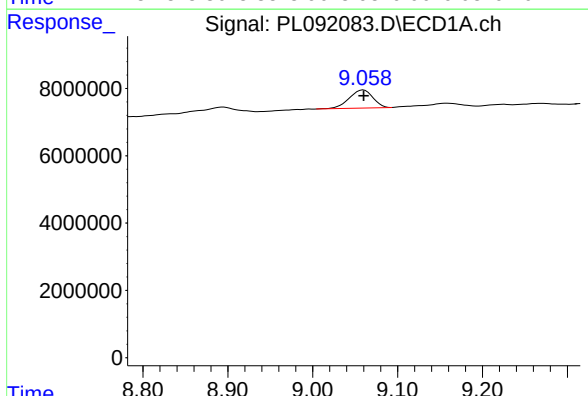

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 10460157
Conc: 6.39 ng/ml

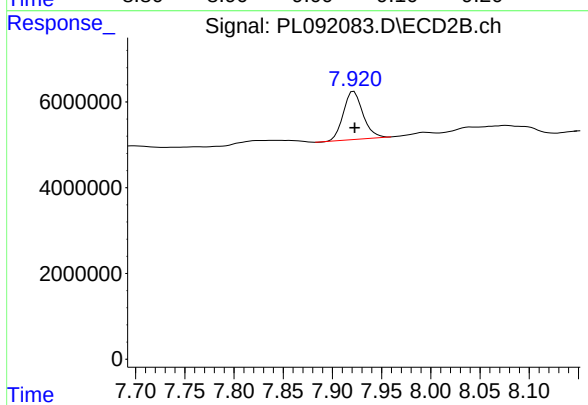

#28 Decachlorobiphenyl

R.T.: 7.922 min
Delta R.T.: 0.000 min
Response: 15500056
Conc: 6.20 ng/ml