

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
 Data File : PL040435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2018 15:03
 Operator : AJ\SJ
 Sample : J5081-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 02:32:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.807	158.0E6	64134931	21.591	20.310
28)	SA Decachlor...	7.815	8.730	178.3E6	57761627	18.759	18.240
Target Compounds							
7)	B delta-BHC	0.000	4.820	0	4201508	N.D.	0.910 #
15)	B Endosulfa...	5.867f	0.000	27404790	0	2.751	N.D. #
16)	A 4,4'-DDD	0.000	6.515f	0	11274100	N.D.	3.549 #
20)	A Methoxychlor	6.499f	0.000	45959434	0	9.515	N.D. #
23)	Chlordane-1	0.000	4.820	0	4201508	N.D.	27.225 #
27)	Chlordane-5	5.867	0.000	27404790	0	67.892	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
Data File : PL040435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2018 15:03
Operator : AJ\SJ
Sample : J5081-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 02:32:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

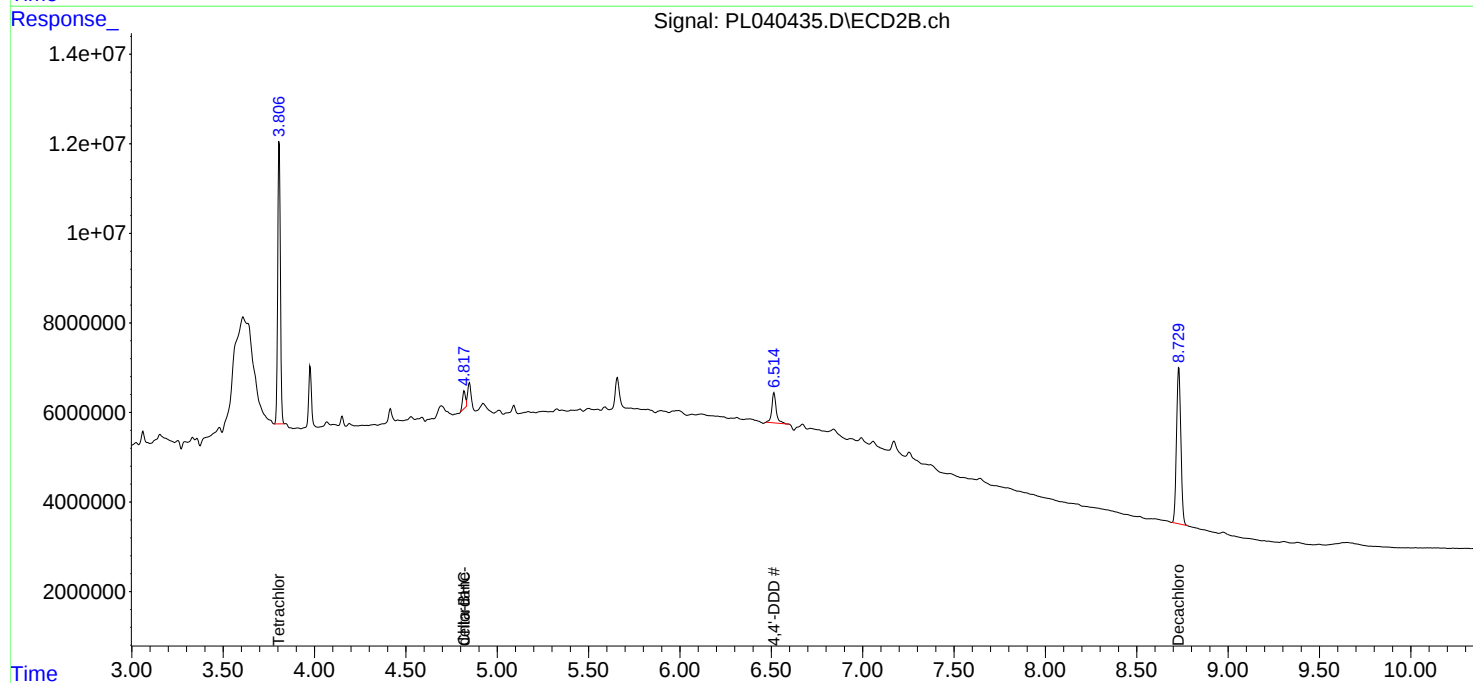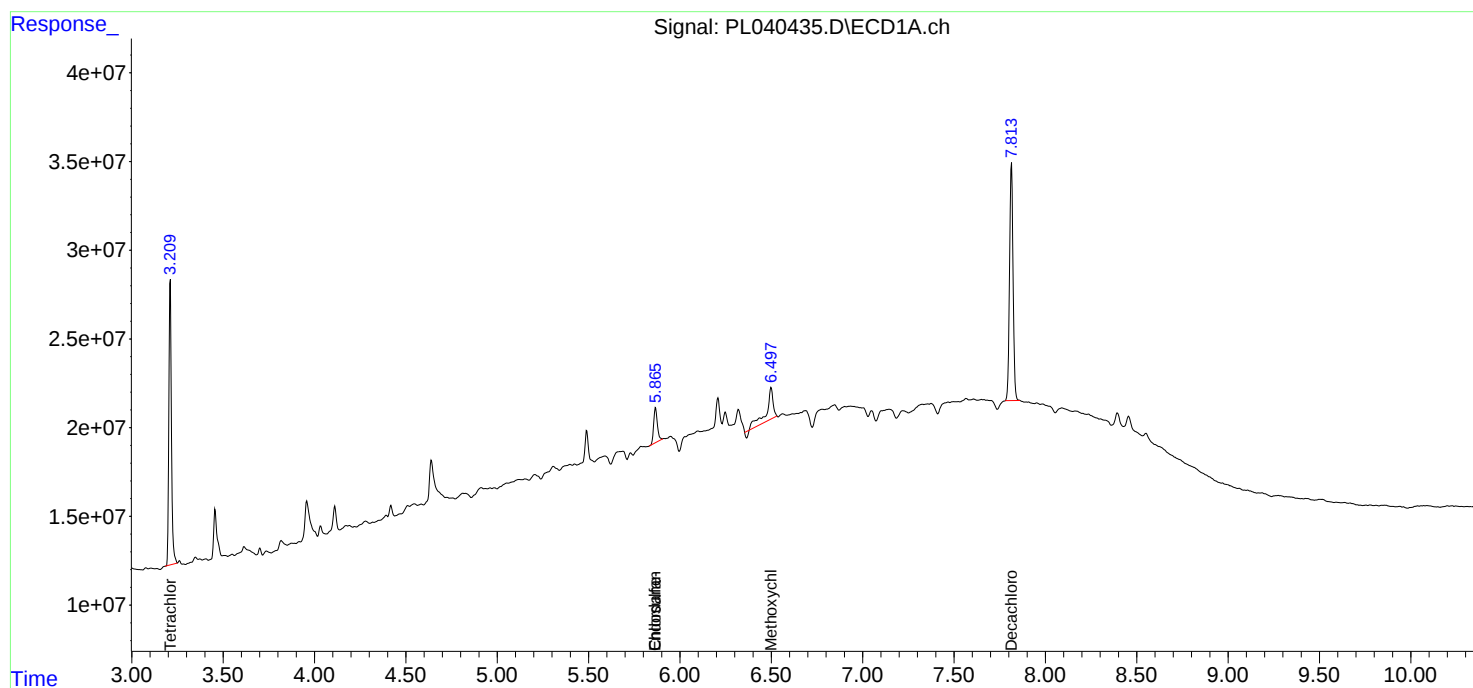


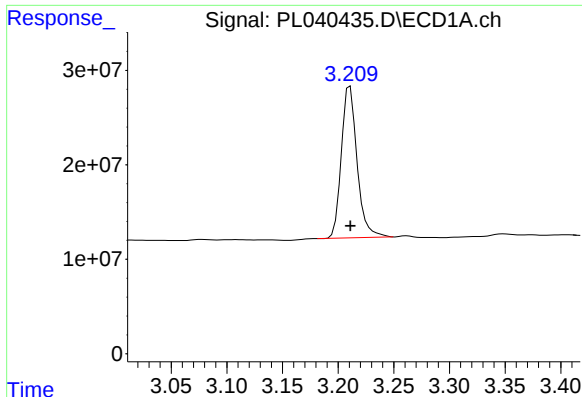

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: 0.000 min
Response: 158045756
Conc: 21.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

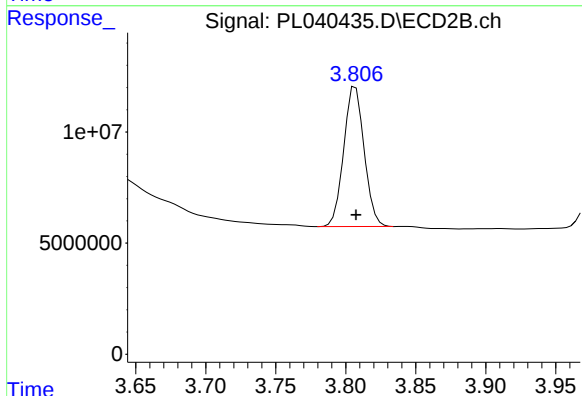


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 64134931
Conc: 20.31 ng/ml

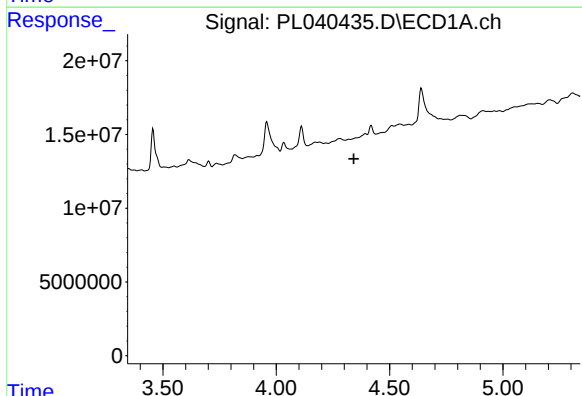


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

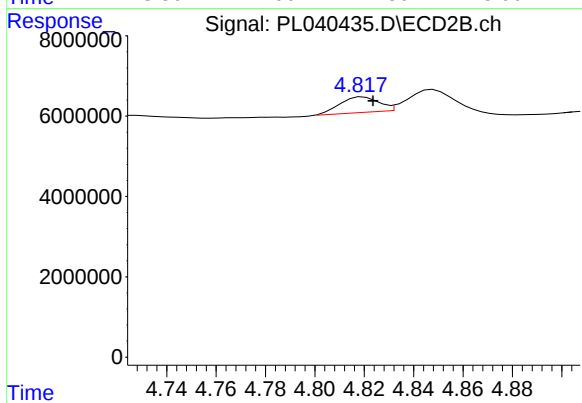

#7 delta-BHC


R.T.: 4.820 min
Delta R.T.: -0.004 min
Response: 4201508
Conc: 0.91 ng/ml

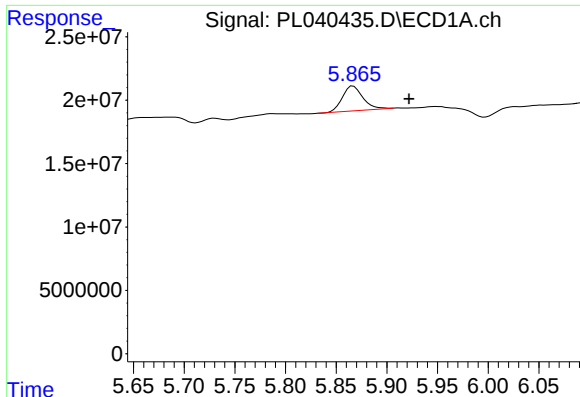

#15 Endosulfan II


R.T.: 5.867 min
Delta R.T.: -0.055 min
Response: 27404790
Conc: 2.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

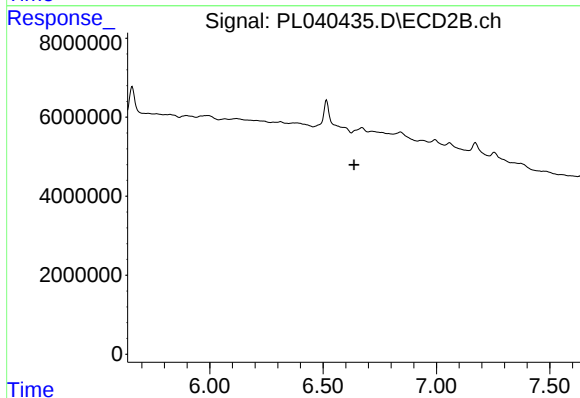


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

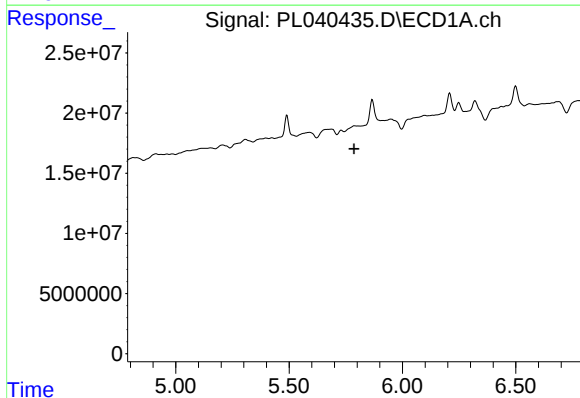


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.787 min
Response: 0
Conc: N.D.

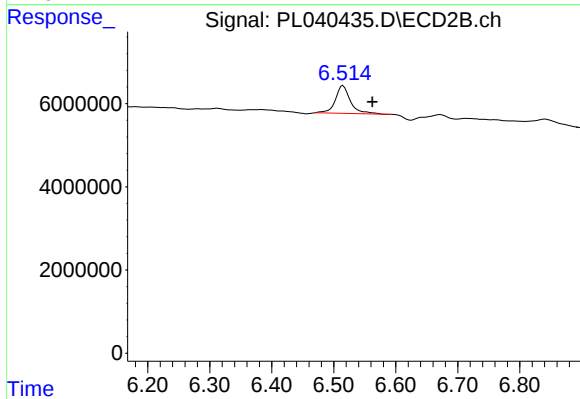

#16 4,4'-DDD


R.T.: 6.515 min
Delta R.T.: -0.047 min
Response: 11274100
Conc: 3.55 ng/ml

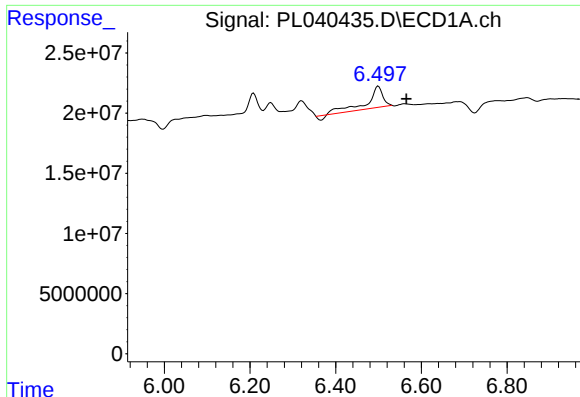

#20 Methoxychlor


R.T.: 6.499 min
Delta R.T.: -0.066 min
Response: 45959434
Conc: 9.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

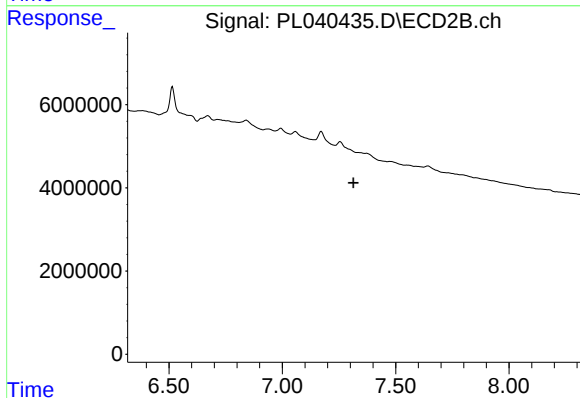


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.314 min
Response: 0
Conc: N.D.

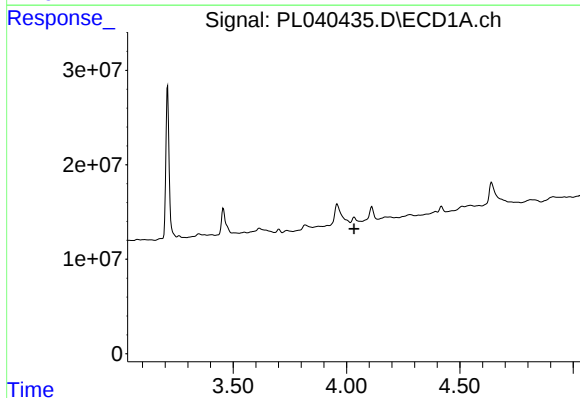


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.034 min
Response: 0
Conc: N.D.

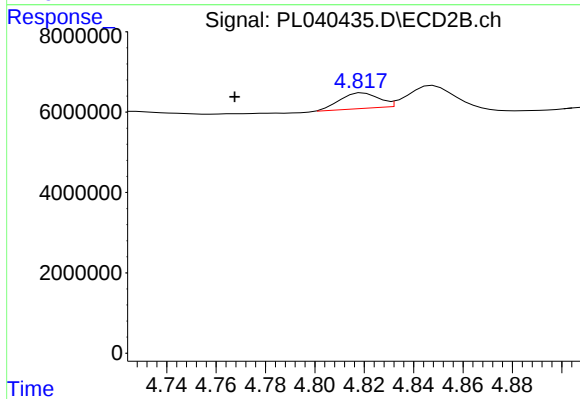

#23 Chlordane-1


R.T.: 4.820 min
Delta R.T.: 0.052 min
Response: 4201508
Conc: 27.22 ng/ml

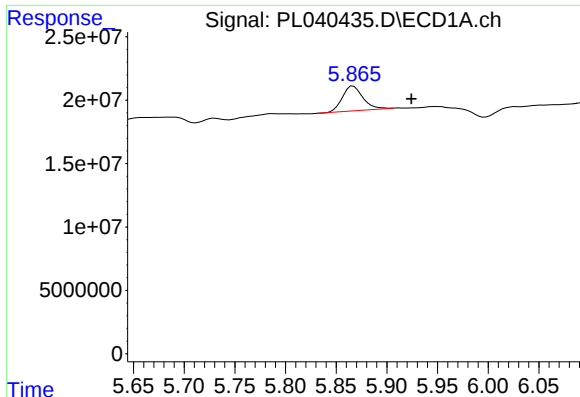

#27 Chlordane-5


R.T.: 5.867 min
Delta R.T.: -0.057 min
Response: 27404790
Conc: 67.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

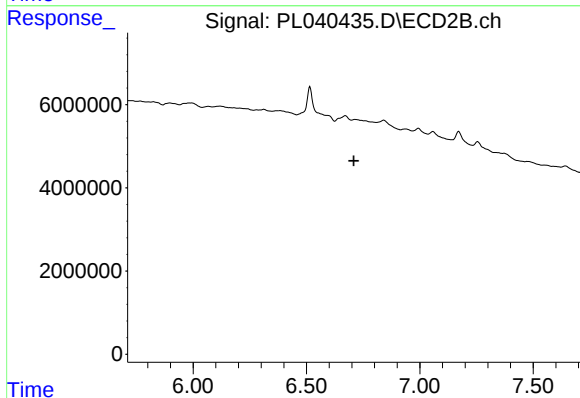


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

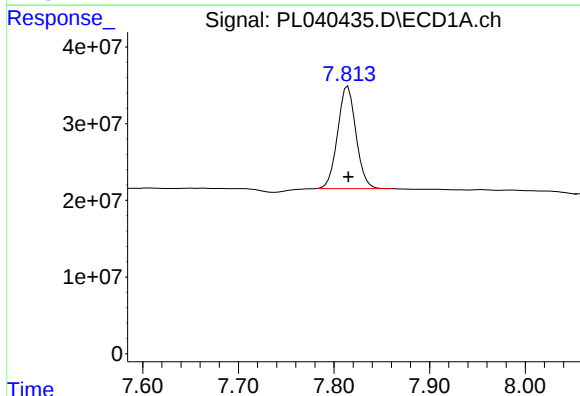

#28 Decachlorobiphenyl

R.T.: 7.815 min
Delta R.T.: 0.000 min
Response: 178322661
Conc: 18.76 ng/ml

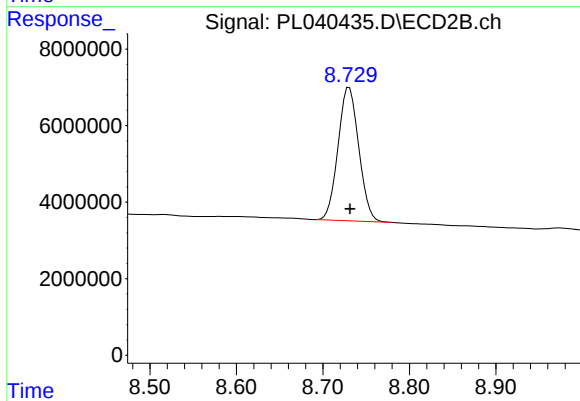

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.001 min
Response: 57761627
Conc: 18.24 ng/ml