

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
 Data File : PL040461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2018 21:11
 Operator : AJ\SJ
 Sample : J5097-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 04:44:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.807	157.3E6	64123997	21.487	20.306
28)	SA Decachlor...	7.816	8.731	202.1E6	67775460	21.257	21.402
Target Compounds							
7)	B delta-BHC	0.000	4.818	0	6447536	N.D.	1.397 #
12)	B 4,4'-DDE	5.306	0.000	35027829	0	3.169	N.D. #
15)	B Endosulfa...	5.868f	0.000	26586772	0	2.669	N.D. #
16)	A 4,4'-DDD	0.000	6.515f	0	10859817	N.D.	3.418 #
19)	B Endosulfa...	6.322	0.000	4320865	0	0.451	N.D. #
20)	A Methoxychlor	6.501f	0.000	228.7E6	0	47.346	N.D. #
23)	Chlordane-1	0.000	4.818	0	6447536	N.D.	41.778 #
27)	Chlordane-5	5.868	0.000	26586772	0	65.865	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
Data File : PL040461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2018 21:11
Operator : AJ\SJ
Sample : J5097-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 04:44:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

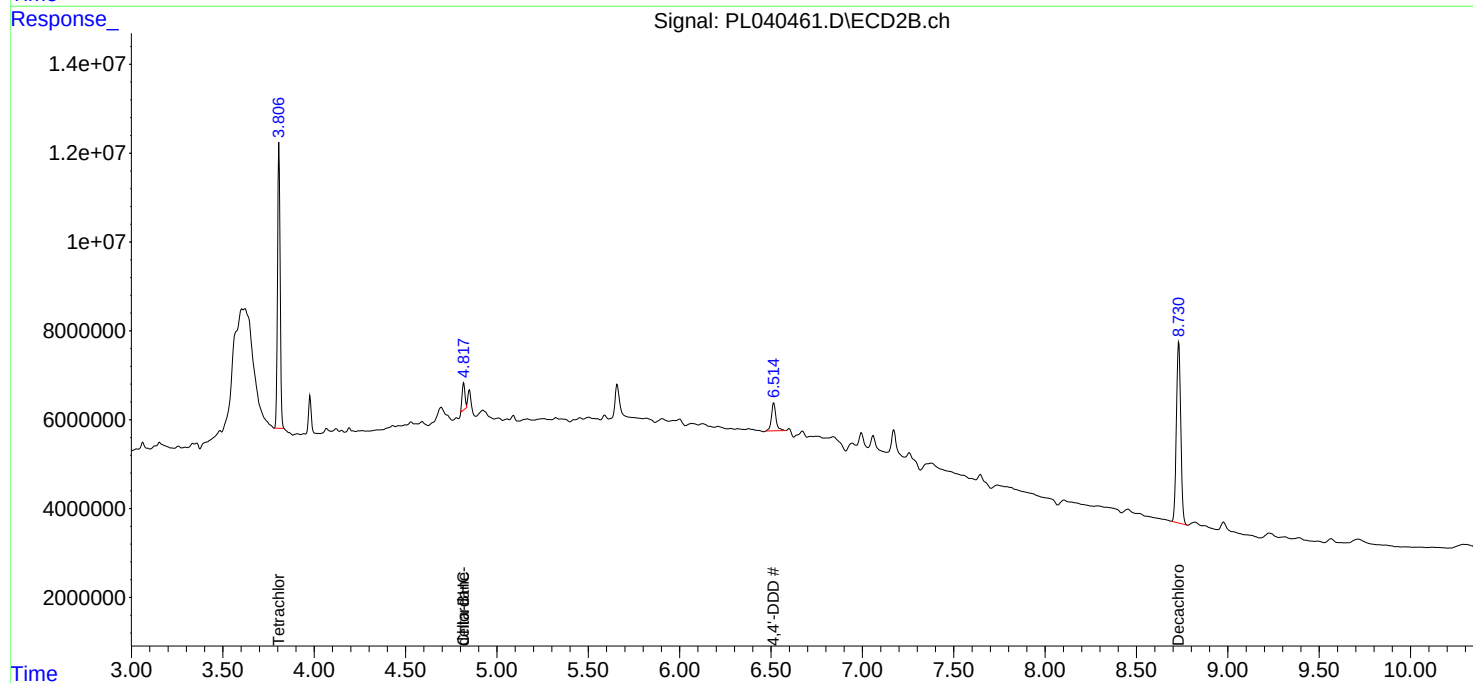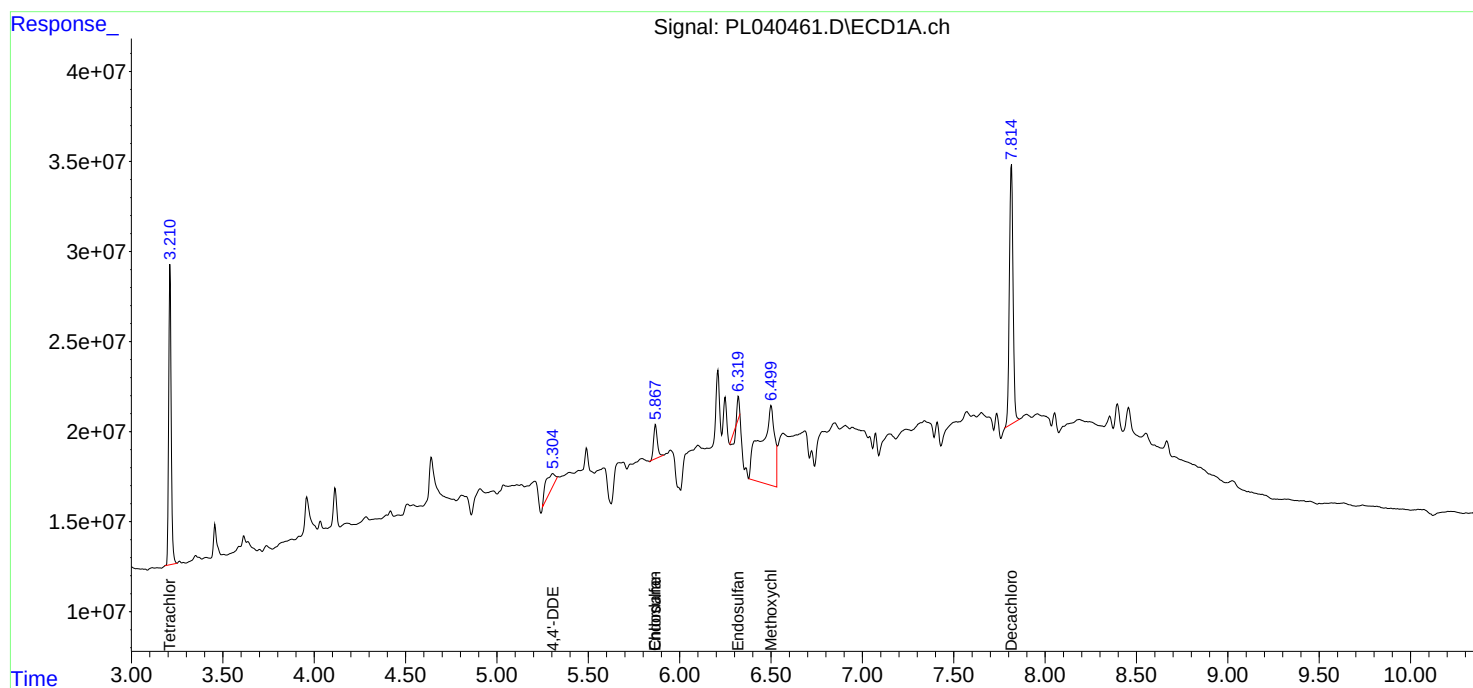


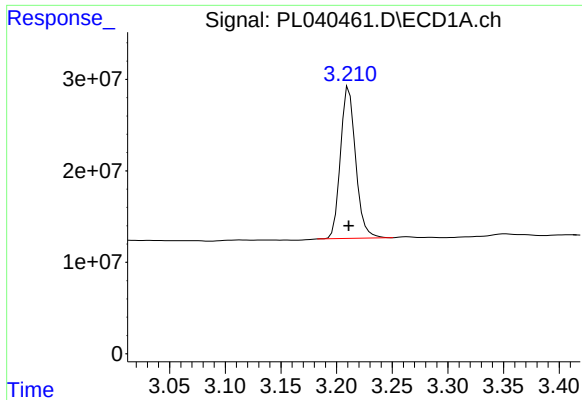

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: 0.000 min
Response: 157285394
Conc: 21.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

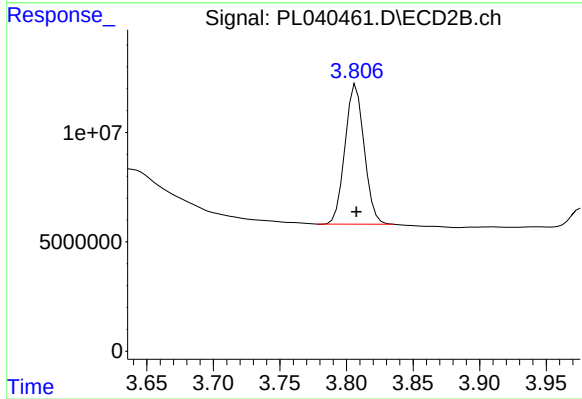


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 64123997
Conc: 20.31 ng/ml

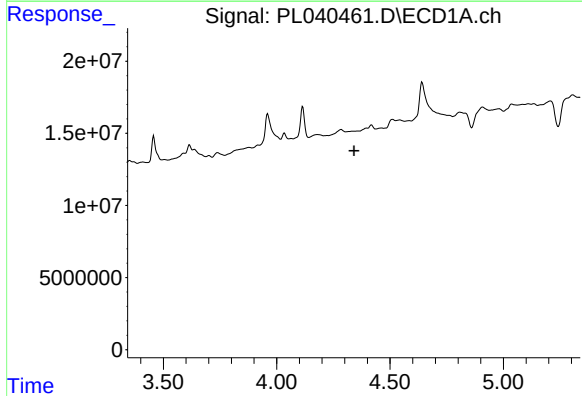


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

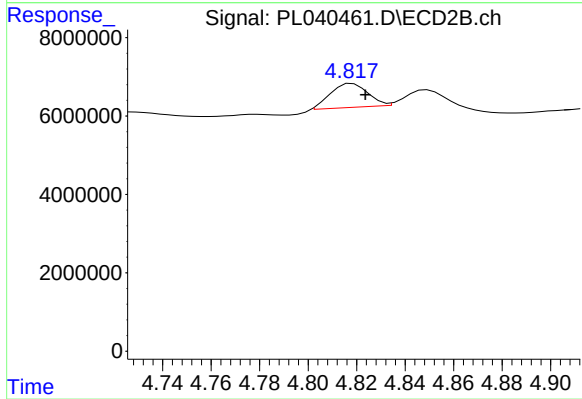

#7 delta-BHC


R.T.: 4.818 min
Delta R.T.: -0.005 min
Response: 6447536
Conc: 1.40 ng/ml

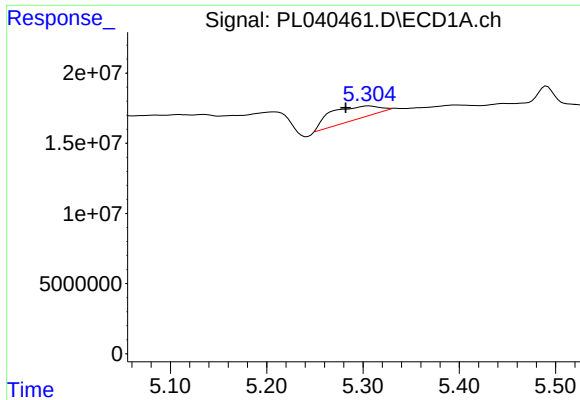

#12 4,4'-DDE


R.T.: 5.306 min
Delta R.T.: 0.024 min
Response: 35027829
Conc: 3.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

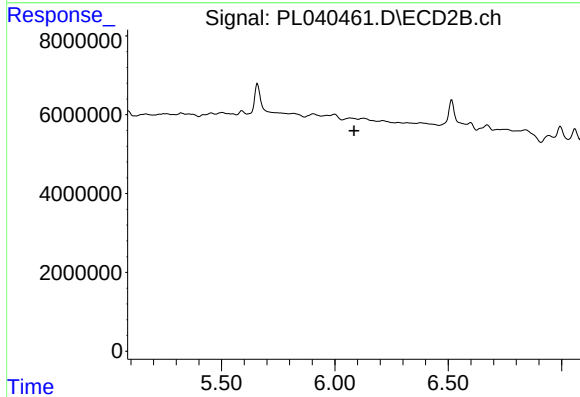


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.084 min
Response: 0
Conc: N.D.

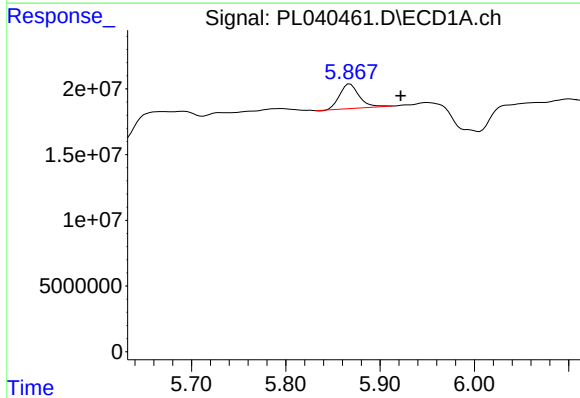


#15 Endosulfan II

R.T.: 5.868 min
Delta R.T.: -0.054 min
Response: 26586772
Conc: 2.67 ng/ml

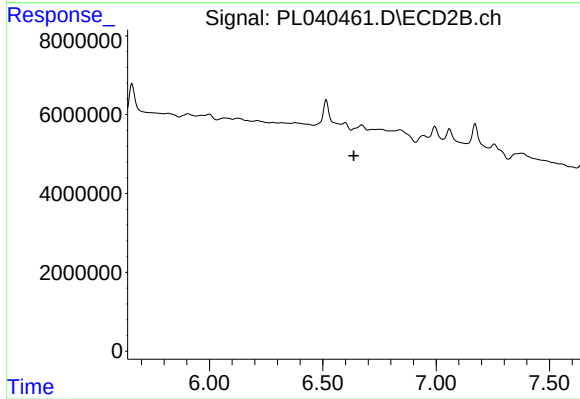

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

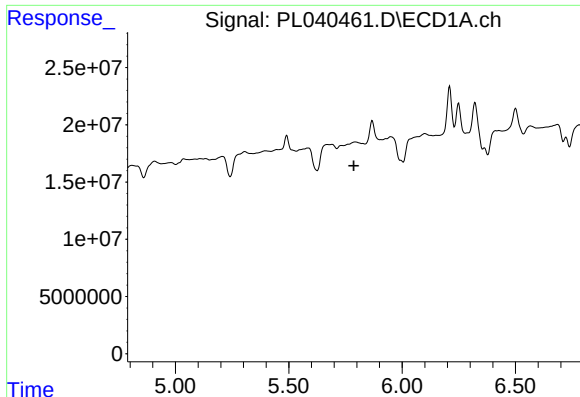

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.787 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

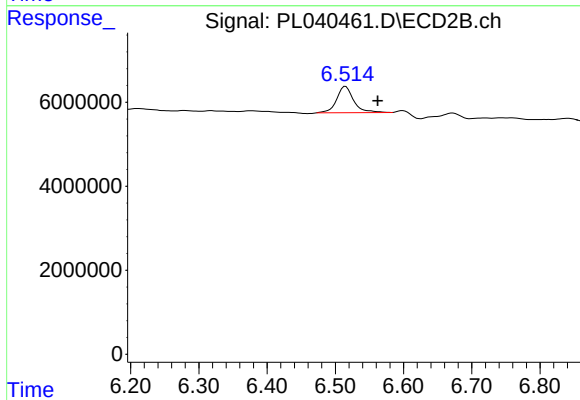


#16 4,4'-DDD

R.T.: 6.515 min
Delta R.T.: -0.047 min
Response: 10859817
Conc: 3.42 ng/ml

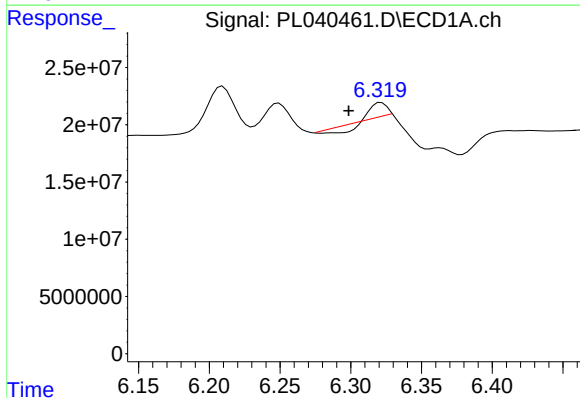


#19 Endosulfan Sulfate

R.T.: 6.322 min
Delta R.T.: 0.023 min
Response: 4320865
Conc: 0.45 ng/ml

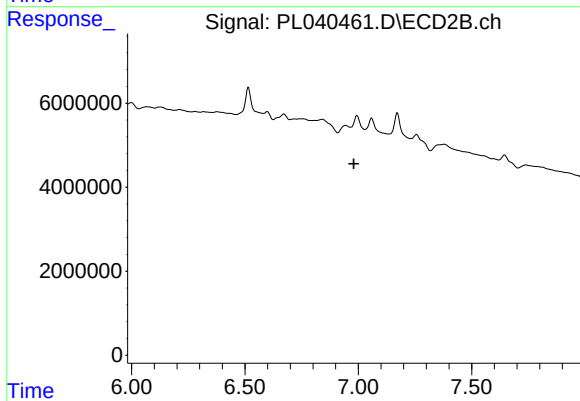

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.980 min
Response: 0
Conc: N.D.

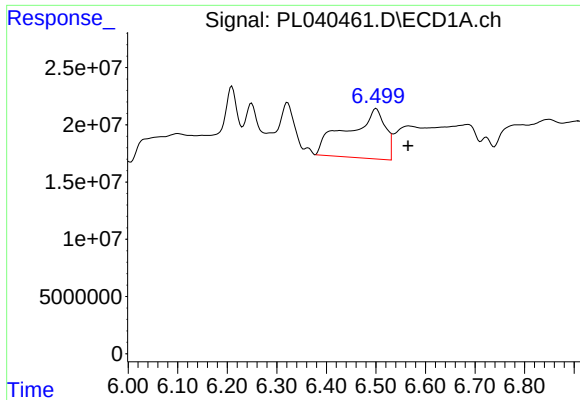

#20 Methoxychlor


R.T.: 6.501 min
Delta R.T.: -0.064 min
Response: 228695847
Conc: 47.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

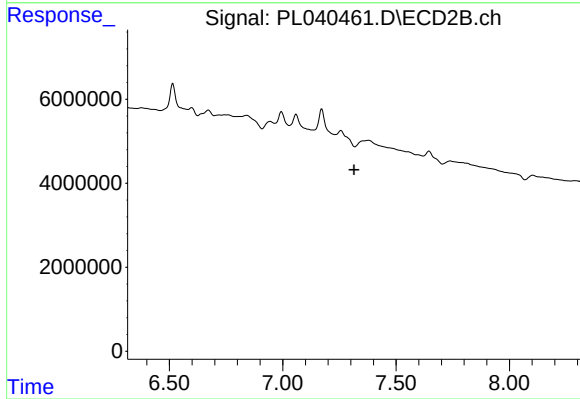


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.314 min
Response: 0
Conc: N.D.

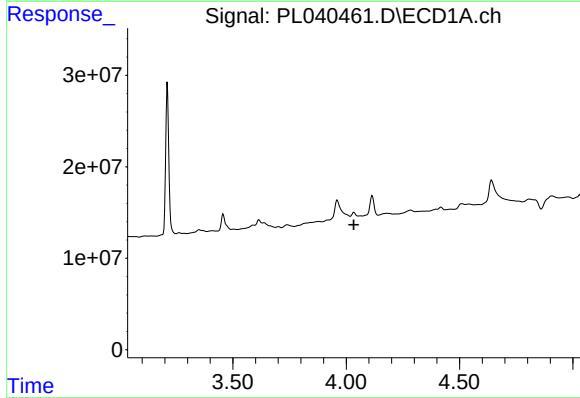


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.034 min
Response: 0
Conc: N.D.

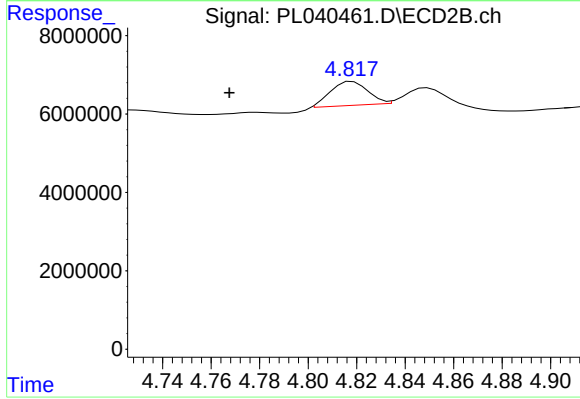

#23 Chlordane-1


R.T.: 4.818 min
Delta R.T.: 0.051 min
Response: 6447536
Conc: 41.78 ng/ml

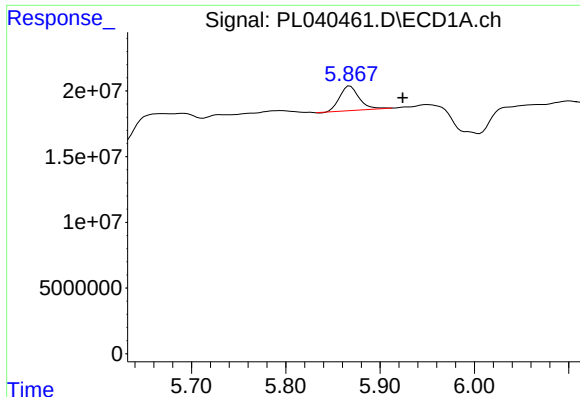

#27 Chlordane-5


R.T.: 5.868 min
Delta R.T.: -0.056 min
Response: 26586772
Conc: 65.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

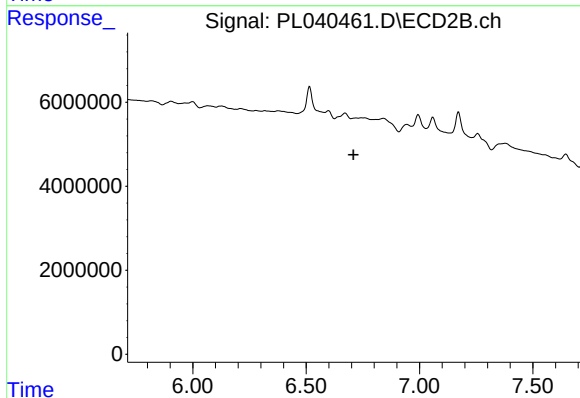


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

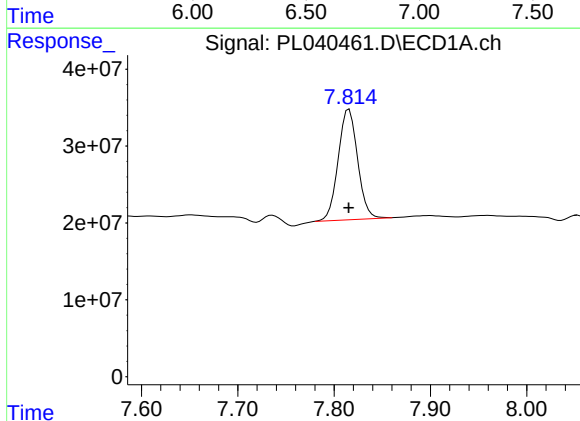

#28 Decachlorobiphenyl

R.T.: 7.816 min
Delta R.T.: 0.000 min
Response: 202064558
Conc: 21.26 ng/ml

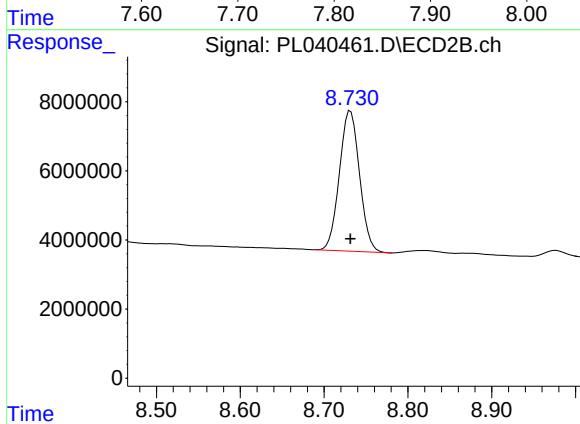

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 67775460
Conc: 21.40 ng/ml