

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
 Data File : PL040466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2018 22:36
 Operator : AJ\SJ
 Sample : J5077-03
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 04:45:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.807	78771878	32963592	10.761	10.439
28)	SA Decachlor...	7.815	8.731	88001945	29260421	9.258	9.240
Target Compounds							
3)	MA gamma-BHC...	0.000	4.461	0	7221846	N.D.	1.591 #
12)	B 4,4'-DDE	5.283	6.085	33302550	11034677	3.013	2.741
13)	MA Dieldrin	0.000	6.161f	0	6419827	N.D.	1.680 #
14)	MA Endrin	5.714f	0.000	23680198	0	2.384	N.D. #
15)	B Endosulfa...	0.000	6.573f	0	15749445	N.D.	4.505 #
16)	A 4,4'-DDD	0.000	6.573	0	15749445	N.D.	4.957 #
17)	MA 4,4'-DDT	6.015	6.833	48795646	4525340	6.034	1.485 #
21)	B Endrin ke...	0.000	7.424	0	6190988	N.D.	2.014 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
Data File : PL040466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2018 22:36
Operator : AJ\SJ
Sample : J5077-03
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 04:45:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

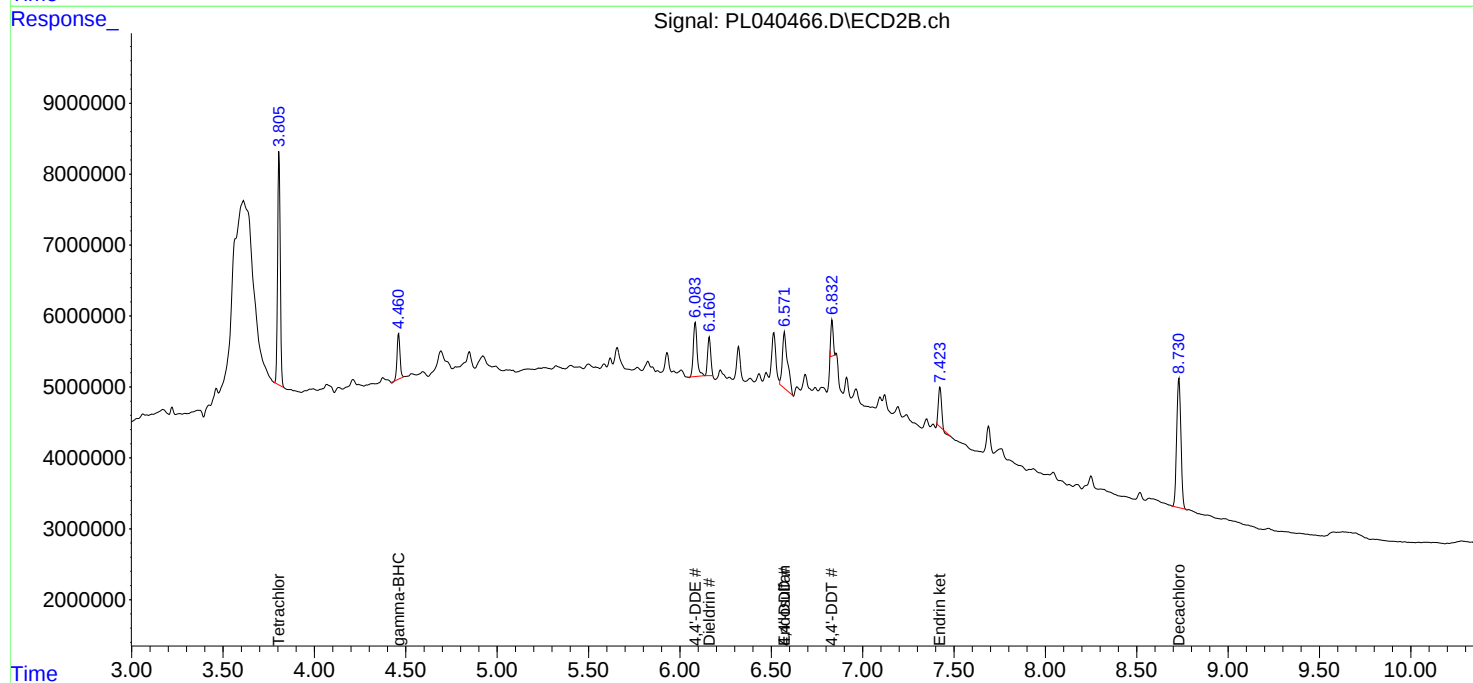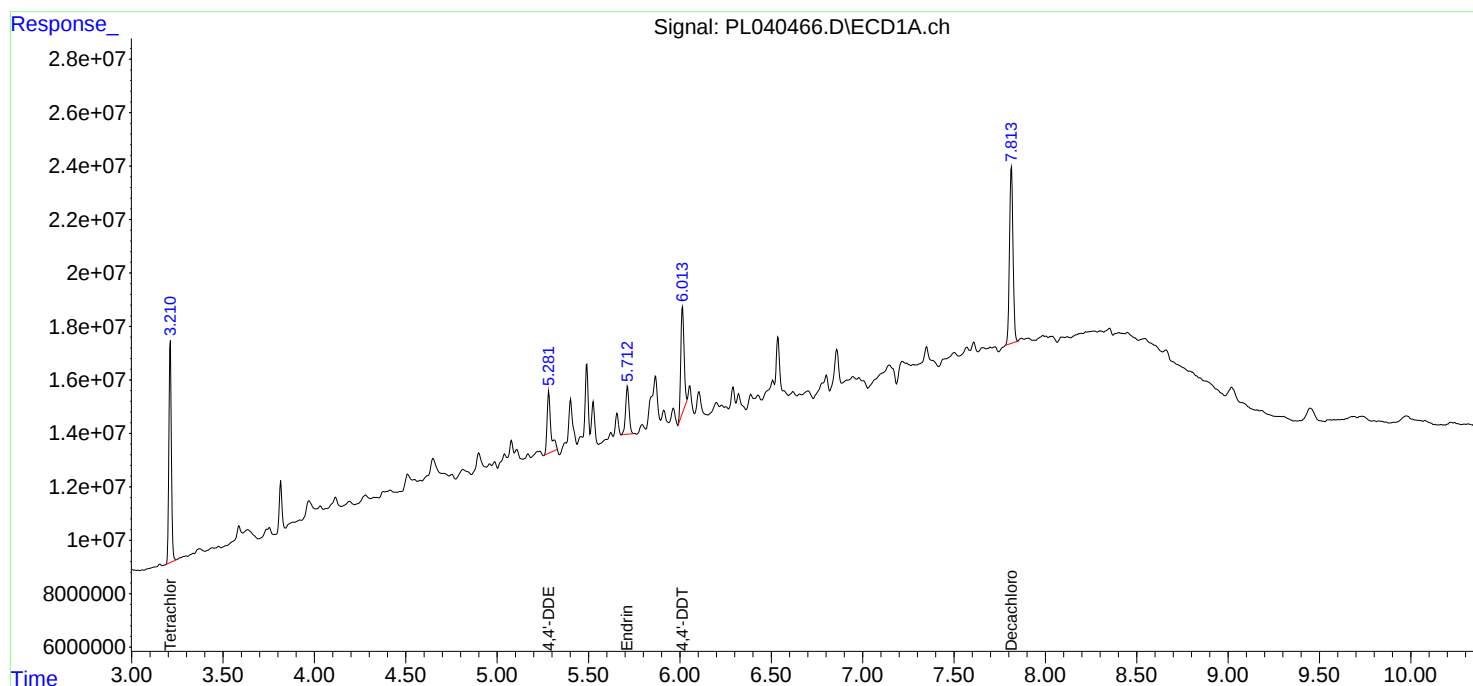


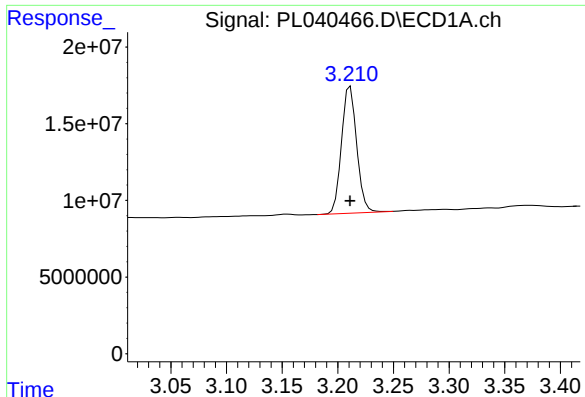

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: 0.000 min
Response: 78771878
Conc: 10.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

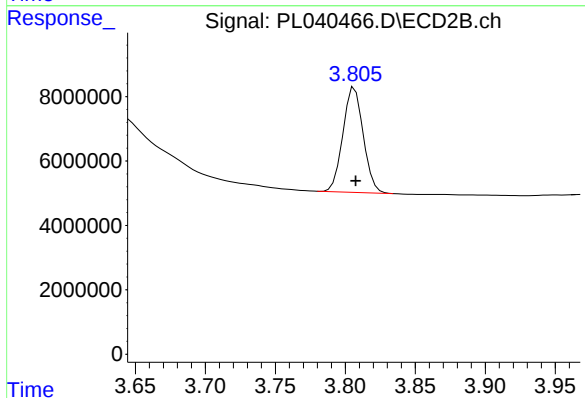


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 32963592
Conc: 10.44 ng/ml

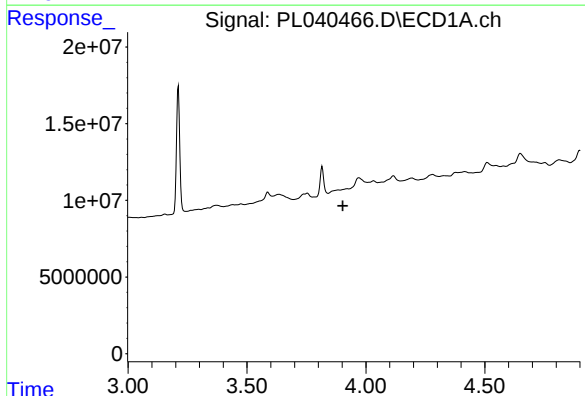


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.902 min
Response: 0
Conc: N.D.

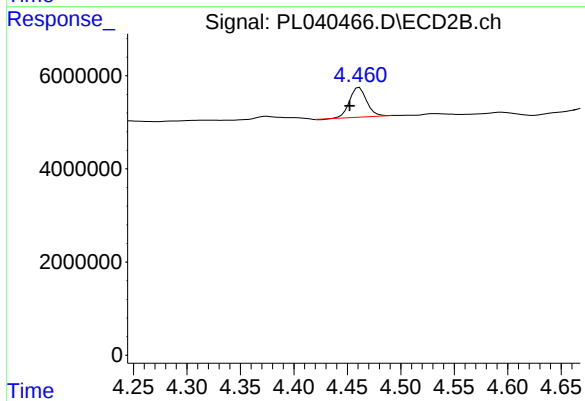

#3 gamma-BHC (Lindane)


R.T.: 4.461 min
Delta R.T.: 0.009 min
Response: 7221846
Conc: 1.59 ng/ml

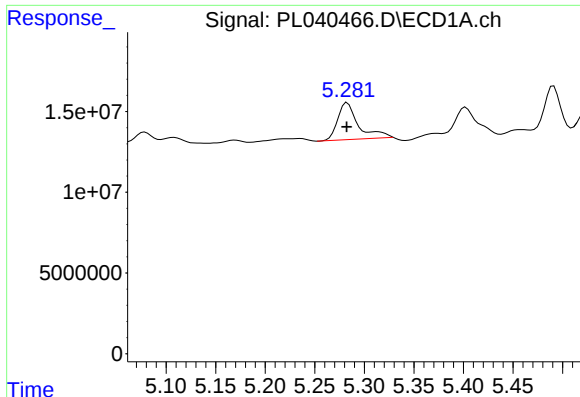

#12 4,4'-DDE


R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 33302550
Conc: 3.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

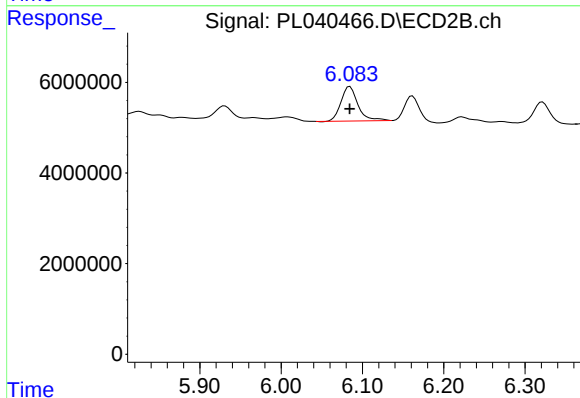


#12 4,4'-DDE

R.T.: 6.085 min
Delta R.T.: 0.000 min
Response: 11034677
Conc: 2.74 ng/ml

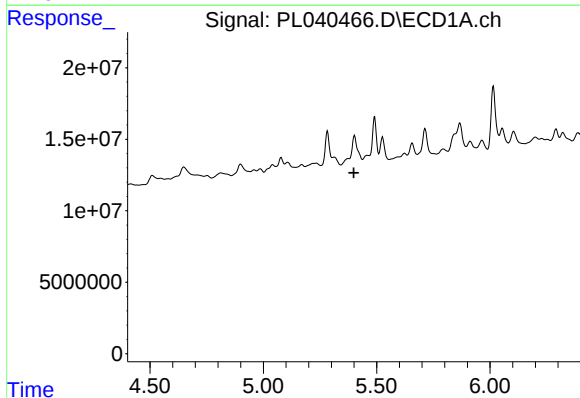


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.399 min
Response: 0
Conc: N.D.

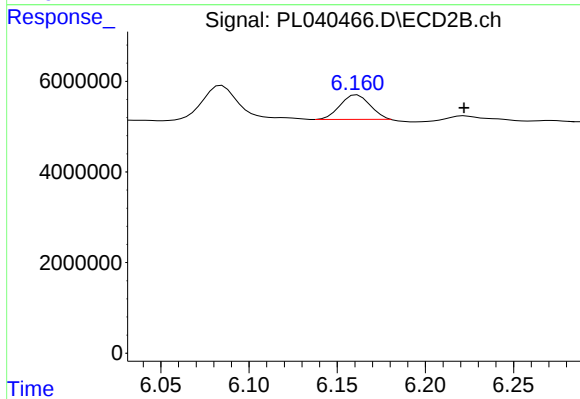

#13 Dieldrin


R.T.: 6.161 min
Delta R.T.: -0.061 min
Response: 6419827
Conc: 1.68 ng/ml

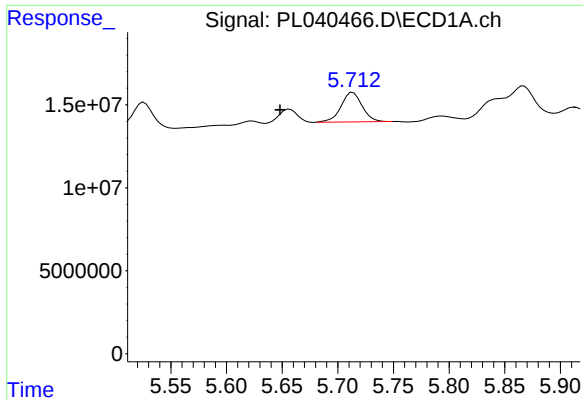

#14 Endrin


R.T.: 5.714 min
Delta R.T.: 0.066 min
Response: 23680198
Conc: 2.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

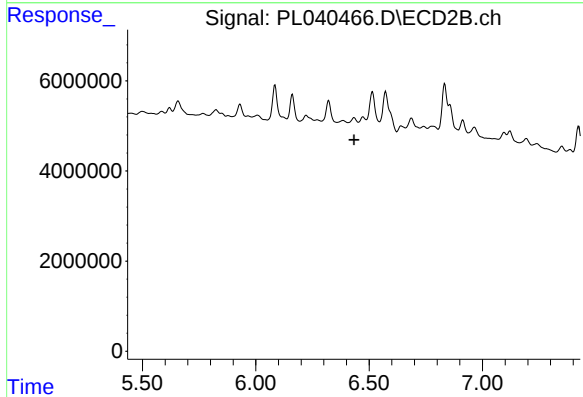


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

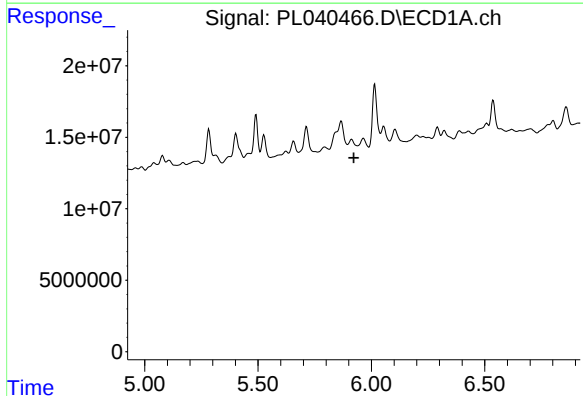


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.922 min
Response: 0
Conc: N.D.

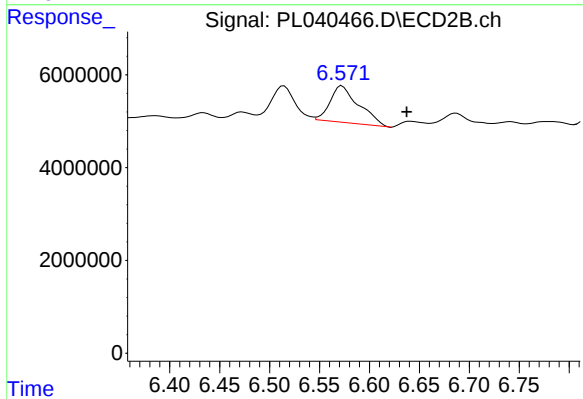

#15 Endosulfan II


R.T.: 6.573 min
Delta R.T.: -0.065 min
Response: 15749445
Conc: 4.51 ng/ml

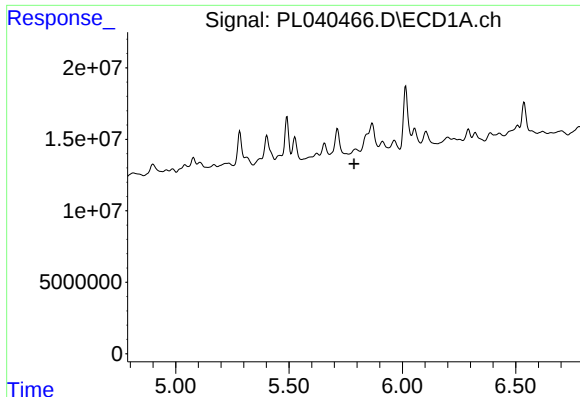

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.787 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

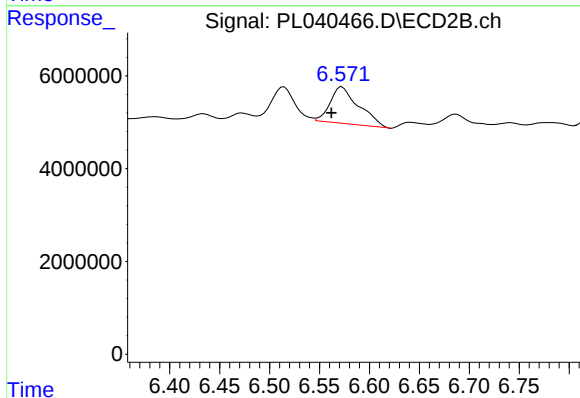


#16 4,4'-DDD

R.T.: 6.573 min
Delta R.T.: 0.011 min
Response: 15749445
Conc: 4.96 ng/ml

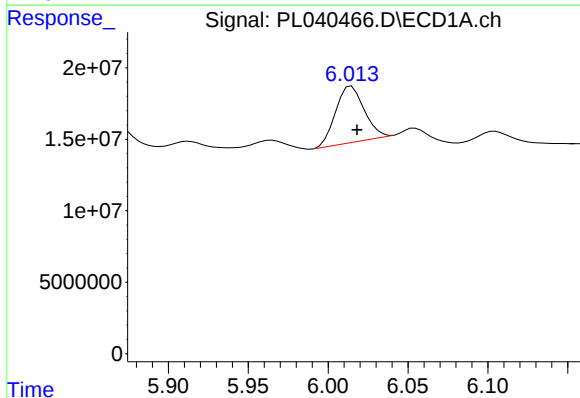


#17 4,4'-DDT

R.T.: 6.015 min
Delta R.T.: -0.004 min
Response: 48795646
Conc: 6.03 ng/ml

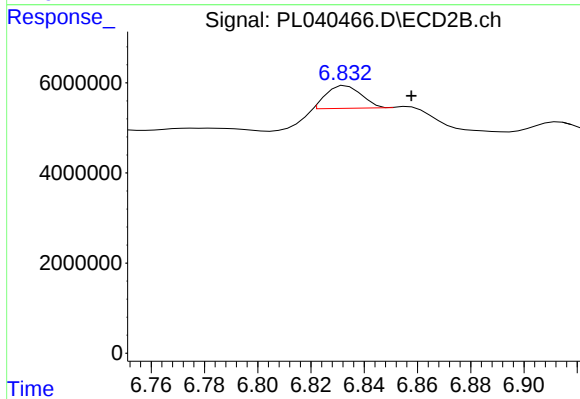

#17 4,4'-DDT


R.T.: 6.833 min
Delta R.T.: -0.024 min
Response: 4525340
Conc: 1.49 ng/ml

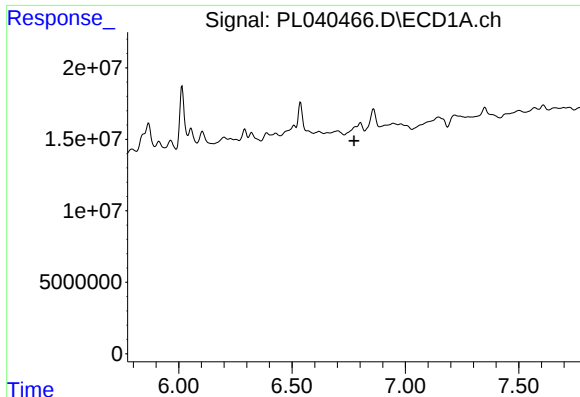

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

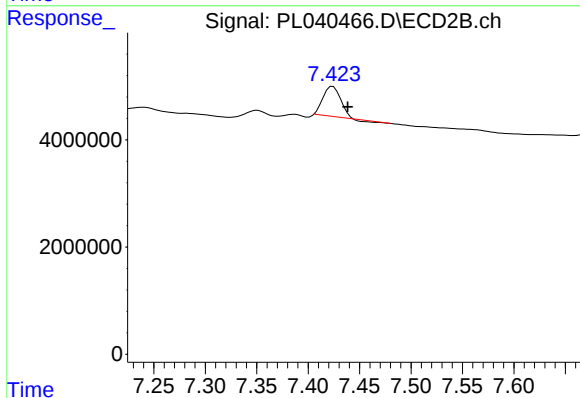


#21 Endrin ketone

R.T.: 7.424 min
Delta R.T.: -0.014 min
Response: 6190988
Conc: 2.01 ng/ml

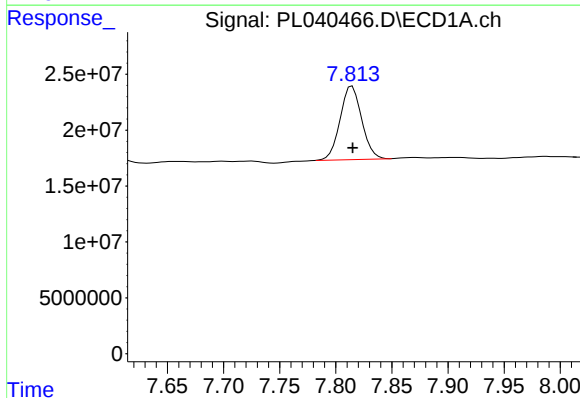

#28 Decachlorobiphenyl

R.T.: 7.815 min
Delta R.T.: 0.000 min
Response: 88001945
Conc: 9.26 ng/ml

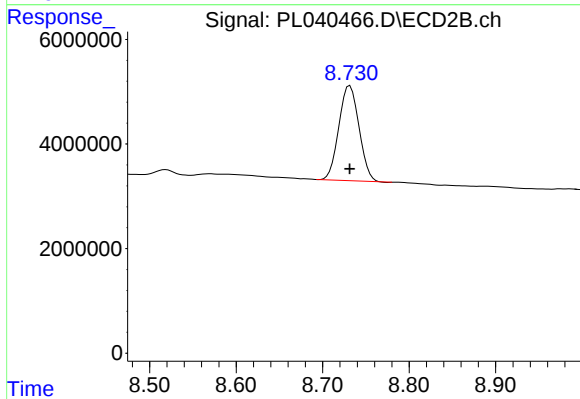

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 29260421
Conc: 9.24 ng/ml