

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
 Data File : PL040474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2018 00:29
 Operator : AJ\SJ
 Sample : J5093-01
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 04:47:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.807	57931269	24726835	7.914	7.830
28)	SA Decachlor...	7.815	8.731	44234663	13022955	4.653	4.112
Target Compounds							
9)	A Endosulfan I	5.112f	5.929f	16247044	6661604	1.612	1.790
10)	B gamma-Chl...	5.077	0.000	48362359	0	4.453	N.D. #
11)	B alpha-Chl...	5.112	5.929	16247044	6661604	1.551	1.697
12)	B 4,4'-DDE	5.283	0.000	33042731	0	2.989	N.D. #
15)	B Endosulfa...	5.868f	0.000	25453816	0	2.555	N.D. #
16)	A 4,4'-DDD	0.000	6.515f	0	9310810	N.D.	2.931 #
25)	Chlordane-3	5.077	0.000	48362359	0	37.649	N.D. #
26)	Chlordane-4	5.112	5.929	16247044	6661604	13.712	10.094 #
27)	Chlordane-5	5.868	0.000	25453816	0	63.058	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
Data File : PL040474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2018 00:29
Operator : AJ\SJ
Sample : J5093-01
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 04:47:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

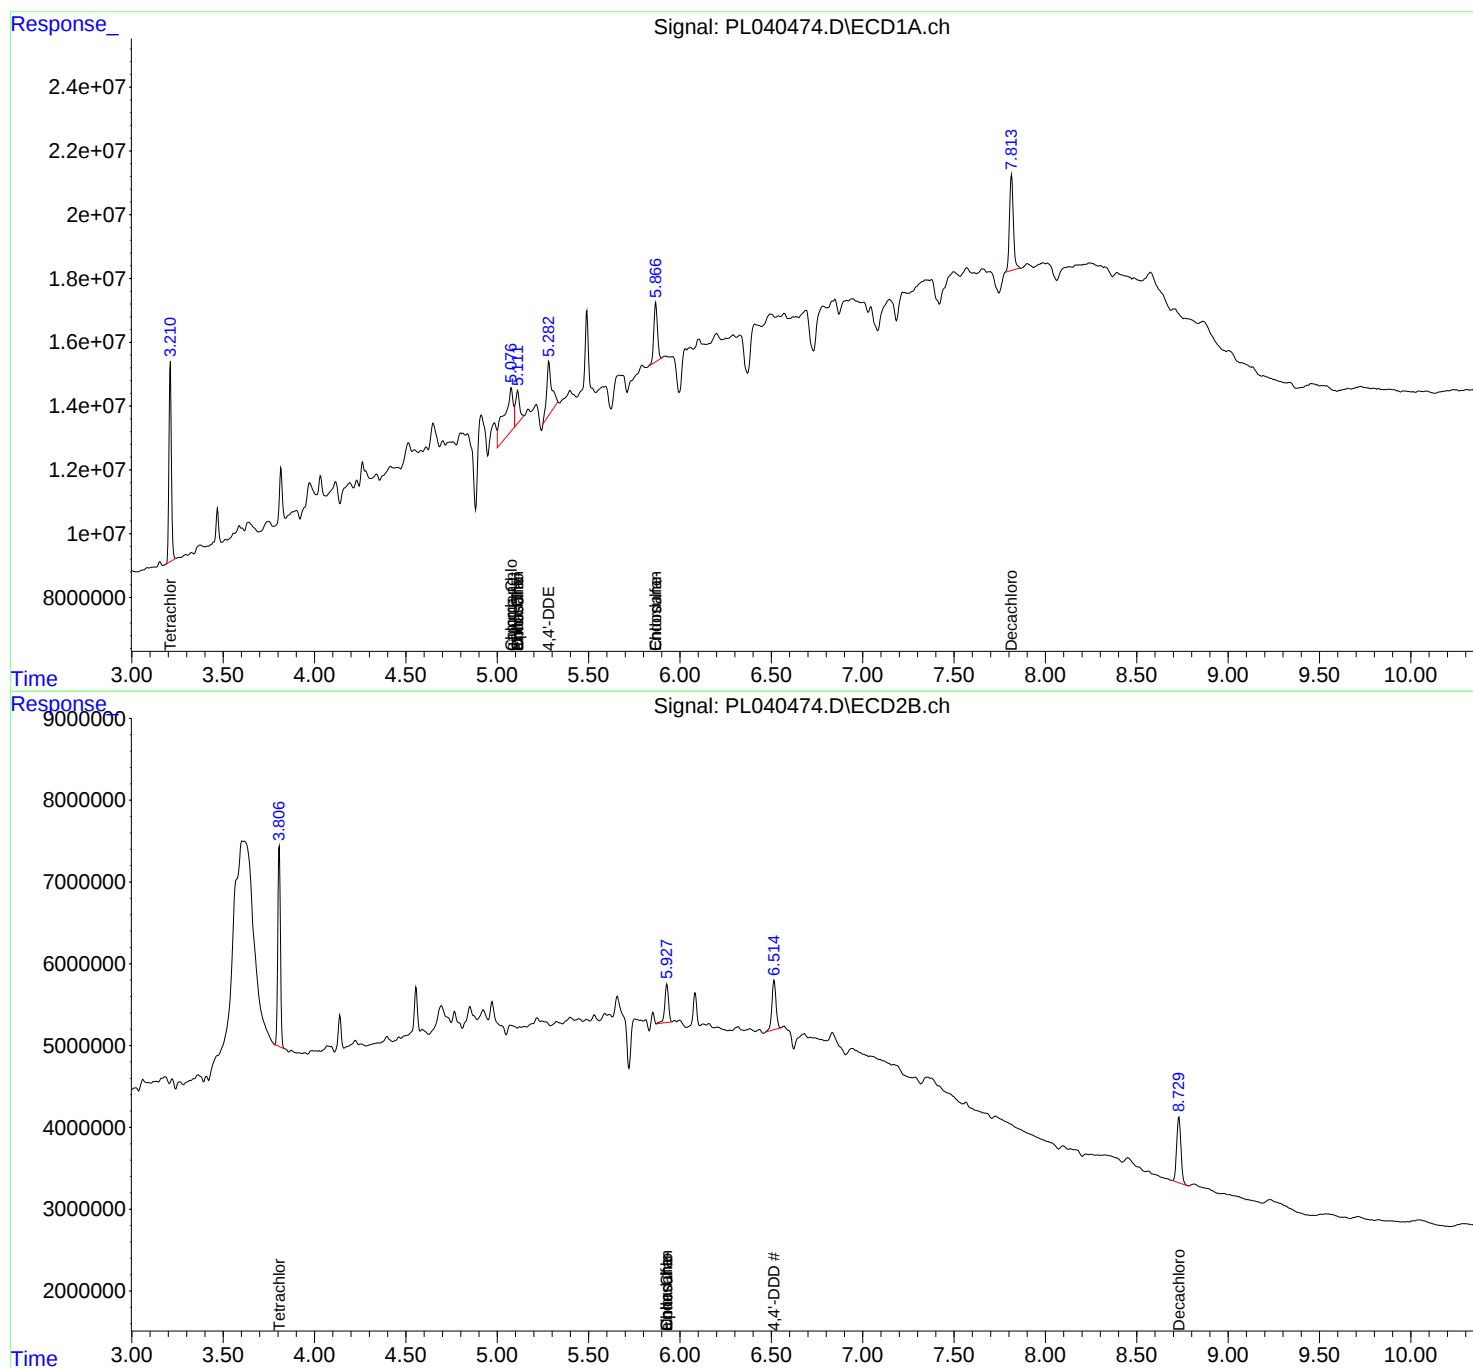


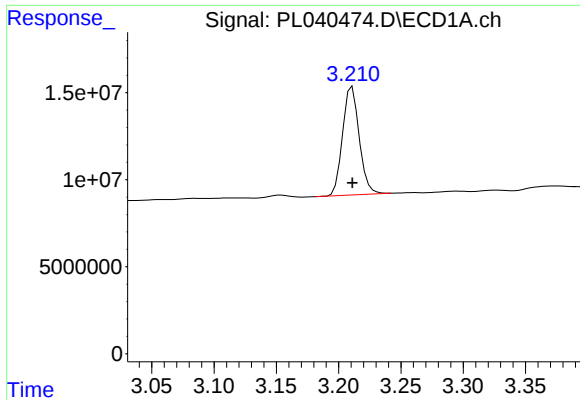

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: 0.000 min
Response: 57931269
Conc: 7.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

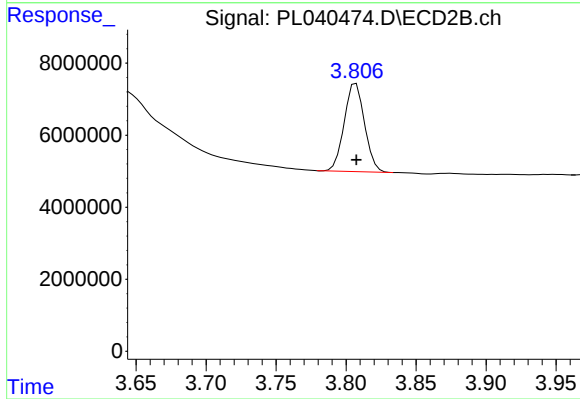


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 24726835
Conc: 7.83 ng/ml

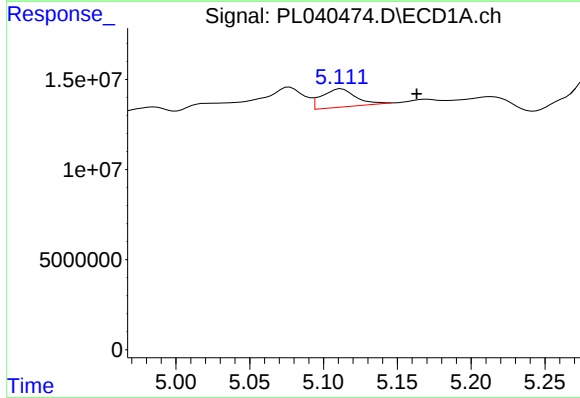


#9 Endosulfan I

R.T.: 5.112 min
Delta R.T.: -0.051 min
Response: 16247044
Conc: 1.61 ng/ml

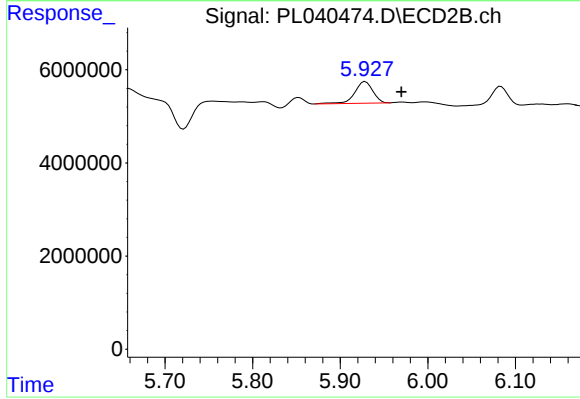

#9 Endosulfan I


R.T.: 5.929 min
Delta R.T.: -0.041 min
Response: 6661604
Conc: 1.79 ng/ml

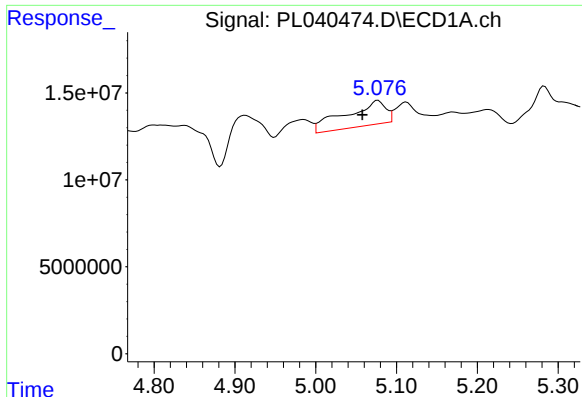

#10 gamma-Chlordane


R.T.: 5.077 min
Delta R.T.: 0.019 min
Response: 48362359
Conc: 4.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

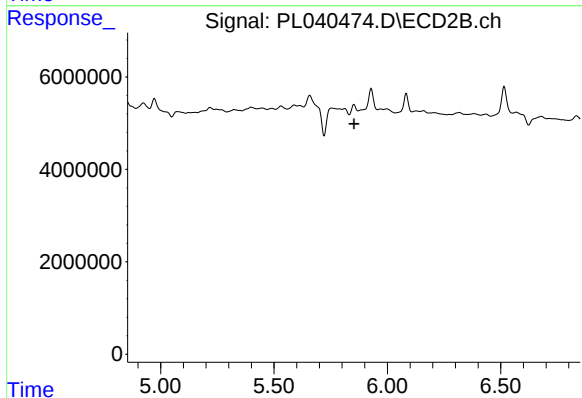


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.853 min
Response: 0
Conc: N.D.

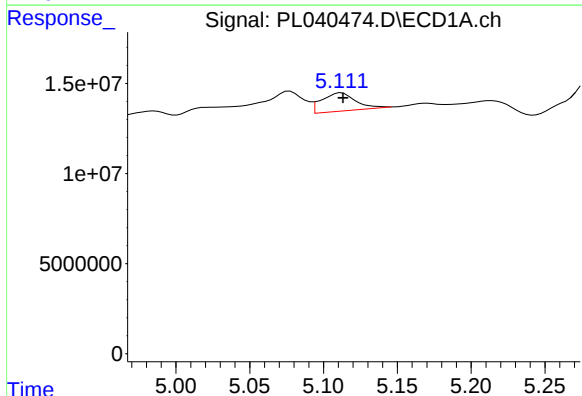


#11 alpha-Chlordane

R.T.: 5.112 min
Delta R.T.: -0.001 min
Response: 16247044
Conc: 1.55 ng/ml

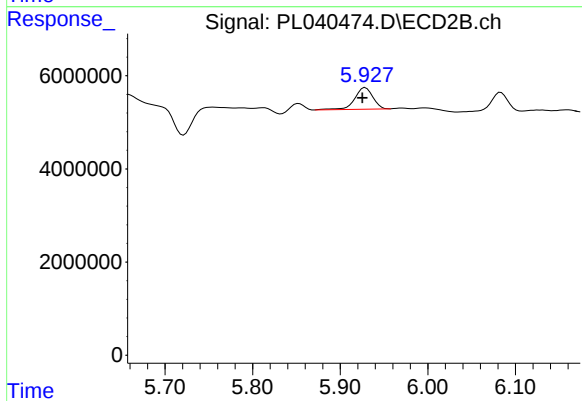

#11 alpha-Chlordane


R.T.: 5.929 min
Delta R.T.: 0.003 min
Response: 6661604
Conc: 1.70 ng/ml

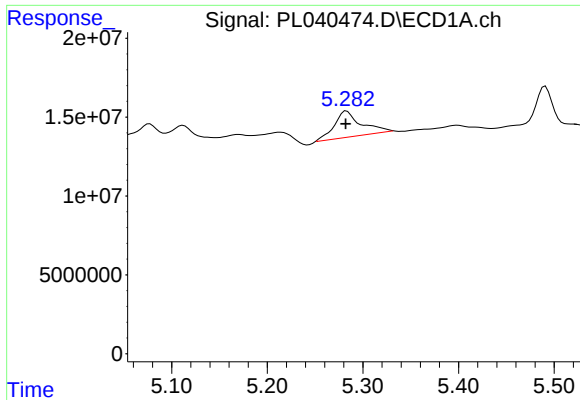

#12 4,4'-DDE


R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 33042731
Conc: 2.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

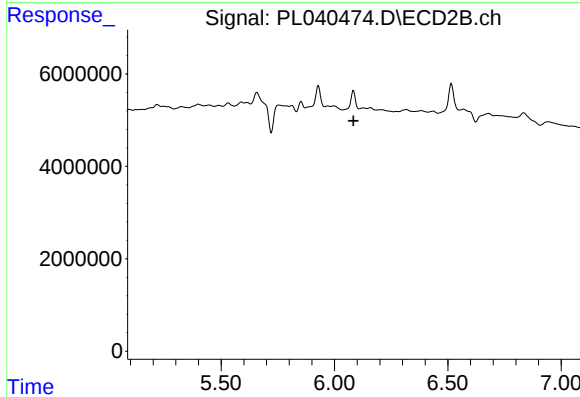


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.084 min
Response: 0
Conc: N.D.

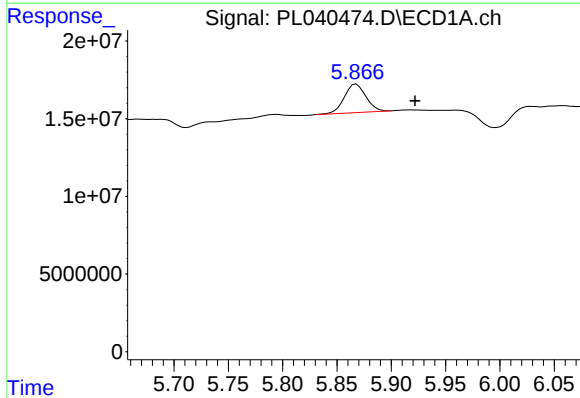


#15 Endosulfan II

R.T.: 5.868 min
Delta R.T.: -0.054 min
Response: 25453816
Conc: 2.55 ng/ml

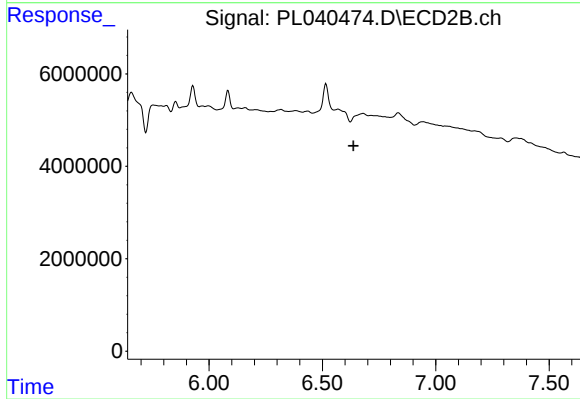

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

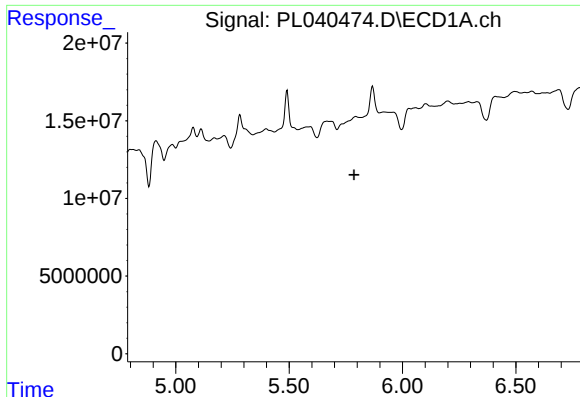

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.787 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

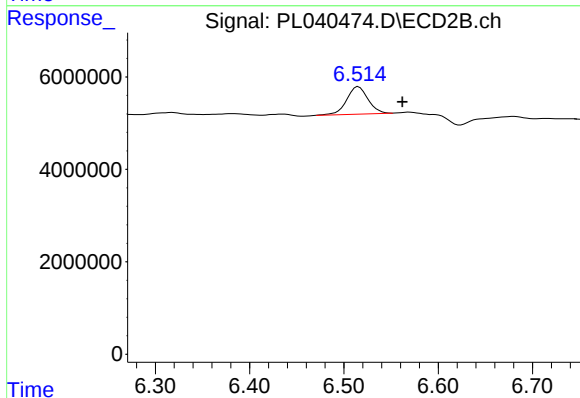


#16 4,4'-DDD

R.T.: 6.515 min
Delta R.T.: -0.047 min
Response: 9310810
Conc: 2.93 ng/ml

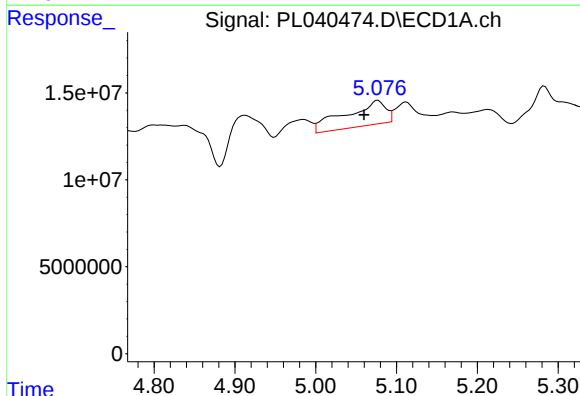


#25 Chlordane-3

R.T.: 5.077 min
Delta R.T.: 0.017 min
Response: 48362359
Conc: 37.65 ng/ml

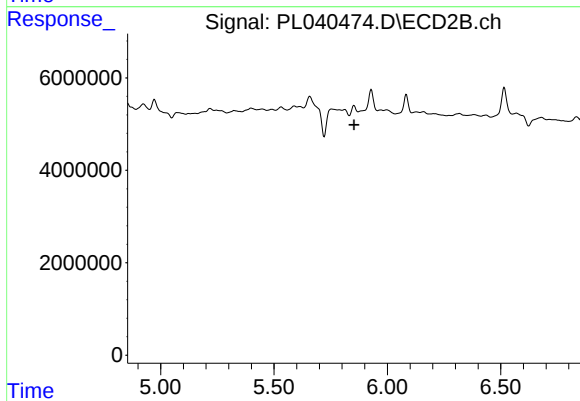

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.854 min
Response: 0
Conc: N.D.

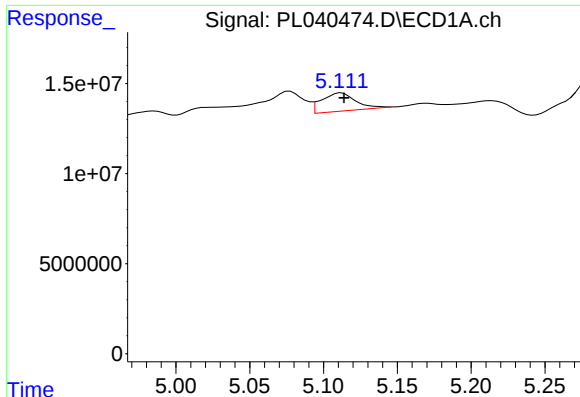

#26 Chlordane-4


R.T.: 5.112 min
Delta R.T.: -0.002 min
Response: 16247044
Conc: 13.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

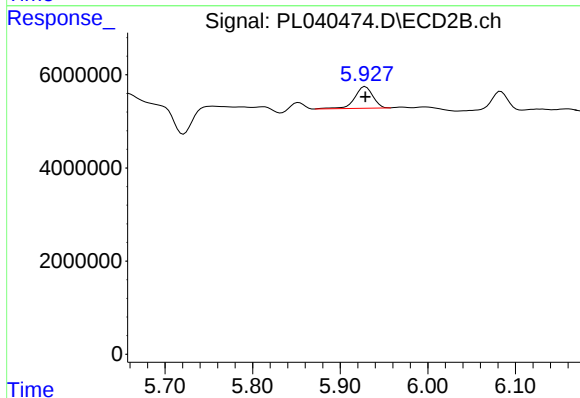


#26 Chlordane-4

R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 6661604
Conc: 10.09 ng/ml

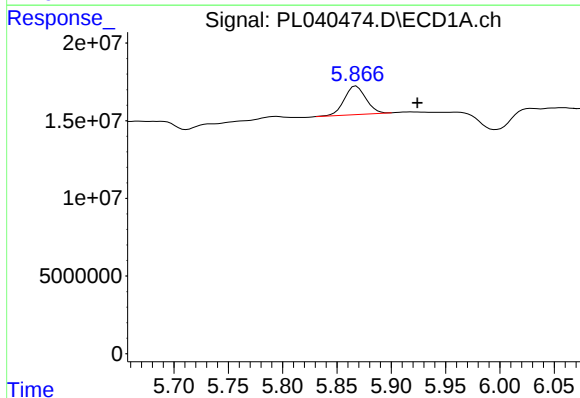


#27 Chlordane-5

R.T.: 5.868 min
Delta R.T.: -0.056 min
Response: 25453816
Conc: 63.06 ng/ml

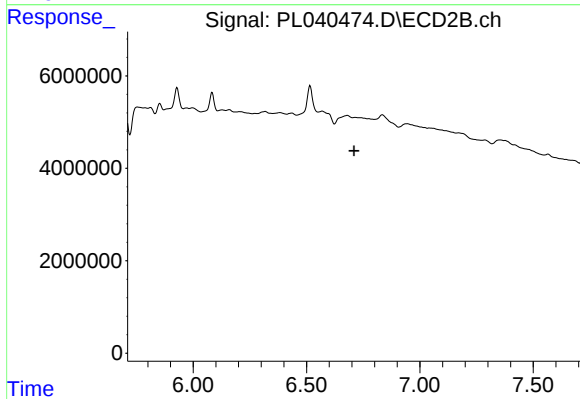

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

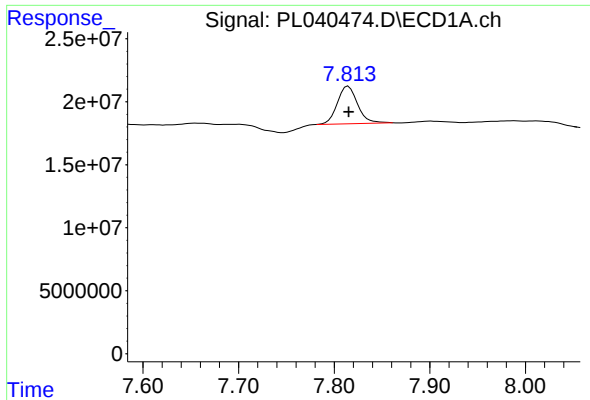

#28 Decachlorobiphenyl

R.T.: 7.815 min
Delta R.T.: 0.000 min
Response: 44234663
Conc: 4.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

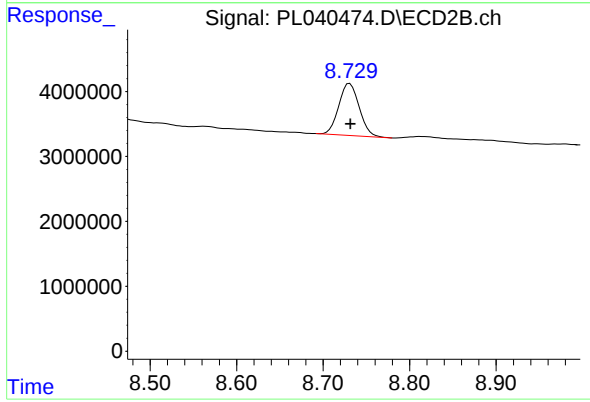

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 13022955
Conc: 4.11 ng/ml