

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
 Data File : PL040478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2018 01:26
 Operator : AJ\SJ
 Sample : J5099-02
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 04:48:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.807	161.8E6	66260979	22.107	20.983
28)	SA Decachlor...	7.815	8.732	209.1E6	67120464	21.999	21.195
Target Compounds							
4)	MA Heptachlor	4.115f	0.000	189310	0	0.016	N.D. #
6)	B beta-BHC	4.115f	0.000	189310	0	0.045	N.D. #
7)	B delta-BHC	0.000	4.818	0	8018892	N.D.	1.737 #
15)	B Endosulfa...	5.868f	0.000	25254735	0	2.535	N.D. #
16)	A 4,4'-DDD	0.000	6.516f	0	9089509	N.D.	2.861 #
19)	B Endosulfa...	6.321	0.000	13317422	0	1.391	N.D. #
20)	A Methoxychlor	6.500f	0.000	70216345	0	14.537	N.D. #
23)	Chlordane-1	0.000	4.818	0	8018892	N.D.	51.960 #
27)	Chlordane-5	5.868	0.000	25254735	0	62.565	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
Data File : PL040478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2018 01:26
Operator : AJ\SJ
Sample : J5099-02
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 04:48:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

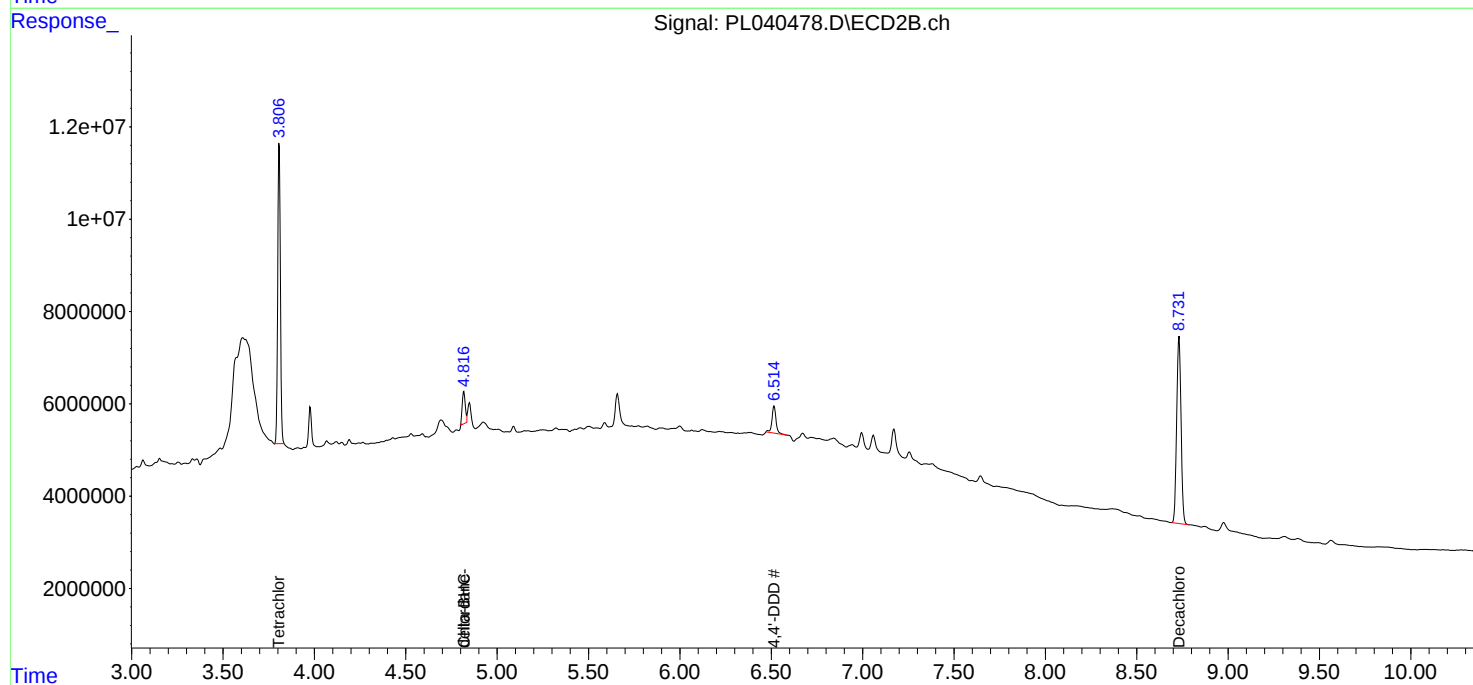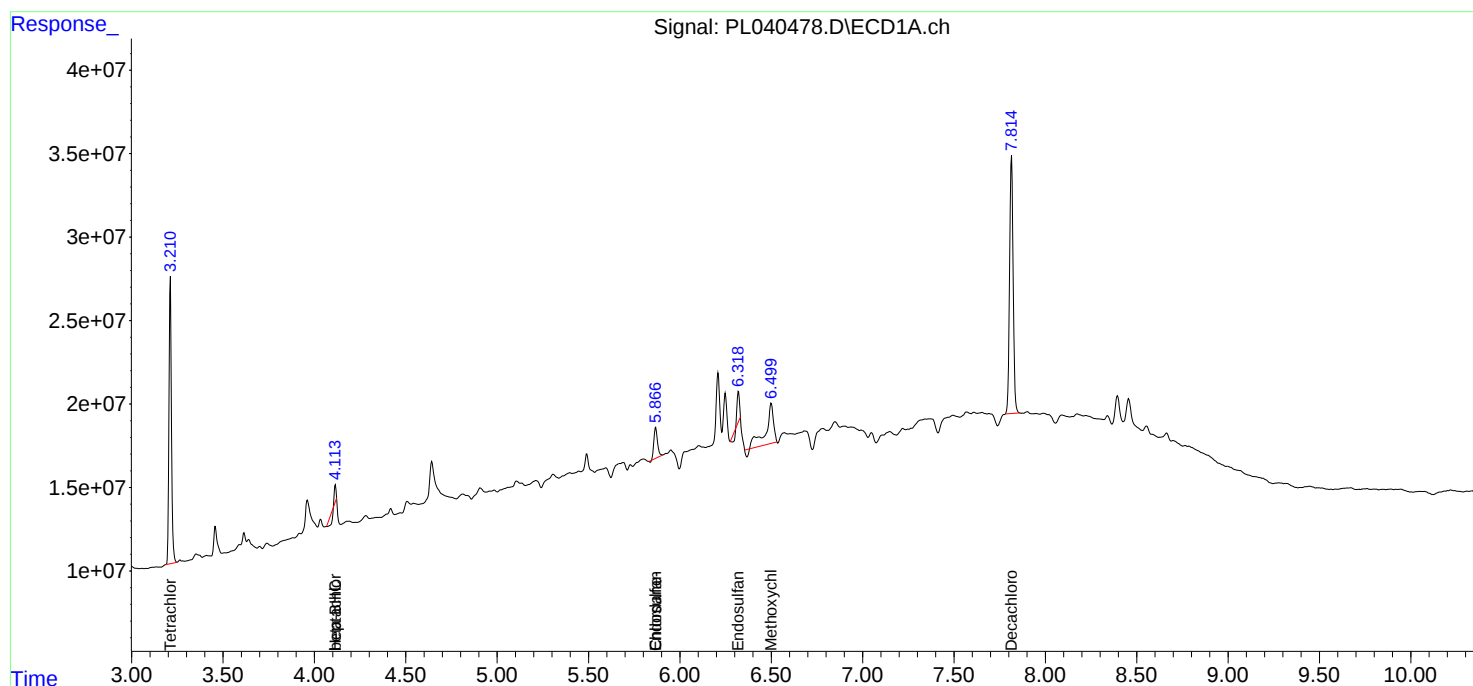


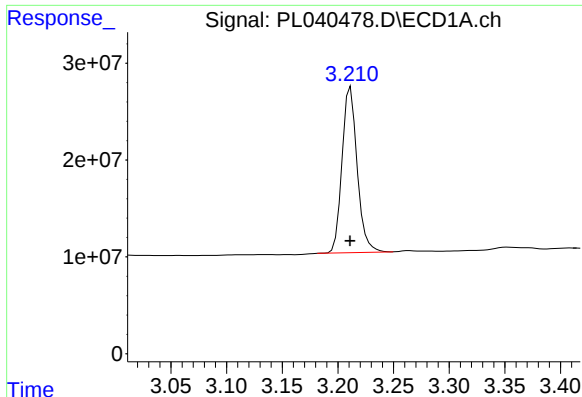

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: 0.000 min
Response: 161826795
Conc: 22.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

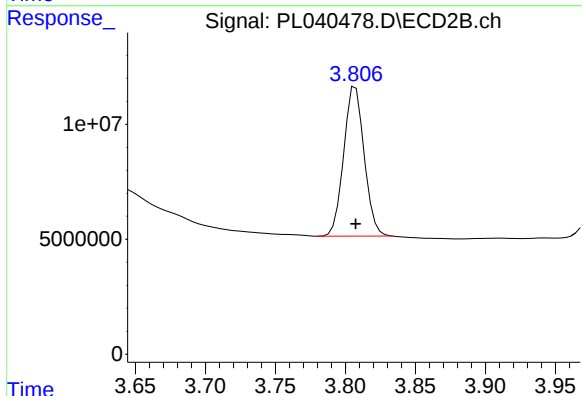


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 66260979
Conc: 20.98 ng/ml

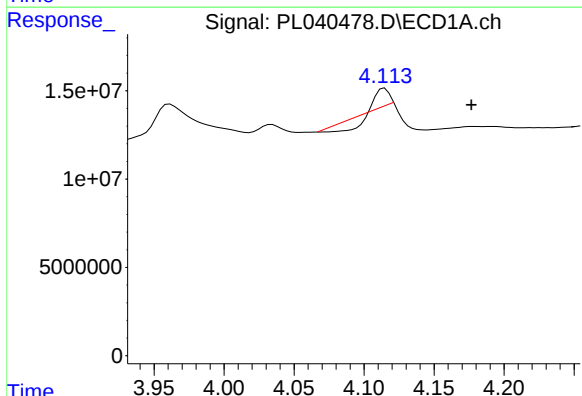


#4 Heptachlor

R.T.: 4.115 min
Delta R.T.: -0.062 min
Response: 189310
Conc: 0.02 ng/ml

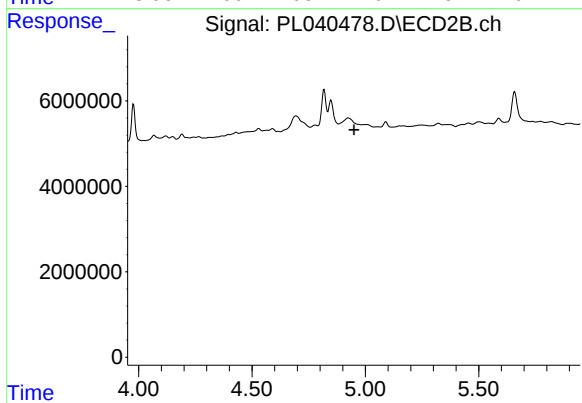

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.951 min
Response: 0
Conc: N.D.

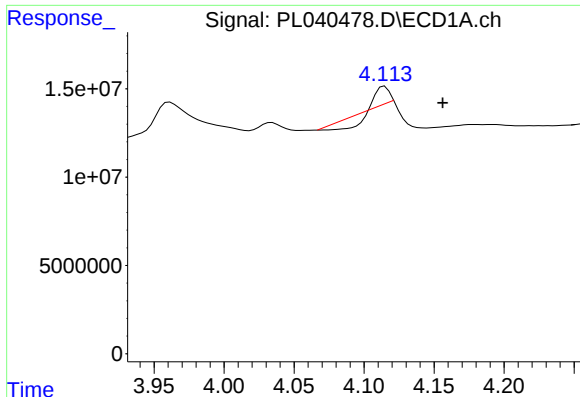

#6 beta-BHC


R.T.: 4.115 min
Delta R.T.: -0.041 min
Response: 189310
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

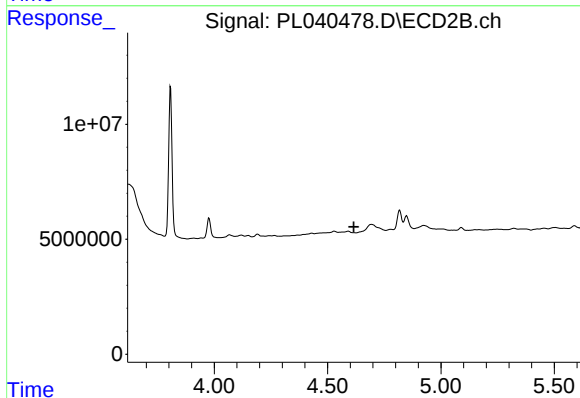


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.615 min
Response: 0
Conc: N.D.

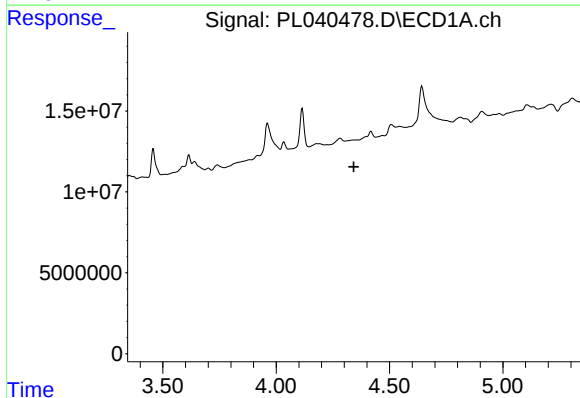


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

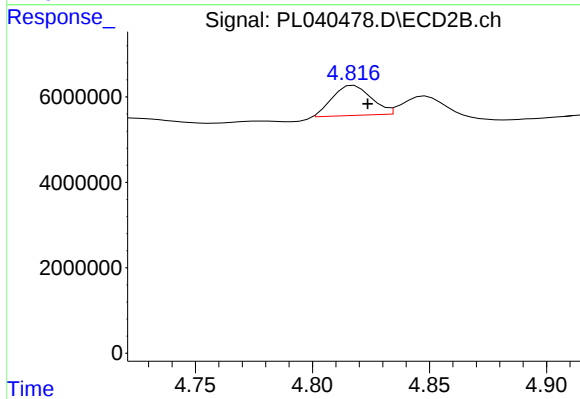

#7 delta-BHC


R.T.: 4.818 min
Delta R.T.: -0.006 min
Response: 8018892
Conc: 1.74 ng/ml

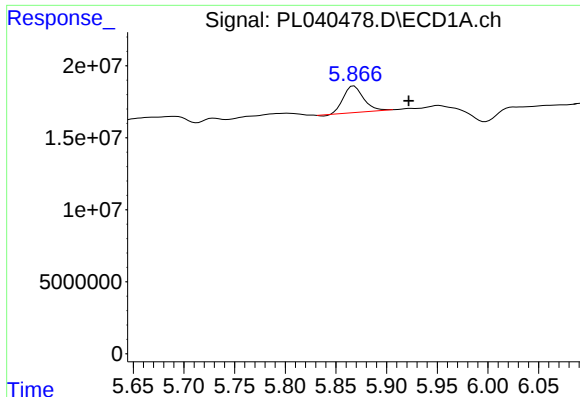

#15 Endosulfan II


R.T.: 5.868 min
Delta R.T.: -0.054 min
Response: 25254735
Conc: 2.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

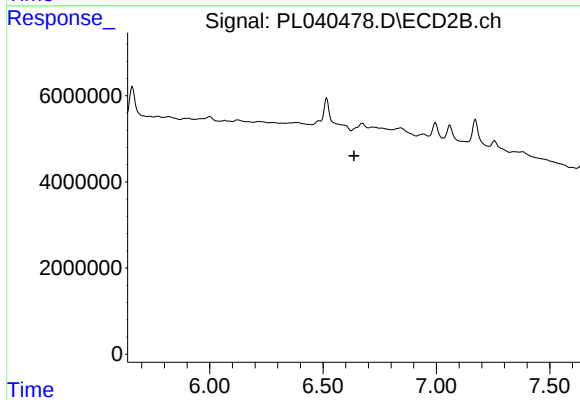


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

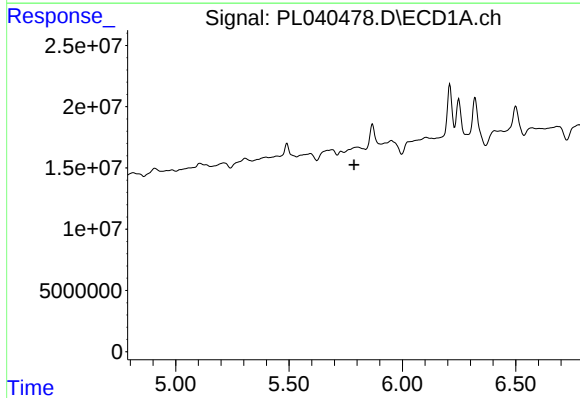


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.787 min
Response: 0
Conc: N.D.

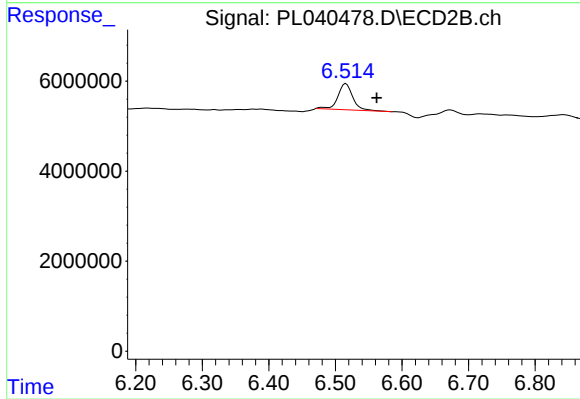

#16 4,4'-DDD


R.T.: 6.516 min
Delta R.T.: -0.046 min
Response: 9089509
Conc: 2.86 ng/ml

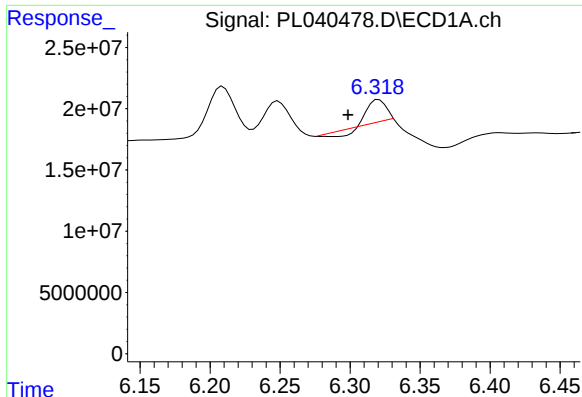

#19 Endosulfan Sulfate


R.T.: 6.321 min
Delta R.T.: 0.022 min
Response: 13317422
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

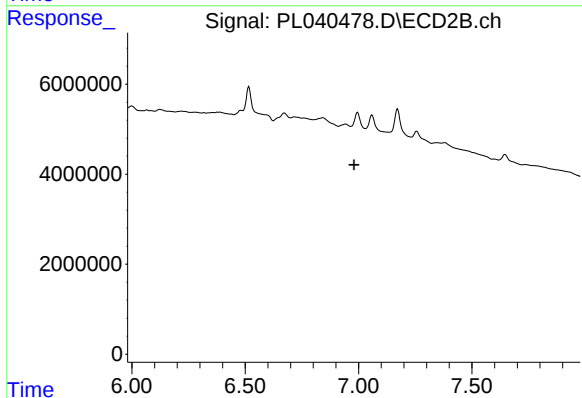


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.980 min
Response: 0
Conc: N.D.

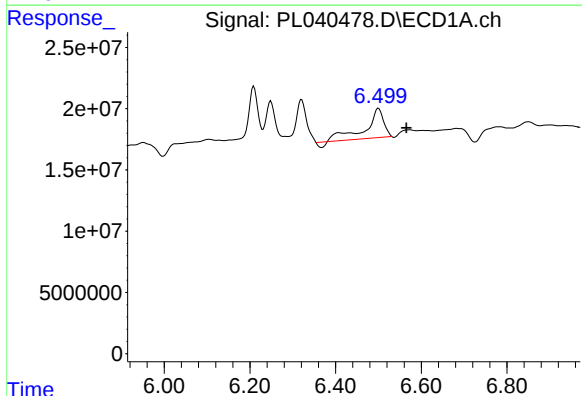


#20 Methoxychlor

R.T.: 6.500 min
Delta R.T.: -0.065 min
Response: 70216345
Conc: 14.54 ng/ml

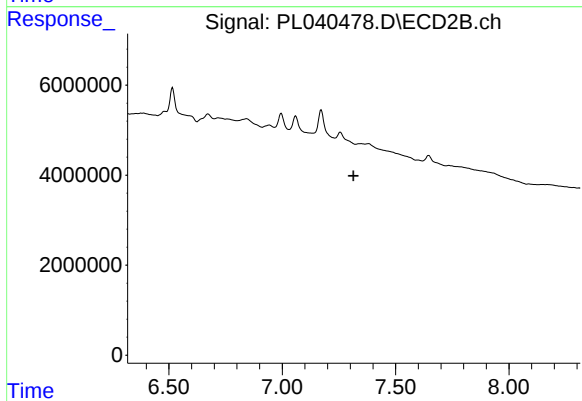

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.314 min
Response: 0
Conc: N.D.

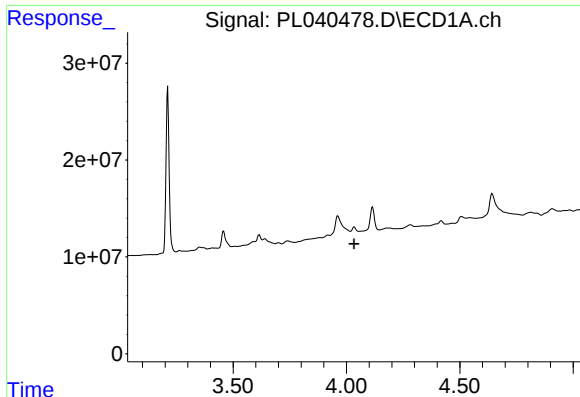

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

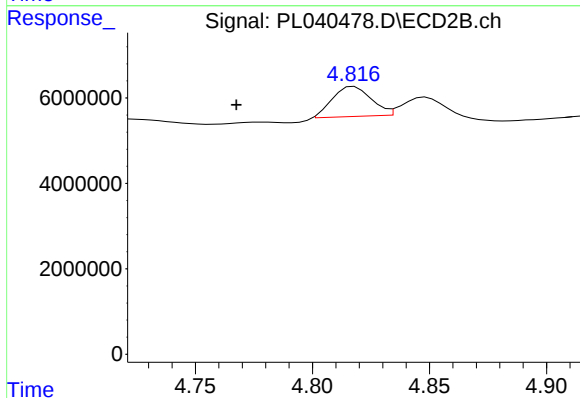


#23 Chlordane-1

R.T.: 4.818 min
Delta R.T.: 0.050 min
Response: 8018892
Conc: 51.96 ng/ml

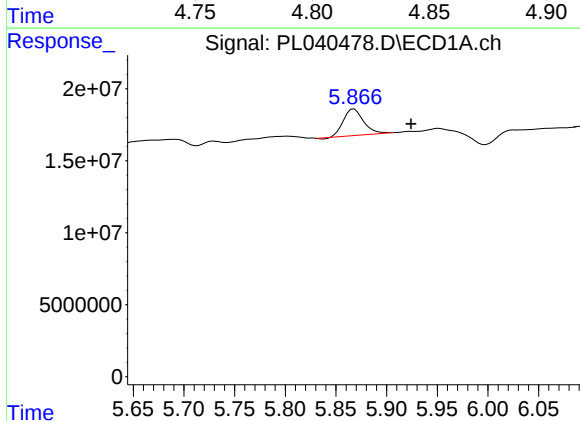


#27 Chlordane-5

R.T.: 5.868 min
Delta R.T.: -0.056 min
Response: 25254735
Conc: 62.57 ng/ml

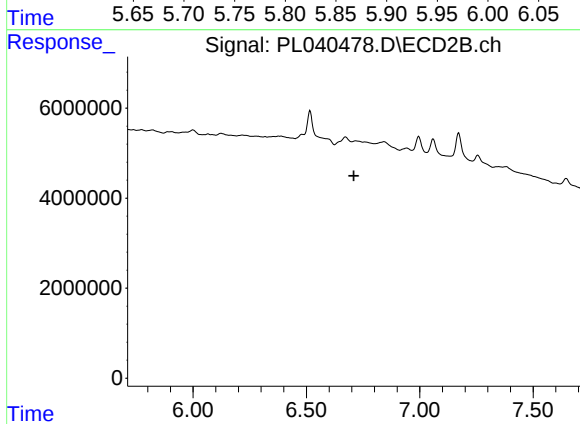

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

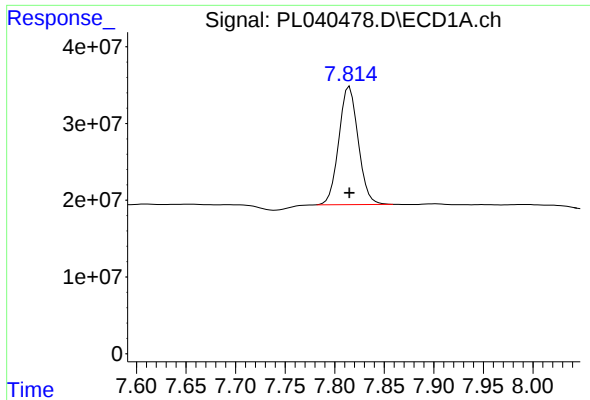

#28 Decachlorobiphenyl

R.T.: 7.815 min
Delta R.T.: 0.000 min
Response: 209121770
Conc: 22.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

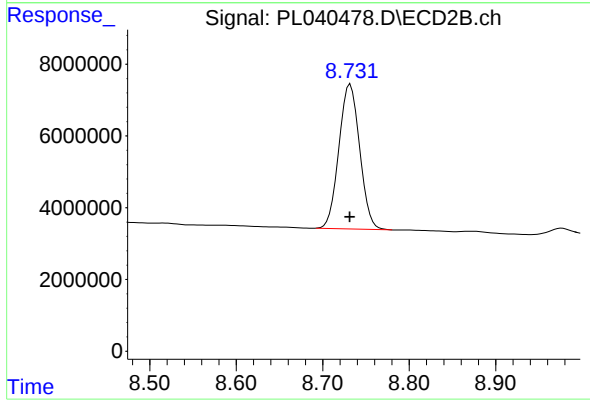

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: 0.000 min
Response: 67120464
Conc: 21.19 ng/ml