

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
 Data File : PL040479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2018 01:40
 Operator : AJ\SJ
 Sample : J5100-04
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 04:48:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.211	3.807	158.7E6	64476235	21.685	20.418
28)	SA Decachlor...	7.815	8.732	210.8E6	68260487	22.175	21.555
Target Compounds							
4)	MA Heptachlor	4.115f	0.000	1798012	0	0.153	N.D. #
6)	B beta-BHC	4.115f	0.000	1798012	0	0.426	N.D. #
7)	B delta-BHC	0.000	4.818	0	7686910	N.D.	1.665 #
15)	B Endosulfa...	5.868f	0.000	22961704	0	2.305	N.D. #
16)	A 4,4'-DDD	0.000	6.516f	0	9033194	N.D.	2.843 #
19)	B Endosulfa...	6.321	0.000	9578209	0	1.001	N.D. #
20)	A Methoxychlor	6.500f	0.000	92451321	0	19.140	N.D. #
23)	Chlordane-1	0.000	4.818	0	7686910	N.D.	49.809 #
27)	Chlordane-5	5.868	0.000	22961704	0	56.885	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
Data File : PL040479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2018 01:40
Operator : AJ\SJ
Sample : J5100-04
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 04:48:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

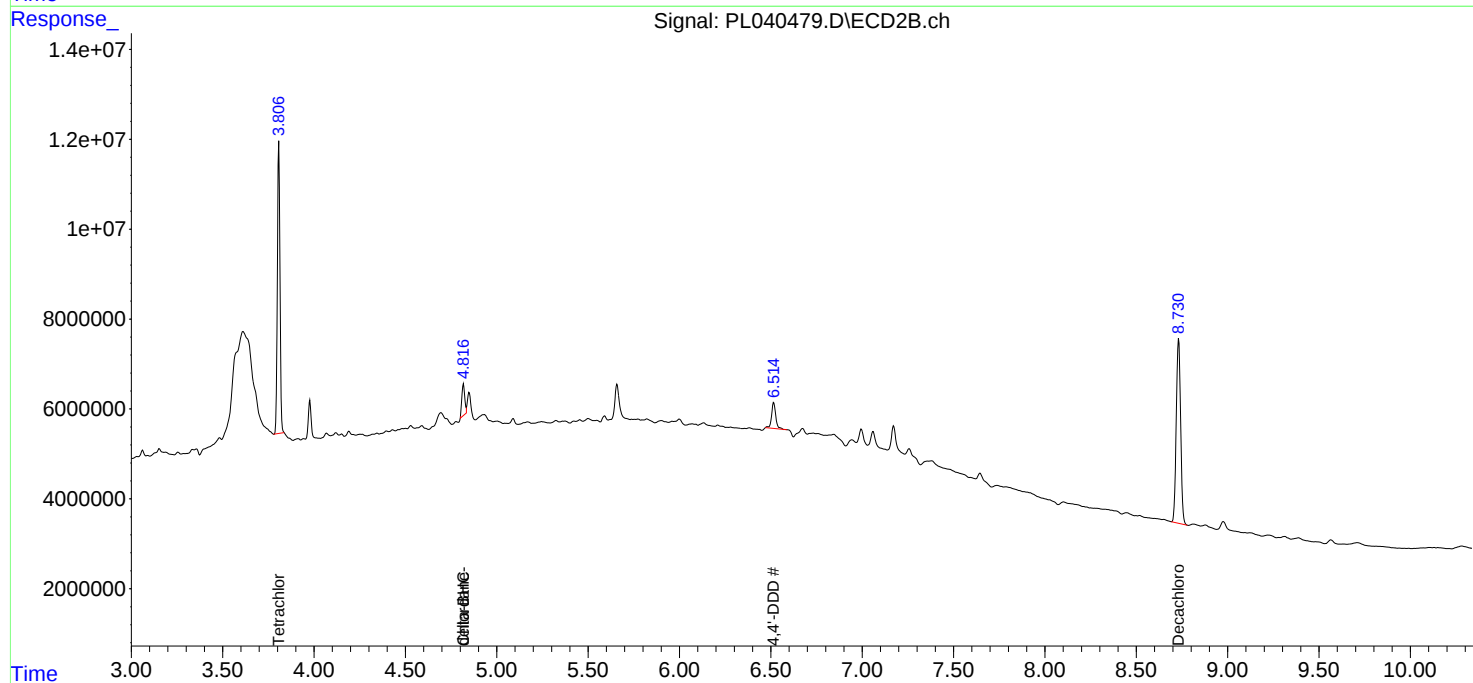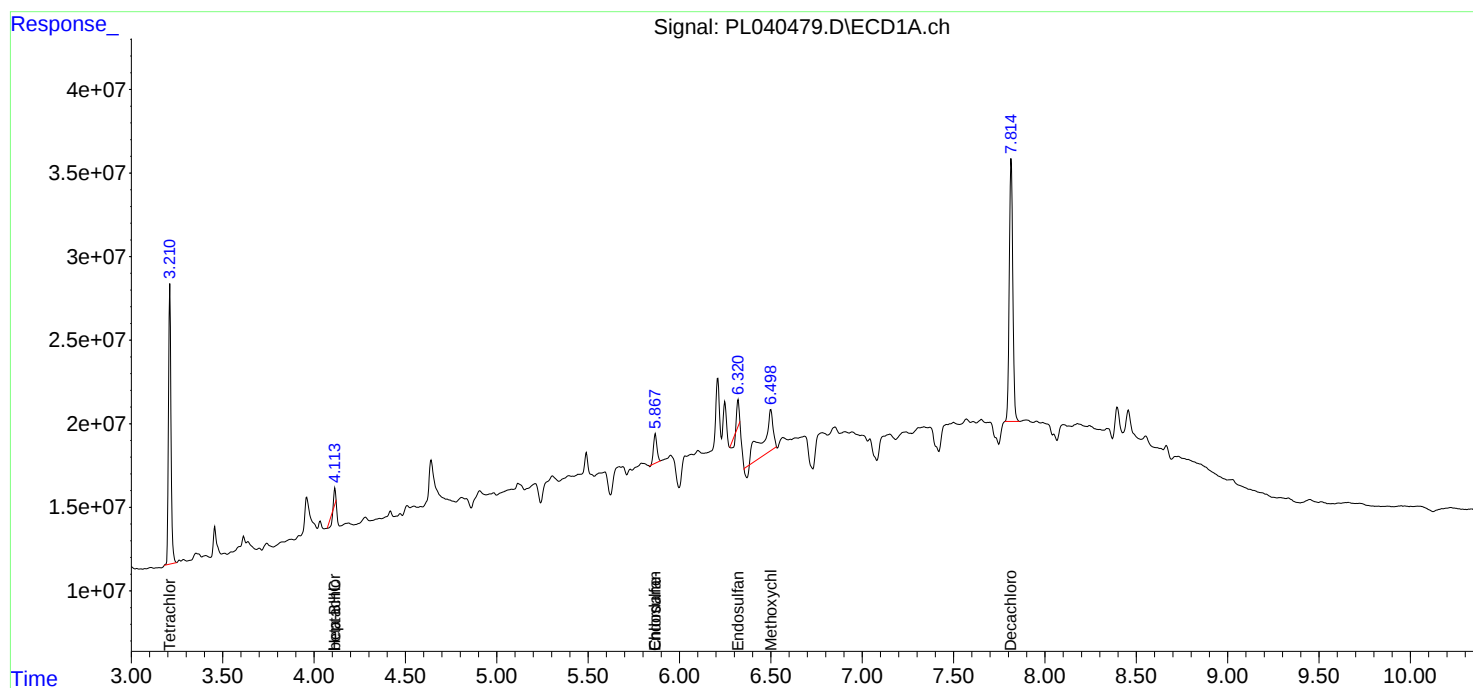


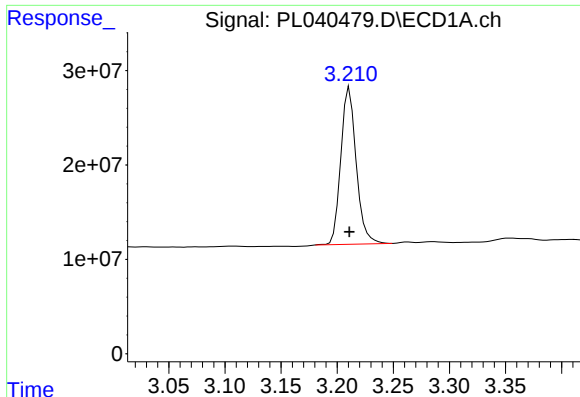

#1 Tetrachloro-m-xylene


R.T.: 3.211 min
Delta R.T.: 0.000 min
Response: 158732972
Conc: 21.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

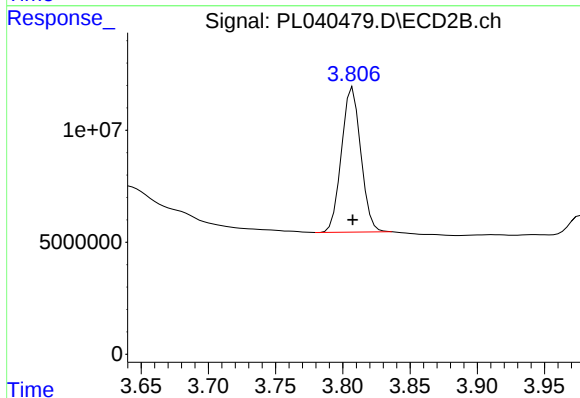


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 64476235
Conc: 20.42 ng/ml

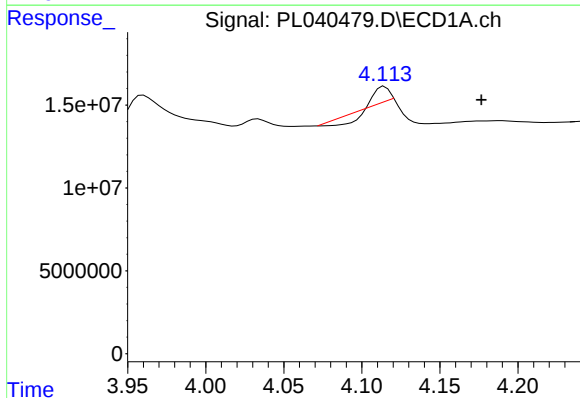


#4 Heptachlor

R.T.: 4.115 min
Delta R.T.: -0.062 min
Response: 1798012
Conc: 0.15 ng/ml

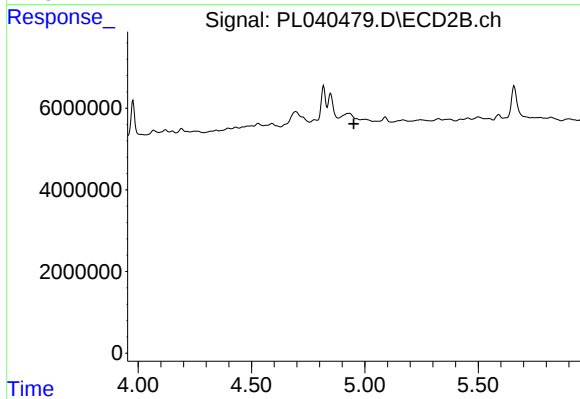

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.951 min
Response: 0
Conc: N.D.

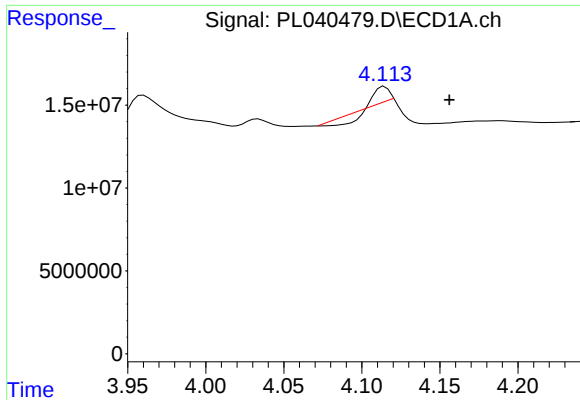

#6 beta-BHC


R.T.: 4.115 min
Delta R.T.: -0.042 min
Response: 1798012
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

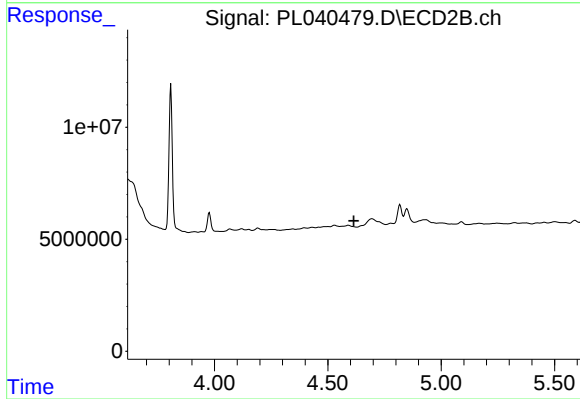


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.615 min
Response: 0
Conc: N.D.

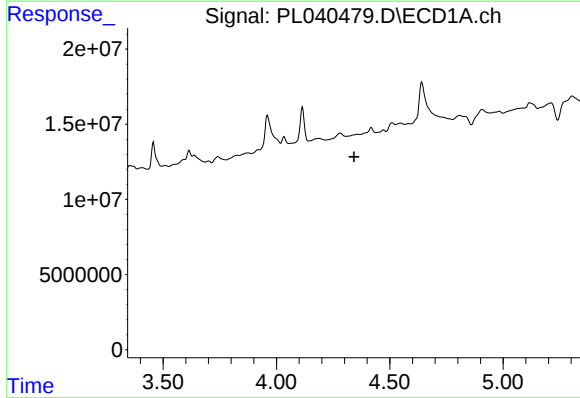


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

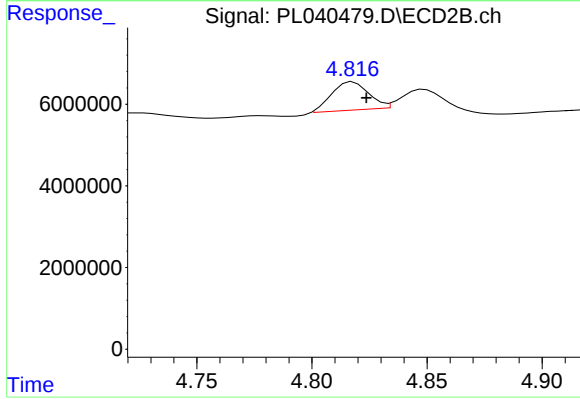

#7 delta-BHC


R.T.: 4.818 min
Delta R.T.: -0.006 min
Response: 7686910
Conc: 1.67 ng/ml

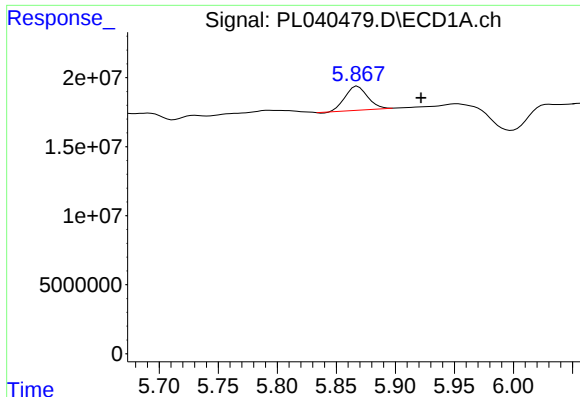

#15 Endosulfan II


R.T.: 5.868 min
Delta R.T.: -0.054 min
Response: 22961704
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

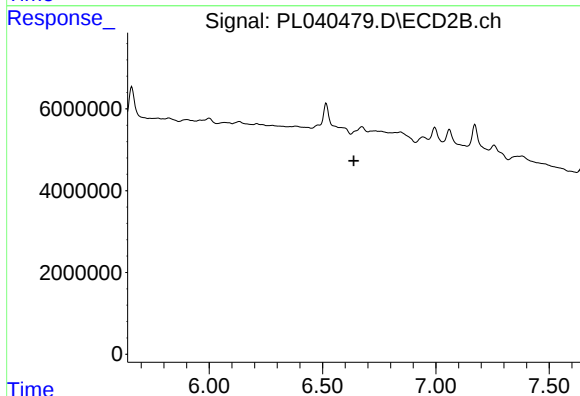


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

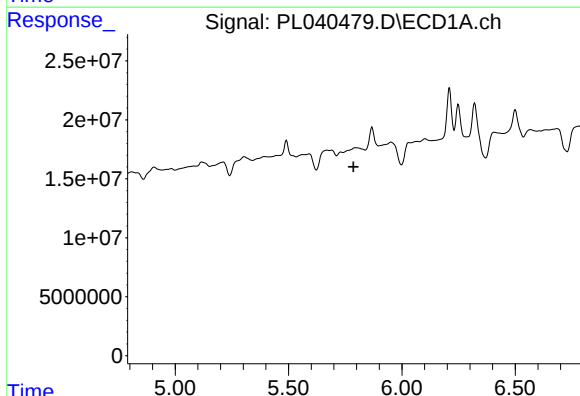


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.787 min
Response: 0
Conc: N.D.

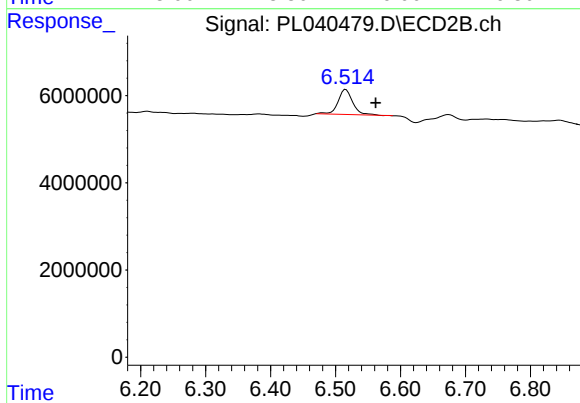

#16 4,4'-DDD


R.T.: 6.516 min
Delta R.T.: -0.046 min
Response: 9033194
Conc: 2.84 ng/ml

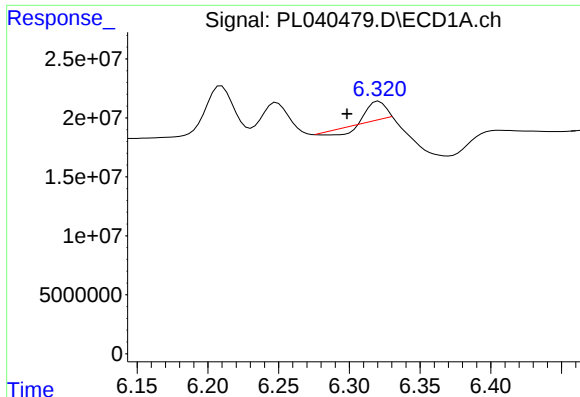

#19 Endosulfan Sulfate


R.T.: 6.321 min
Delta R.T.: 0.022 min
Response: 9578209
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

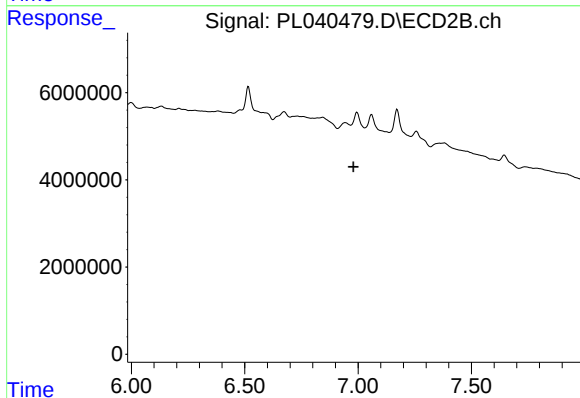


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.980 min
Response: 0
Conc: N.D.

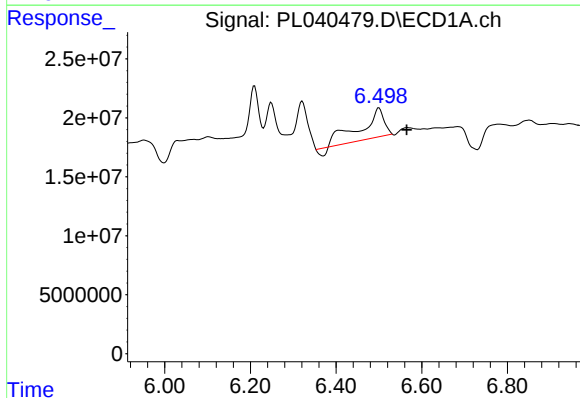


#20 Methoxychlor

R.T.: 6.500 min
Delta R.T.: -0.065 min
Response: 92451321
Conc: 19.14 ng/ml

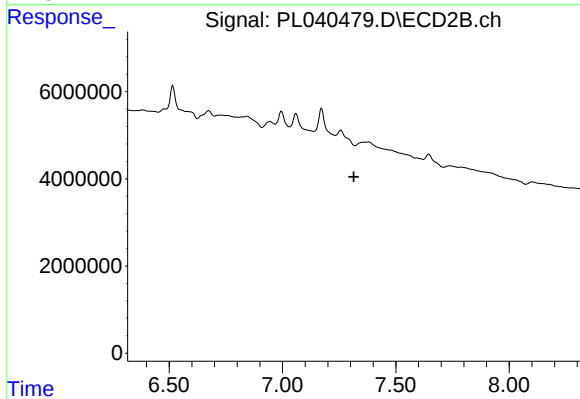

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.314 min
Response: 0
Conc: N.D.

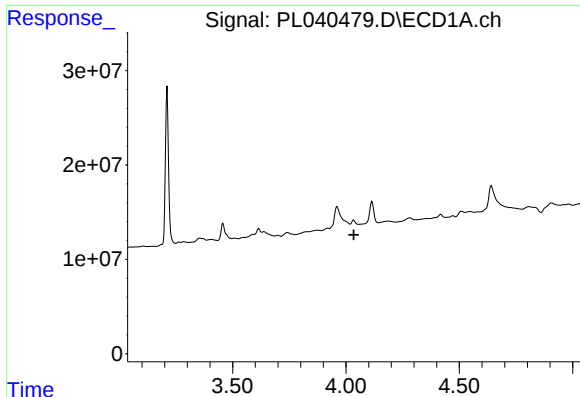

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

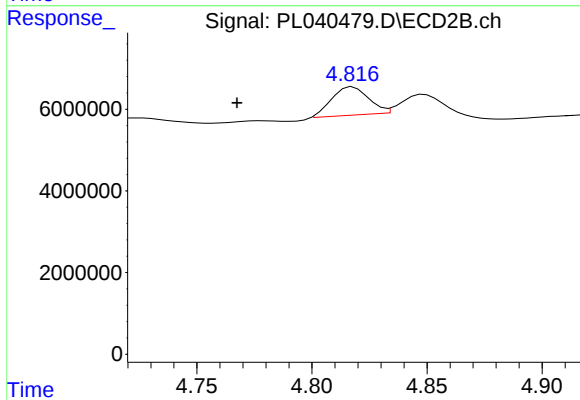


#23 Chlordane-1

R.T.: 4.818 min
Delta R.T.: 0.050 min
Response: 7686910
Conc: 49.81 ng/ml

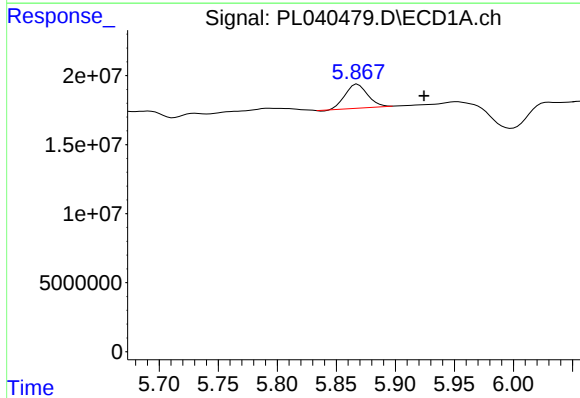


#27 Chlordane-5

R.T.: 5.868 min
Delta R.T.: -0.056 min
Response: 22961704
Conc: 56.88 ng/ml

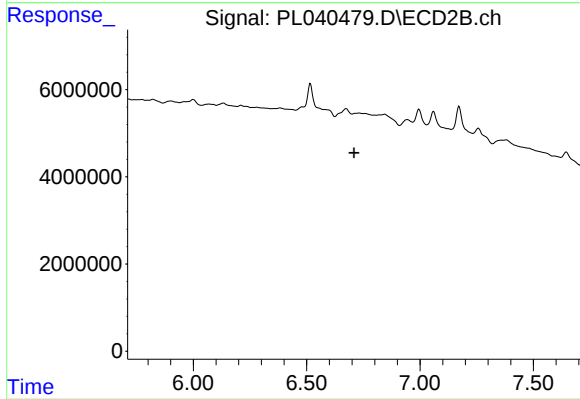

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

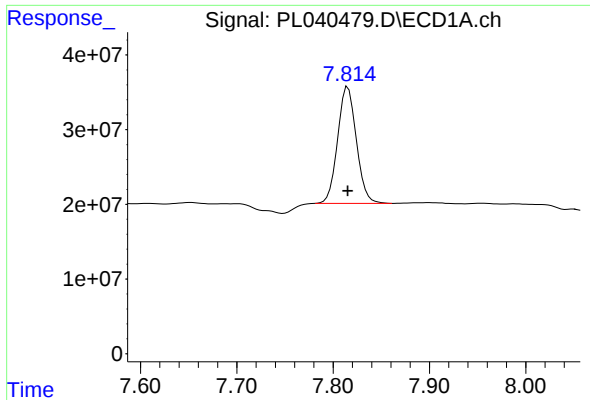

#28 Decachlorobiphenyl


R.T.: 7.815 min

Delta R.T.: 0.000 min

Response: 210787165

Conc: 22.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

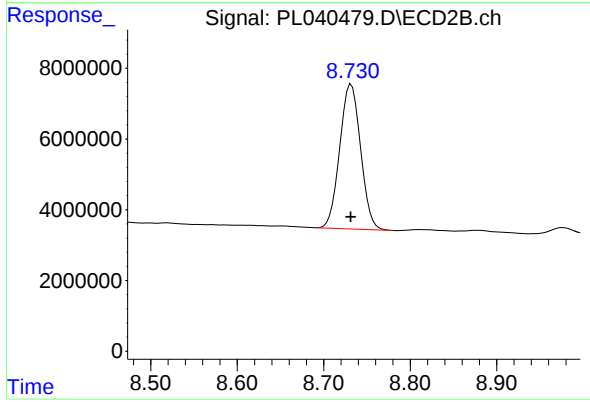

#28 Decachlorobiphenyl

R.T.: 8.732 min

Delta R.T.: 0.000 min

Response: 68260487

Conc: 21.55 ng/ml