

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
 Data File : PL040480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2018 01:54
 Operator : AJ\SJ
 Sample : PB113285BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 04:48:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.212	3.807	145.7E6	59708436	19.907	18.908
28)	SA Decachlor...	7.815	8.731	185.4E6	59323817	19.504	18.733
Target Compounds							
15)	B Endosulfa...	5.868f	0.000	24706680	0	2.480	N.D. #
16)	A 4,4'-DDD	0.000	6.516f	0	9513244	N.D.	2.994 #
19)	B Endosulfa...	6.321	0.000	13575301	0	1.418	N.D. #
20)	A Methoxychlor	6.500f	0.000	85840135	0	17.771	N.D. #
27)	Chlordane-5	5.868	0.000	24706680	0	61.208	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092718\
Data File : PL040480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2018 01:54
Operator : AJ\SJ
Sample : PB113285BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 04:48:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

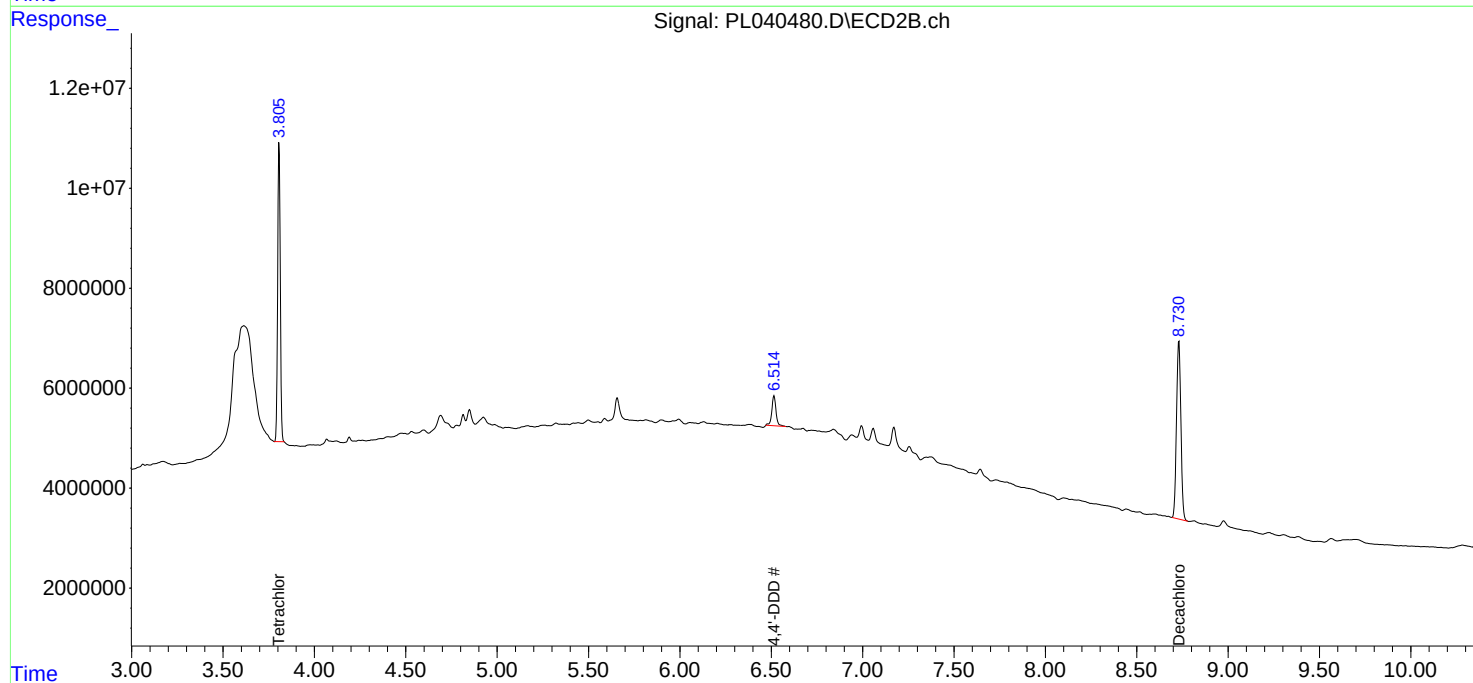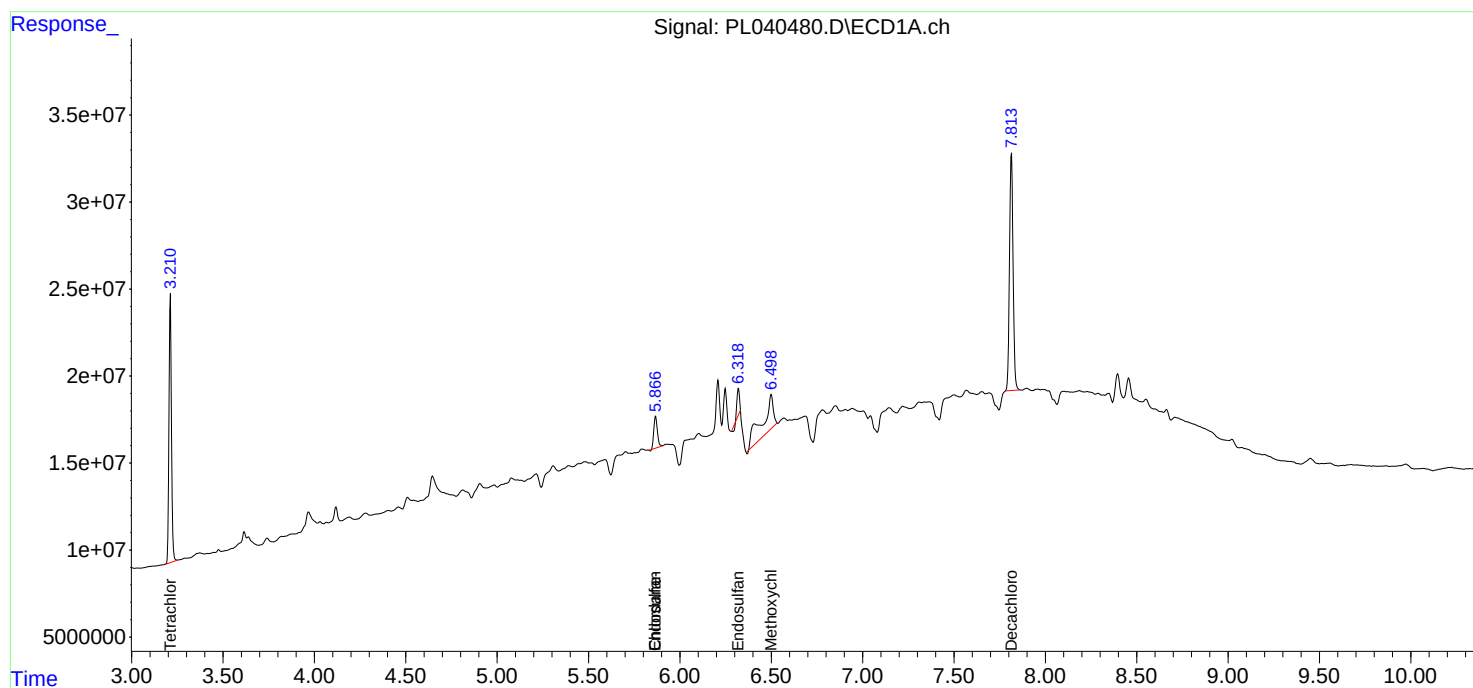


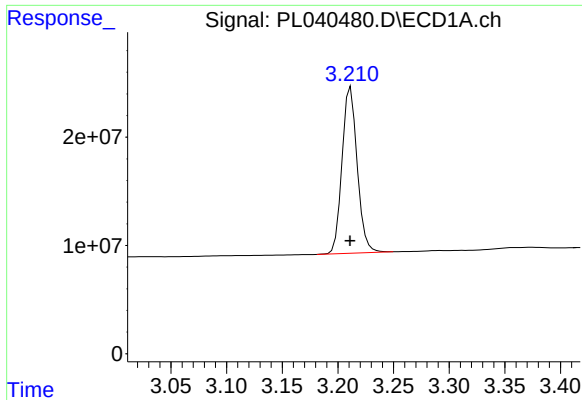

#1 Tetrachloro-m-xylene


R.T.: 3.212 min
Delta R.T.: 0.000 min
Response: 145716852
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

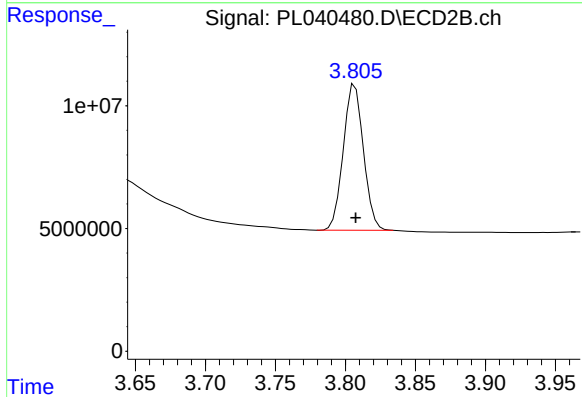


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 59708436
Conc: 18.91 ng/ml

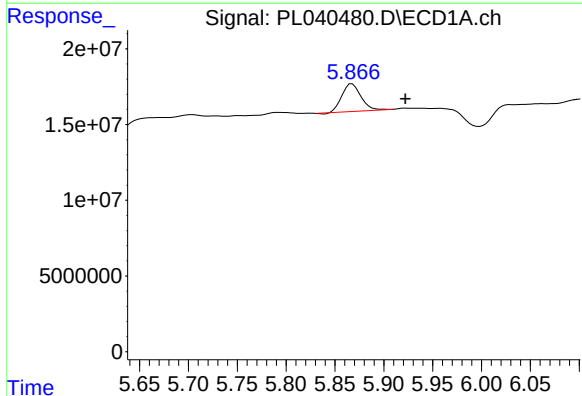


#15 Endosulfan II

R.T.: 5.868 min
Delta R.T.: -0.054 min
Response: 24706680
Conc: 2.48 ng/ml

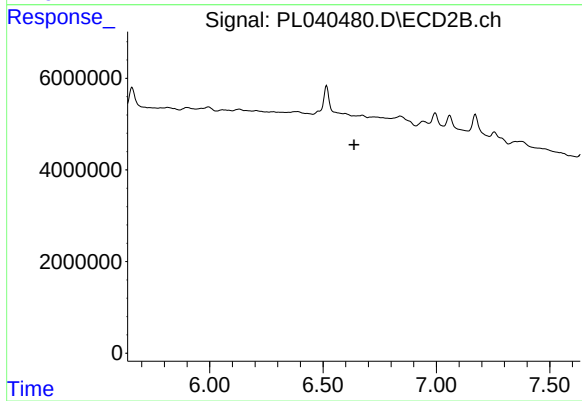

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.637 min
Response: 0
Conc: N.D.

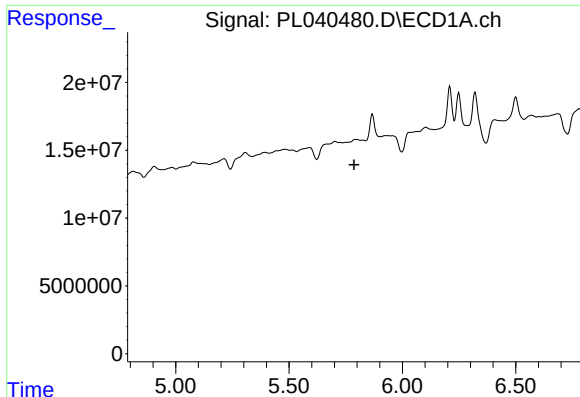

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.787 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

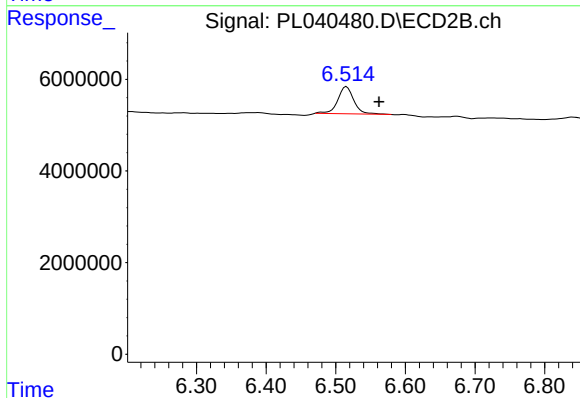


#16 4,4'-DDD

R.T.: 6.516 min
Delta R.T.: -0.047 min
Response: 9513244
Conc: 2.99 ng/ml

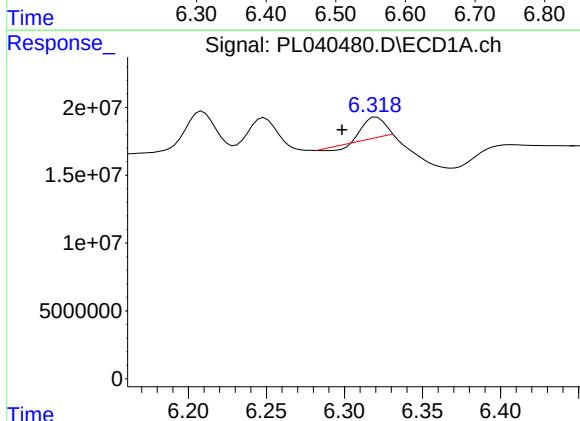


#19 Endosulfan Sulfate

R.T.: 6.321 min
Delta R.T.: 0.022 min
Response: 13575301
Conc: 1.42 ng/ml

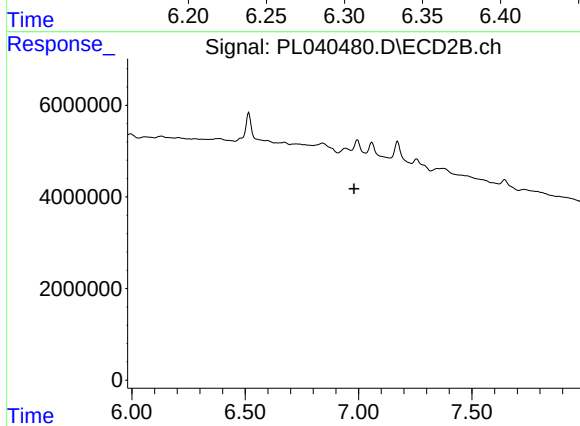

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.980 min
Response: 0
Conc: N.D.

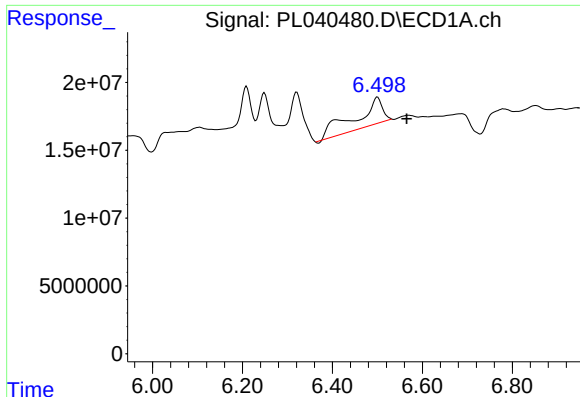

#20 Methoxychlor


R.T.: 6.500 min
Delta R.T.: -0.065 min
Response: 85840135
Conc: 17.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

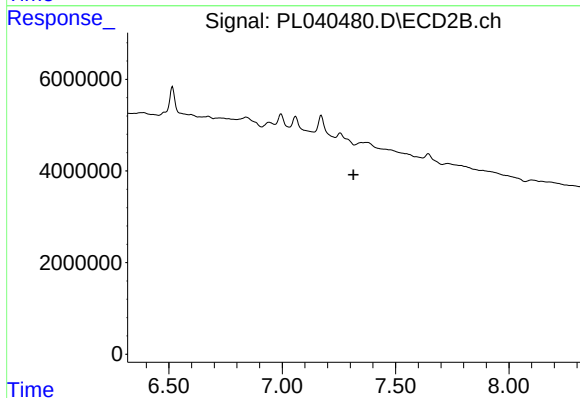


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.314 min
Response: 0
Conc: N.D.

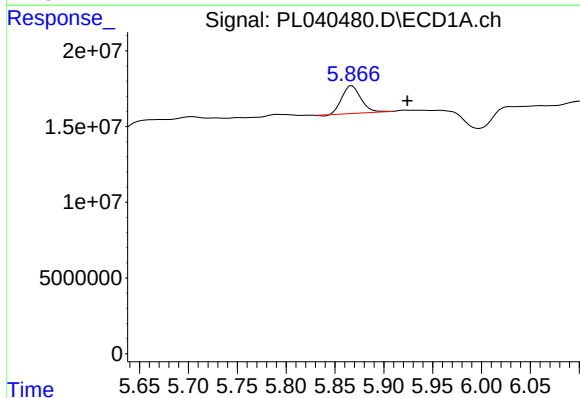


#27 Chlordane-5

R.T.: 5.868 min
Delta R.T.: -0.057 min
Response: 24706680
Conc: 61.21 ng/ml

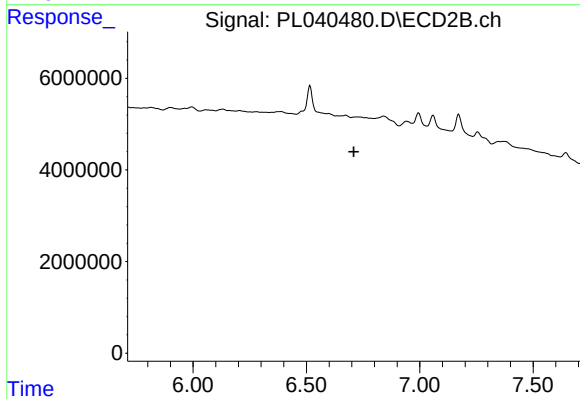

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

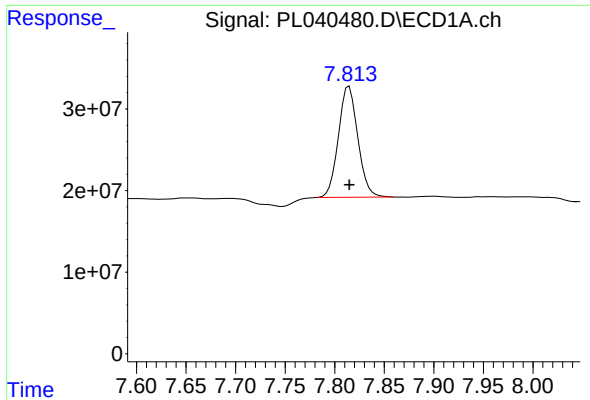

#28 Decachlorobiphenyl

R.T.: 7.815 min
Delta R.T.: 0.000 min
Response: 185401394
Conc: 19.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

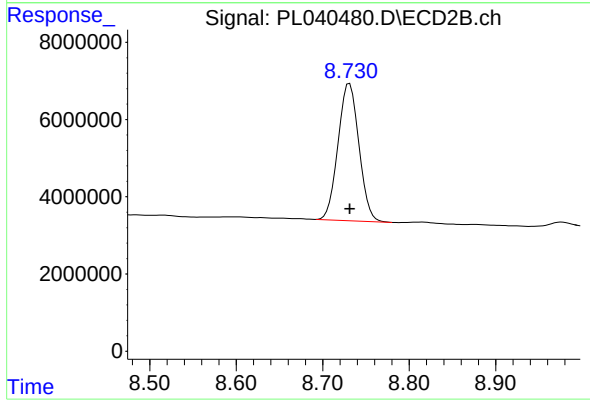

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 59323817
Conc: 18.73 ng/ml