

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092719\
 Data File : PL052784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 12:10
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 14:03:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	4.047	236.3E6	62484500	30.298	28.677
28)	SA Decachlor...	8.346	9.124	208.6E6	66031479	23.854	27.575
Target Compounds							
2)	A alpha-BHC	3.985	0.000	66122774	0	5.500	N.D. #
23)	Chlordane-1	0.000	5.026f	0	412797	N.D.	5.316 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092719\
Data File : PL052784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 12:10
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 14:03:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

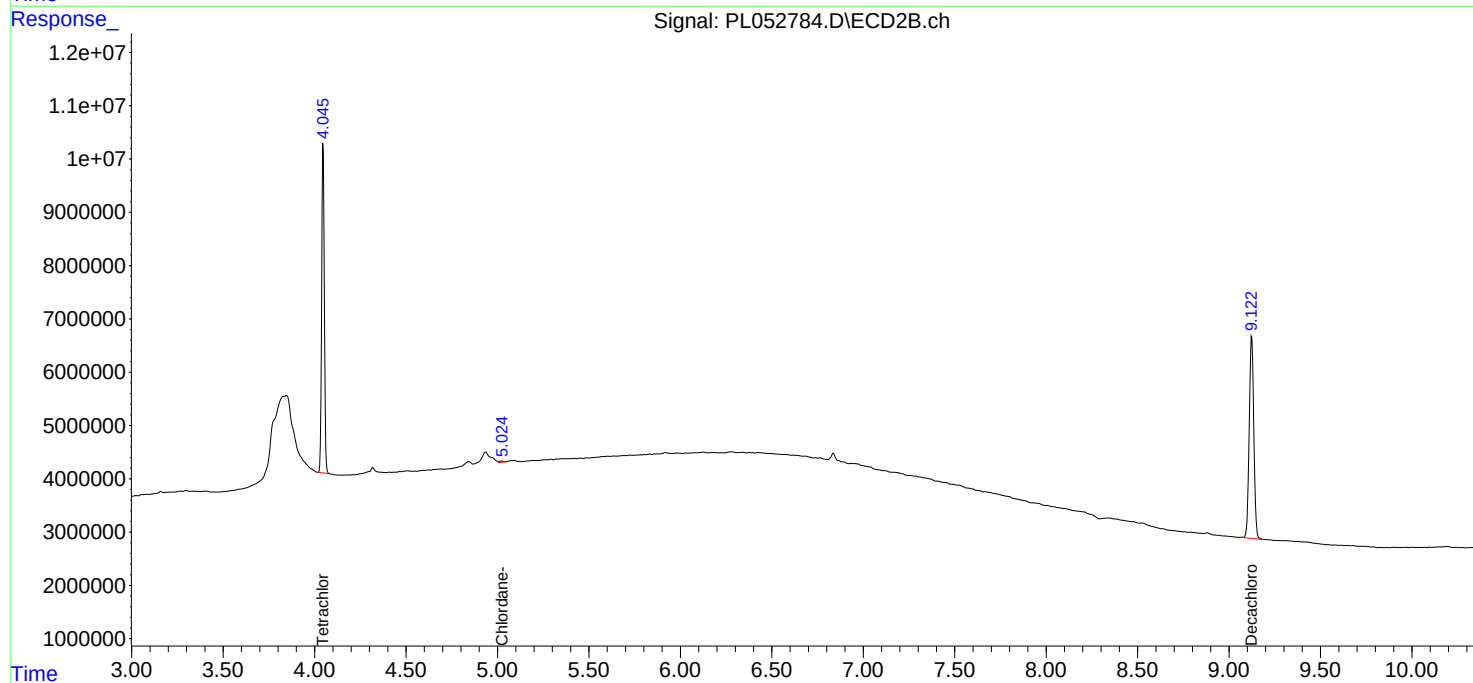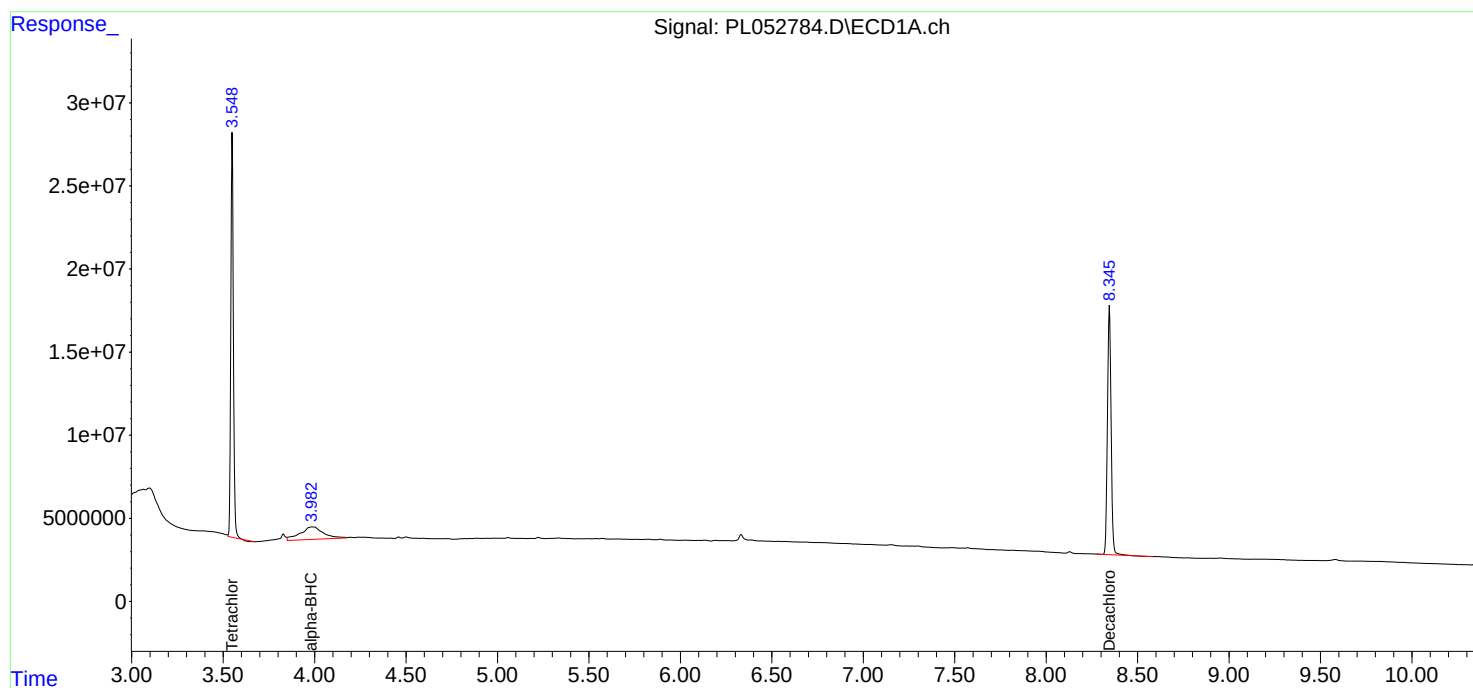


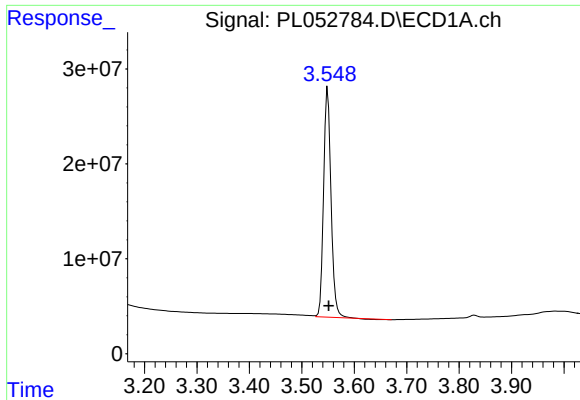

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: -0.001 min
Response: 236257994
Conc: 30.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

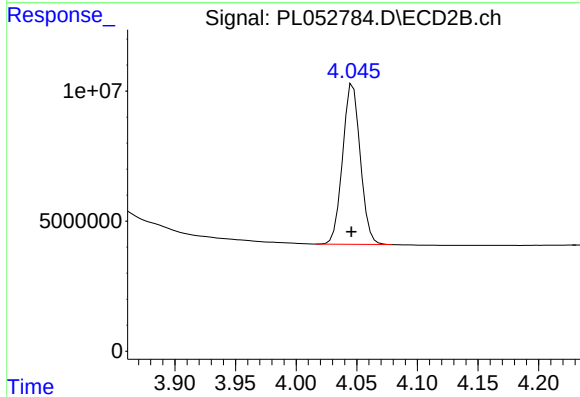


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.001 min
Response: 62484500
Conc: 28.68 ng/ml

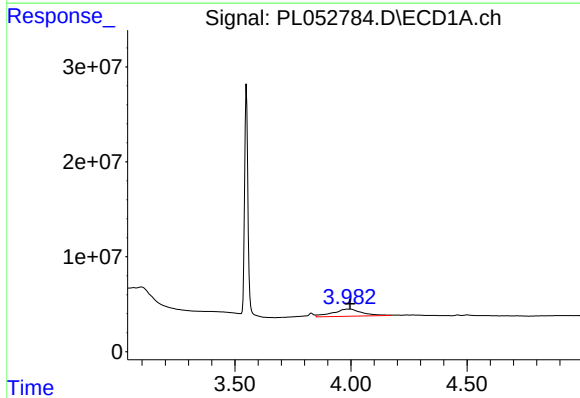


#2 alpha-BHC

R.T.: 3.985 min
Delta R.T.: -0.012 min
Response: 66122774
Conc: 5.50 ng/ml

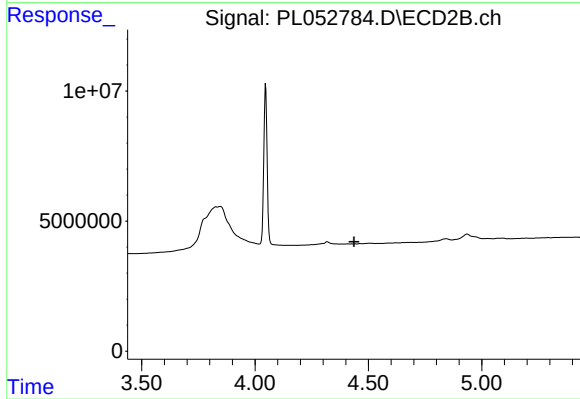

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.437 min
Response: 0
Conc: N.D.

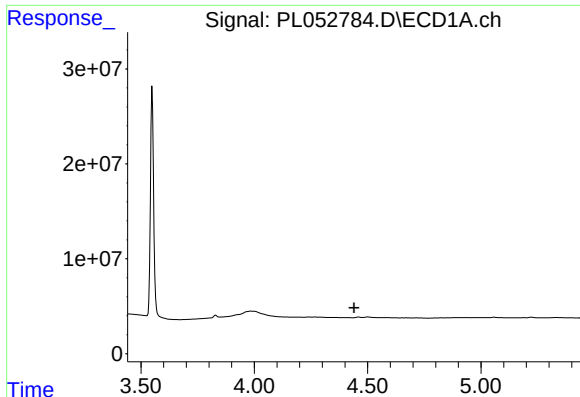

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

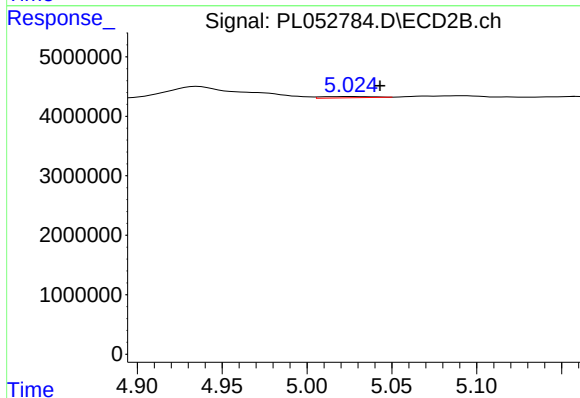


#23 Chlordane-1

R.T.: 5.026 min
Delta R.T.: -0.017 min
Response: 412797
Conc: 5.32 ng/ml

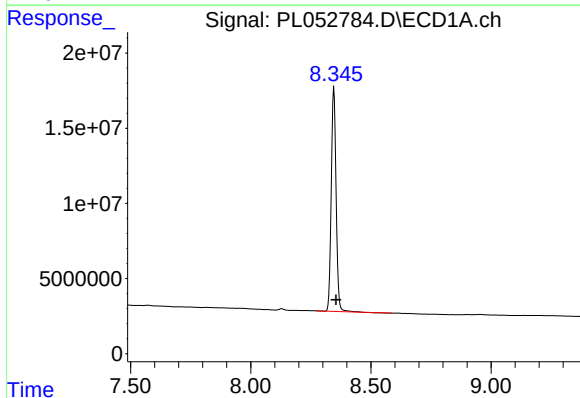

#28 Decachlorobiphenyl

R.T.: 8.346 min
Delta R.T.: -0.008 min
Response: 208589540
Conc: 23.85 ng/ml

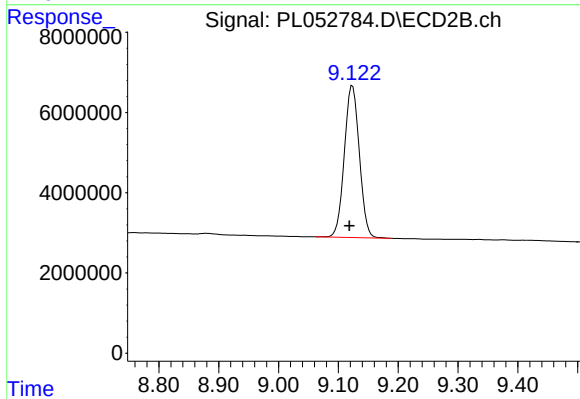

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: 0.005 min
Response: 66031479
Conc: 27.57 ng/ml