

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092722\
 Data File : PL077939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2022 15:05
 Operator : AR\AJ
 Sample : N4844-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-04-092622

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/28/2022
 Supervised By : Ankita Jodhani 09/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 23:48:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.414	2.623	16436862	34705007	10.254m	11.690m
2) SA Decachlor...	8.906	7.722	18403547	30469975	14.240	12.138

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092722\
Data File : PL077939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2022 15:05
Operator : AR\AJ
Sample : N4844-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SU-04-092622


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/28/2022
Supervised By : Ankita Jodhani 09/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 23:48:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

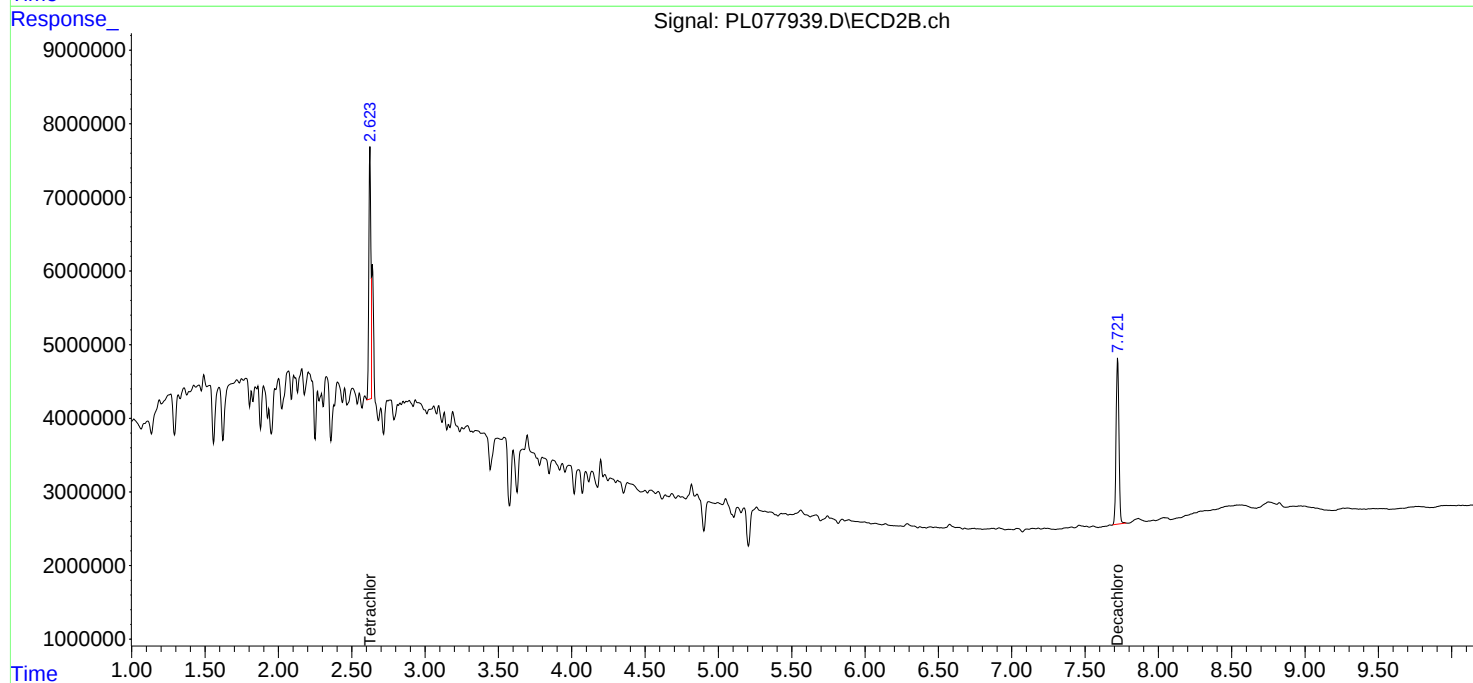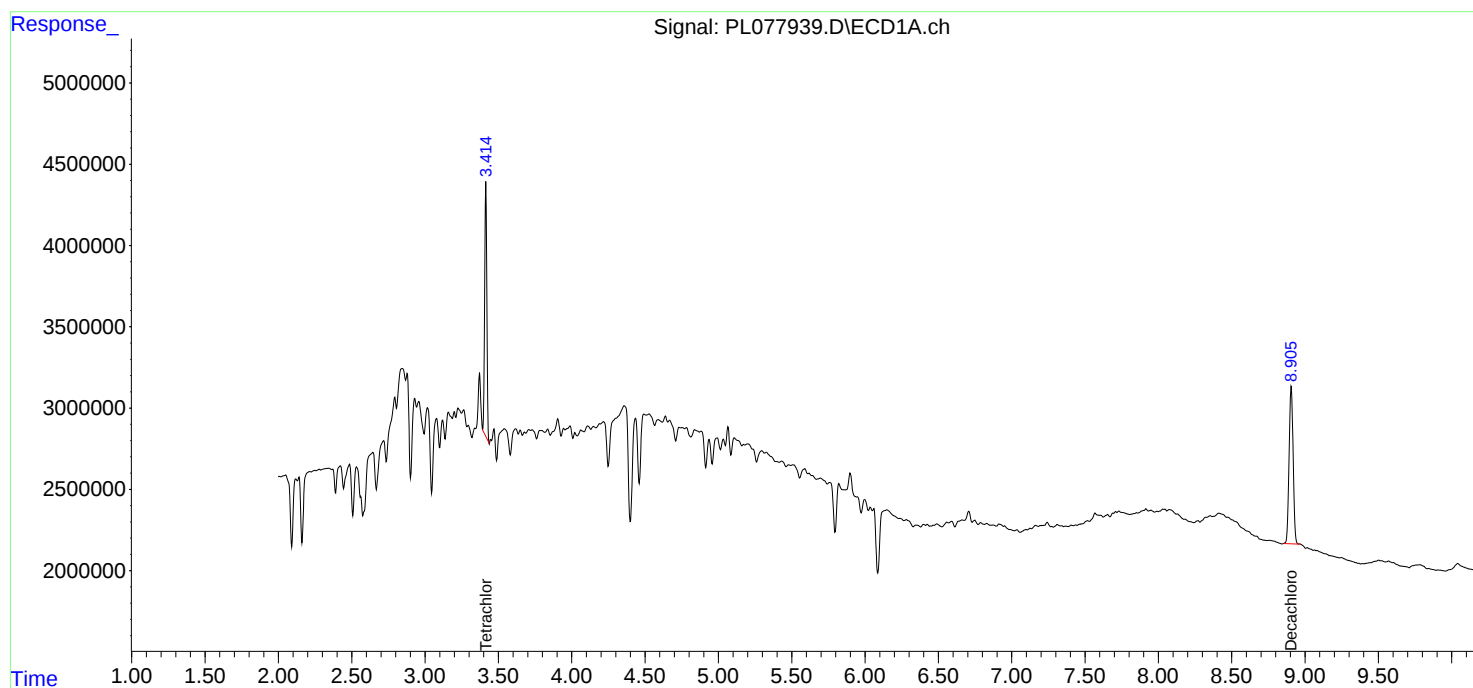

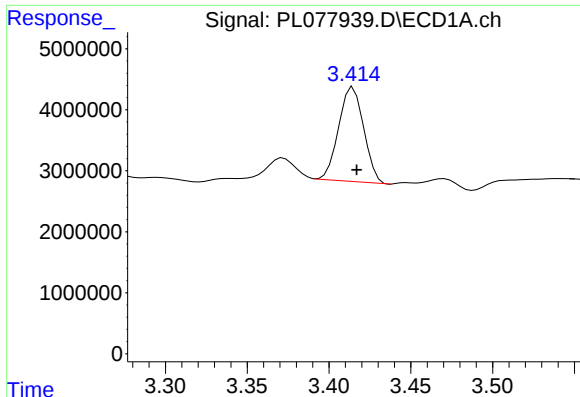


#1 Tetrachloro-m-xylene

R.T.: 3.414 min
Delta R.T.: -0.003 min
Response: 16436862
Conc: 10.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-092622


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/28/2022
Supervised By :Ankita Jodhani 09/28/2022

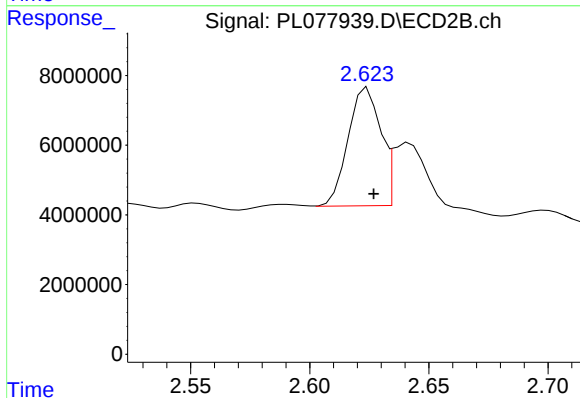


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: -0.004 min
Response: 34705007
Conc: 11.69 ng/ml m

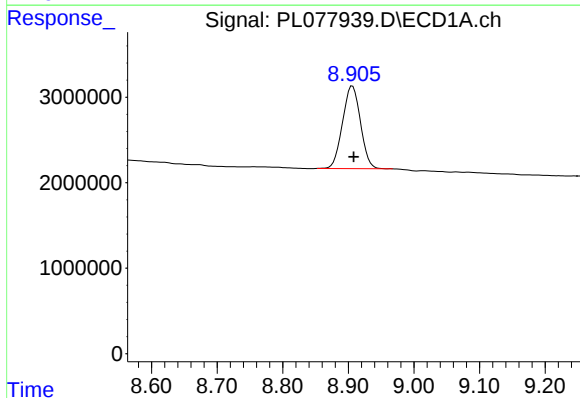

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: -0.002 min
Response: 18403547
Conc: 14.24 ng/ml

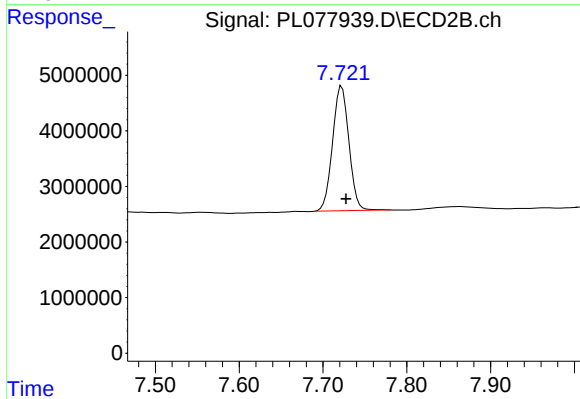

#28 Decachlorobiphenyl

R.T.: 7.722 min
Delta R.T.: -0.005 min
Response: 30469975
Conc: 12.14 ng/ml