

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092724\
 Data File : PL092119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2024 16:31
 Operator : AR\AJ
 Sample : P4194-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MANHOLE-119-KEARNY

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 00:11:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.780	38919800	45239932	17.495	18.038
28)	SA Decachlor...	9.060	7.922	18454599	29258409	11.265	11.694

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092724\
Data File : PL092119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2024 16:31
Operator : AR\AJ
Sample : P4194-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MANHOLE-119-KEARNY

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 00:11:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

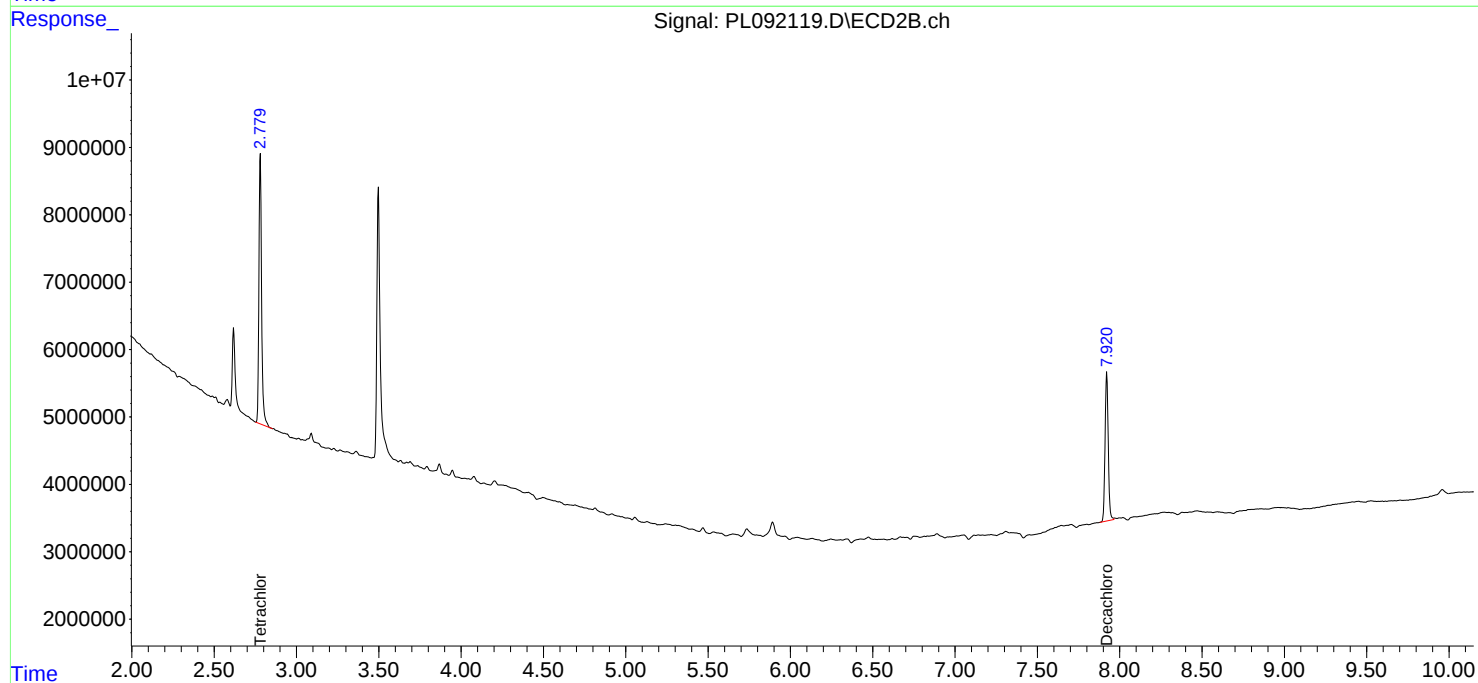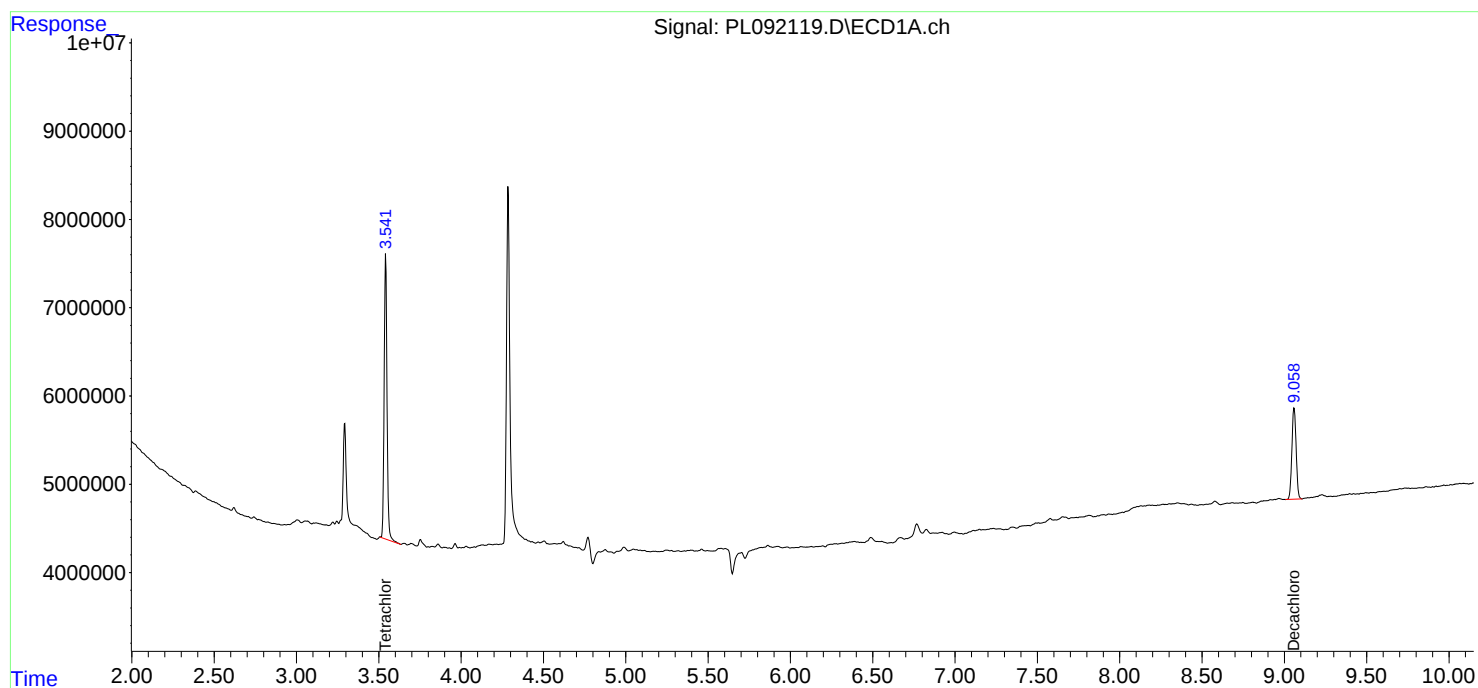


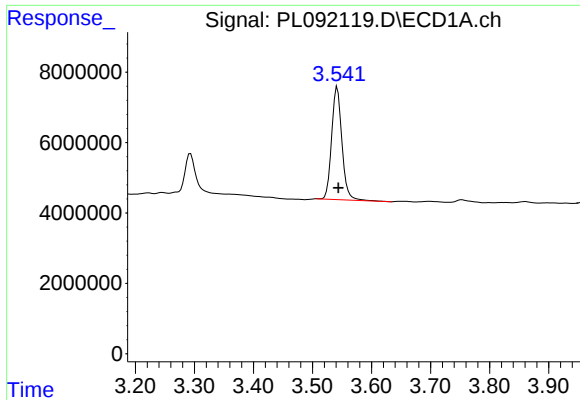

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 38919800
Conc: 17.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
MANHOLE-119-KEARNY

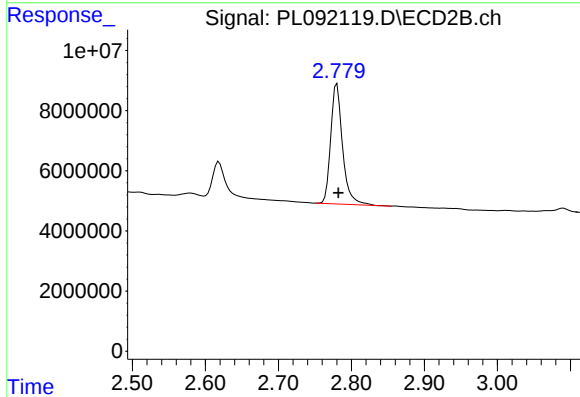


#1 Tetrachloro-m-xylene

R.T.: 2.780 min
Delta R.T.: -0.002 min
Response: 45239932
Conc: 18.04 ng/ml

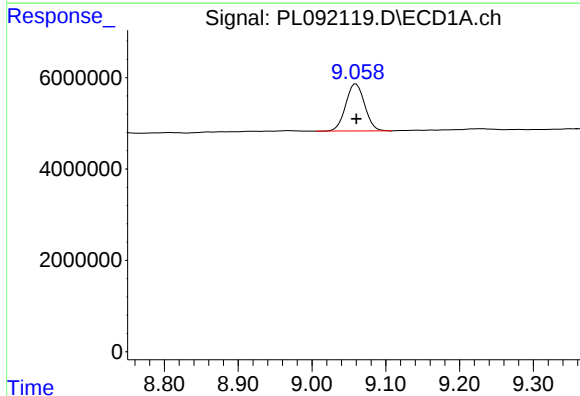

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 18454599
Conc: 11.26 ng/ml

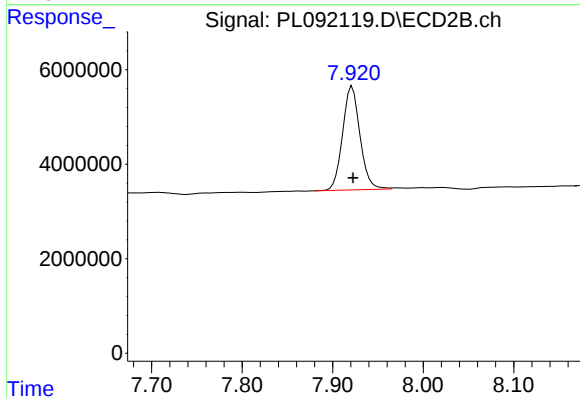

#28 Decachlorobiphenyl

R.T.: 7.922 min
Delta R.T.: 0.000 min
Response: 29258409
Conc: 11.69 ng/ml