

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092818\
 Data File : PL040506.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2018 16:04
 Operator : AJ\SJ
 Sample : PB113334BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 22:46:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.217	3.804	174.4E6	64713355	23.825	20.493
28)	SA Decachlor...	7.821	8.733	248.4E6	71364566	26.128	22.535
Target Compounds							
7)	B delta-BHC	0.000	4.784f	0	5419304	N.D.	1.174 #
8)	B Heptachlo...	0.000	5.642	0	11881051	N.D.	3.095 #
14)	MA Endrin	0.000	6.500f	0	45673805	N.D.	13.981 #
15)	B Endosulfa...	5.862f	0.000	139.5E6	0	14.005	N.D. #
16)	A 4,4'-DDD	0.000	6.500f	0	45673805	N.D.	14.376 #
20)	A Methoxychlor	6.508f	0.000	39415800	0	8.160	N.D. #
23)	Chlordane-1	0.000	4.784	0	5419304	N.D.	35.116 #
27)	Chlordane-5	5.862	0.000	139.5E6	0	345.660	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092818\
Data File : PL040506.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2018 16:04
Operator : AJ\SJ
Sample : PB113334BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 22:46:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

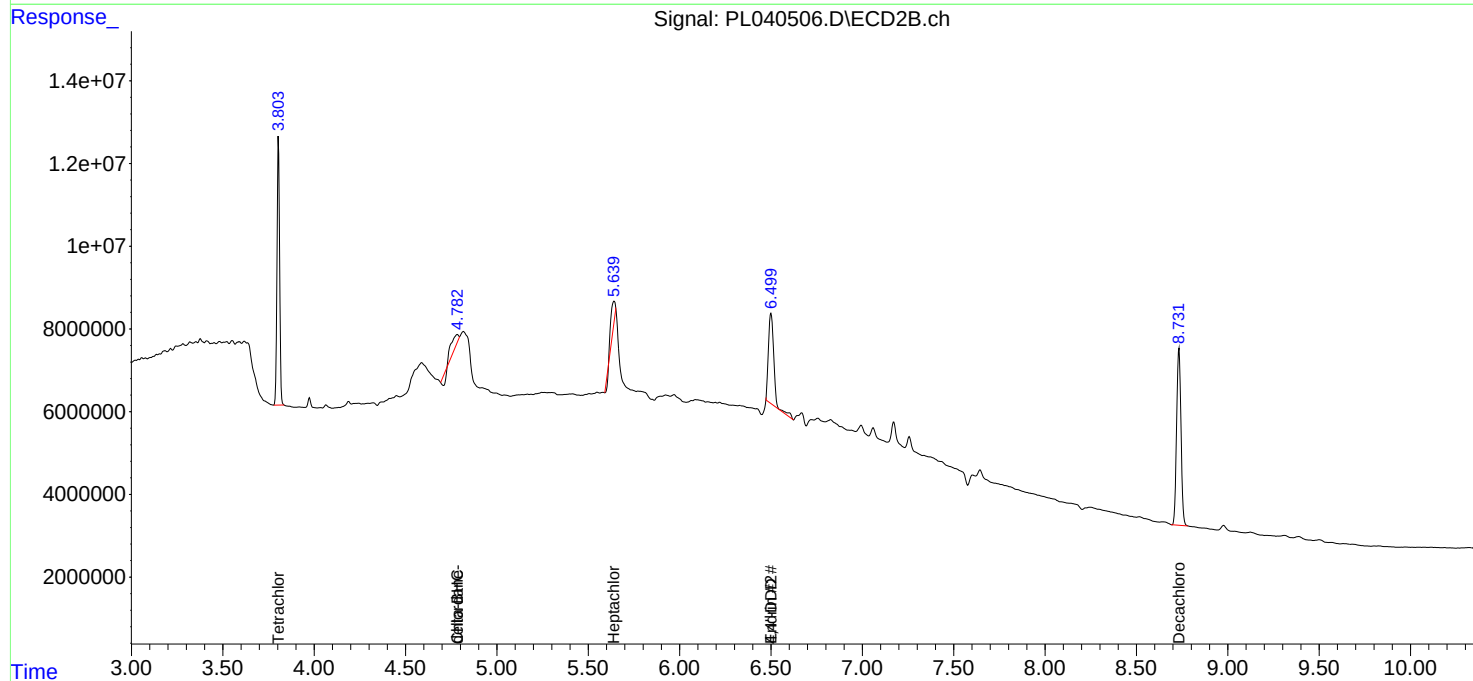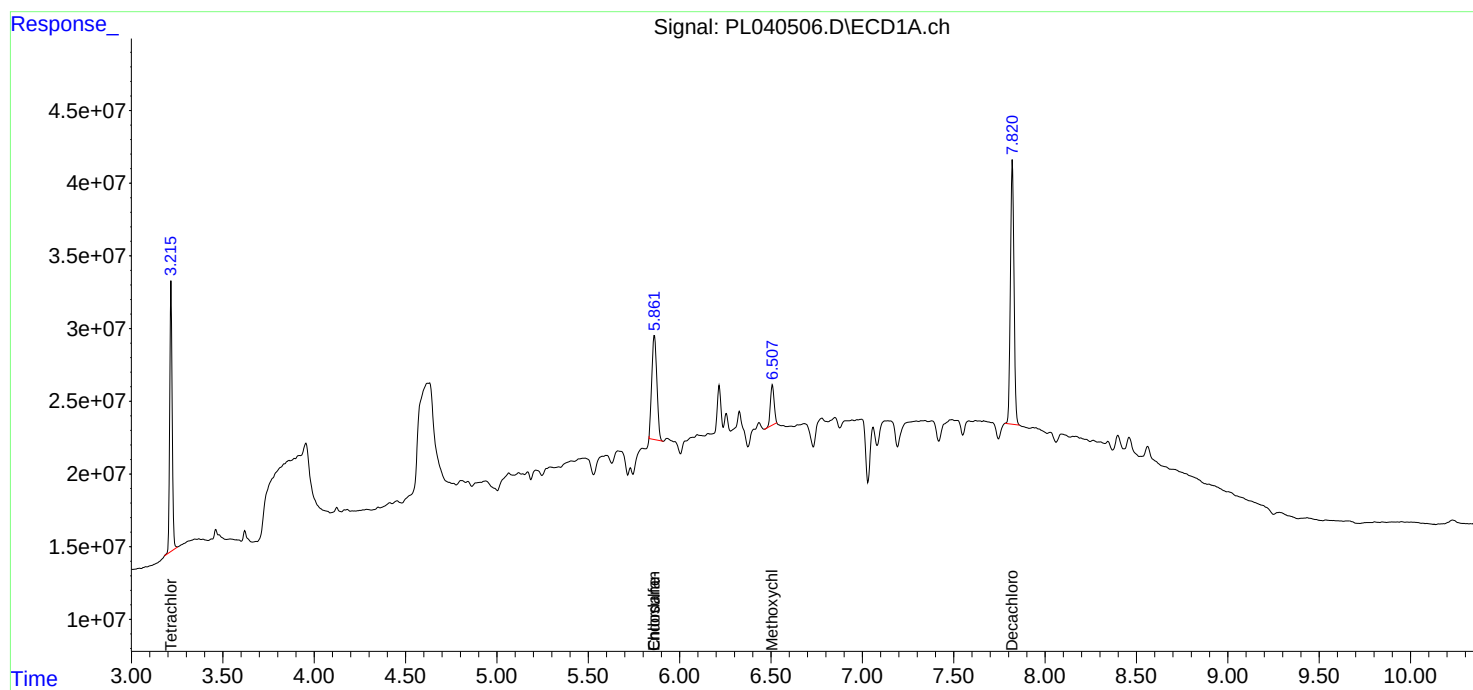


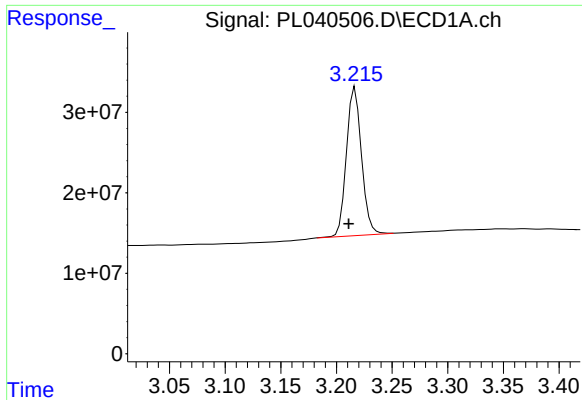

#1 Tetrachloro-m-xylene


R.T.: 3.217 min
Delta R.T.: 0.006 min
Response: 174398441
Conc: 23.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

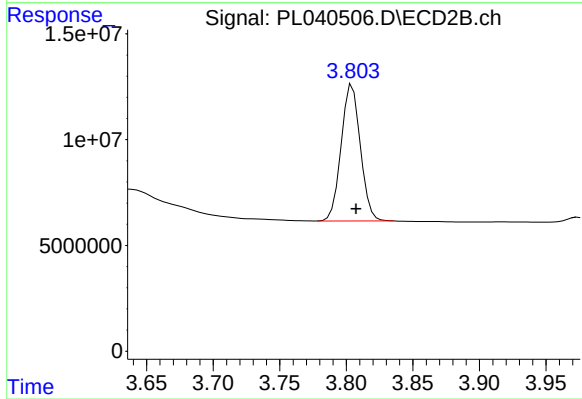


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: -0.003 min
Response: 64713355
Conc: 20.49 ng/ml

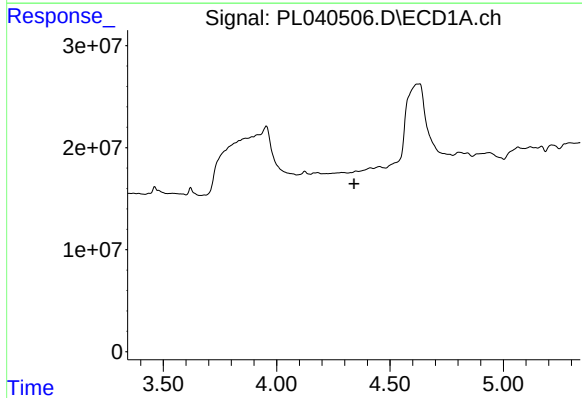


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

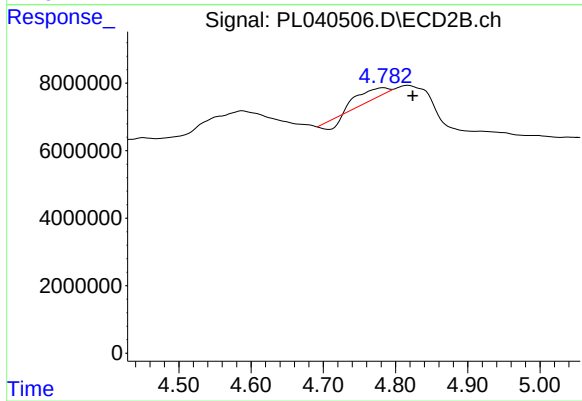

#7 delta-BHC


R.T.: 4.784 min
Delta R.T.: -0.040 min
Response: 5419304
Conc: 1.17 ng/ml

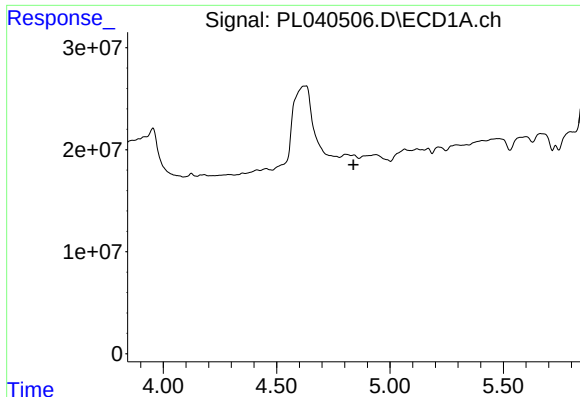

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.839 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

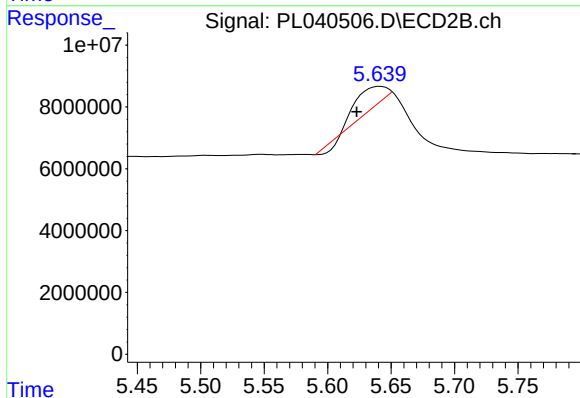


#8 Heptachlor epoxide

R.T.: 5.642 min
Delta R.T.: 0.019 min
Response: 11881051
Conc: 3.10 ng/ml

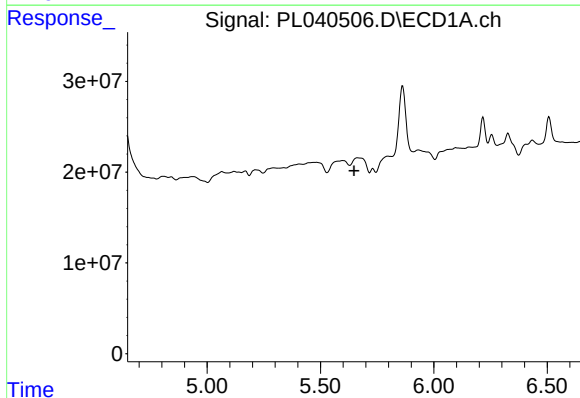


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.648 min
Response: 0
Conc: N.D.

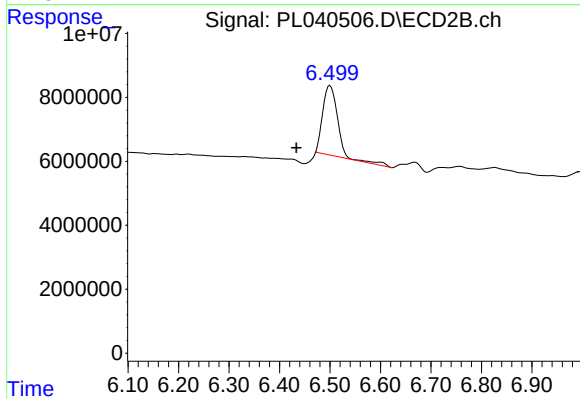

#14 Endrin


R.T.: 6.500 min
Delta R.T.: 0.066 min
Response: 45673805
Conc: 13.98 ng/ml

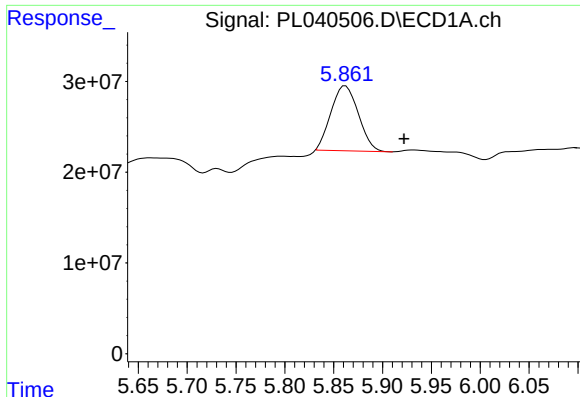

#15 Endosulfan II


R.T.: 5.862 min
Delta R.T.: -0.060 min
Response: 139527329
Conc: 14.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

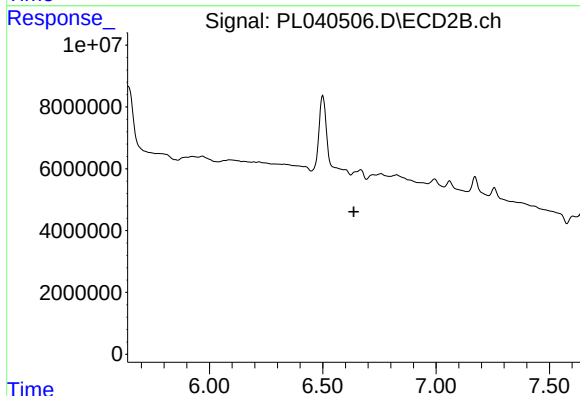


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

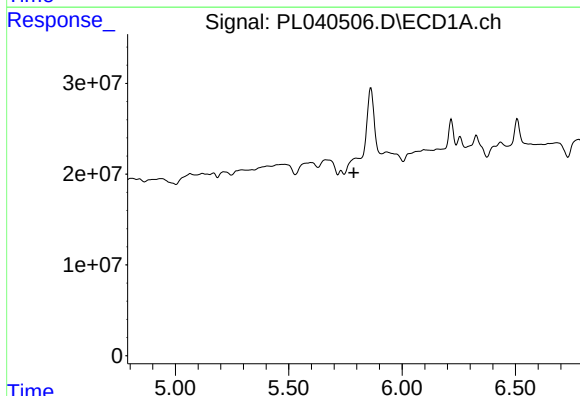


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.787 min
Response: 0
Conc: N.D.

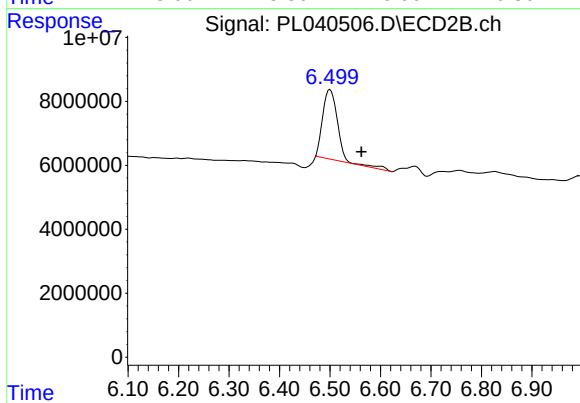

#16 4,4'-DDD


R.T.: 6.500 min
Delta R.T.: -0.062 min
Response: 45673805
Conc: 14.38 ng/ml

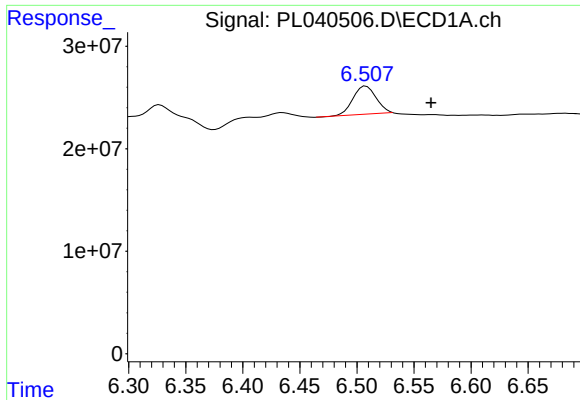

#20 Methoxychlor


R.T.: 6.508 min
Delta R.T.: -0.057 min
Response: 39415800
Conc: 8.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

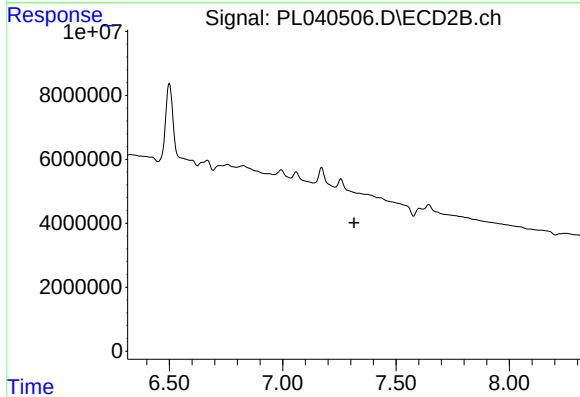


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.314 min
Response: 0
Conc: N.D.

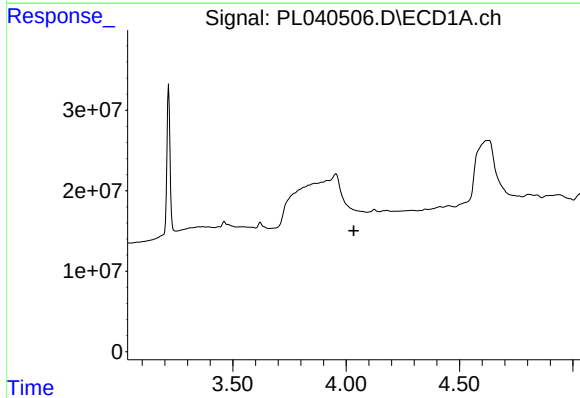


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.034 min
Response: 0
Conc: N.D.

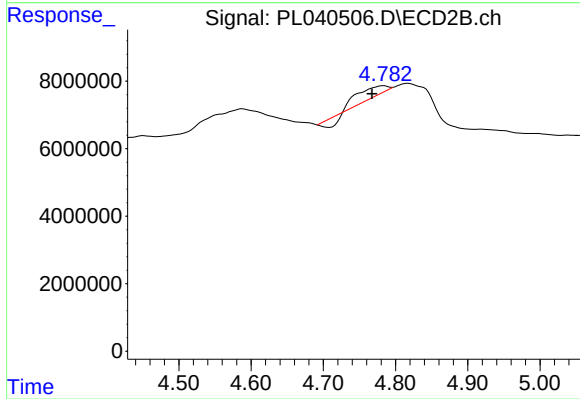

#23 Chlordane-1


R.T.: 4.784 min
Delta R.T.: 0.016 min
Response: 5419304
Conc: 35.12 ng/ml

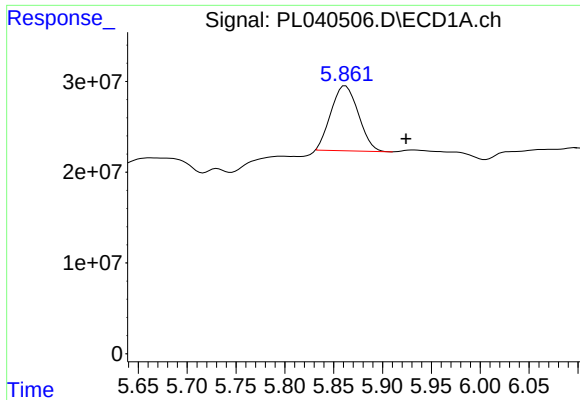

#27 Chlordane-5


R.T.: 5.862 min
Delta R.T.: -0.062 min
Response: 139527329
Conc: 345.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

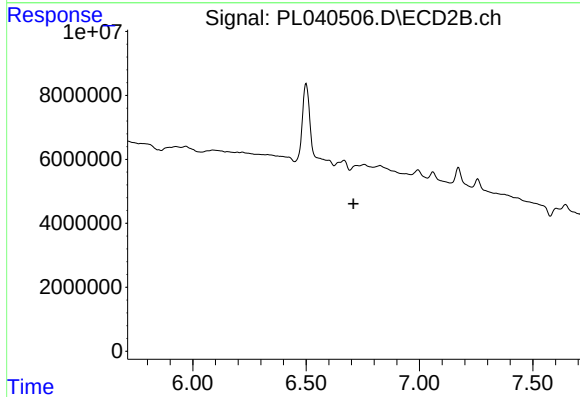


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

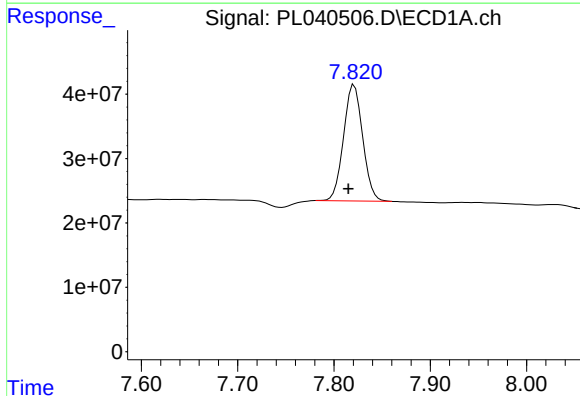

#28 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: 0.006 min
Response: 248368039
Conc: 26.13 ng/ml

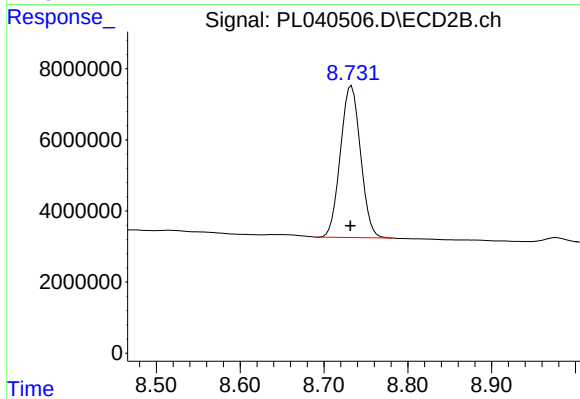

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: 0.001 min
Response: 71364566
Conc: 22.54 ng/ml