

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092820\
 Data File : PL061833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2020 09:25
 Operator : DD\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 17:42:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	84815532	127.0E6	49.717	46.536
28)	SA Decachlor...	8.210	9.095	73016229	102.4E6	44.884	46.526
Target Compounds							
2)	A alpha-BHC	3.894	4.396	123.3E6	190.2E6	50.578	47.613
3)	MA gamma-BHC...	4.177	4.681	110.8E6	174.2E6	50.652	47.064
4)	MA Heptachlor	4.479	5.192	102.4E6	167.0E6	50.190	48.238
5)	MB Aldrin	4.727	5.498	91793675	155.6E6	50.875	48.018
6)	B beta-BHC	4.428	4.853	45757203	70457403	50.100	46.662
7)	B delta-BHC	4.632	5.071	104.7E6	152.3E6	51.072	59.751
8)	B Heptachlo...	5.169	5.887	87294541	134.3E6	50.001	54.177
9)	A Endosulfan I	5.508	6.244	80837679	127.4E6	49.886	46.130
10)	B gamma-Chl...	5.397	6.122	86309990	138.0E6	49.699	47.007
11)	B alpha-Chl...	5.455	6.195	86228575	138.3E6	49.640	46.033
12)	B 4,4'-DDE	5.620	6.352	79117595	127.7E6	50.340	46.797
13)	MA Dieldrin	5.751	6.502	83911548	130.7E6	49.891	46.086
14)	MA Endrin	6.007	6.720	72842557	104.0E6	45.778	42.617
15)	B Endosulfa...	6.280	6.930	75888938	111.0E6	46.937	42.941
16)	A 4,4'-DDD	6.135	6.843	67663063	101.6E6	51.104	45.688
17)	MA 4,4'-DDT	6.375	7.144	62021398	95553921	49.165	43.636
18)	B Endrin al...	6.448	7.055	65065778	95387865	46.271	44.564
19)	B Endosulfa...	6.661	7.278	73440459	106.5E6	47.471	45.470
20)	A Methoxychlor	6.921	7.604	36865806	54173513	45.597	42.996
21)	B Endrin ke...	7.151	7.751	86245621	110.6E6	50.465	47.116
22)	Mirex	7.340	8.207	64390254	80784208	45.930	45.849



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092820\
Data File : PL061833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2020 09:25
Operator : DD\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 17:42:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

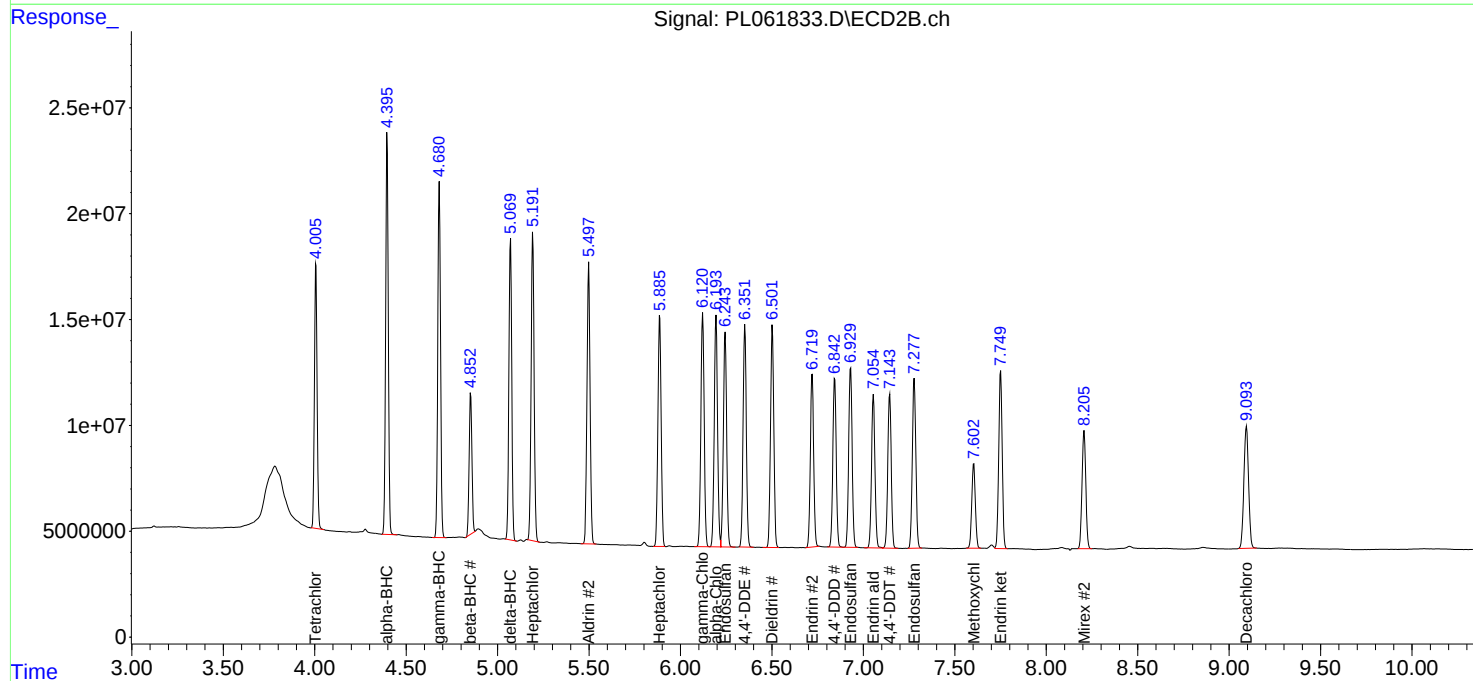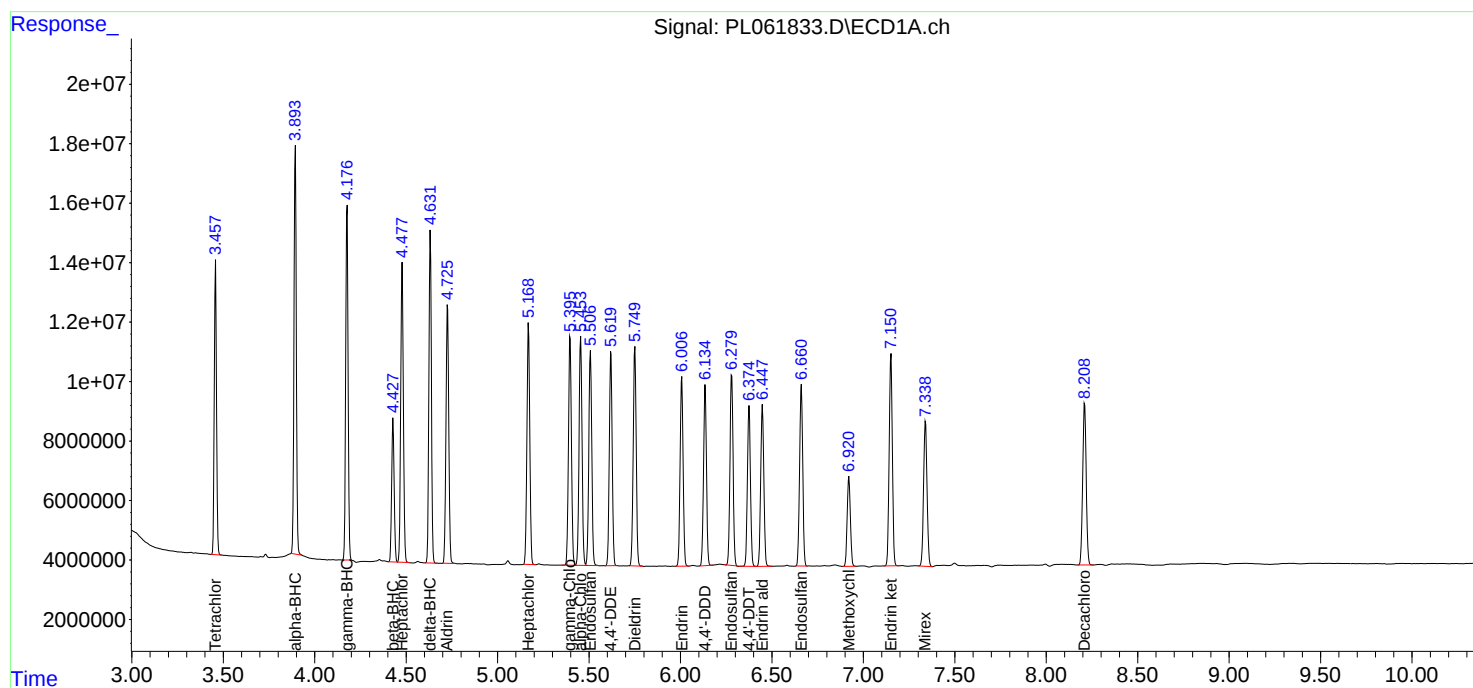


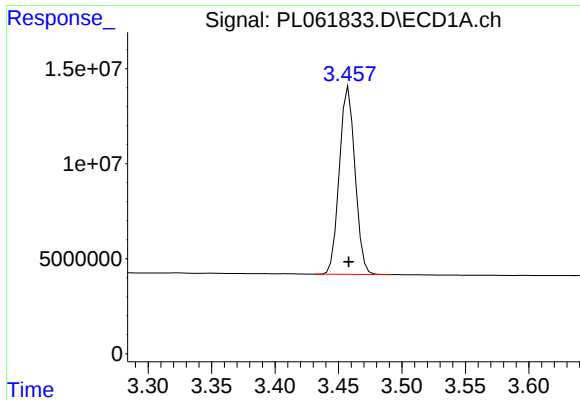

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 84815532
Conc: 49.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

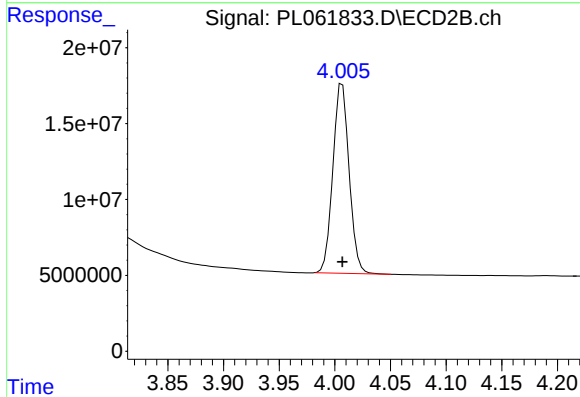


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 126960990
Conc: 46.54 ng/ml

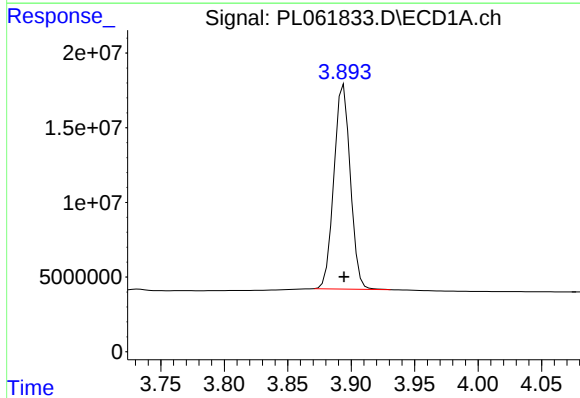


#2 alpha-BHC

R.T.: 3.894 min
Delta R.T.: 0.000 min
Response: 123279854
Conc: 50.58 ng/ml

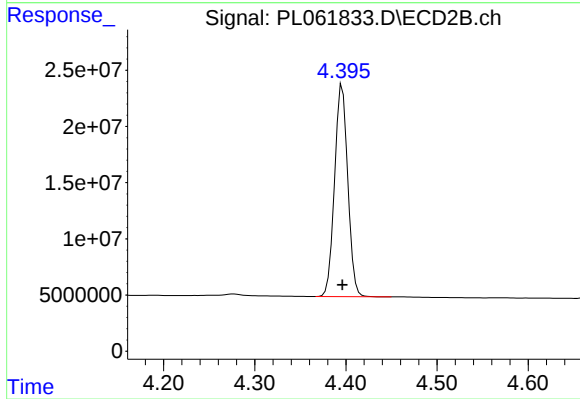

#2 alpha-BHC


R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 190179553
Conc: 47.61 ng/ml

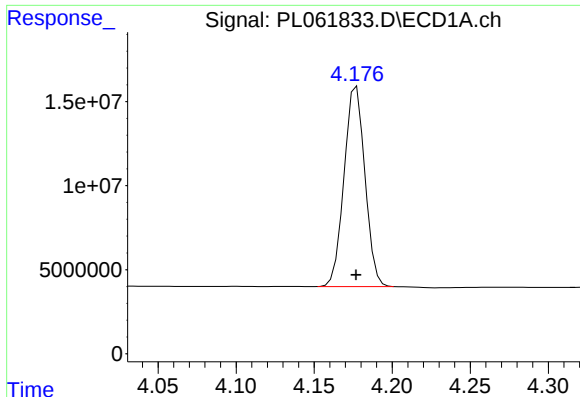

#3 gamma-BHC (Lindane)


R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 110786555
Conc: 50.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

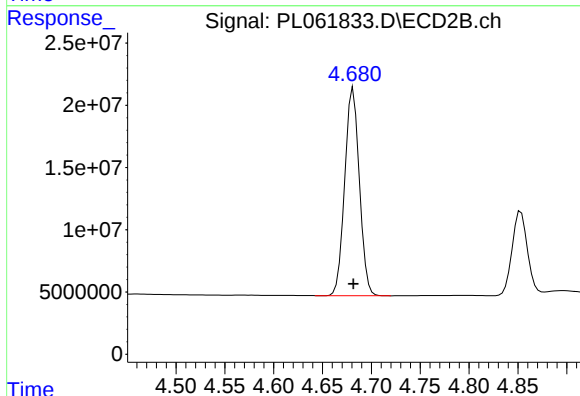


#3 gamma-BHC (Lindane)

R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 174225621
Conc: 47.06 ng/ml

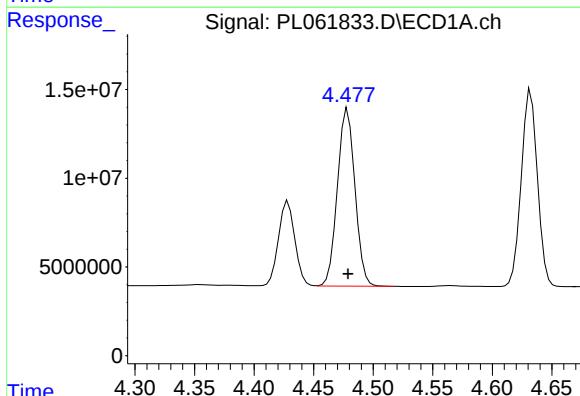


#4 Heptachlor

R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 102420795
Conc: 50.19 ng/ml

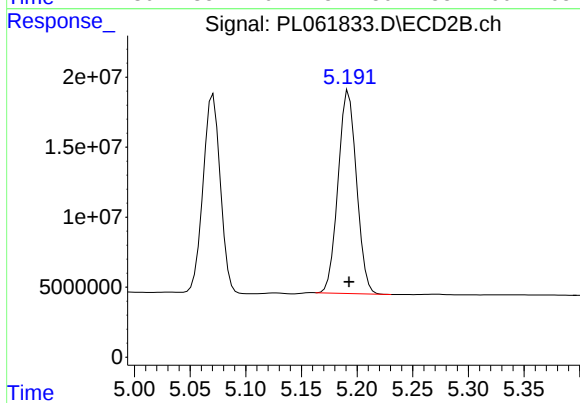

#4 Heptachlor


R.T.: 5.192 min
Delta R.T.: 0.000 min
Response: 167042462
Conc: 48.24 ng/ml

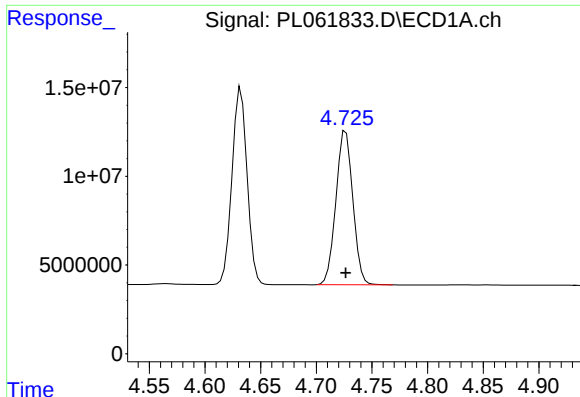

#5 Aldrin


R.T.: 4.727 min
Delta R.T.: 0.000 min
Response: 91793675
Conc: 50.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

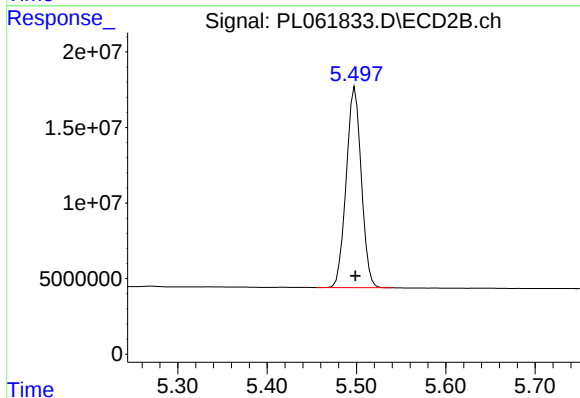


#5 Aldrin

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 155552741
Conc: 48.02 ng/ml

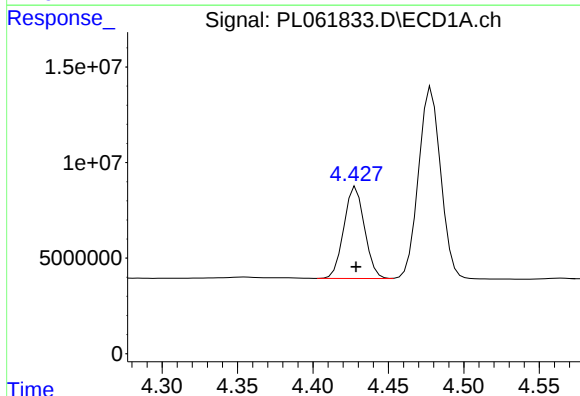


#6 beta-BHC

R.T.: 4.428 min
Delta R.T.: 0.000 min
Response: 45757203
Conc: 50.10 ng/ml

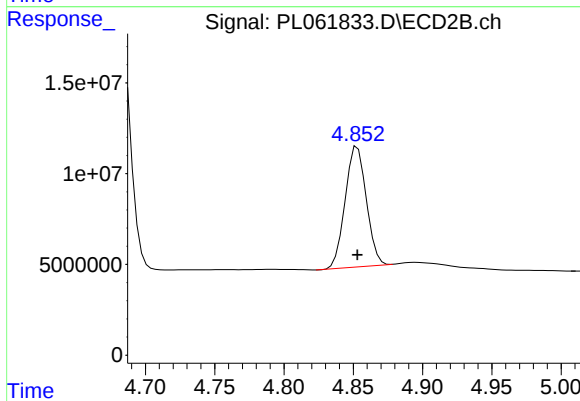

#6 beta-BHC


R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 70457403
Conc: 46.66 ng/ml

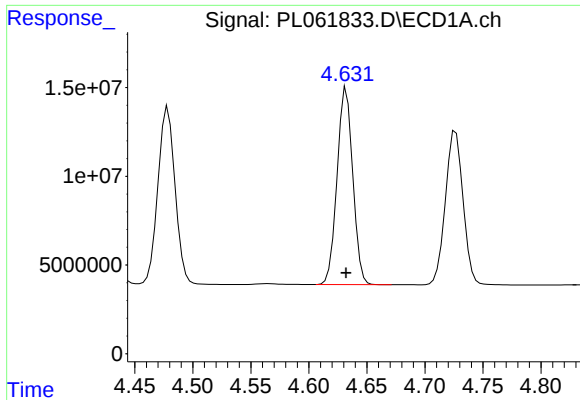

#7 delta-BHC


R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 104709596
Conc: 51.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

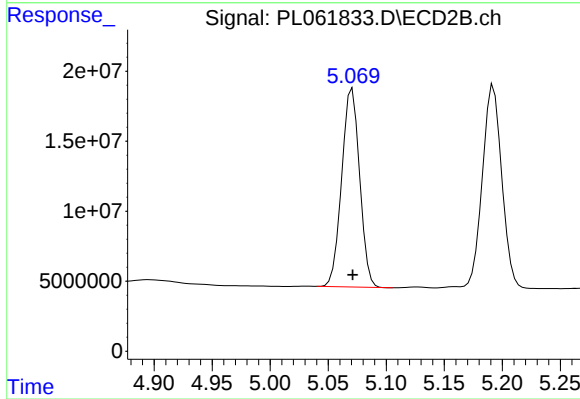


#7 delta-BHC

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 152251741
Conc: 59.75 ng/ml

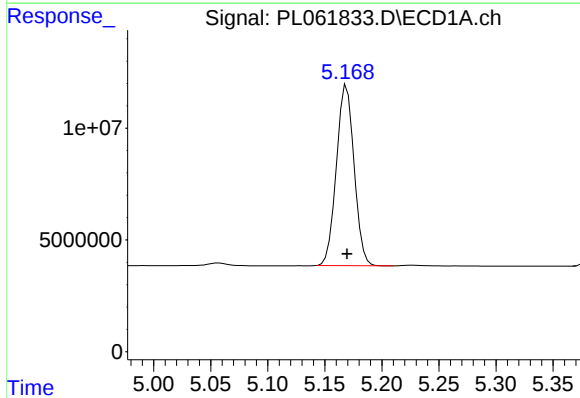


#8 Heptachlor epoxide

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 87294541
Conc: 50.00 ng/ml

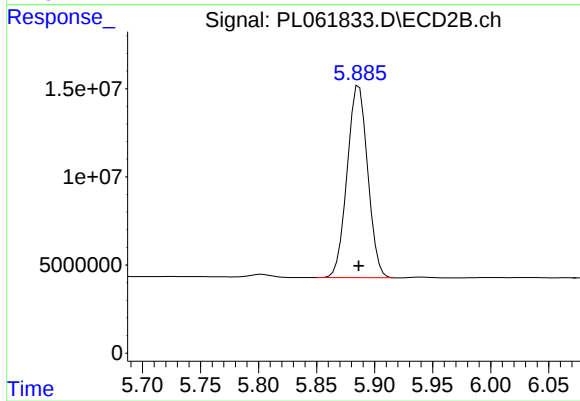

#8 Heptachlor epoxide


R.T.: 5.887 min
Delta R.T.: 0.000 min
Response: 134270153
Conc: 54.18 ng/ml

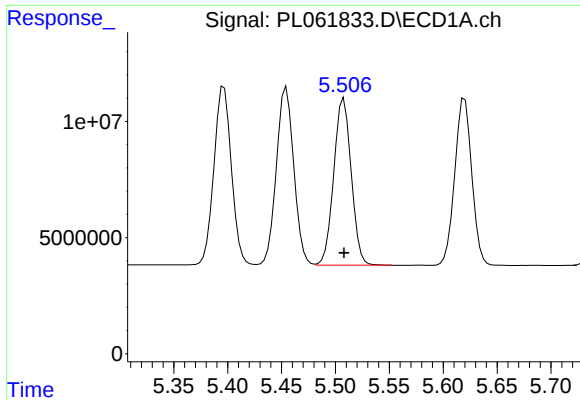

#9 Endosulfan I


R.T.: 5.508 min
Delta R.T.: 0.000 min
Response: 80837679
Conc: 49.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

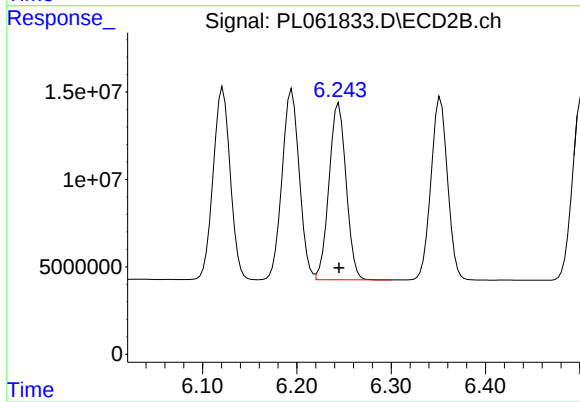


#9 Endosulfan I

R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 127435939
Conc: 46.13 ng/ml

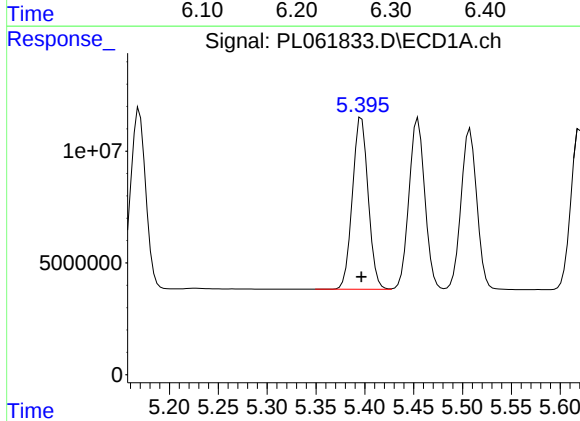


#10 gamma-Chlordane

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 86309990
Conc: 49.70 ng/ml

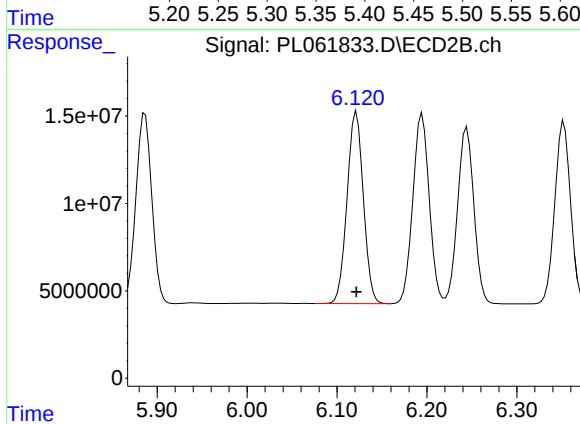

#10 gamma-Chlordane


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 138041723
Conc: 47.01 ng/ml

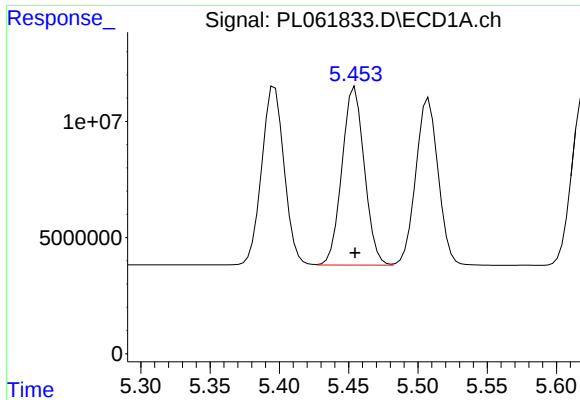

#11 alpha-Chlordane


R.T.: 5.455 min
Delta R.T.: 0.000 min
Response: 86228575
Conc: 49.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

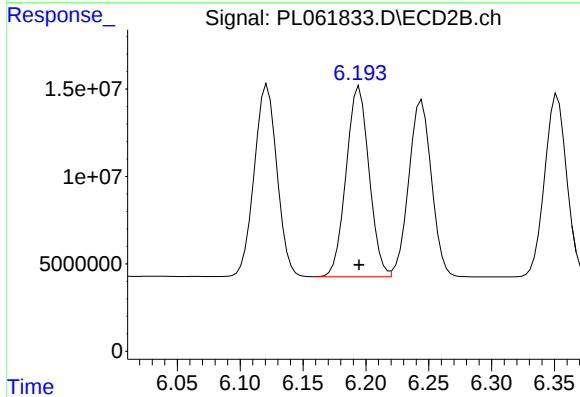


#11 alpha-Chlordane

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 138263228
Conc: 46.03 ng/ml

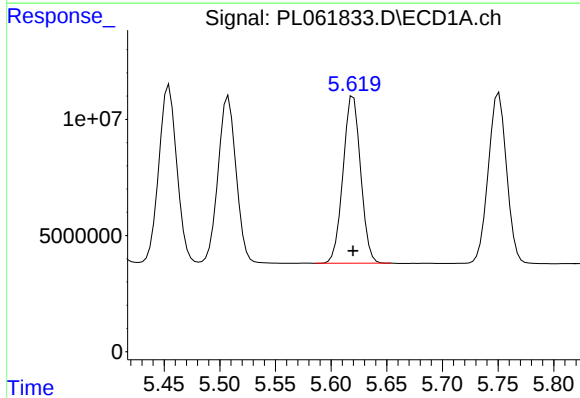


#12 4,4'-DDE

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 79117595
Conc: 50.34 ng/ml

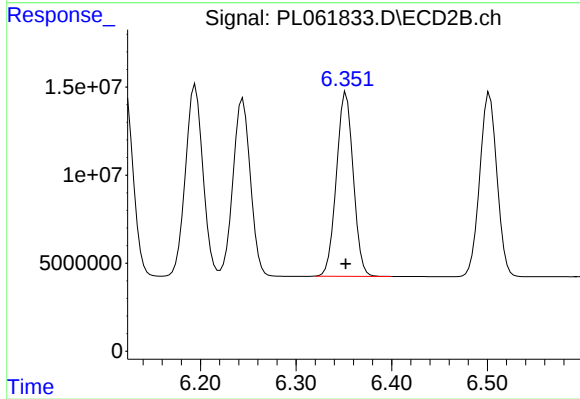

#12 4,4'-DDE


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 127747131
Conc: 46.80 ng/ml

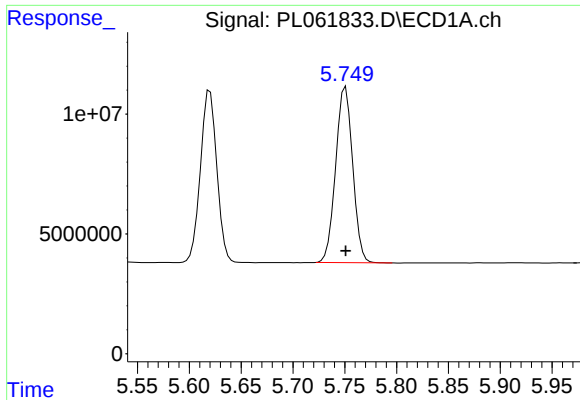

#13 Dieldrin


R.T.: 5.751 min
Delta R.T.: 0.000 min
Response: 83911548
Conc: 49.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

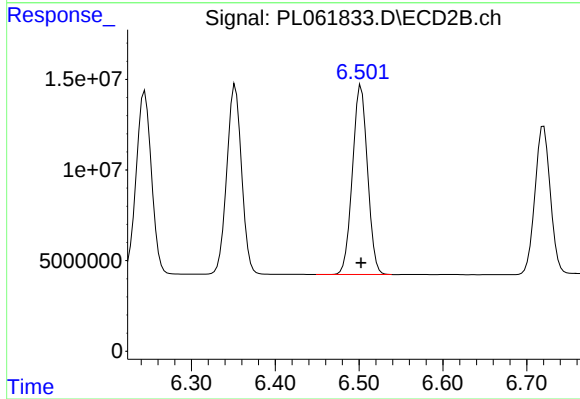


#13 Dieldrin

R.T.: 6.502 min
Delta R.T.: 0.000 min
Response: 130741978
Conc: 46.09 ng/ml

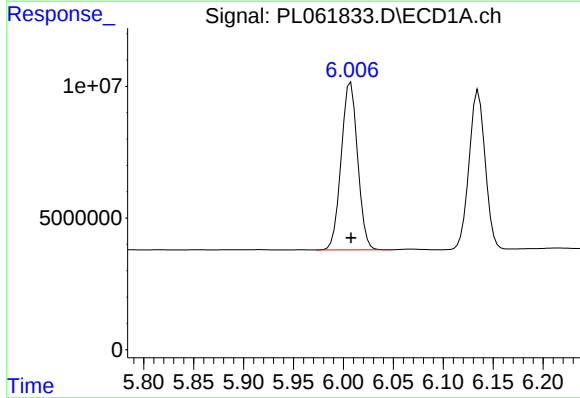


#14 Endrin

R.T.: 6.007 min
Delta R.T.: 0.000 min
Response: 72842557
Conc: 45.78 ng/ml

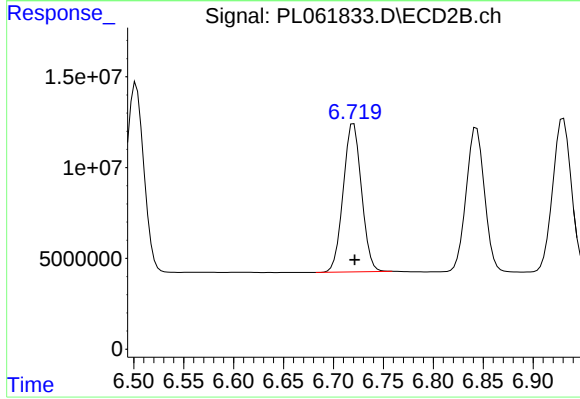

#14 Endrin


R.T.: 6.720 min
Delta R.T.: -0.001 min
Response: 103969096
Conc: 42.62 ng/ml

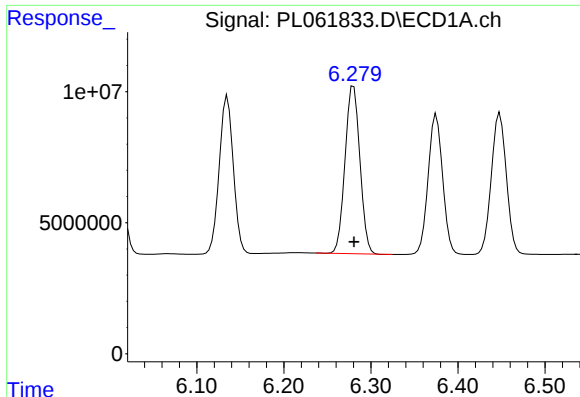

#15 Endosulfan II


R.T.: 6.280 min
Delta R.T.: 0.000 min
Response: 75888938
Conc: 46.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

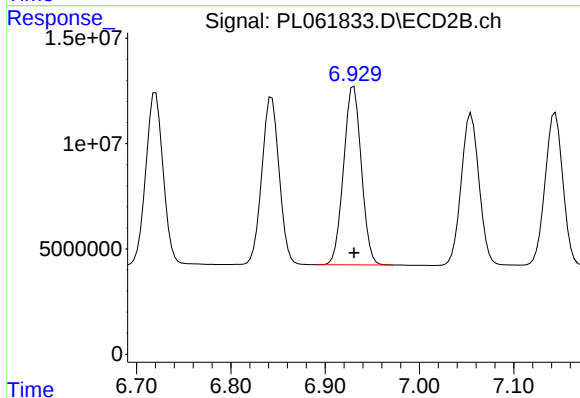


#15 Endosulfan II

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 110989829
Conc: 42.94 ng/ml

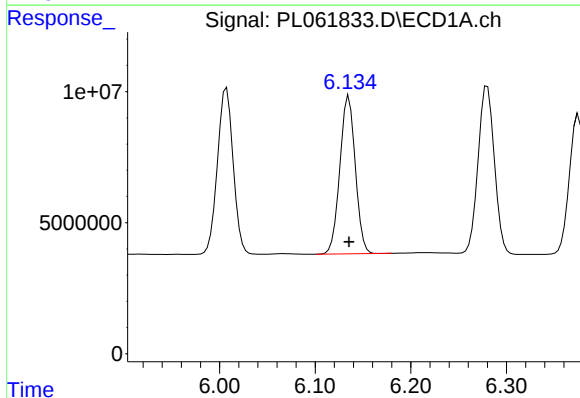


#16 4,4'-DDD

R.T.: 6.135 min
Delta R.T.: 0.000 min
Response: 67663063
Conc: 51.10 ng/ml

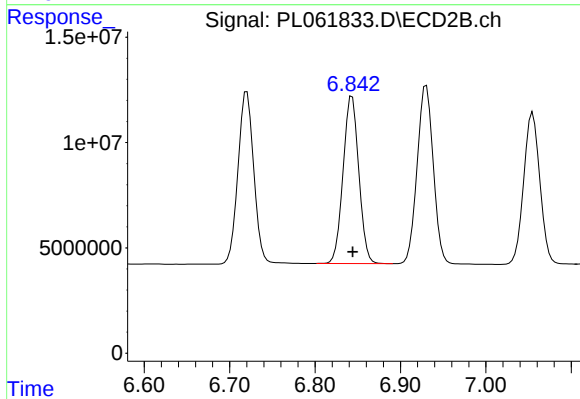

#16 4,4'-DDD


R.T.: 6.843 min
Delta R.T.: 0.000 min
Response: 101567649
Conc: 45.69 ng/ml

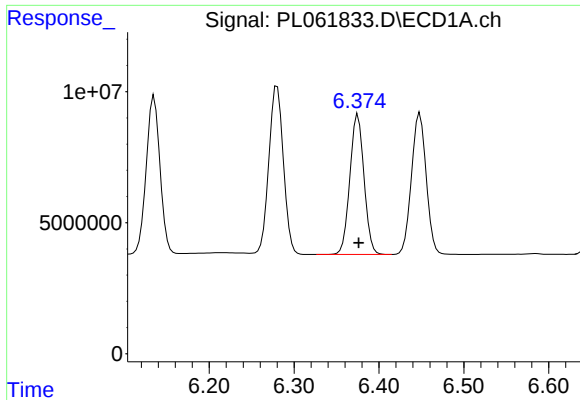

#17 4,4'-DDT


R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 62021398
Conc: 49.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

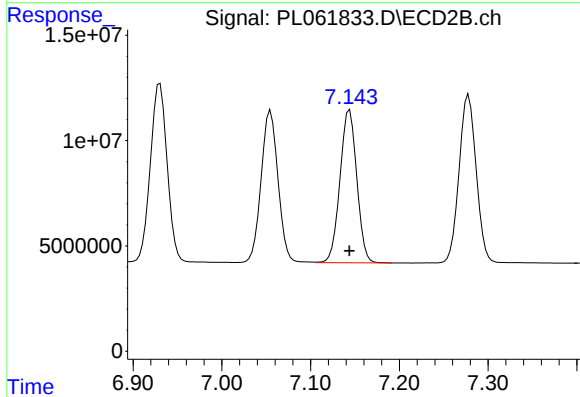


#17 4,4'-DDT

R.T.: 7.144 min
Delta R.T.: 0.000 min
Response: 95553921
Conc: 43.64 ng/ml

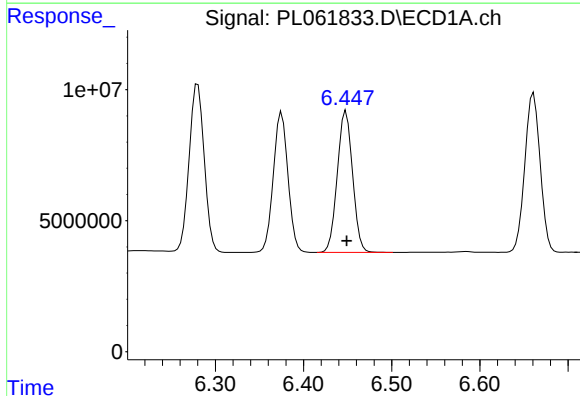


#18 Endrin aldehyde

R.T.: 6.448 min
Delta R.T.: 0.000 min
Response: 65065778
Conc: 46.27 ng/ml

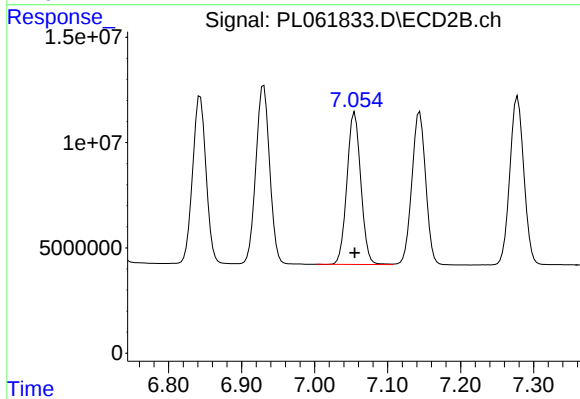

#18 Endrin aldehyde


R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 95387865
Conc: 44.56 ng/ml

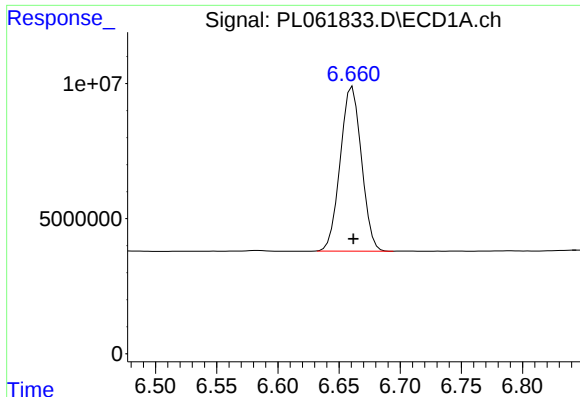

#19 Endosulfan Sulfate


R.T.: 6.661 min
Delta R.T.: 0.000 min
Response: 73440459
Conc: 47.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

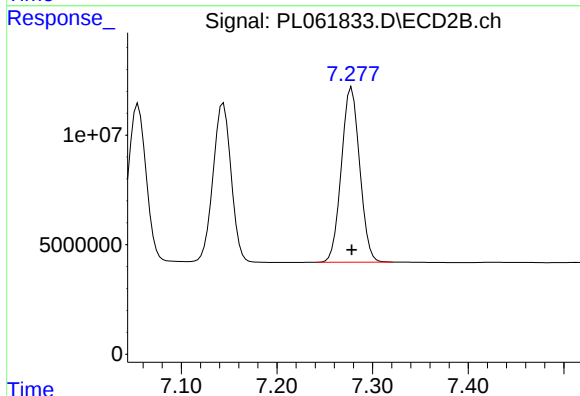


#19 Endosulfan Sulfate

R.T.: 7.278 min
Delta R.T.: 0.000 min
Response: 106471500
Conc: 45.47 ng/ml

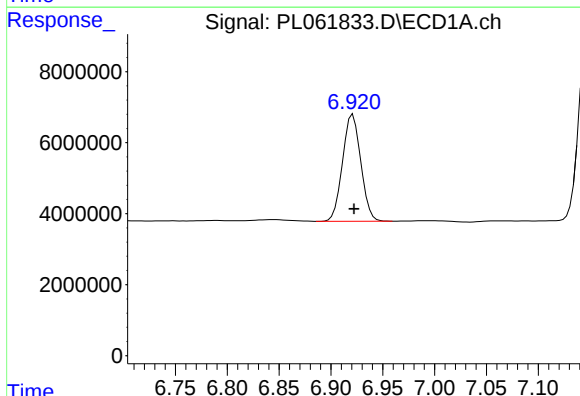


#20 Methoxychlor

R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 36865806
Conc: 45.60 ng/ml

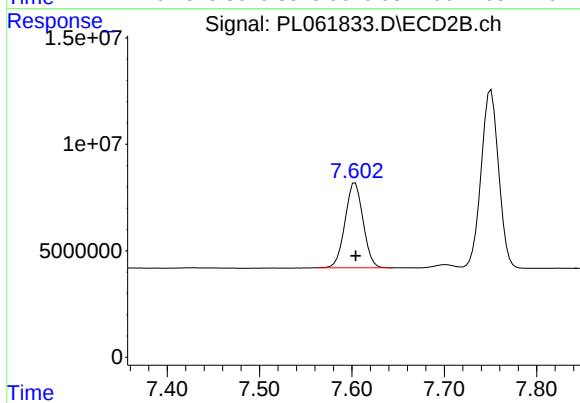

#20 Methoxychlor


R.T.: 7.604 min
Delta R.T.: 0.000 min
Response: 54173513
Conc: 43.00 ng/ml

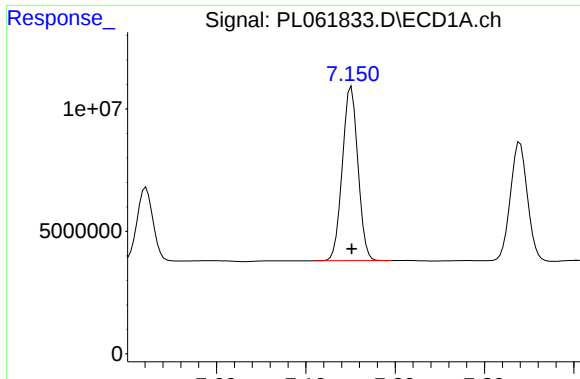

#21 Endrin ketone


R.T.: 7.151 min
Delta R.T.: 0.000 min
Response: 86245621
Conc: 50.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

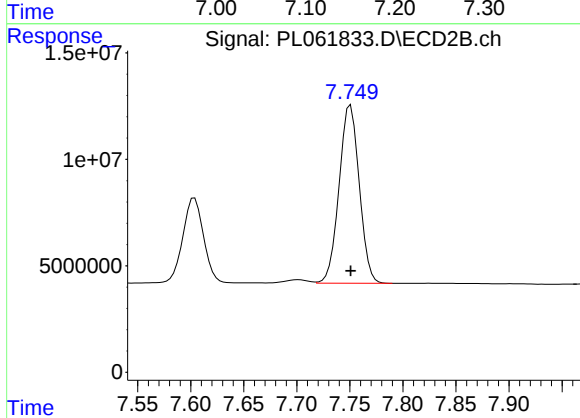


#21 Endrin ketone

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 110581452
Conc: 47.12 ng/ml

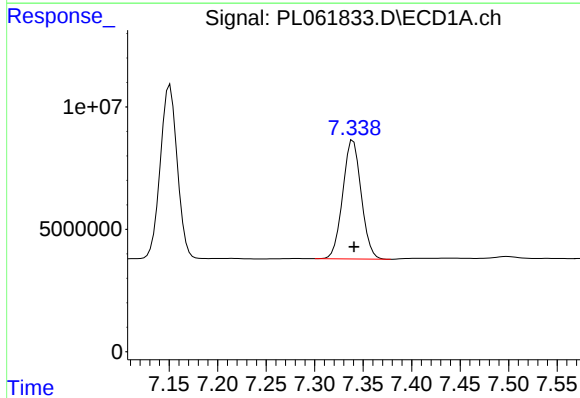


#22 Mirex

R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 64390254
Conc: 45.93 ng/ml

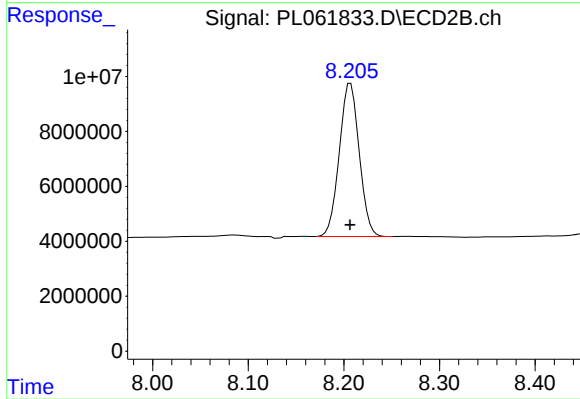

#22 Mirex


R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 80784208
Conc: 45.85 ng/ml

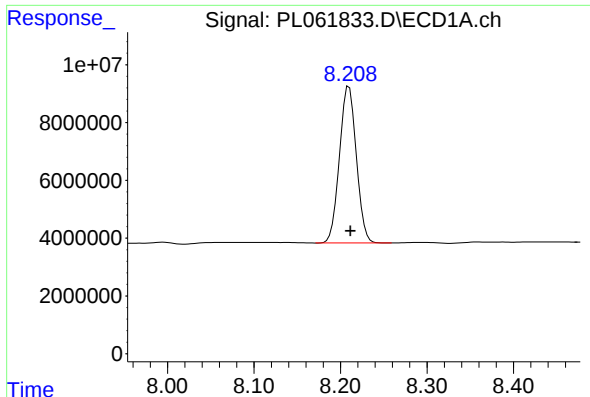

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: -0.002 min
Response: 73016229
Conc: 44.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

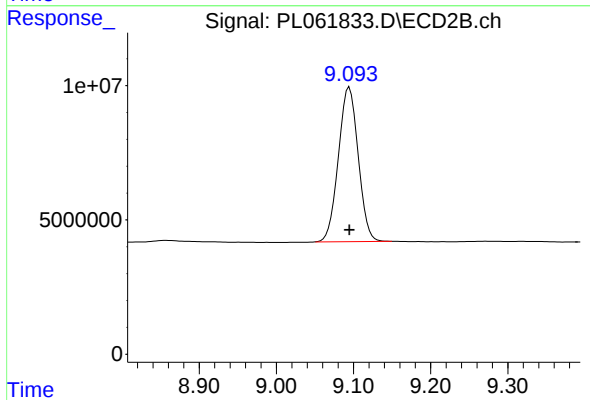

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 102419686
Conc: 46.53 ng/ml