

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092823\
 Data File : PL085564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 05:09
 Operator : AR\AJ
 Sample : 04627-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 280-300FB-BACKFILL-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 06:50:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 26 01:26:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.651	49887198	20995478	19.397	18.504
28)	SA Decachlor...	8.942	7.824	40323468	21935546	19.649	18.476

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092823\
Data File : PL085564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 05:09
Operator : AR\AJ
Sample : 04627-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
280-300FB-BACKFILL-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 06:50:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 26 01:26:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

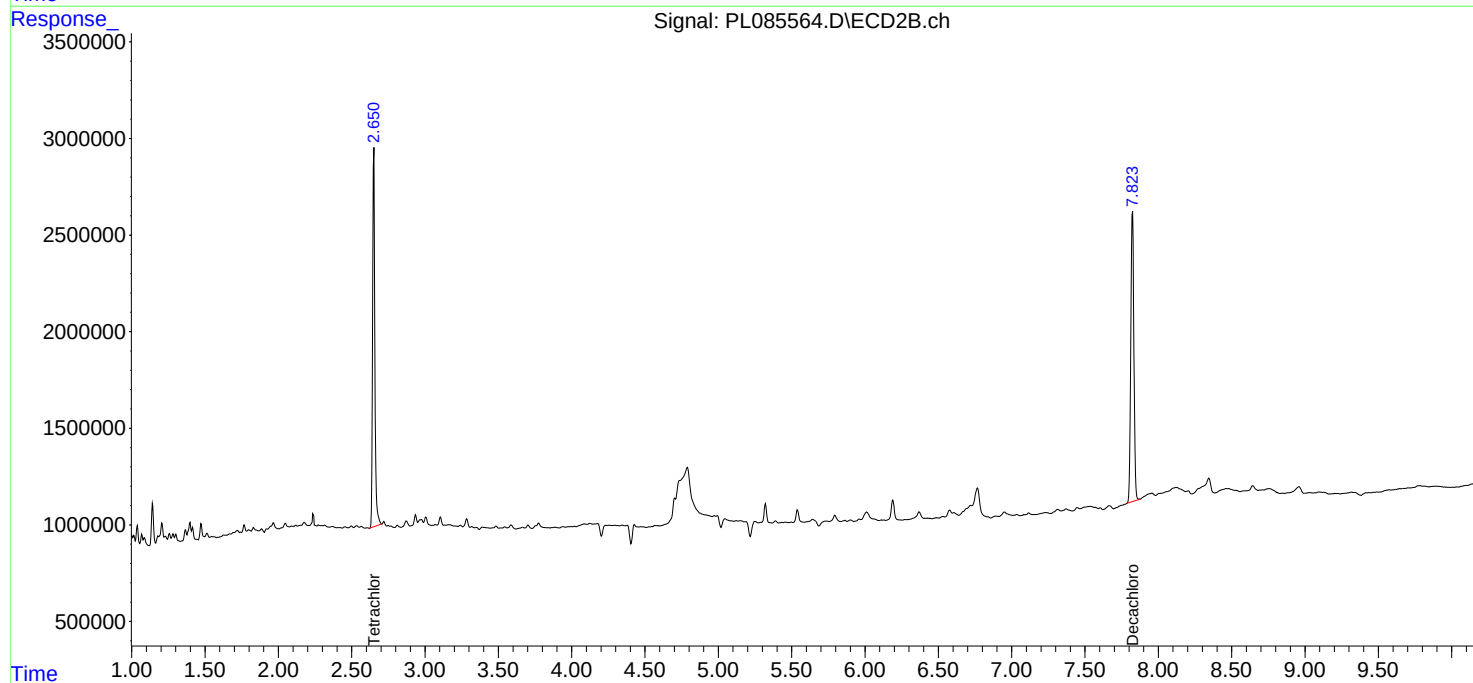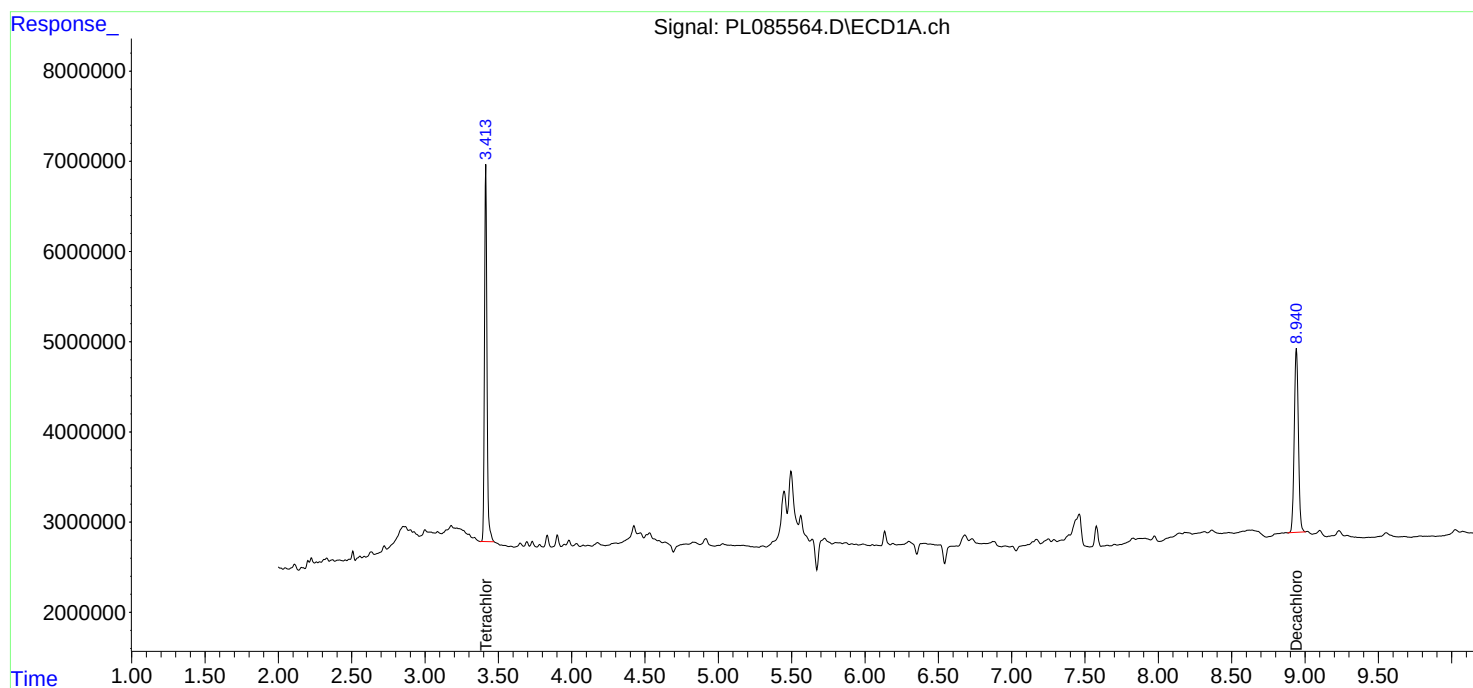


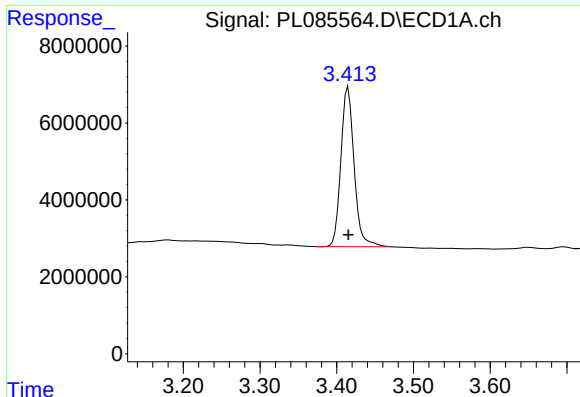

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: 0.000 min
Response: 49887198
Conc: 19.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
280-300FB-BACKFILL-01

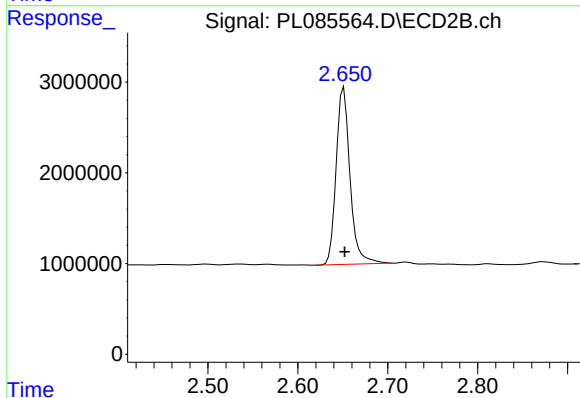


#1 Tetrachloro-m-xylene

R.T.: 2.651 min
Delta R.T.: 0.000 min
Response: 20995478
Conc: 18.50 ng/ml

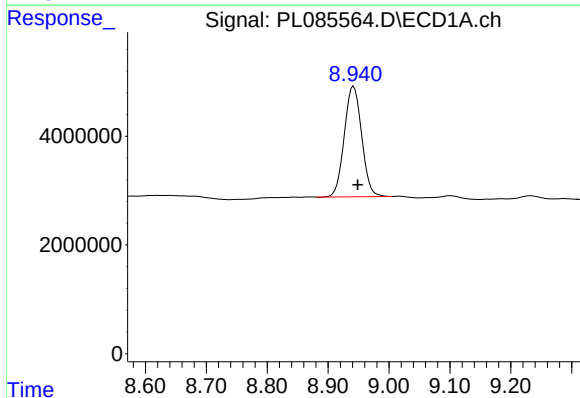

#28 Decachlorobiphenyl

R.T.: 8.942 min
Delta R.T.: -0.007 min
Response: 40323468
Conc: 19.65 ng/ml

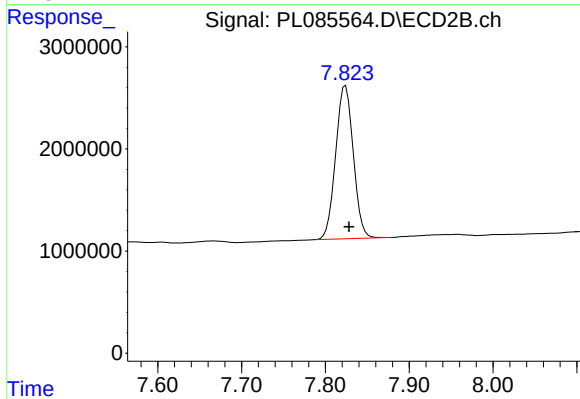

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: -0.004 min
Response: 21935546
Conc: 18.48 ng/ml