

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092919\
 Data File : PL052820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 23:53
 Operator : SG\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 04:48:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 04:45:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	4.048	898.1E6	189.7E6	74.238	73.451
28)	SA Decachlor...	8.346	9.124	699.4E6	200.4E6	73.685	72.333
Target Compounds							
23)	Chlordane-1	4.436	5.045	261.5E6	73667245	753.166	748.474
24)	Chlordane-2	4.942	5.513	288.0E6	82110003	730.658	781.578
25)	Chlordane-3	5.518	6.159	899.0E6	321.3E6	759.196	758.203
26)	Chlordane-4	5.577	6.233	744.3E6	387.1E6	748.871	763.159
27)	Chlordane-5	6.419	7.038	296.6E6	62127539	757.679	732.833


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092919\
Data File : PL052820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 23:53
Operator : SG\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 04:48:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 04:45:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

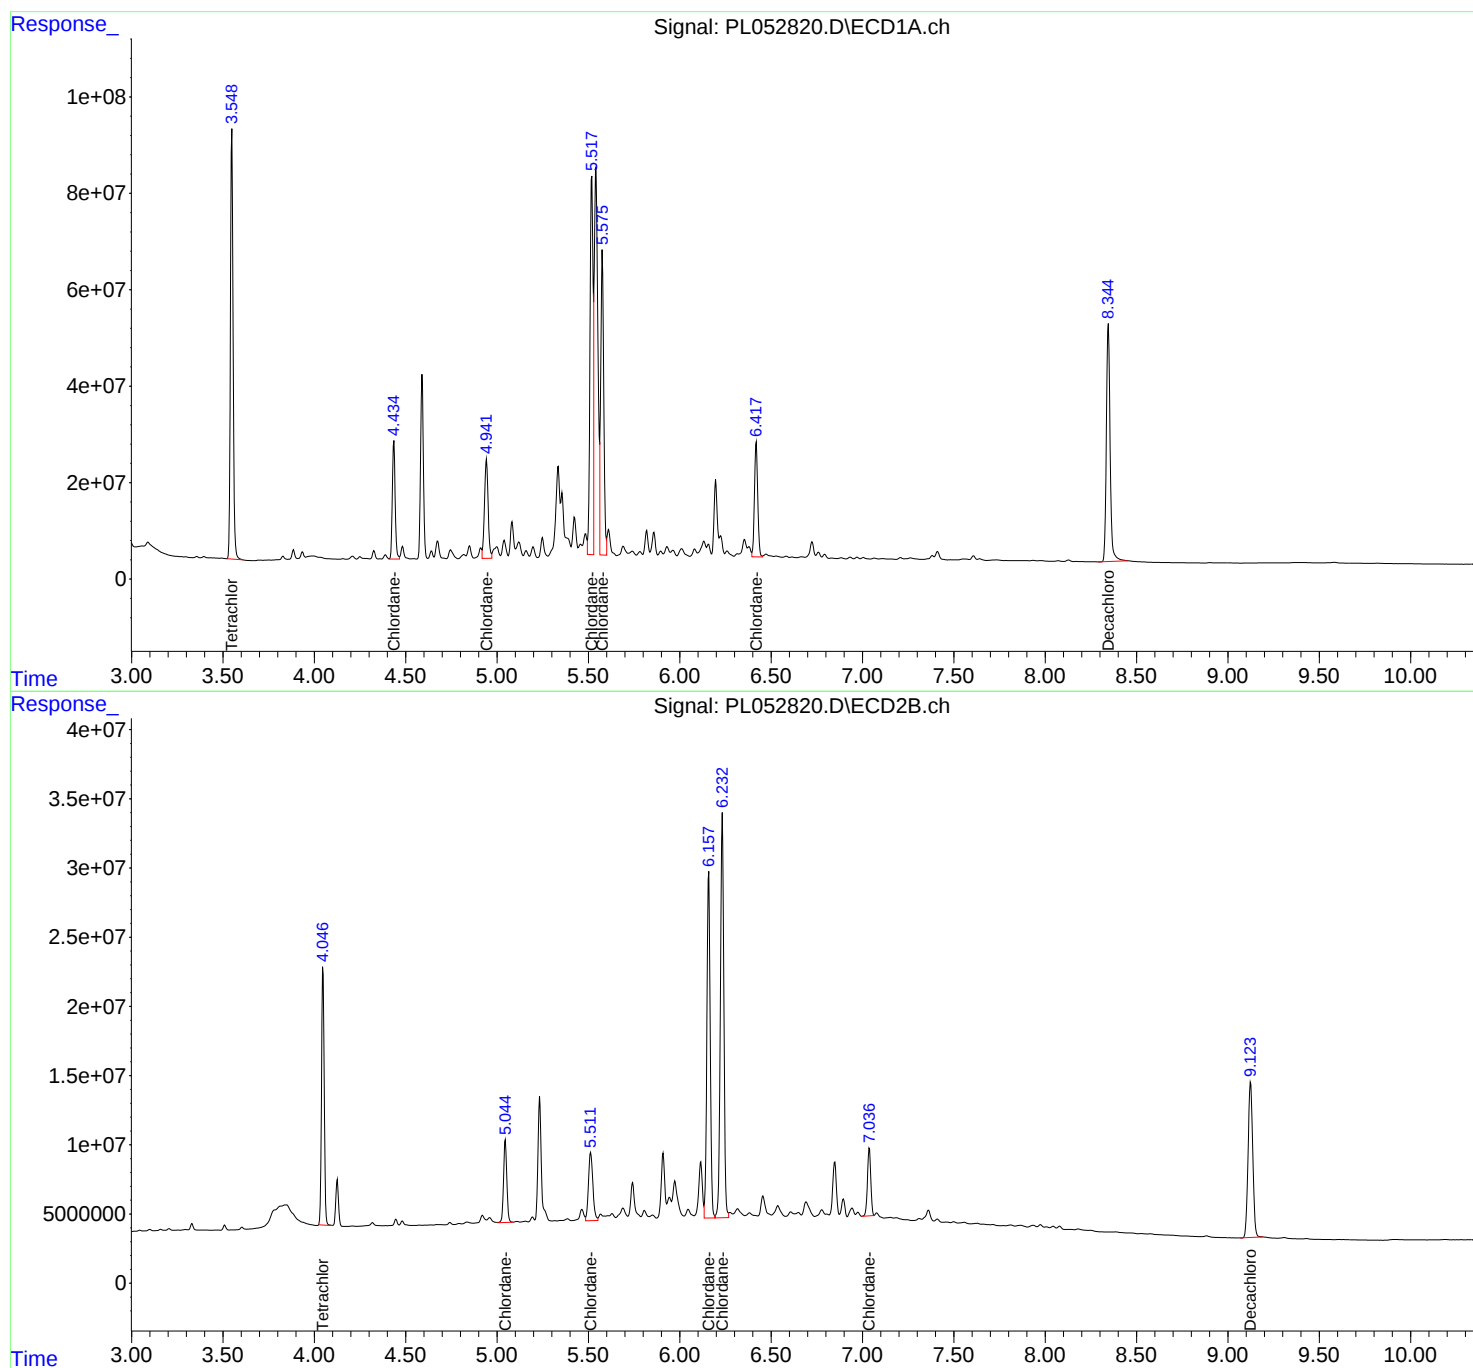


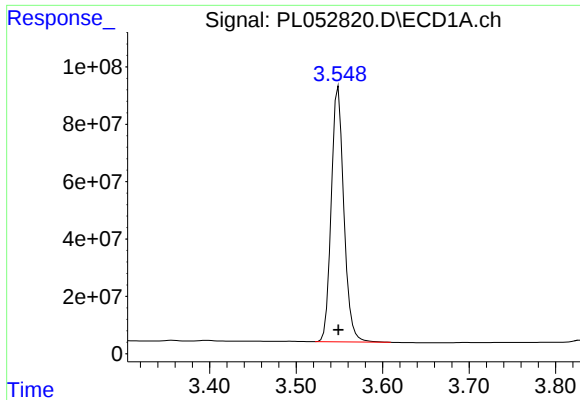

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 898111700
Conc: 74.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

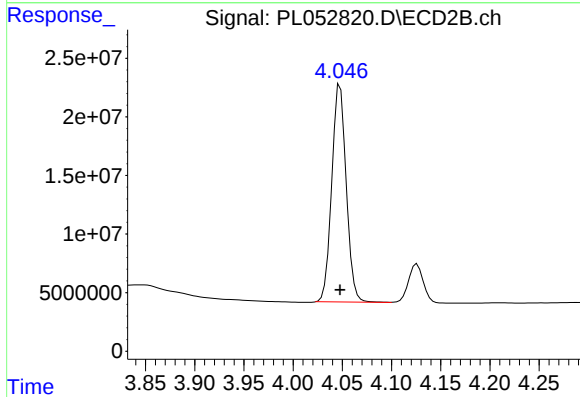


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 189724310
Conc: 73.45 ng/ml

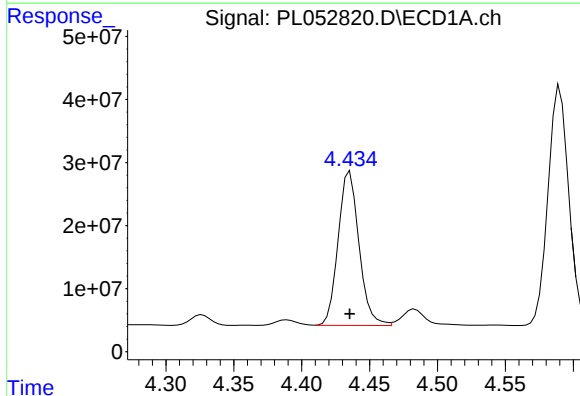


#23 Chlordane-1

R.T.: 4.436 min
Delta R.T.: 0.000 min
Response: 261456262
Conc: 753.17 ng/ml

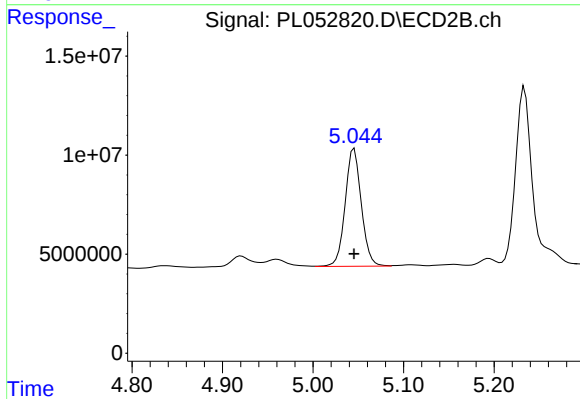

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 73667245
Conc: 748.47 ng/ml

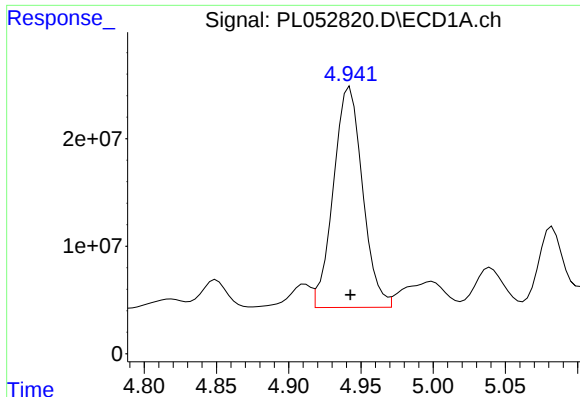

#24 Chlordane-2


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 288018620
Conc: 730.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

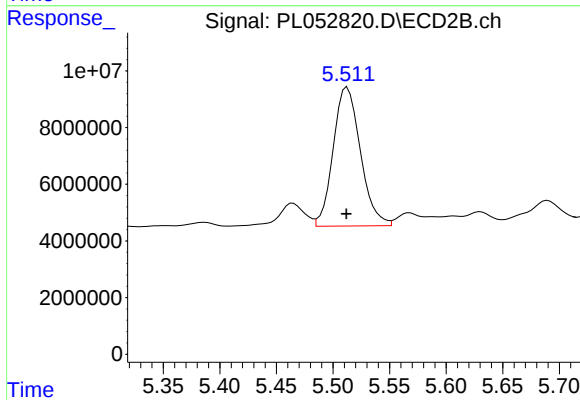


#24 Chlordane-2

R.T.: 5.513 min
Delta R.T.: 0.000 min
Response: 82110003
Conc: 781.58 ng/ml

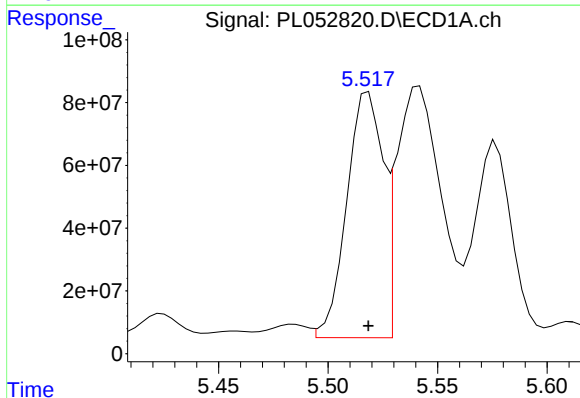


#25 Chlordane-3

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 899037685
Conc: 759.20 ng/ml

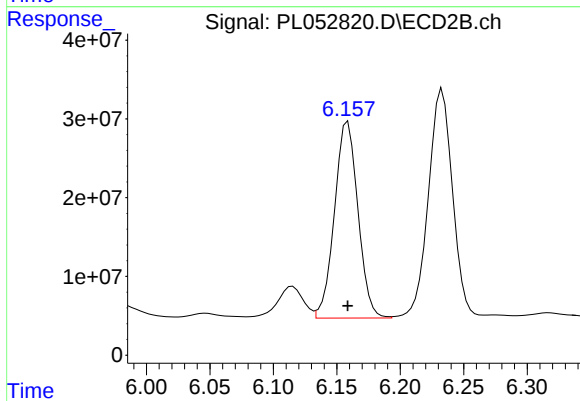

#25 Chlordane-3


R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 321277976
Conc: 758.20 ng/ml

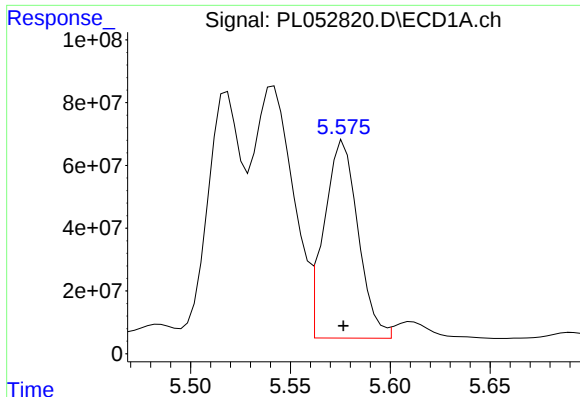

#26 Chlordane-4


R.T.: 5.577 min
Delta R.T.: 0.000 min
Response: 744250692
Conc: 748.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

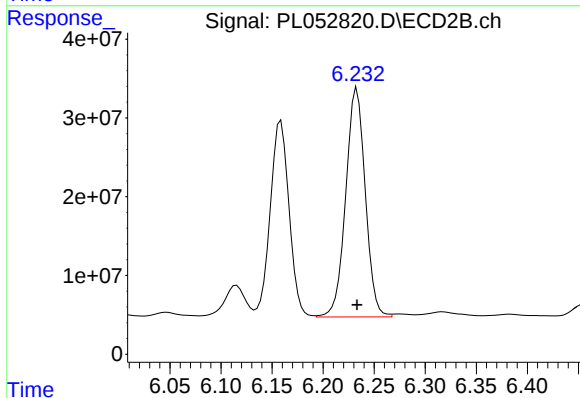


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 387149687
Conc: 763.16 ng/ml

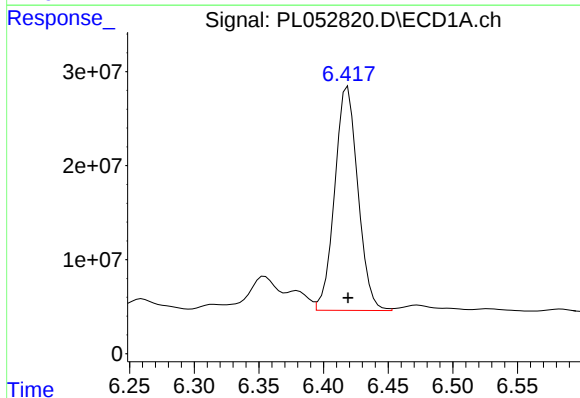


#27 Chlordane-5

R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 296554408
Conc: 757.68 ng/ml

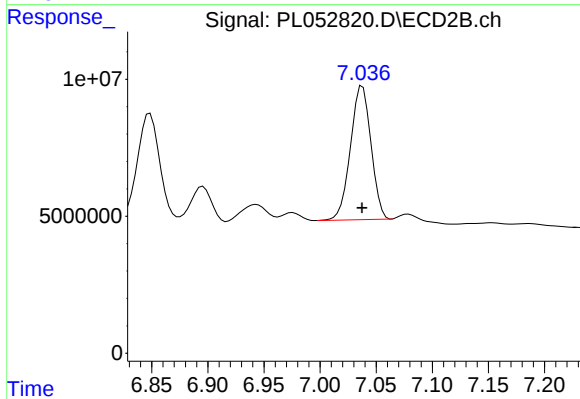

#27 Chlordane-5


R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 62127539
Conc: 732.83 ng/ml

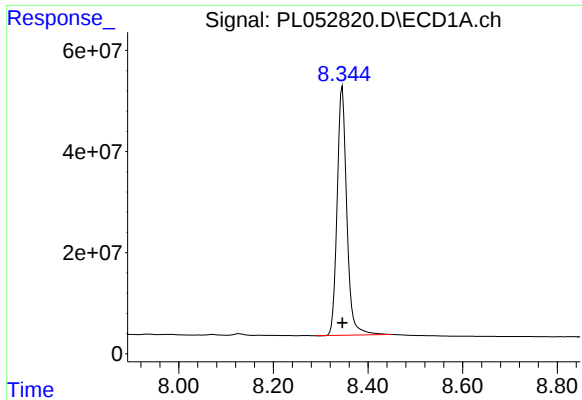

#28 Decachlorobiphenyl

R.T.: 8.346 min
Delta R.T.: 0.000 min
Response: 699384225
Conc: 73.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

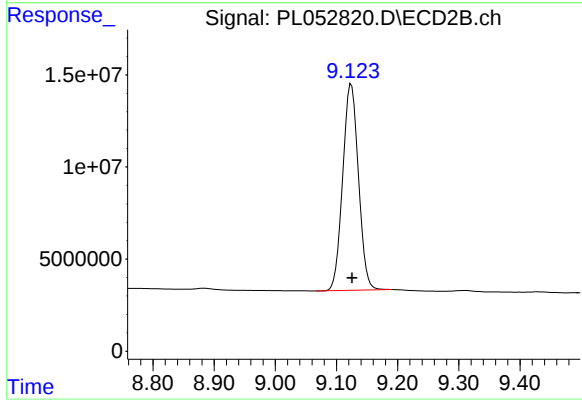

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: -0.001 min
Response: 200355283
Conc: 72.33 ng/ml