

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092919\
 Data File : PL052821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2019 00:07
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 04:48:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 04:45:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	4.048	604.9E6	129.2E6	50.000	50.000
28)	SA Decachlor...	8.346	9.125	474.6E6	138.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.435	5.045	173.6E6	49211621	500.000	500.000
24)	Chlordane-2	4.943	5.512	197.1E6	52528381	500.000	500.000
25)	Chlordane-3	5.518	6.159	592.1E6	211.9E6	500.000	500.000
26)	Chlordane-4	5.577	6.233	496.9E6	253.6E6	500.000	500.000
27)	Chlordane-5	6.419	7.037	195.7E6	42388615	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092919\
Data File : PL052821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2019 00:07
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 04:48:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 04:45:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

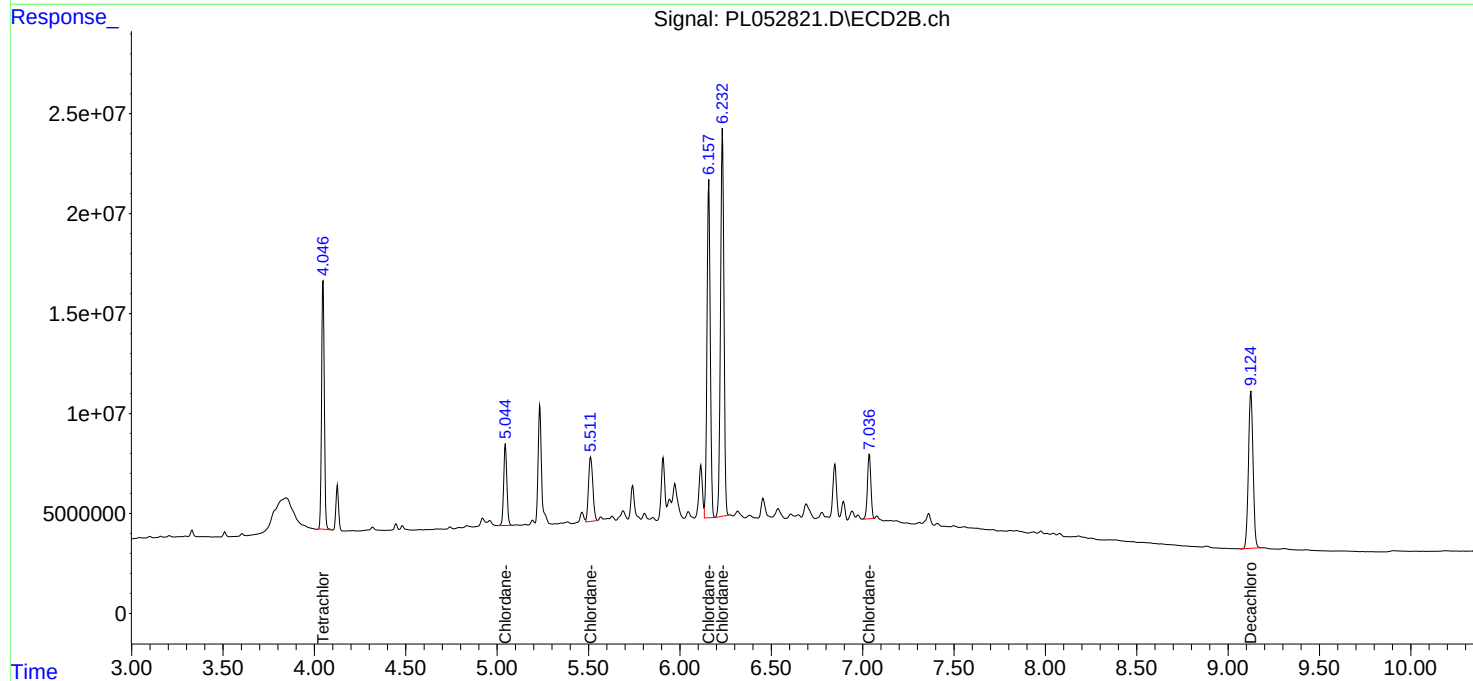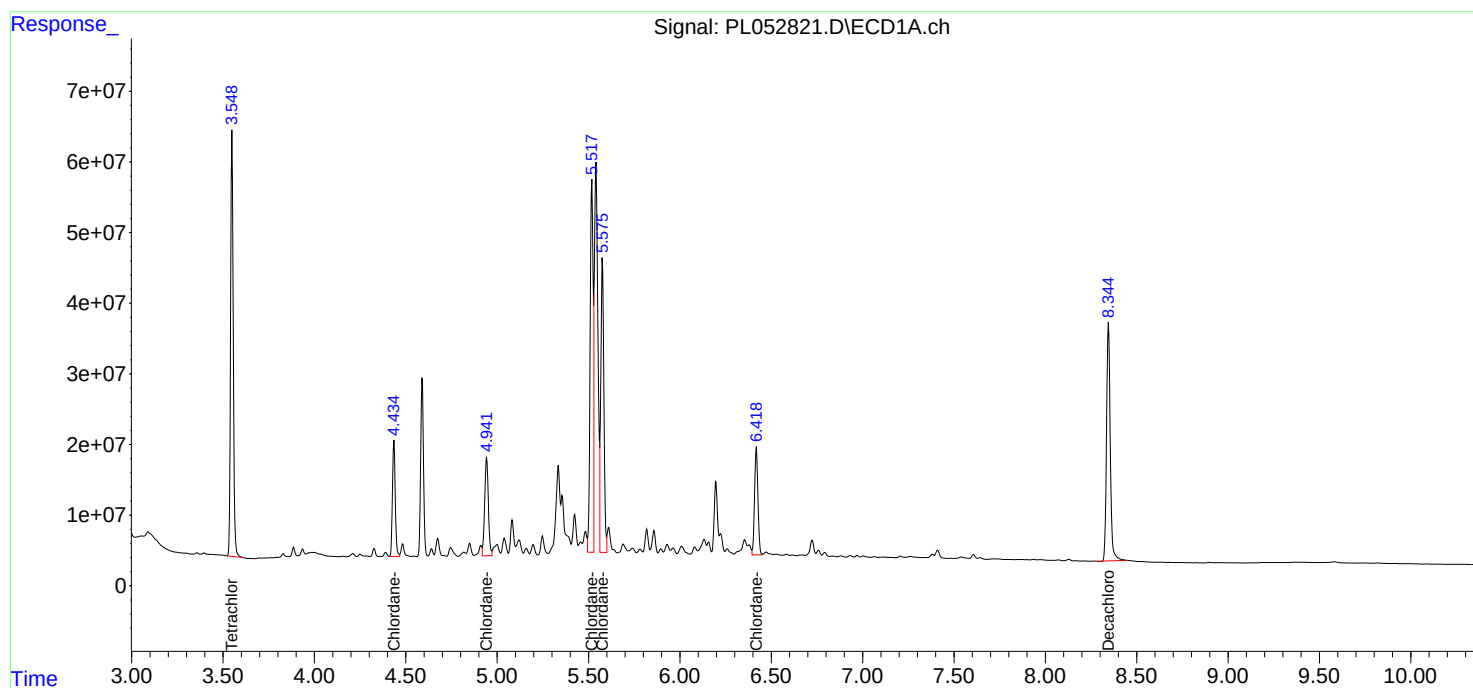


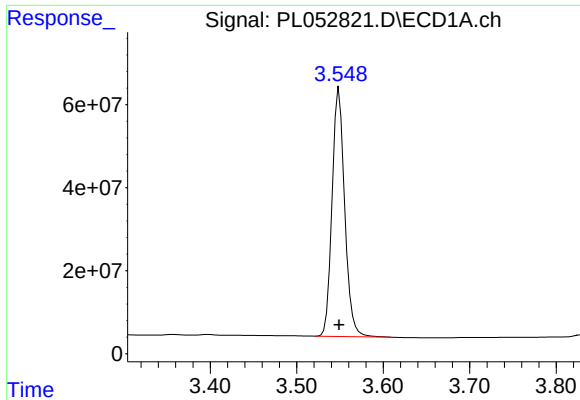

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 604886493
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

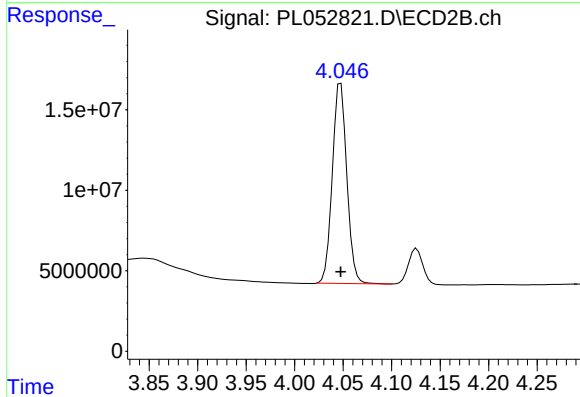


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 129150325
Conc: 50.00 ng/ml

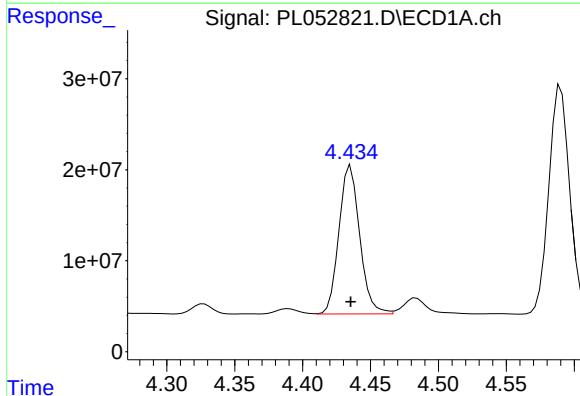


#23 Chlordane-1

R.T.: 4.435 min
Delta R.T.: 0.000 min
Response: 173571566
Conc: 500.00 ng/ml

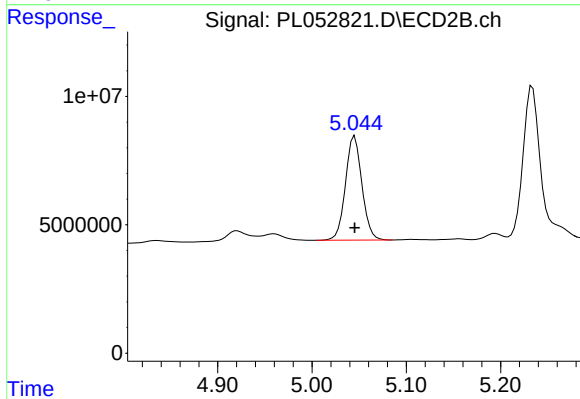

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 49211621
Conc: 500.00 ng/ml

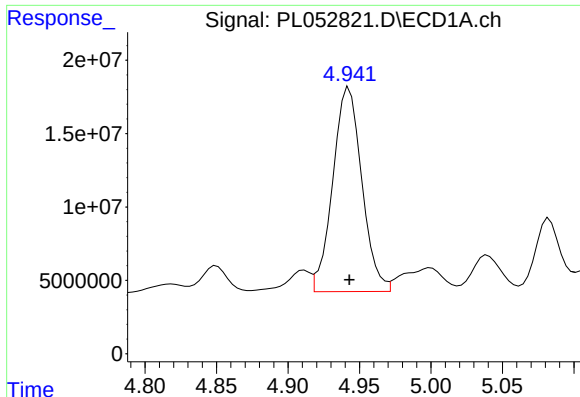

#24 Chlordane-2


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 197095247
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

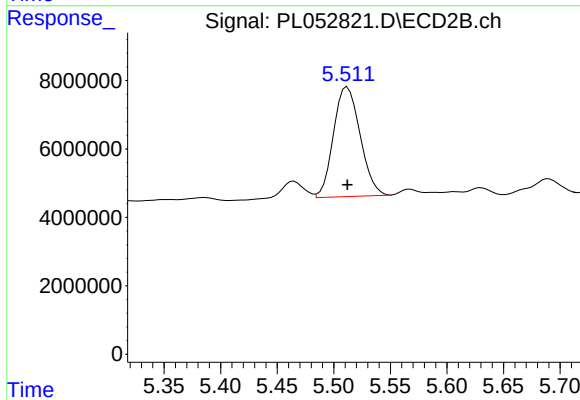


#24 Chlordane-2

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 52528381
Conc: 500.00 ng/ml

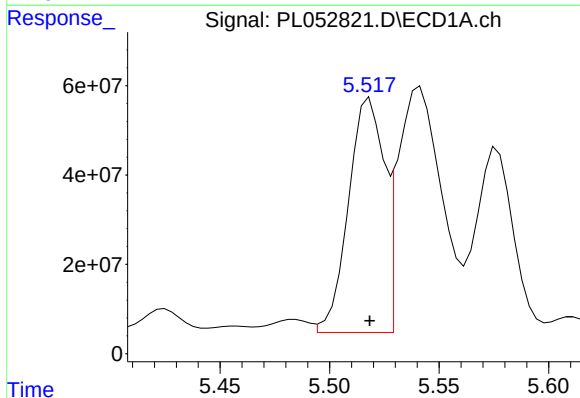


#25 Chlordane-3

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 592098560
Conc: 500.00 ng/ml

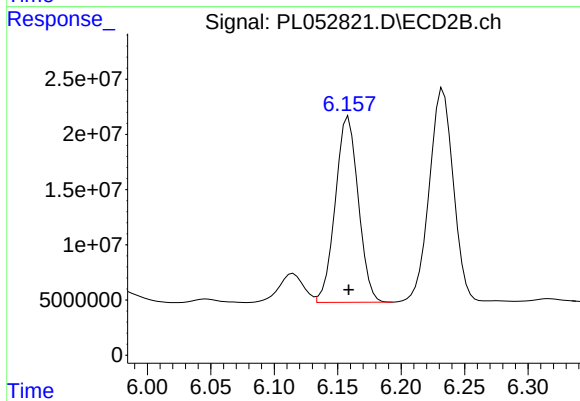

#25 Chlordane-3


R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 211868054
Conc: 500.00 ng/ml

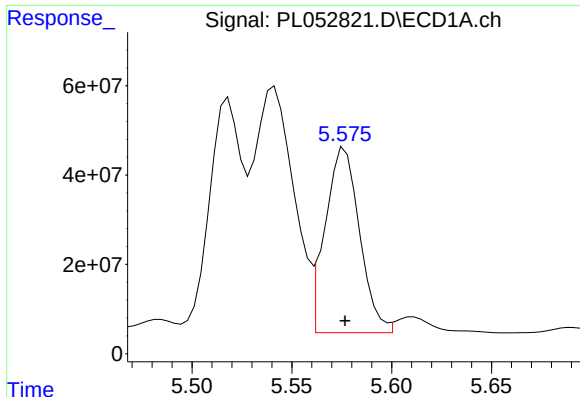

#26 Chlordane-4


R.T.: 5.577 min
Delta R.T.: 0.000 min
Response: 496914896
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

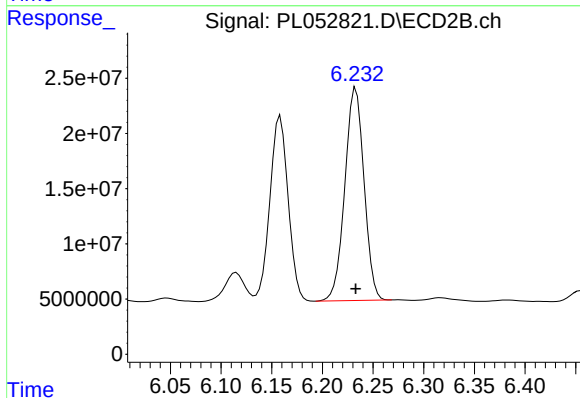


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 253649290
Conc: 500.00 ng/ml

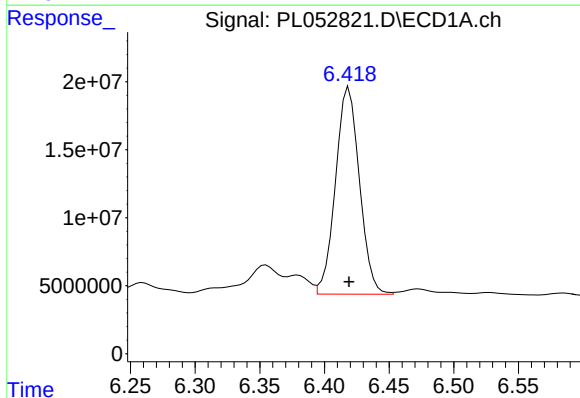


#27 Chlordane-5

R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 195699176
Conc: 500.00 ng/ml

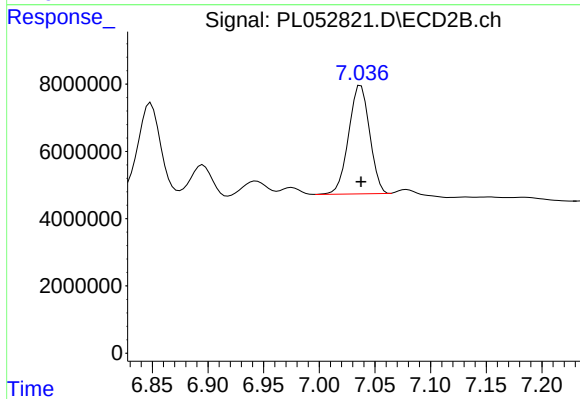

#27 Chlordane-5


R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 42388615
Conc: 500.00 ng/ml

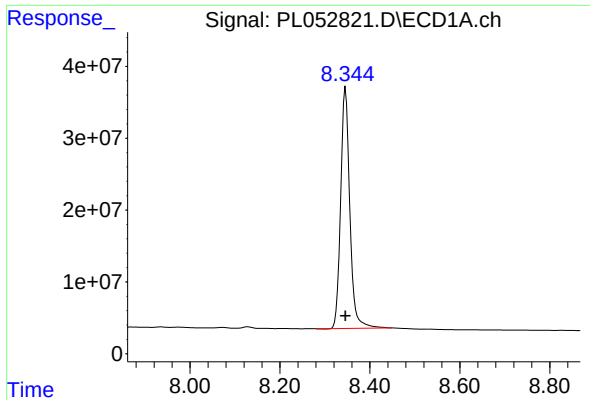

#28 Decachlorobiphenyl

R.T.: 8.346 min
Delta R.T.: 0.000 min
Response: 474574185
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

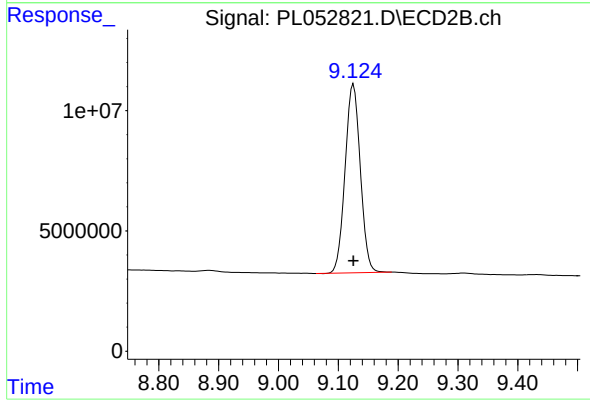

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 138494857
Conc: 50.00 ng/ml