

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092919\
 Data File : PL052830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2019 02:13
 Operator : SG\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL092919CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 08:41:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:36:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	4.048	597.1E6	129.2E6	49.099	49.218
28)	SA Decachlor...	8.345	9.124	477.4E6	141.5E6	47.913	49.253
Target Compounds							
23)	Chlordane-1	4.436	5.045	173.8E6	50555211	500.253	498.426
24)	Chlordane-2	4.942	5.512	197.3E6	57572705	496.616	514.399
25)	Chlordane-3	5.518	6.158	604.1E6	218.5E6	521.343	501.708
26)	Chlordane-4	5.577	6.233	498.5E6	265.5E6	522.315	500.045
27)	Chlordane-5	6.419	7.038	196.8E6	46970645	498.924	532.491



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092919\
Data File : PL052830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2019 02:13
Operator : SG\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL092919CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 08:41:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:36:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

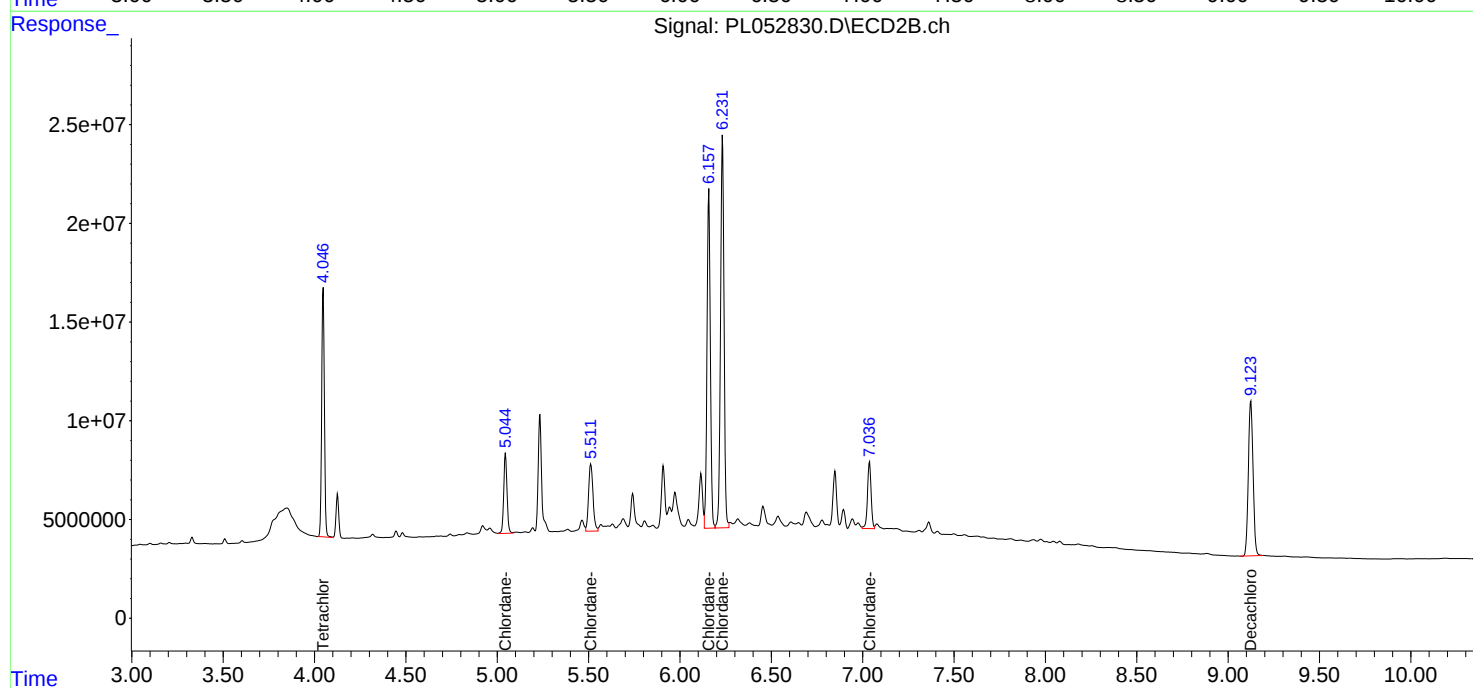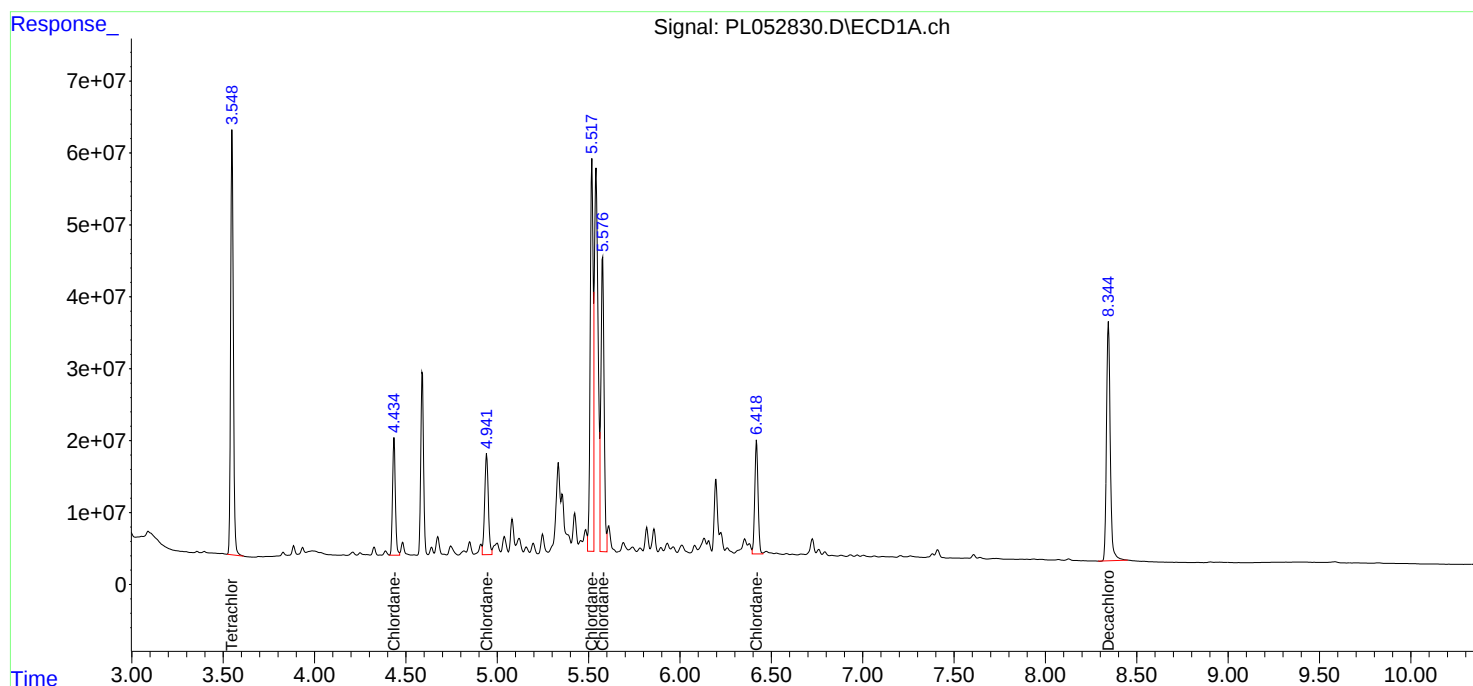


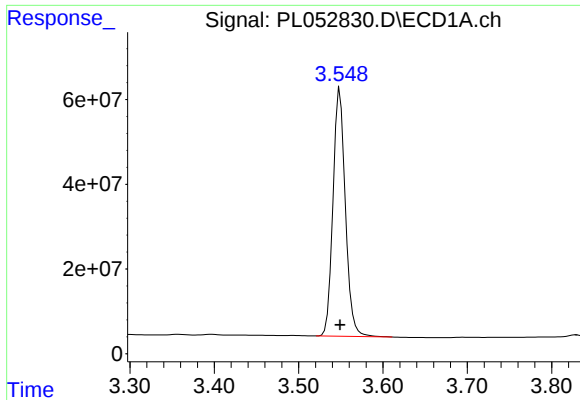

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 597052571
Conc: 49.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092919CHLOR

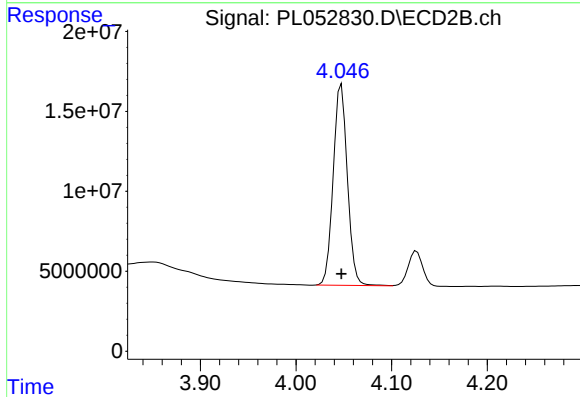


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 129240137
Conc: 49.22 ng/ml

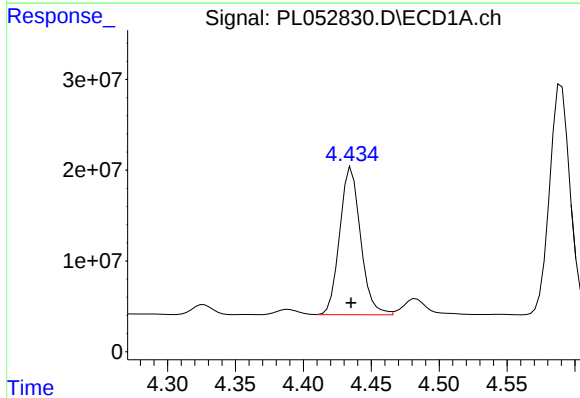


#23 Chlordane-1

R.T.: 4.436 min
Delta R.T.: 0.000 min
Response: 173848651
Conc: 500.25 ng/ml

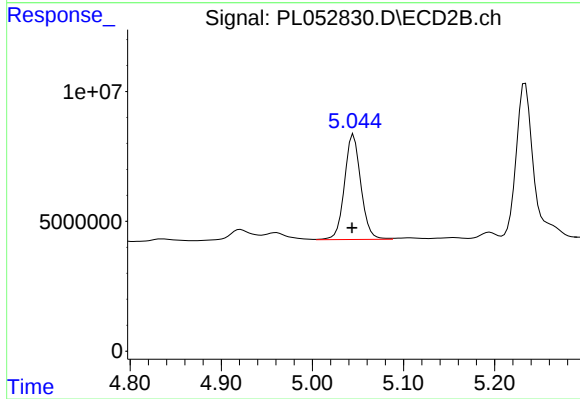

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.002 min
Response: 50555211
Conc: 498.43 ng/ml

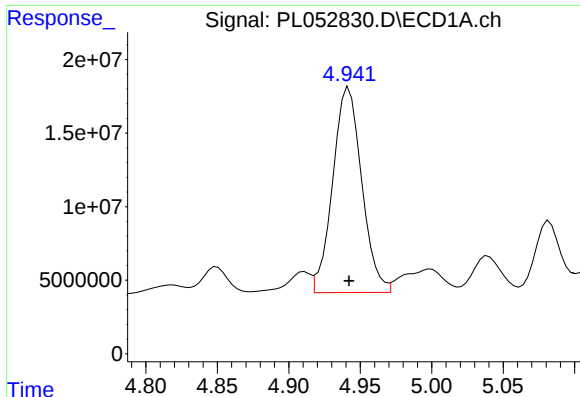

#24 Chlordane-2


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 197298776
Conc: 496.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092919CHLOR

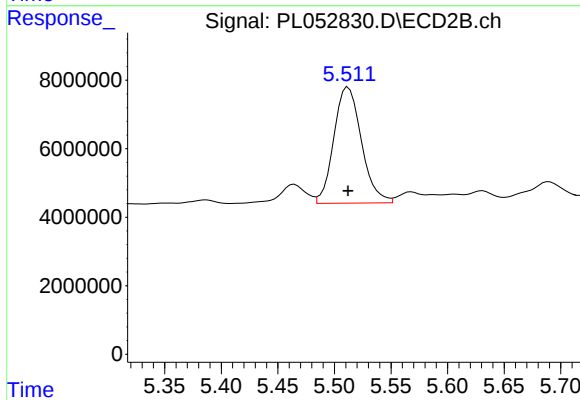


#24 Chlordane-2

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 57572705
Conc: 514.40 ng/ml

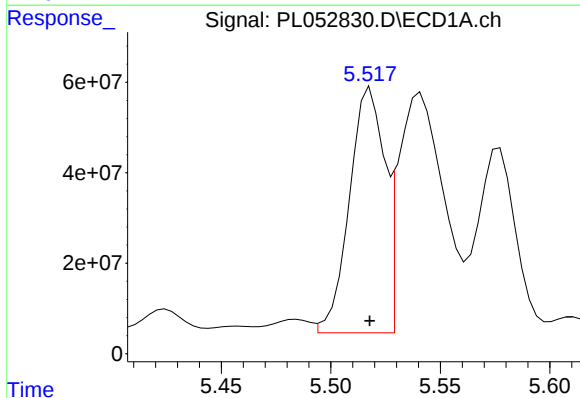


#25 Chlordane-3

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 604079571
Conc: 521.34 ng/ml

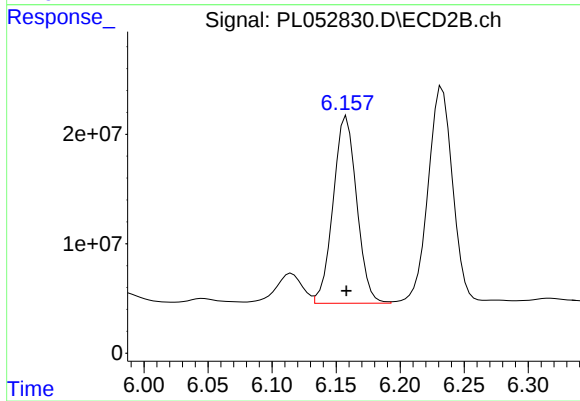

#25 Chlordane-3


R.T.: 6.158 min
Delta R.T.: 0.000 min
Response: 218498394
Conc: 501.71 ng/ml

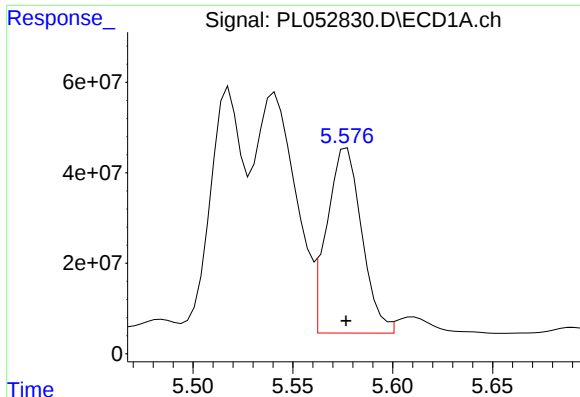

#26 Chlordane-4


R.T.: 5.577 min
Delta R.T.: 0.000 min
Response: 498503022
Conc: 522.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092919CHLOR

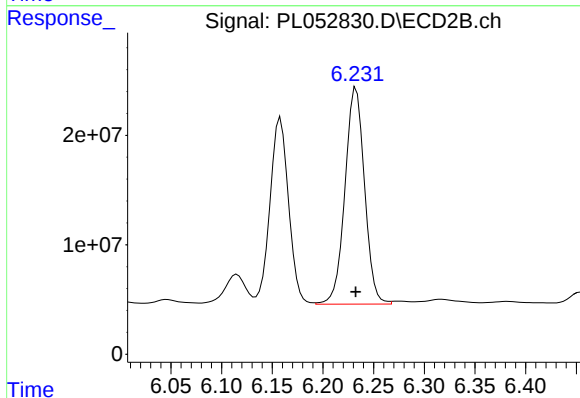


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 265522237
Conc: 500.04 ng/ml

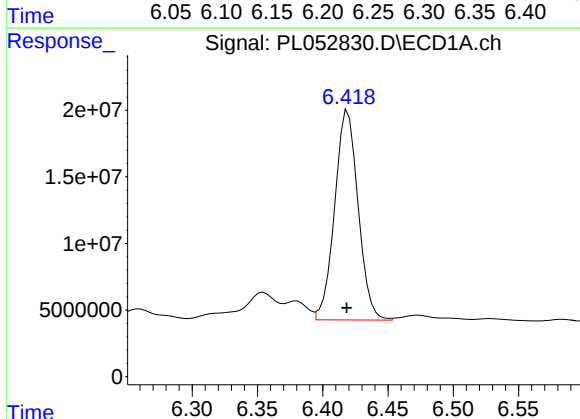


#27 Chlordane-5

R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 196792720
Conc: 498.92 ng/ml

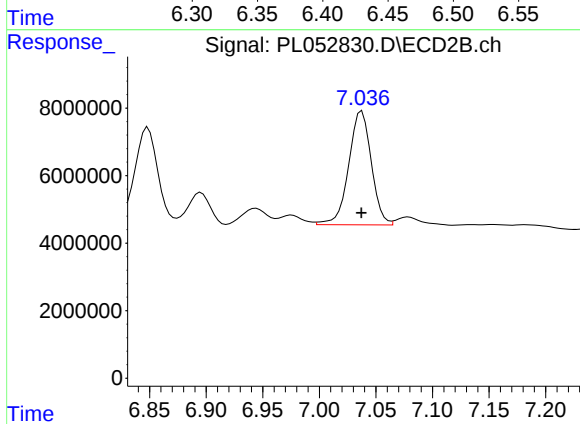

#27 Chlordane-5


R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 46970645
Conc: 532.49 ng/ml

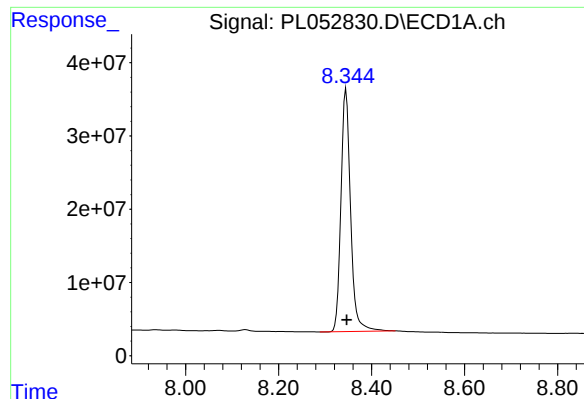

#28 Decachlorobiphenyl

R.T.: 8.345 min
Delta R.T.: -0.002 min
Response: 477414308
Conc: 47.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092919CHLOR

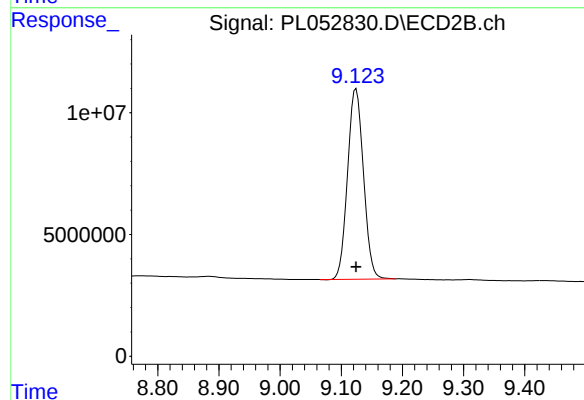

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: 0.000 min
Response: 141485715
Conc: 49.25 ng/ml