

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092919\
 Data File : PL052819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 23:39
 Operator : SG\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 04:48:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 04:45:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	4.047	1208.9E6	262.1E6	99.926	101.457
28)	SA Decachlor...	8.345	9.124	923.3E6	265.9E6	97.274	96.004
Target Compounds							
23)	Chlordane-1	4.436	5.045	358.2E6	100.2E6	1031.957	1018.028
24)	Chlordane-2	4.942	5.512	387.2E6	111.0E6	982.303	1056.172
25)	Chlordane-3	5.519	6.158	1229.9E6	443.5E6	1038.601	1046.529
26)	Chlordane-4	5.577	6.233	1014.6E6	529.6E6	1020.946	1043.980
27)	Chlordane-5	6.419	7.037	408.6E6	85673154	1043.910	1010.568



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092919\
Data File : PL052819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 23:39
Operator : SG\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 04:48:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 04:45:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

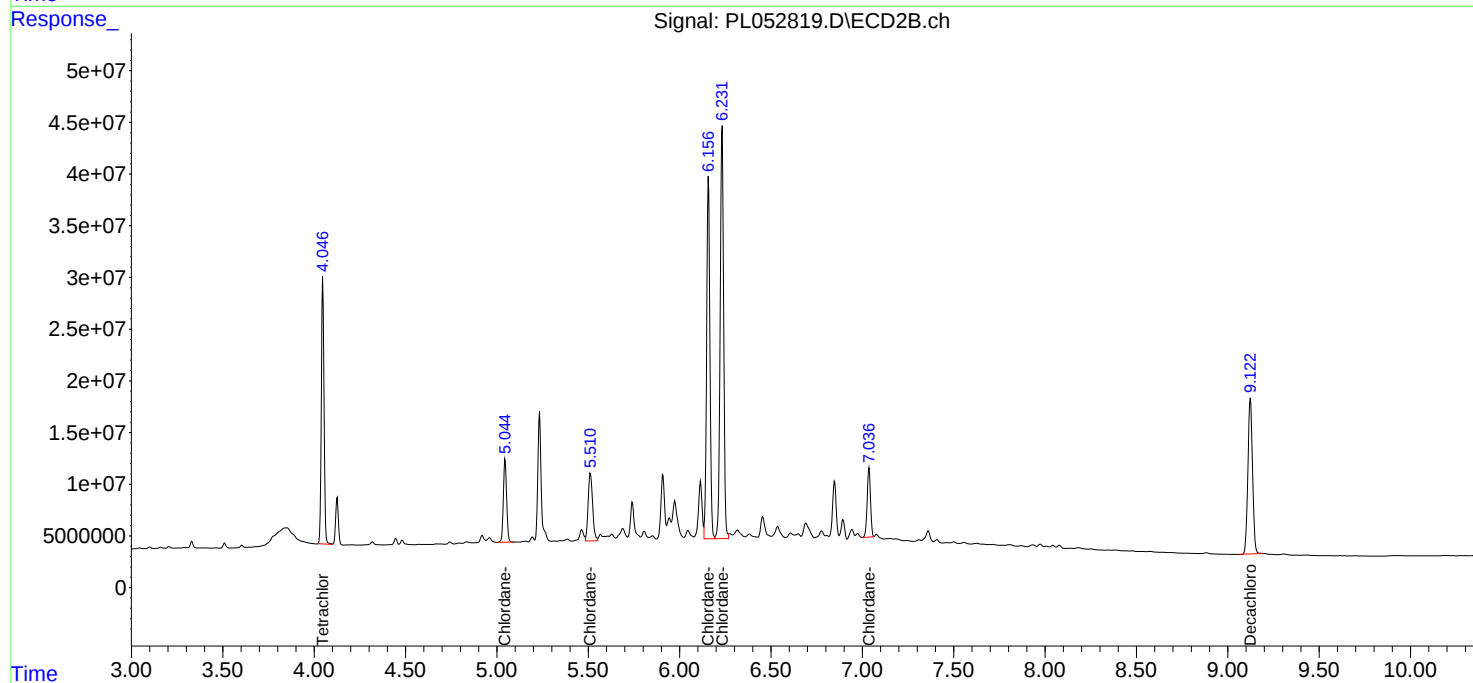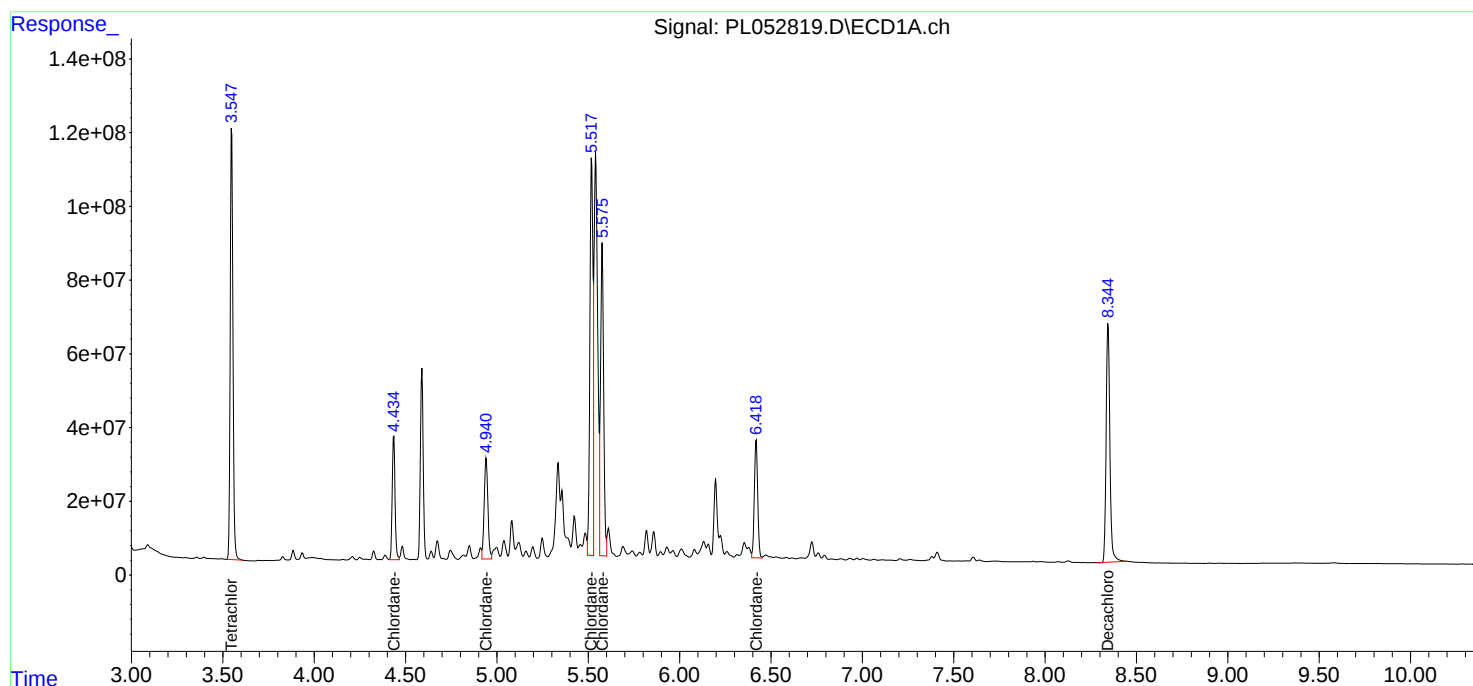


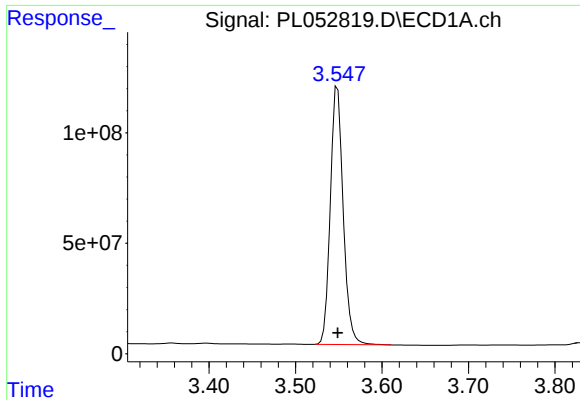

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 1208874340
Conc: 99.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

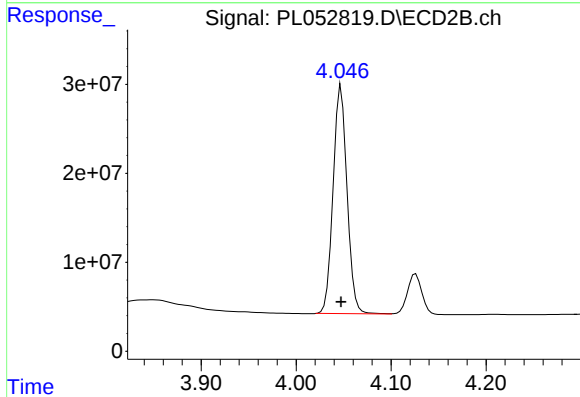


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 262064443
Conc: 101.46 ng/ml

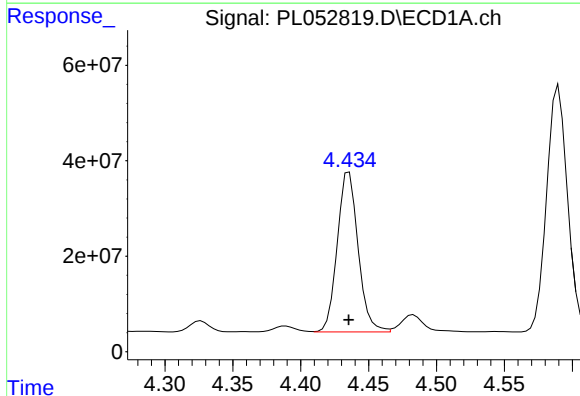


#23 Chlordane-1

R.T.: 4.436 min
Delta R.T.: 0.000 min
Response: 358236827
Conc: 1031.96 ng/ml

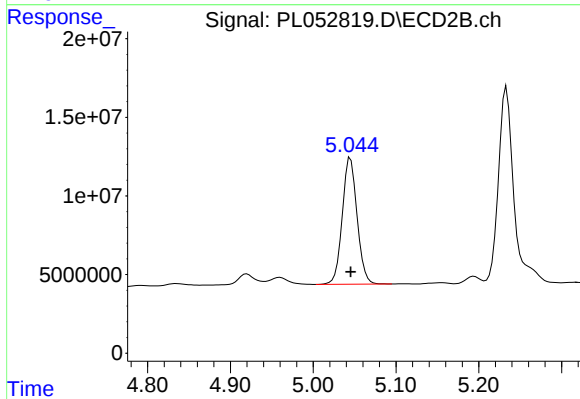

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 100197619
Conc: 1018.03 ng/ml

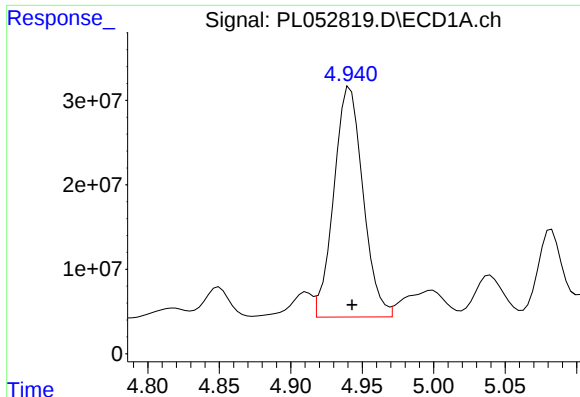

#24 Chlordane-2


R.T.: 4.942 min
Delta R.T.: -0.001 min
Response: 387214616
Conc: 982.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

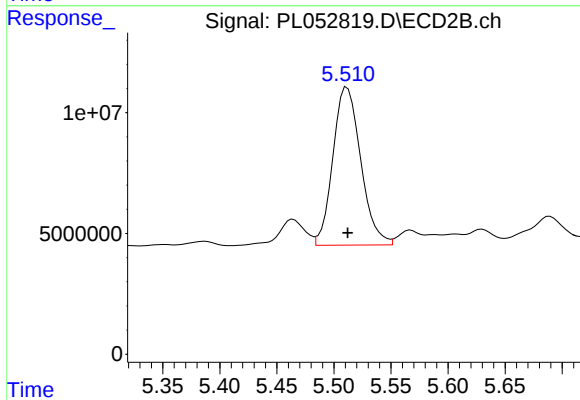


#24 Chlordane-2

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 110958021
Conc: 1056.17 ng/ml

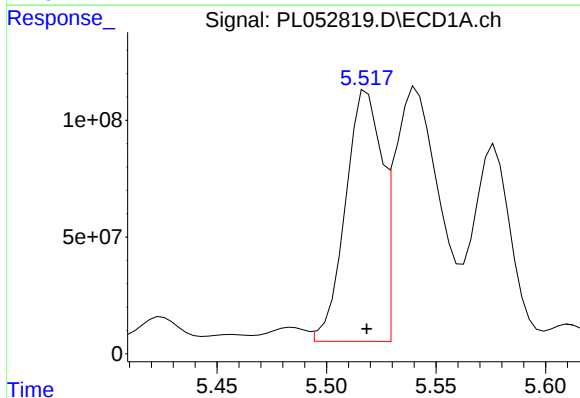


#25 Chlordane-3

R.T.: 5.519 min
Delta R.T.: 0.000 min
Response: 1229908116
Conc: 1038.60 ng/ml

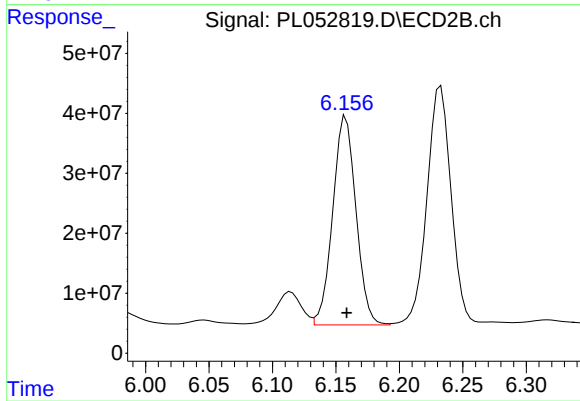

#25 Chlordane-3


R.T.: 6.158 min
Delta R.T.: 0.000 min
Response: 443452260
Conc: 1046.53 ng/ml

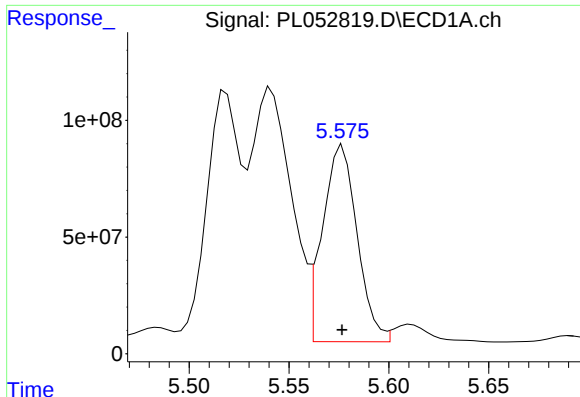

#26 Chlordane-4


R.T.: 5.577 min
Delta R.T.: 0.000 min
Response: 1014646470
Conc: 1020.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

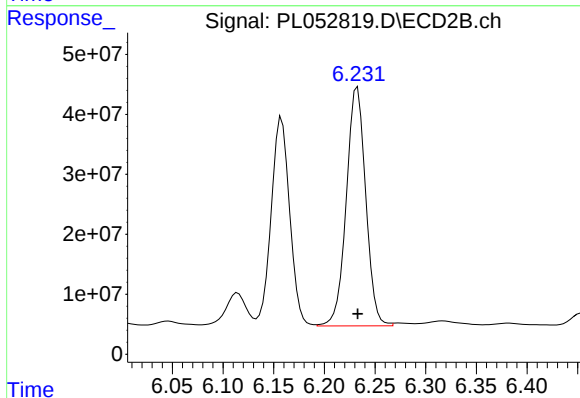


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 529609603
Conc: 1043.98 ng/ml

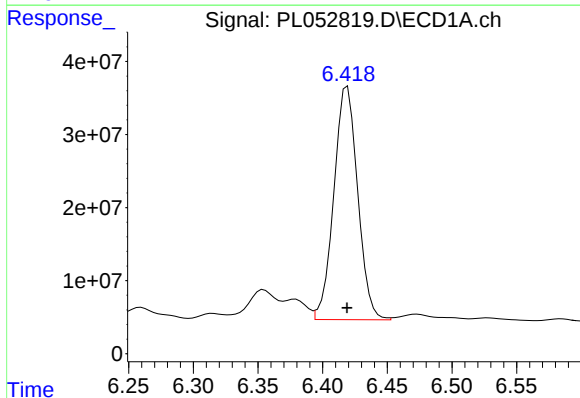


#27 Chlordane-5

R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 408584702
Conc: 1043.91 ng/ml

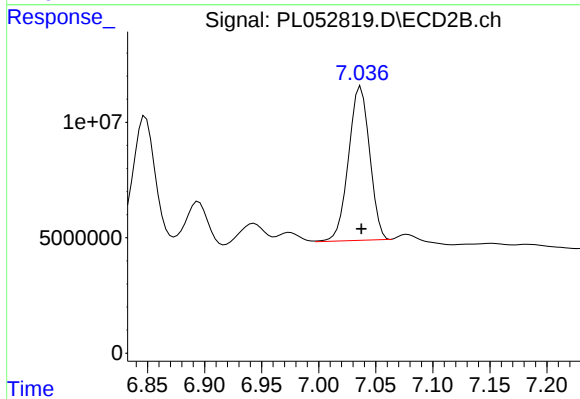

#27 Chlordane-5


R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 85673154
Conc: 1010.57 ng/ml

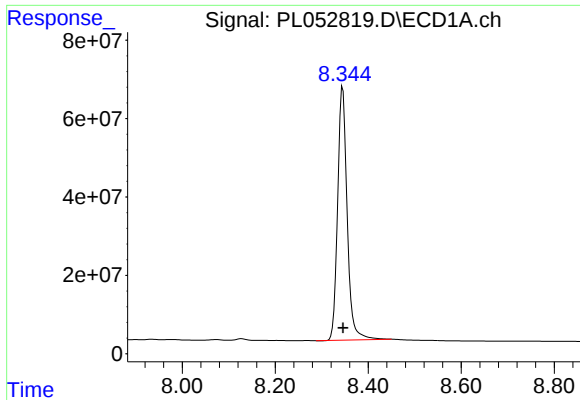

#28 Decachlorobiphenyl

R.T.: 8.345 min
Delta R.T.: 0.000 min
Response: 923272007
Conc: 97.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

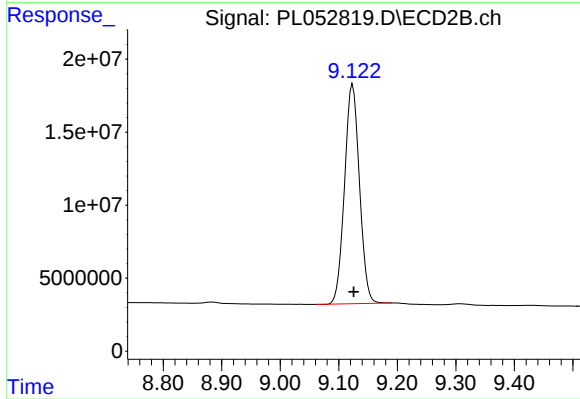

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: -0.002 min
Response: 265920289
Conc: 96.00 ng/ml