

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092920\
 Data File : PL061852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2020 14:57
 Operator : DD\AJ
 Sample : L4158-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 01:10:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.007	31172164	44032150	18.272	16.139
28)	SA Decachlor...	8.211	9.097	32932424	45715197	20.244	20.767
Target Compounds							
2)	A alpha-BHC	0.000	4.368f	0	6744652	N.D.	1.689 #
3)	MA gamma-BHC...	0.000	4.682	0	3734965	N.D.	1.009 #
4)	MA Heptachlor	0.000	5.197	0	7719144	N.D.	2.229 #
17)	MA 4,4'-DDT	6.404f	0.000	5366968	0	4.254	N.D. #
24)	Chlordane-2	0.000	5.462	0	2578098	N.D.	25.053 #
27)	Chlordane-5	0.000	7.025f	0	5656205	N.D.	77.823 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092920\
Data File : PL061852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 14:57
Operator : DD\AJ
Sample : L4158-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 01:10:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

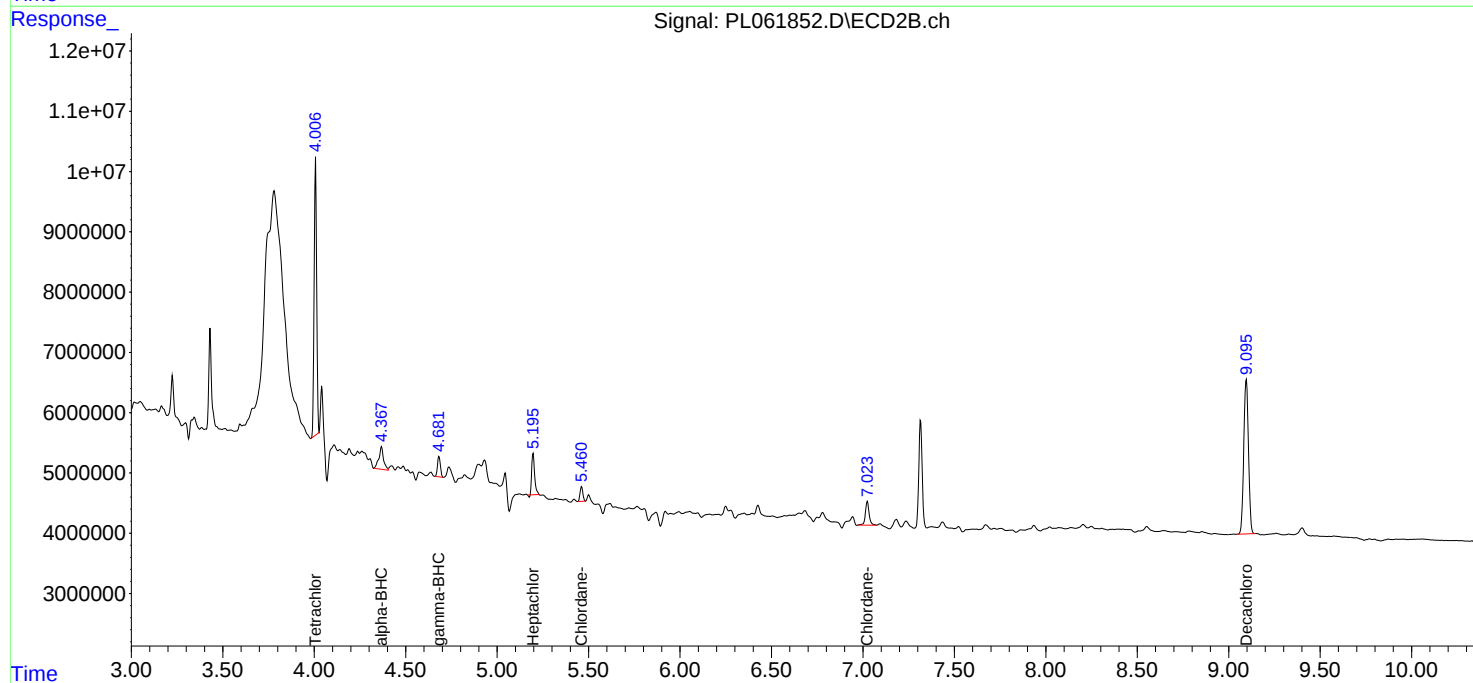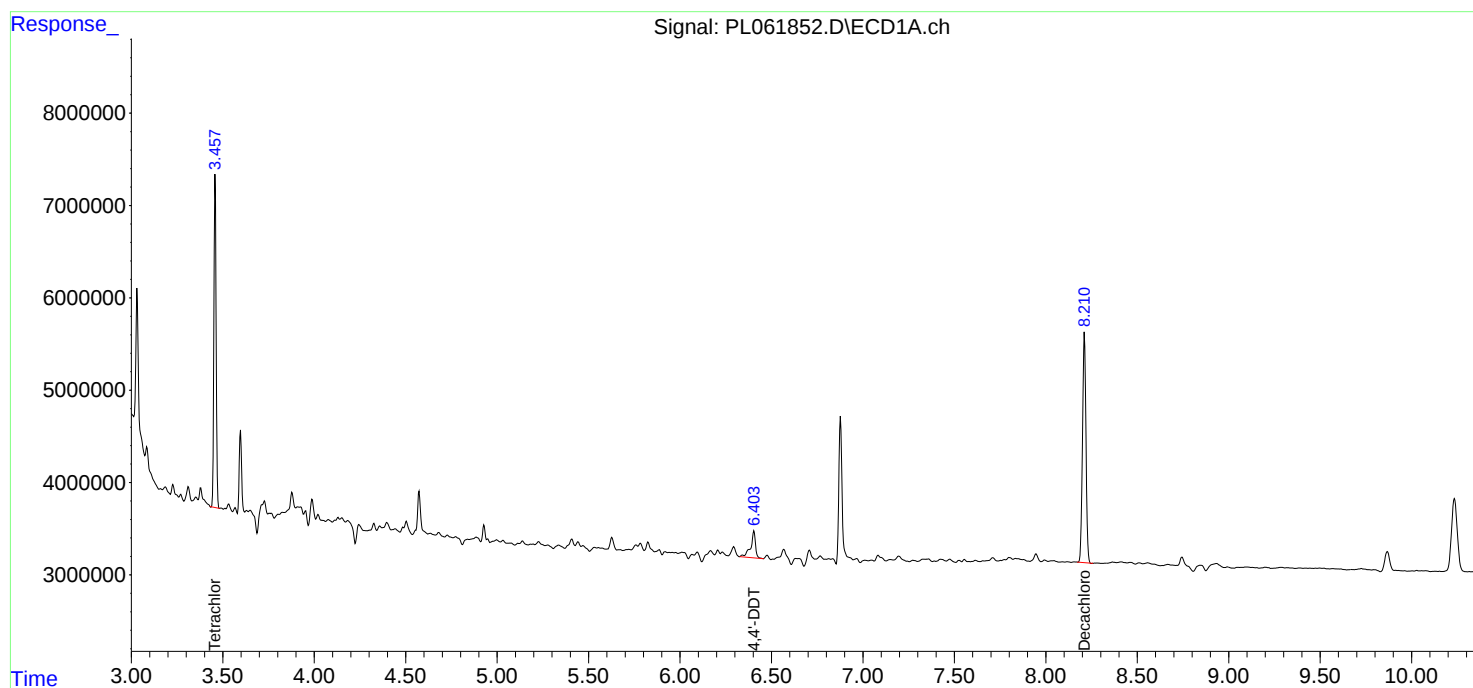


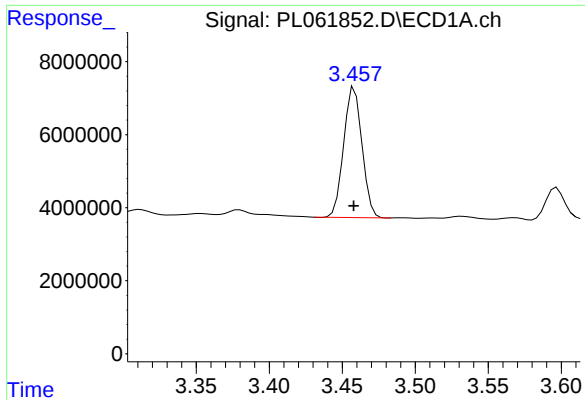

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 31172164
Conc: 18.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

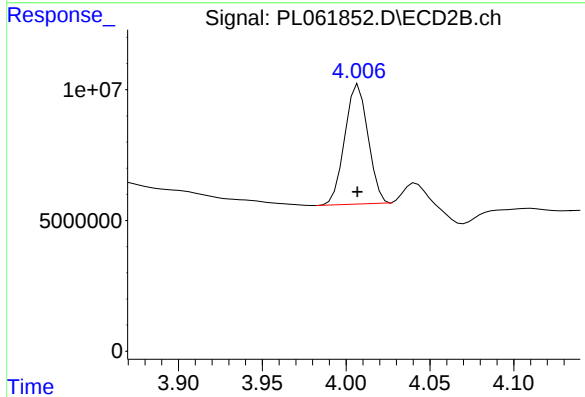


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 44032150
Conc: 16.14 ng/ml

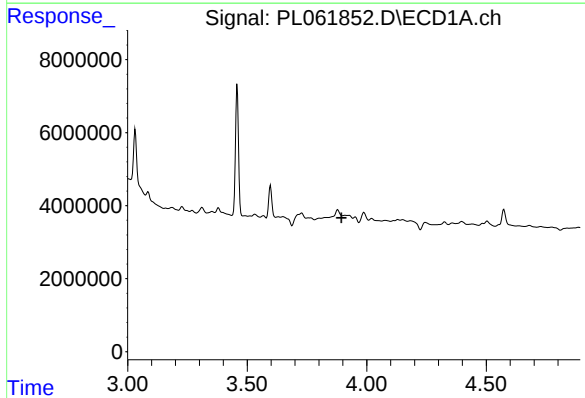


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.894 min
Response: 0
Conc: N.D.

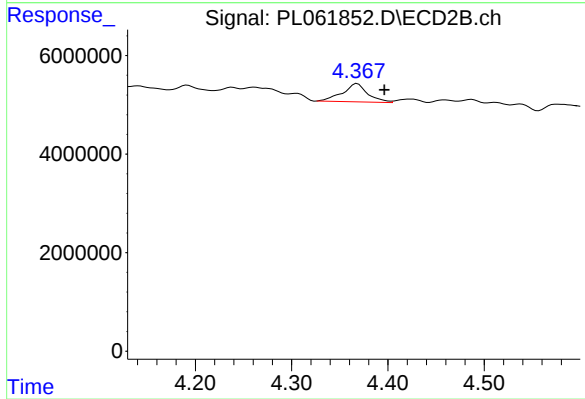

#2 alpha-BHC


R.T.: 4.368 min
Delta R.T.: -0.028 min
Response: 6744652
Conc: 1.69 ng/ml

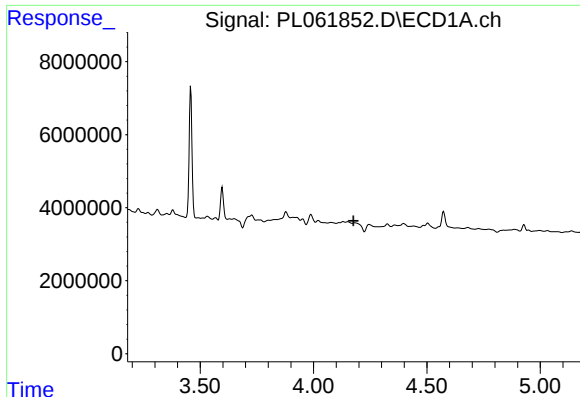

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

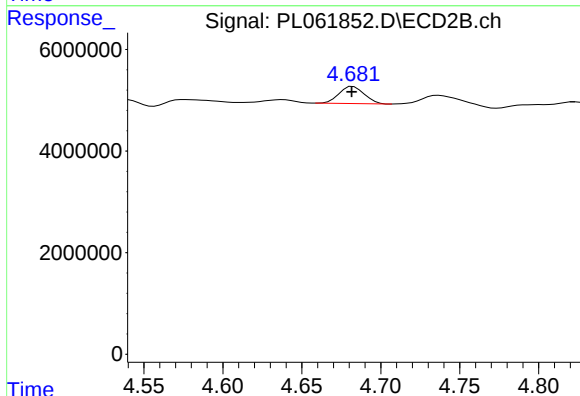


#3 gamma-BHC (Lindane)

R.T.: 4.682 min
Delta R.T.: 0.000 min
Response: 3734965
Conc: 1.01 ng/ml

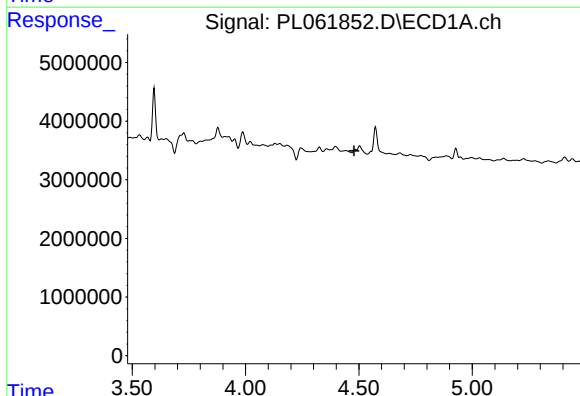


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

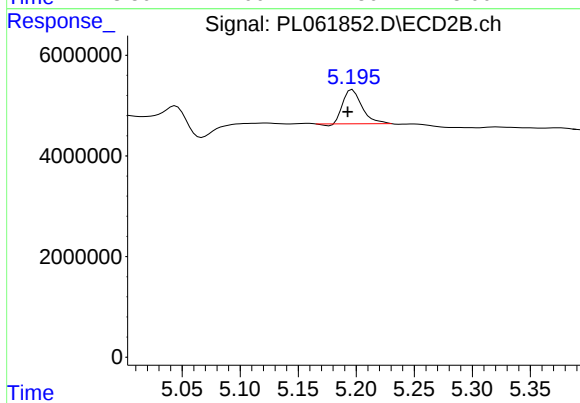

#4 Heptachlor


R.T.: 5.197 min
Delta R.T.: 0.004 min
Response: 7719144
Conc: 2.23 ng/ml

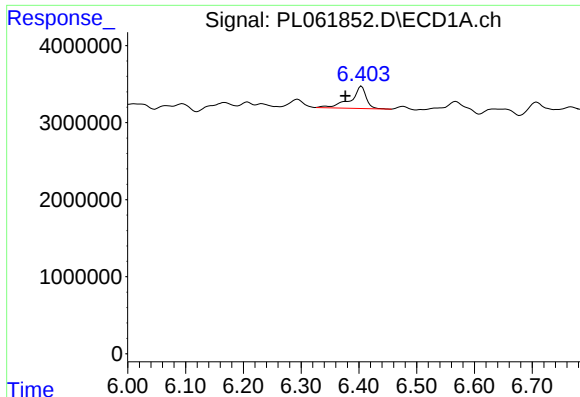

#17 4,4'-DDT


R.T.: 6.404 min
Delta R.T.: 0.028 min
Response: 5366968
Conc: 4.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

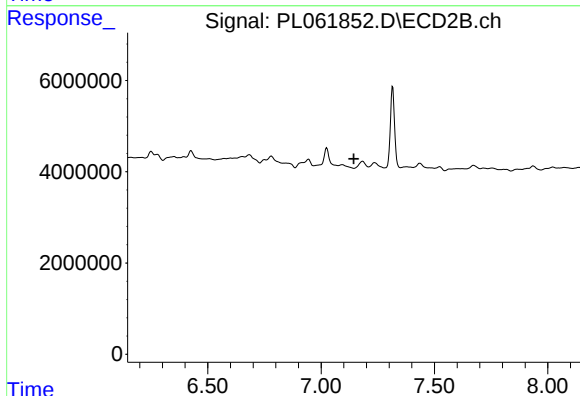


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

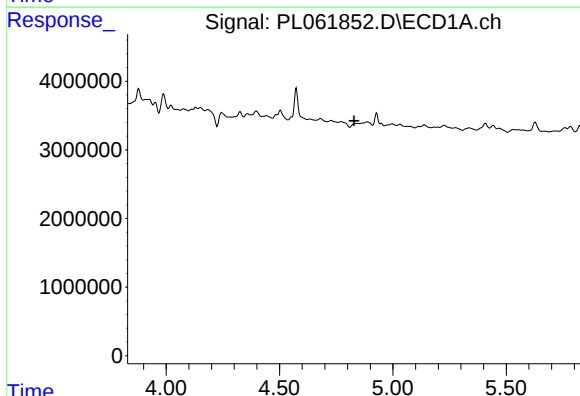


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.829 min
Response: 0
Conc: N.D.

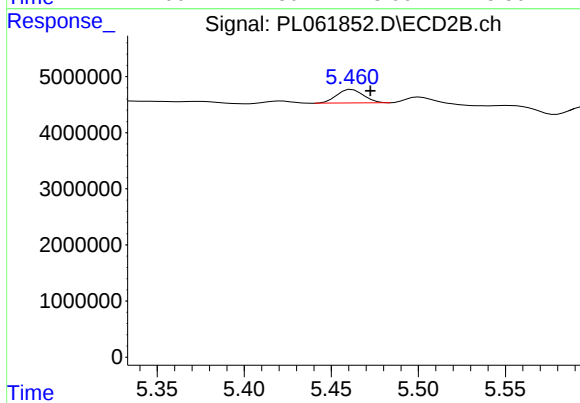

#24 Chlordane-2


R.T.: 5.462 min
Delta R.T.: -0.011 min
Response: 2578098
Conc: 25.05 ng/ml

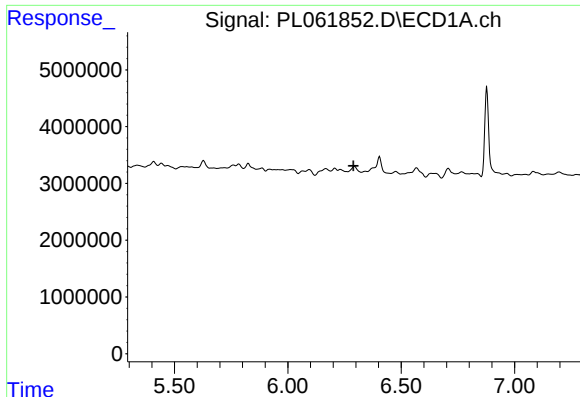

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

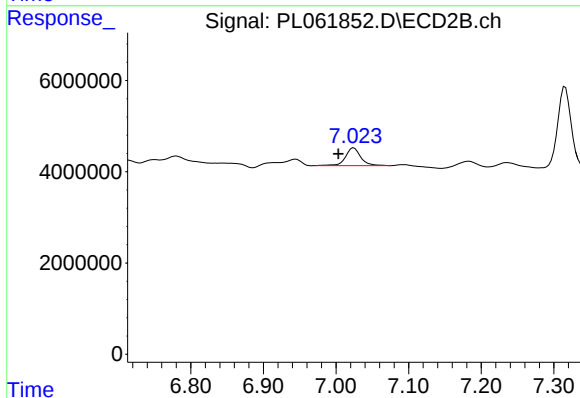


#27 Chlordane-5

R.T.: 7.025 min
Delta R.T.: 0.001 min
Response: 5656205
Conc: 77.82 ng/ml

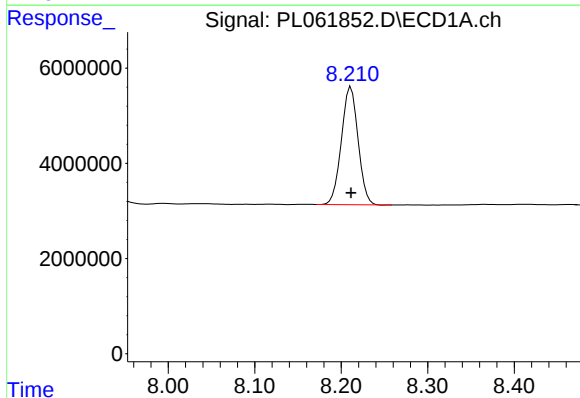

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 32932424
Conc: 20.24 ng/ml

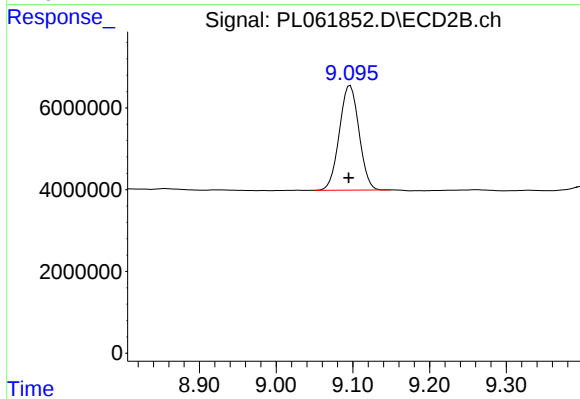

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.002 min
Response: 45715197
Conc: 20.77 ng/ml