

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092920\
 Data File : PL061859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2020 16:37
 Operator : DD\AJ
 Sample : L3869-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 01:12:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	26841182	35231922	15.734	12.914
28)	SA Decachlor...	8.210	9.096	22288734	32425952	13.701	14.730
Target Compounds							
5)	MB Aldrin	0.000	5.473f	0	5105869	N.D.	1.576 #
9)	A Endosulfan I	5.523	0.000	3032947	0	1.872	N.D. #
10)	B gamma-Chl...	5.399	6.123	9338864	7705303	5.377	2.624 #
11)	B alpha-Chl...	0.000	6.196	0	10726546	N.D.	3.571 #
23)	Chlordane-1	4.325	0.000	6278940	0	126.807	N.D. #
24)	Chlordane-2	0.000	5.473	0	5105869	N.D.	49.617 #
25)	Chlordane-3	5.399	6.123	9338864	7705303	59.414	21.028 #
26)	Chlordane-4	0.000	6.196	0	10726546	N.D.	23.894 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092920\
Data File : PL061859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 16:37
Operator : DD\AJ
Sample : L3869-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 01:12:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

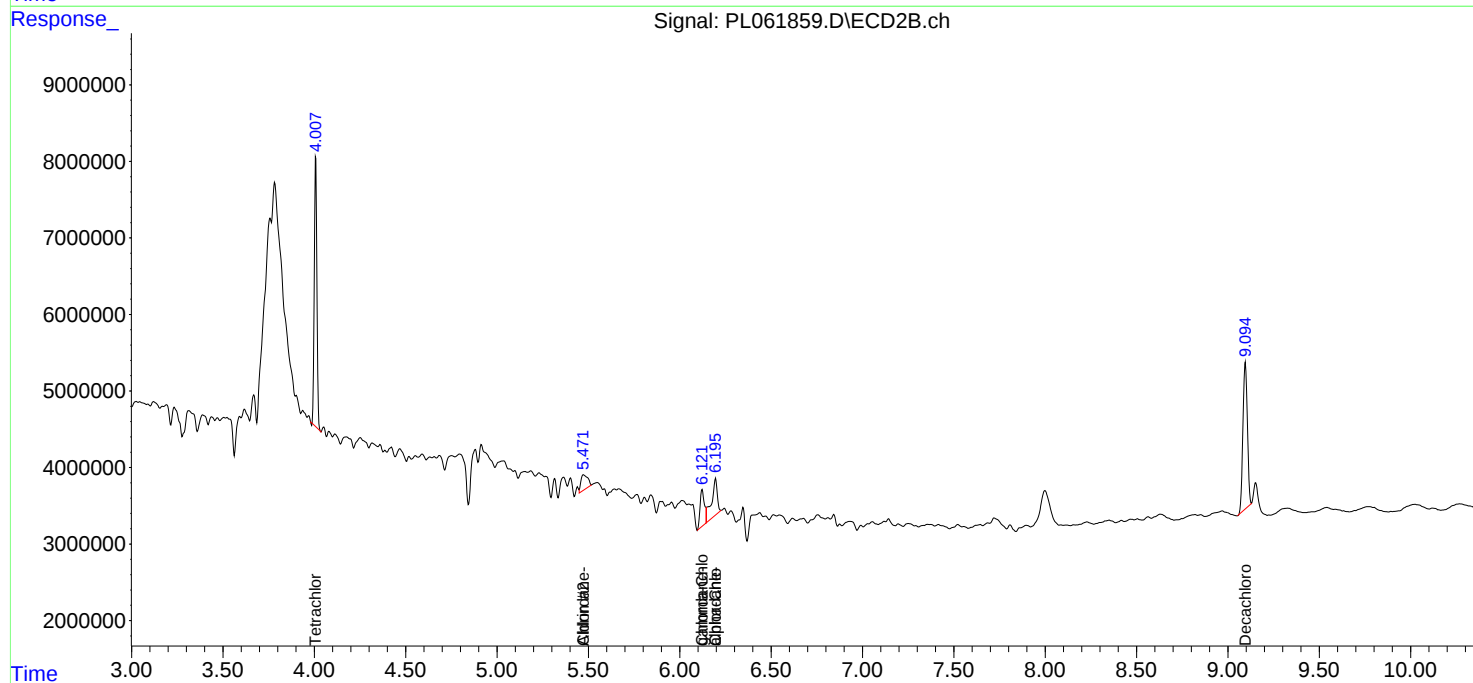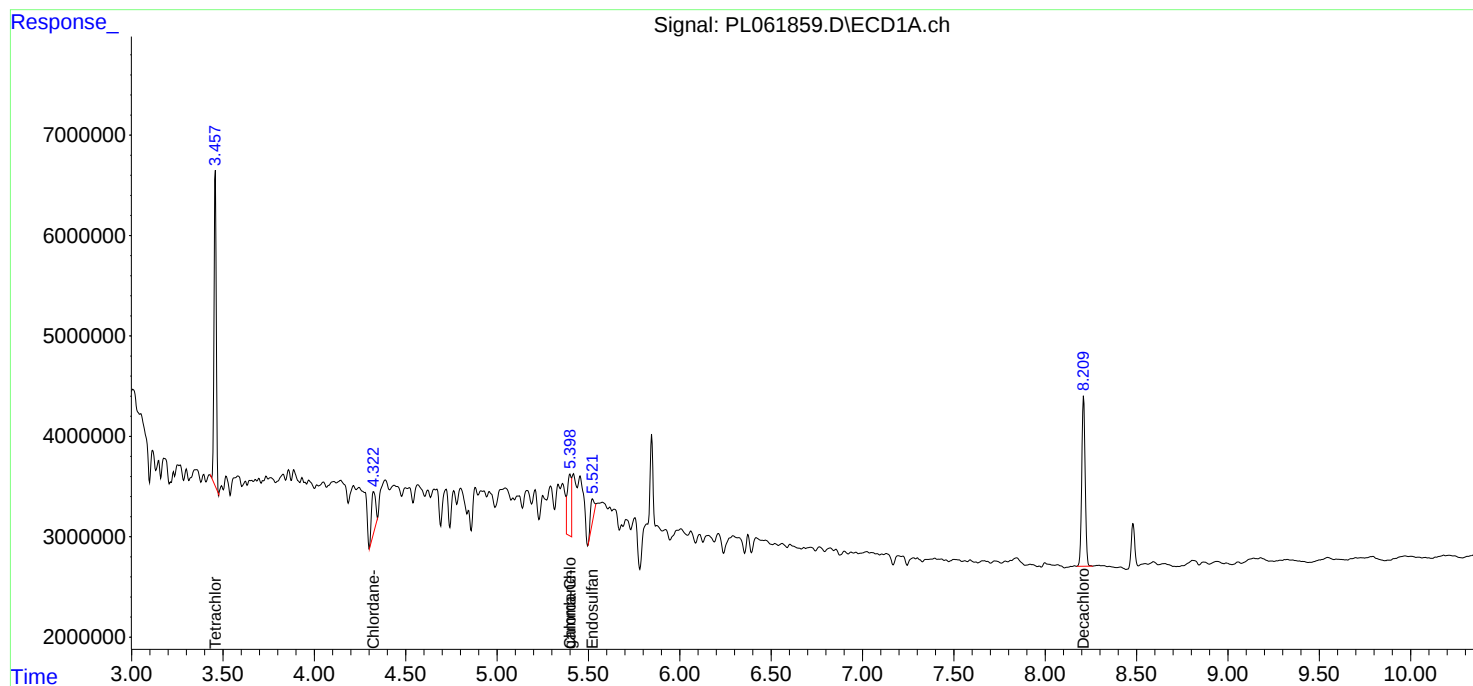


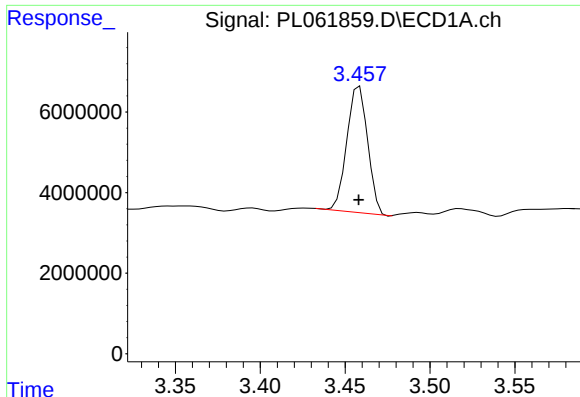

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 26841182
Conc: 15.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

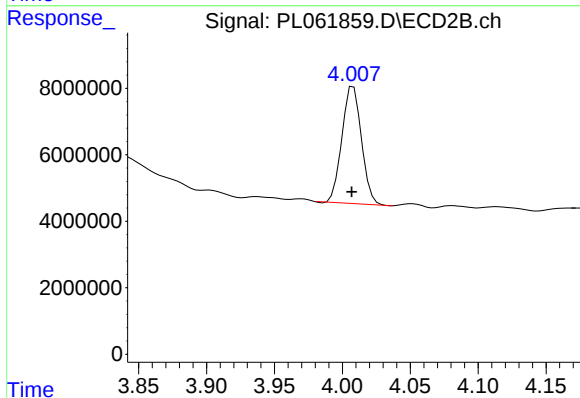


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.001 min
Response: 35231922
Conc: 12.91 ng/ml

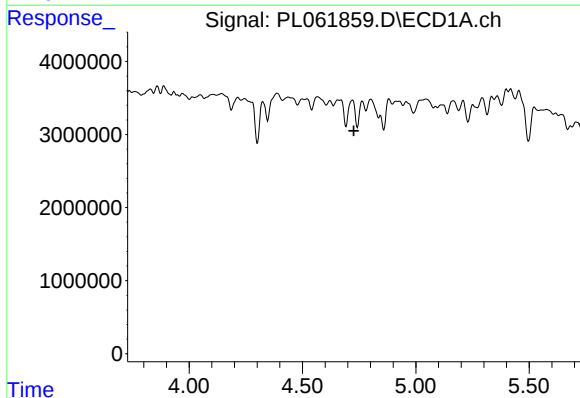


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

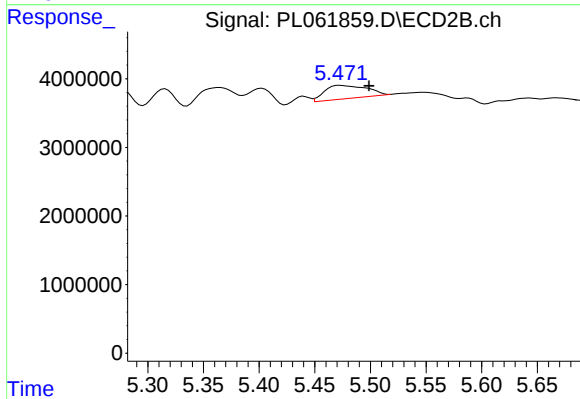

#5 Aldrin


R.T.: 5.473 min
Delta R.T.: -0.026 min
Response: 5105869
Conc: 1.58 ng/ml

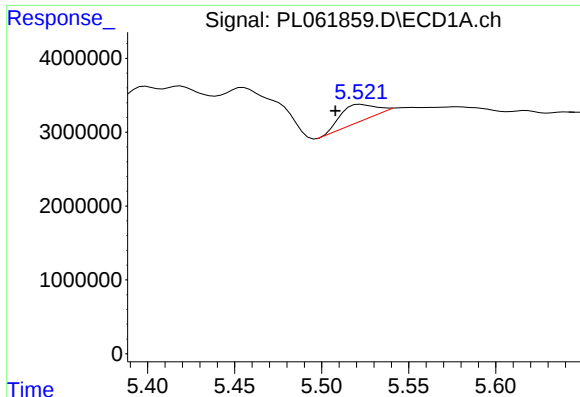

#9 Endosulfan I


R.T.: 5.523 min
Delta R.T.: 0.015 min
Response: 3032947
Conc: 1.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

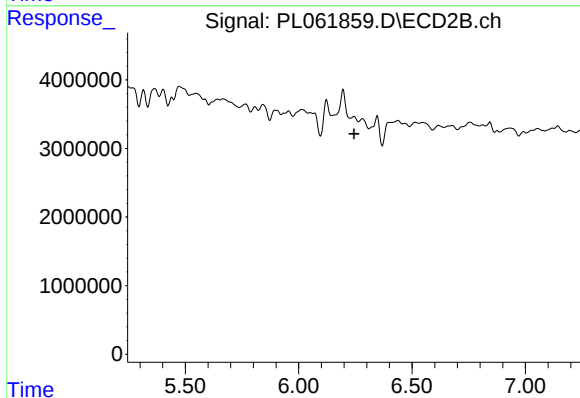


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

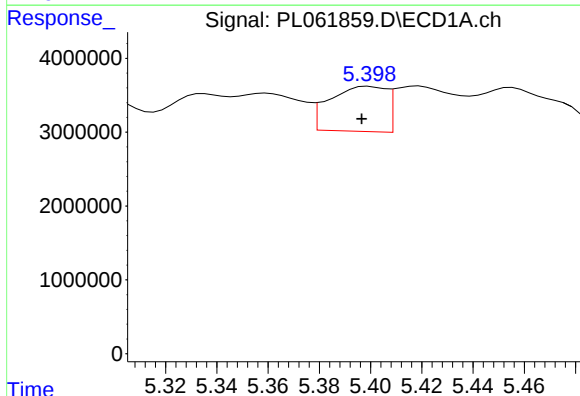


#10 gamma-Chlordane

R.T.: 5.399 min
Delta R.T.: 0.003 min
Response: 9338864
Conc: 5.38 ng/ml

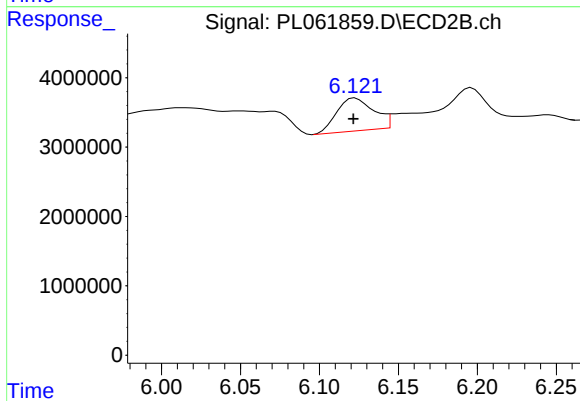

#10 gamma-Chlordane


R.T.: 6.123 min
Delta R.T.: 0.001 min
Response: 7705303
Conc: 2.62 ng/ml

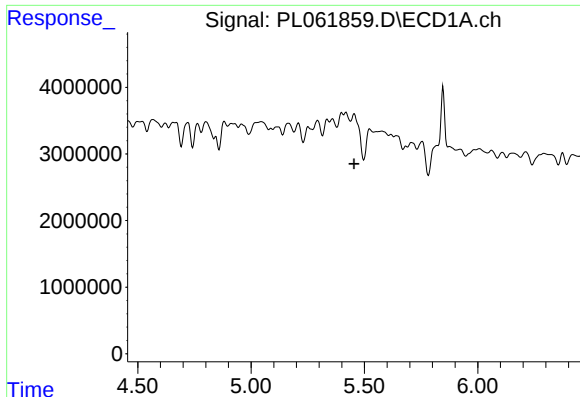

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

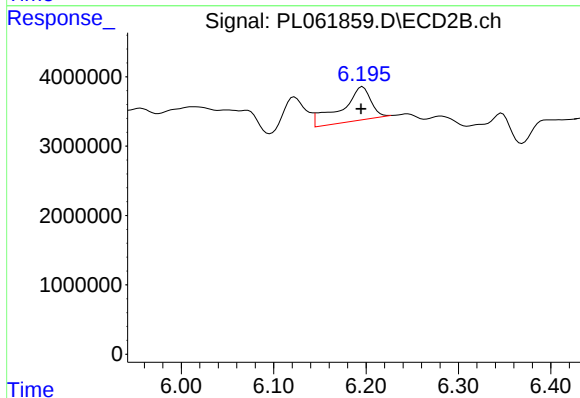


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: 0.002 min
Response: 10726546
Conc: 3.57 ng/ml

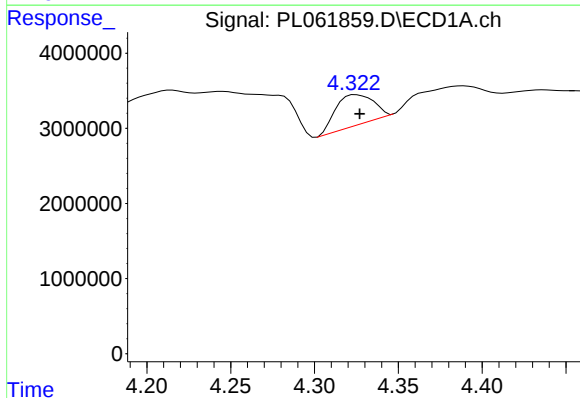


#23 Chlordane-1

R.T.: 4.325 min
Delta R.T.: -0.002 min
Response: 6278940
Conc: 126.81 ng/ml

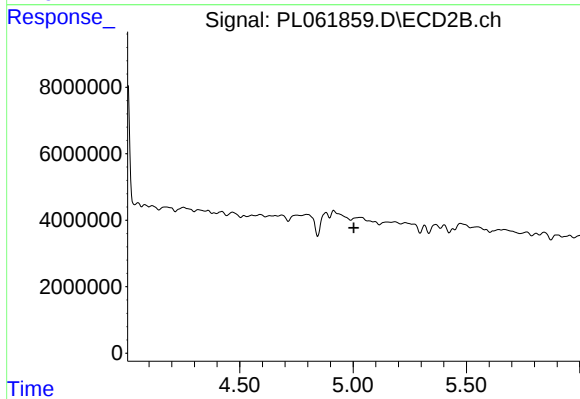

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.004 min
Response: 0
Conc: N.D.

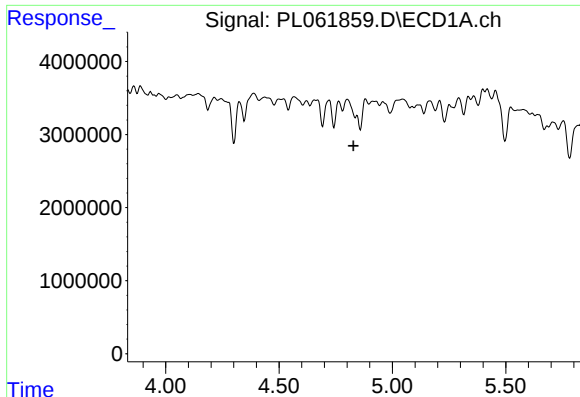

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.829 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

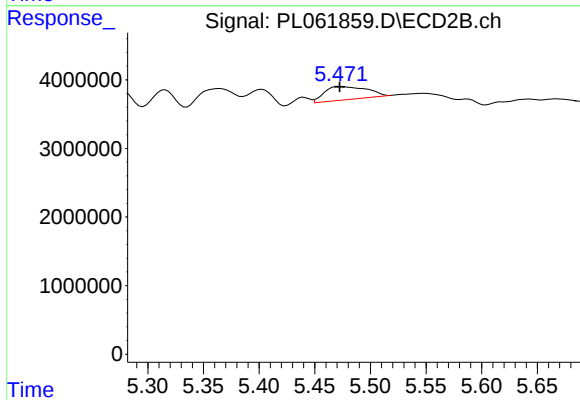


#24 Chlordane-2

R.T.: 5.473 min
Delta R.T.: 0.000 min
Response: 5105869
Conc: 49.62 ng/ml

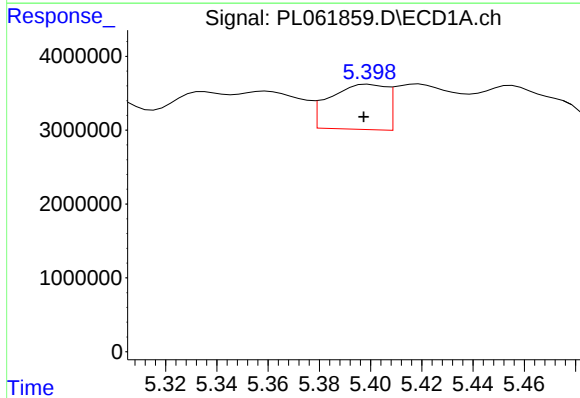


#25 Chlordane-3

R.T.: 5.399 min
Delta R.T.: 0.002 min
Response: 9338864
Conc: 59.41 ng/ml

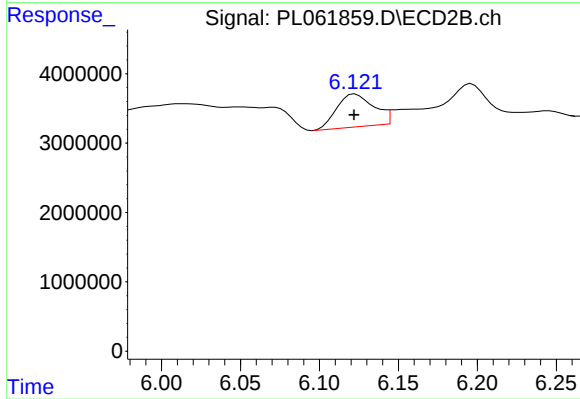

#25 Chlordane-3


R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 7705303
Conc: 21.03 ng/ml

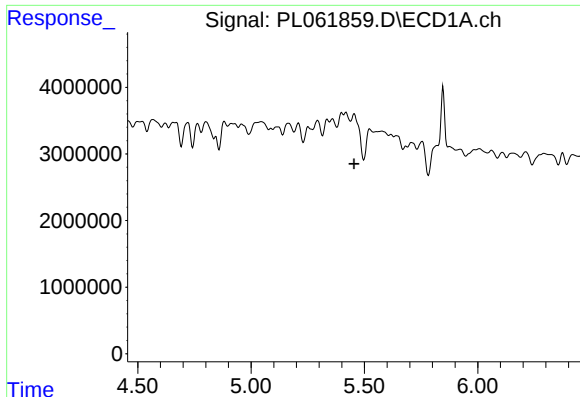

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

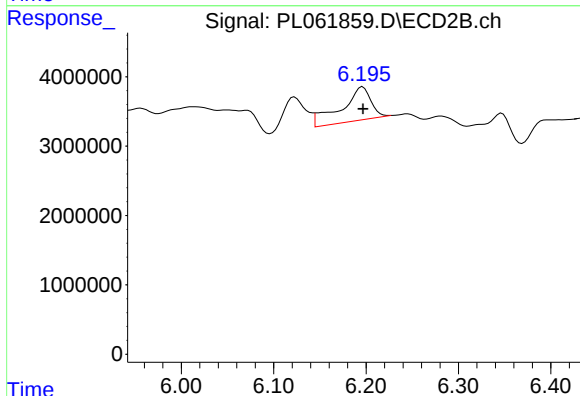


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 10726546
Conc: 23.89 ng/ml

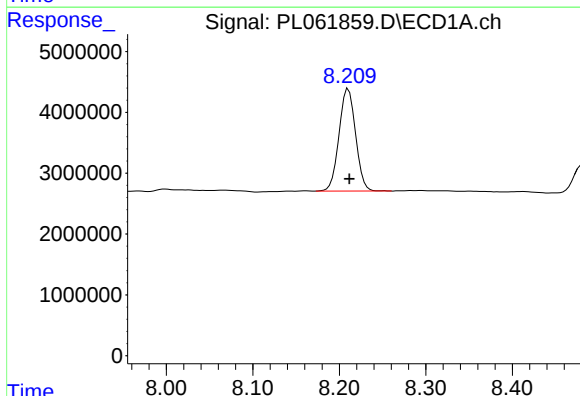

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 22288734
Conc: 13.70 ng/ml

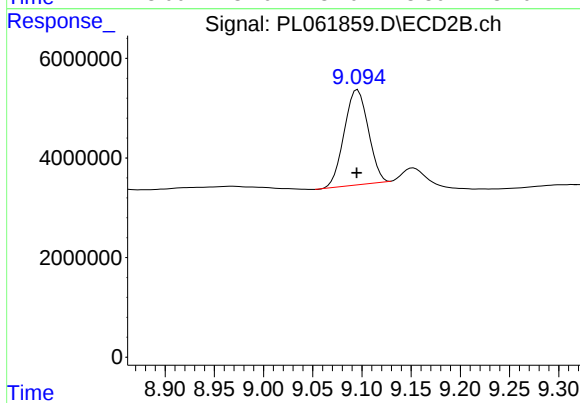

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.000 min
Response: 32425952
Conc: 14.73 ng/ml