

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092920\
 Data File : PL061860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2020 16:51
 Operator : DD\AJ
 Sample : L4173-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 01:12:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.008	19457483	27776078	11.406	10.181
28)	SA Decachlor...	8.211	9.096	11983624	17685799	7.367	8.034
Target Compounds							
10)	B gamma-Chl...	5.386	0.000	8698184	0	5.009	N.D. #
25)	Chlordane-3	5.386	0.000	8698184	0	55.338	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092920\
Data File : PL061860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 16:51
Operator : DD\AJ
Sample : L4173-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 01:12:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

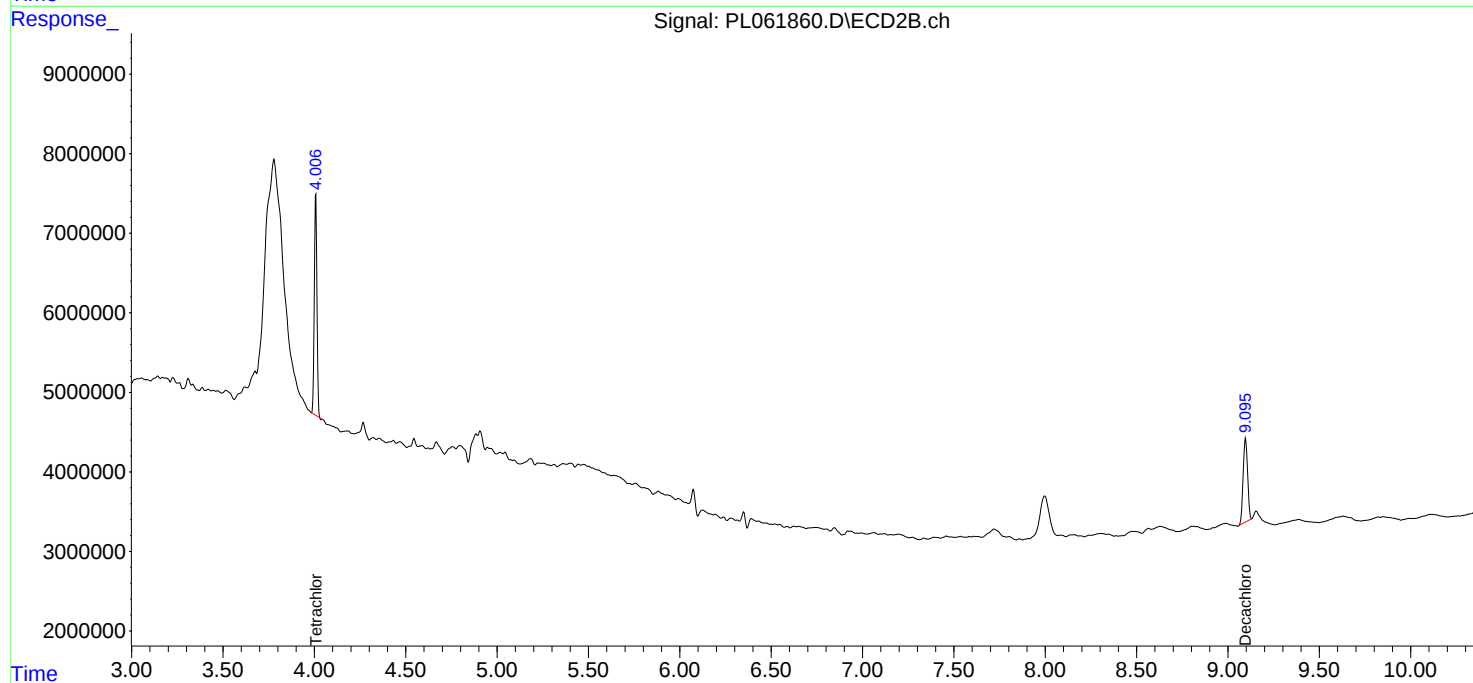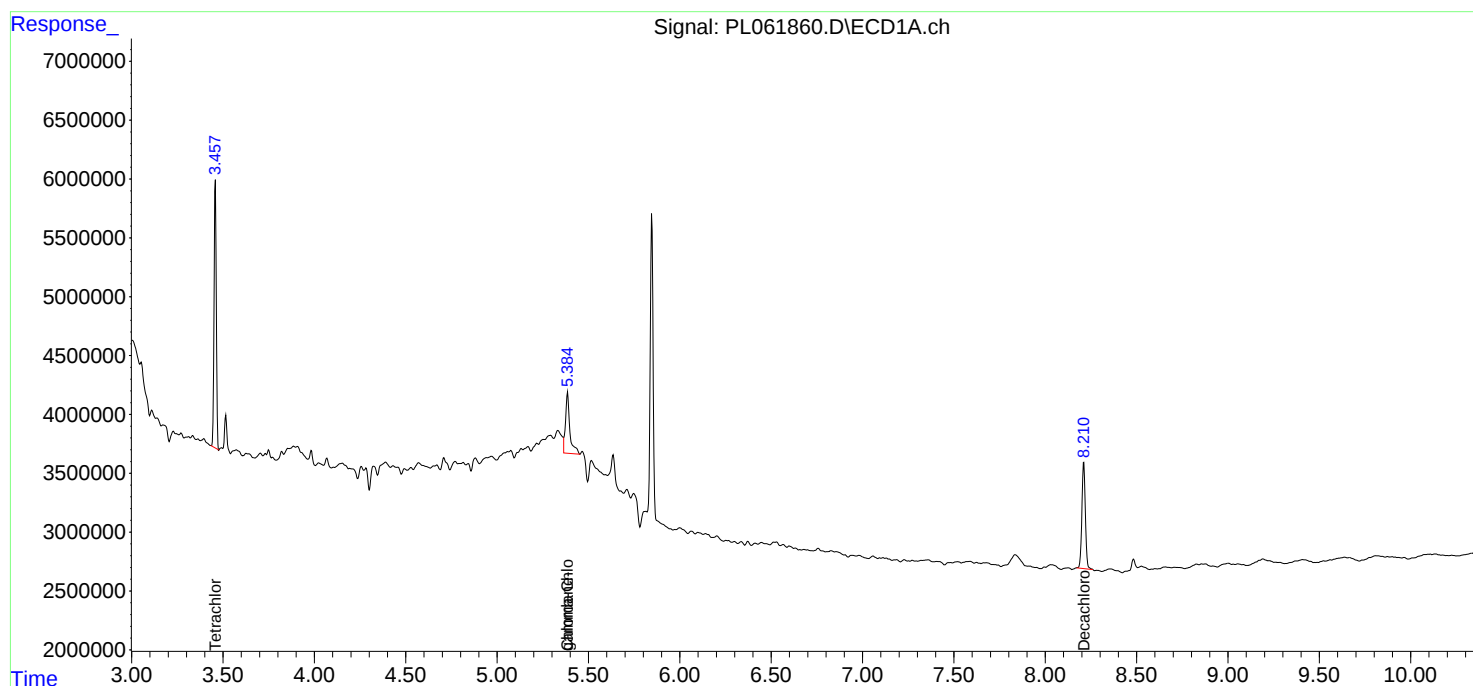


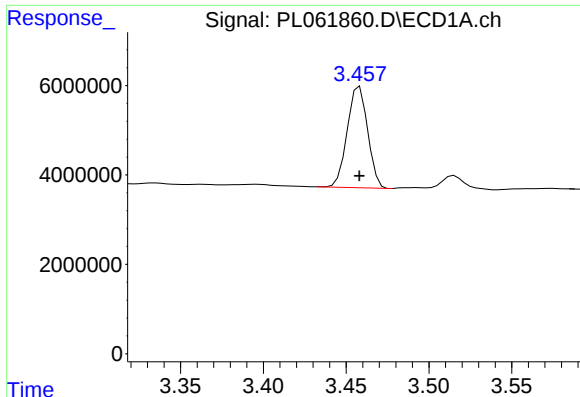

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 19457483
Conc: 11.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

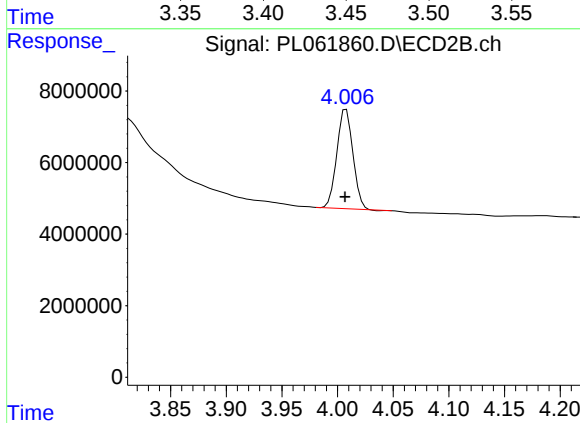


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 27776078
Conc: 10.18 ng/ml

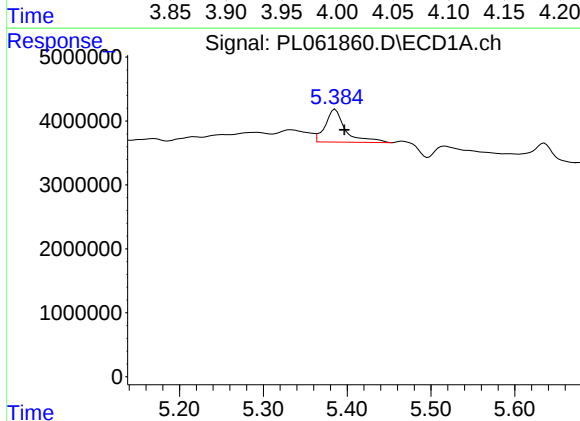


#10 gamma-Chlordane

R.T.: 5.386 min
Delta R.T.: -0.011 min
Response: 8698184
Conc: 5.01 ng/ml

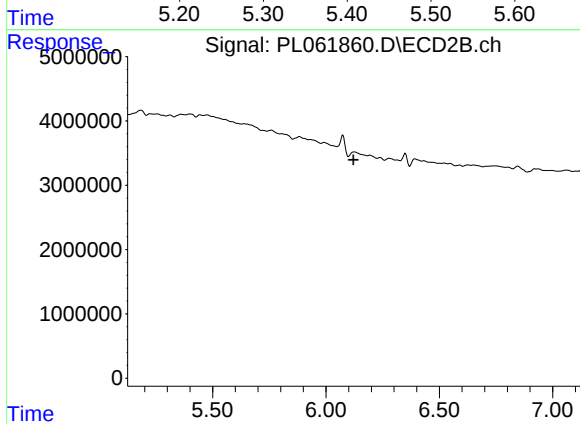

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

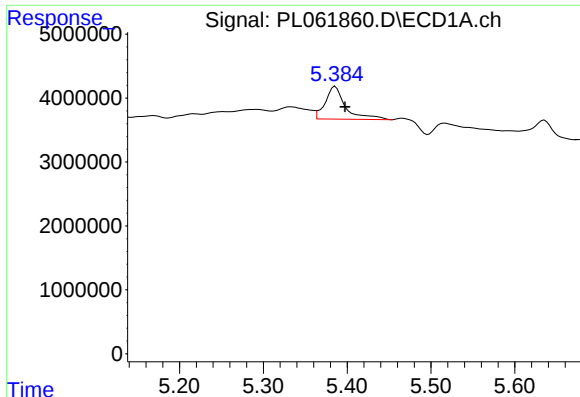

#25 Chlordane-3


R.T.: 5.386 min
Delta R.T.: -0.011 min
Response: 8698184
Conc: 55.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

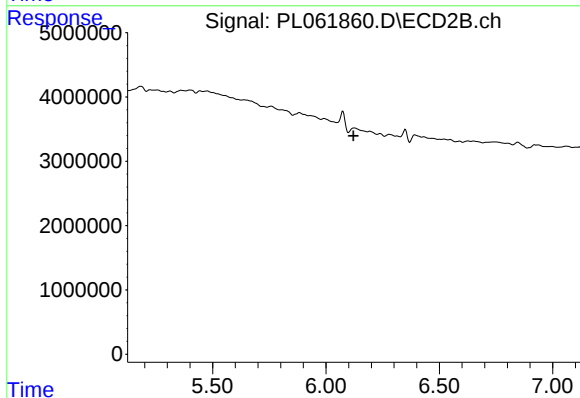


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

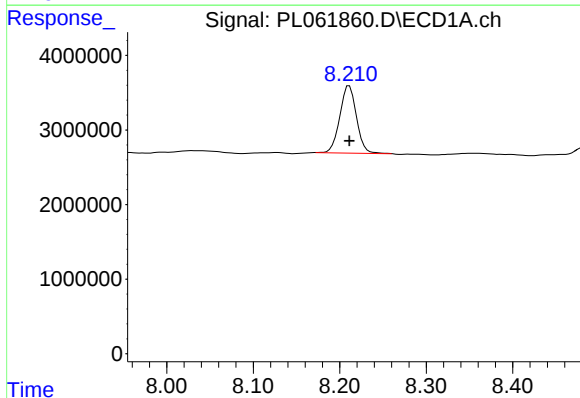

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 11983624
Conc: 7.37 ng/ml

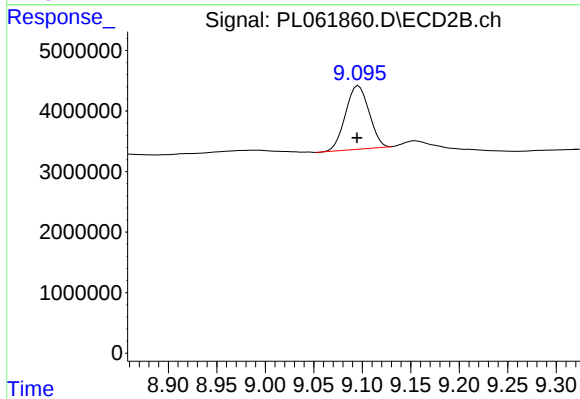

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.001 min
Response: 17685799
Conc: 8.03 ng/ml