

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092920\
 Data File : PL061864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2020 17:48
 Operator : DD\AJ
 Sample : L4173-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3-(0-6FT)

Manual Integrations
 APPROVED

Ankita
 9/30/2020 4:00:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 01:13:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.477f	4.008	24898460	38181513	14.595m	13.995
28)	SA Decachlor...	8.230f	9.096	20422433	28278499	12.554	12.846

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092920\
Data File : PL061864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 17:48
Operator : DD\AJ
Sample : L4173-10
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-3-(0-6FT)


Manual Integrations
APPROVED

Ankita
9/30/2020 4:00:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 01:13:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

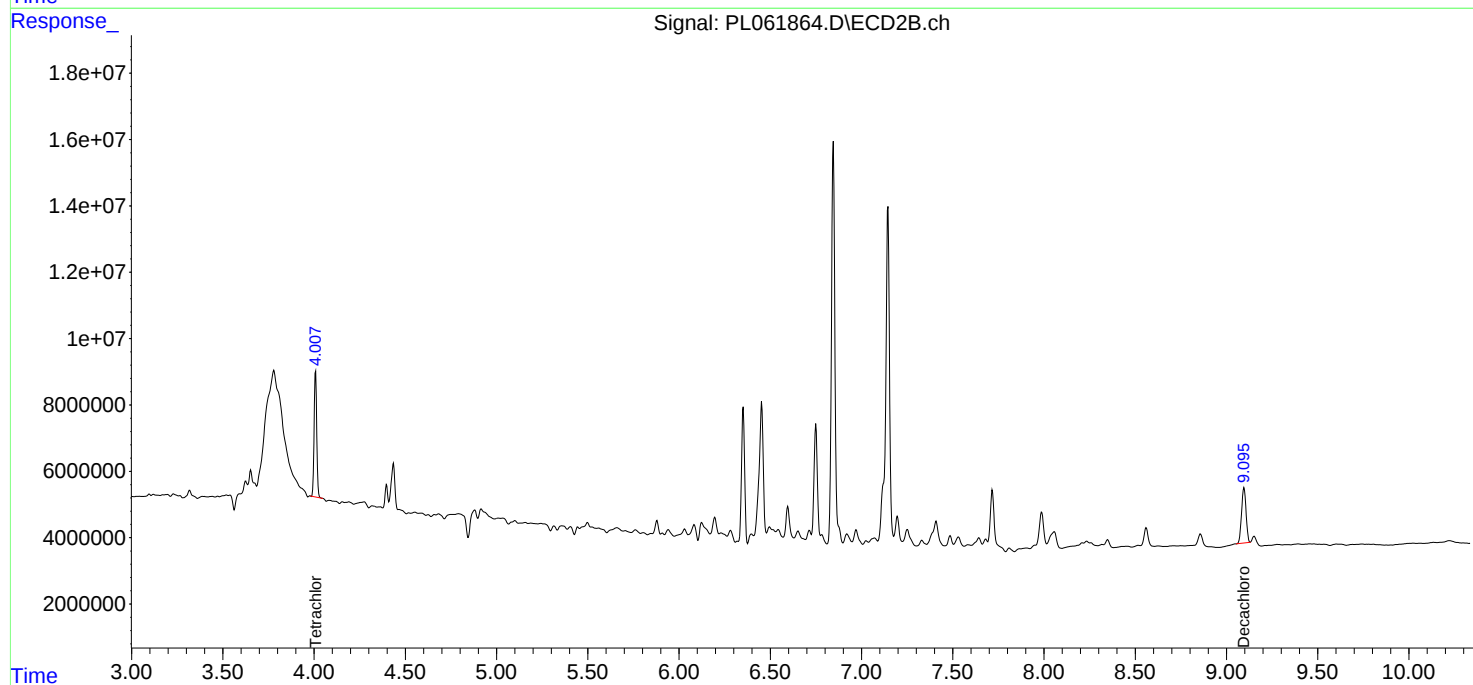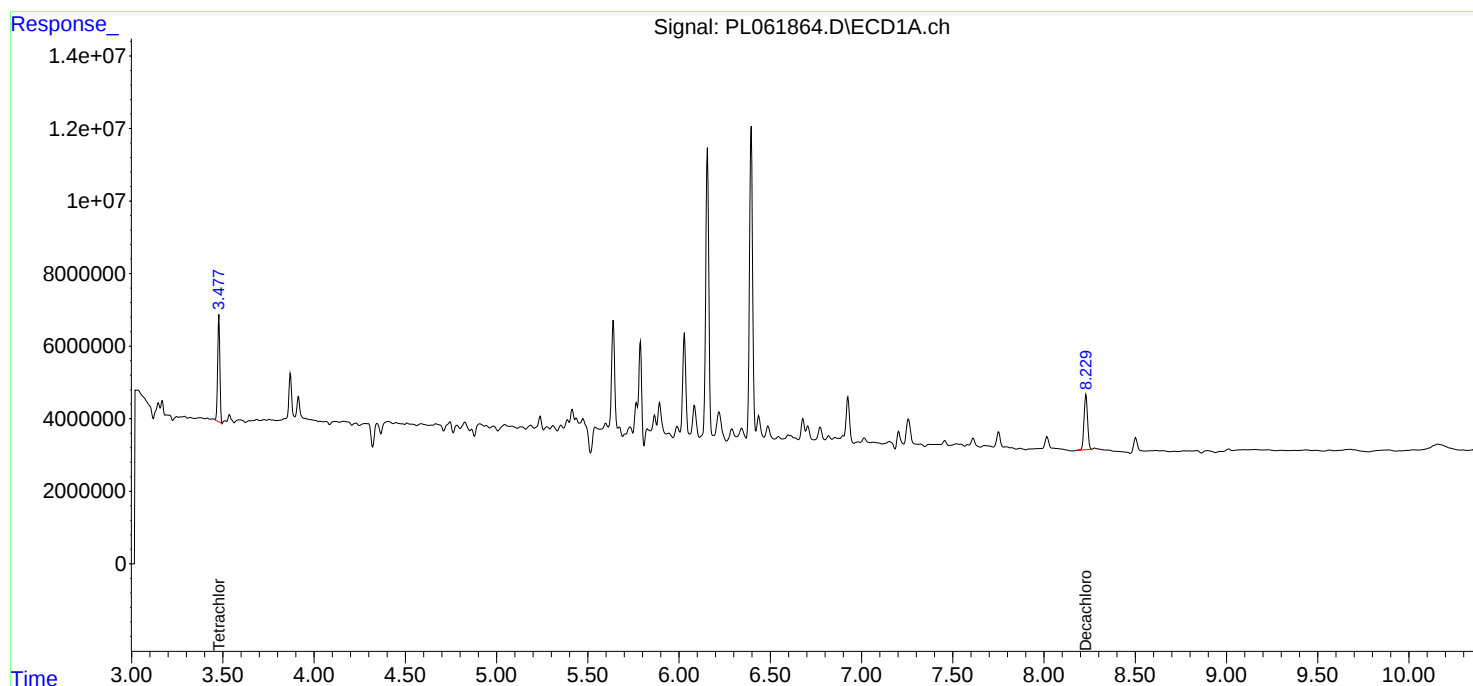

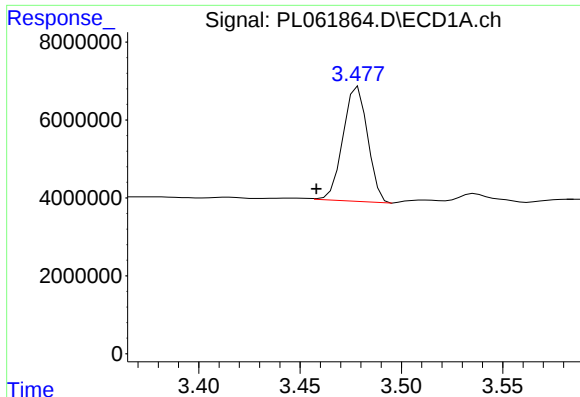


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: 0.019 min
Response: 24898460
Conc: 14.59 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-3-(0-6FT)


Manual Integrations
APPROVED

Ankita
9/30/2020 4:00:26 PM

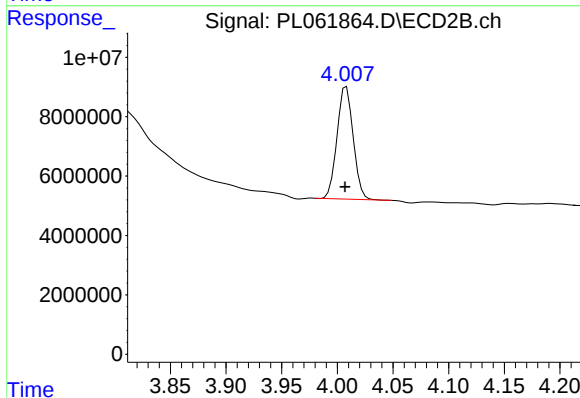


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.001 min
Response: 38181513
Conc: 13.99 ng/ml

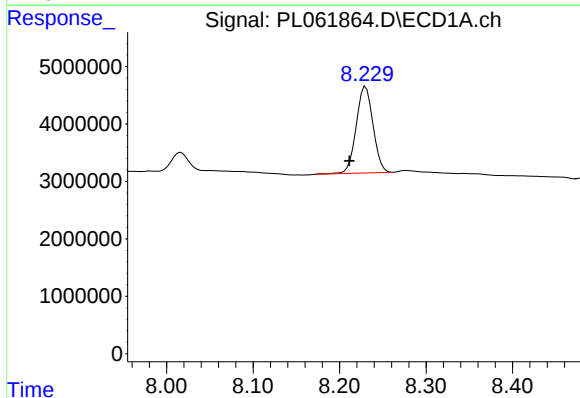

#28 Decachlorobiphenyl

R.T.: 8.230 min
Delta R.T.: 0.019 min
Response: 20422433
Conc: 12.55 ng/ml

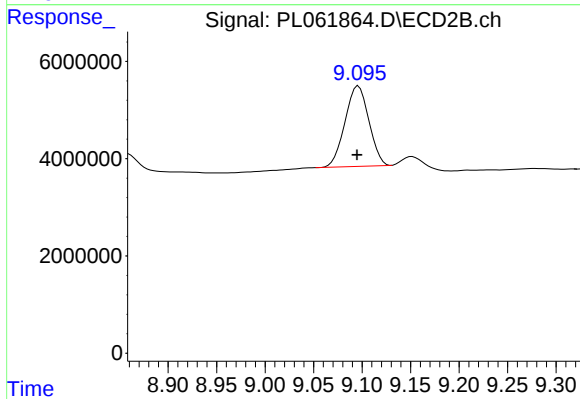

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.002 min
Response: 28278499
Conc: 12.85 ng/ml