

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092922\
 Data File : PL077976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2022 12:59
 Operator : AR\AJ
 Sample : PB147984BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 23:31:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.623	34439230	57878477	21.484	19.496
28)	SA Decachlor...	8.908	7.722	31091651	47575369	24.057	18.953
Target Compounds							
7)	B delta-BHC	4.674	0.000	461076	0	0.225	N.D. #
8)	B Heptachlo...	5.597f	0.000	485610	0	0.279	N.D. #
10)	B gamma-Chl...	0.000	4.791	0	465844	N.D.	0.137 #
12)	B 4,4'-DDE	0.000	5.046	0	287164	N.D.	0.088 #
15)	B Endosulfa...	6.706	0.000	1275745	0	0.924	N.D. #
21)	B Endrin ke...	7.569f	0.000	281225	0	0.204	N.D. #
25)	Chlordane-3	0.000	4.791	0	465844	N.D.	1.354 #
27)	Chlordane-5	0.000	5.552f	0	1296122	N.D.	13.775 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092922\
Data File : PL077976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2022 12:59
Operator : AR\AJ
Sample : PB147984BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 23:31:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

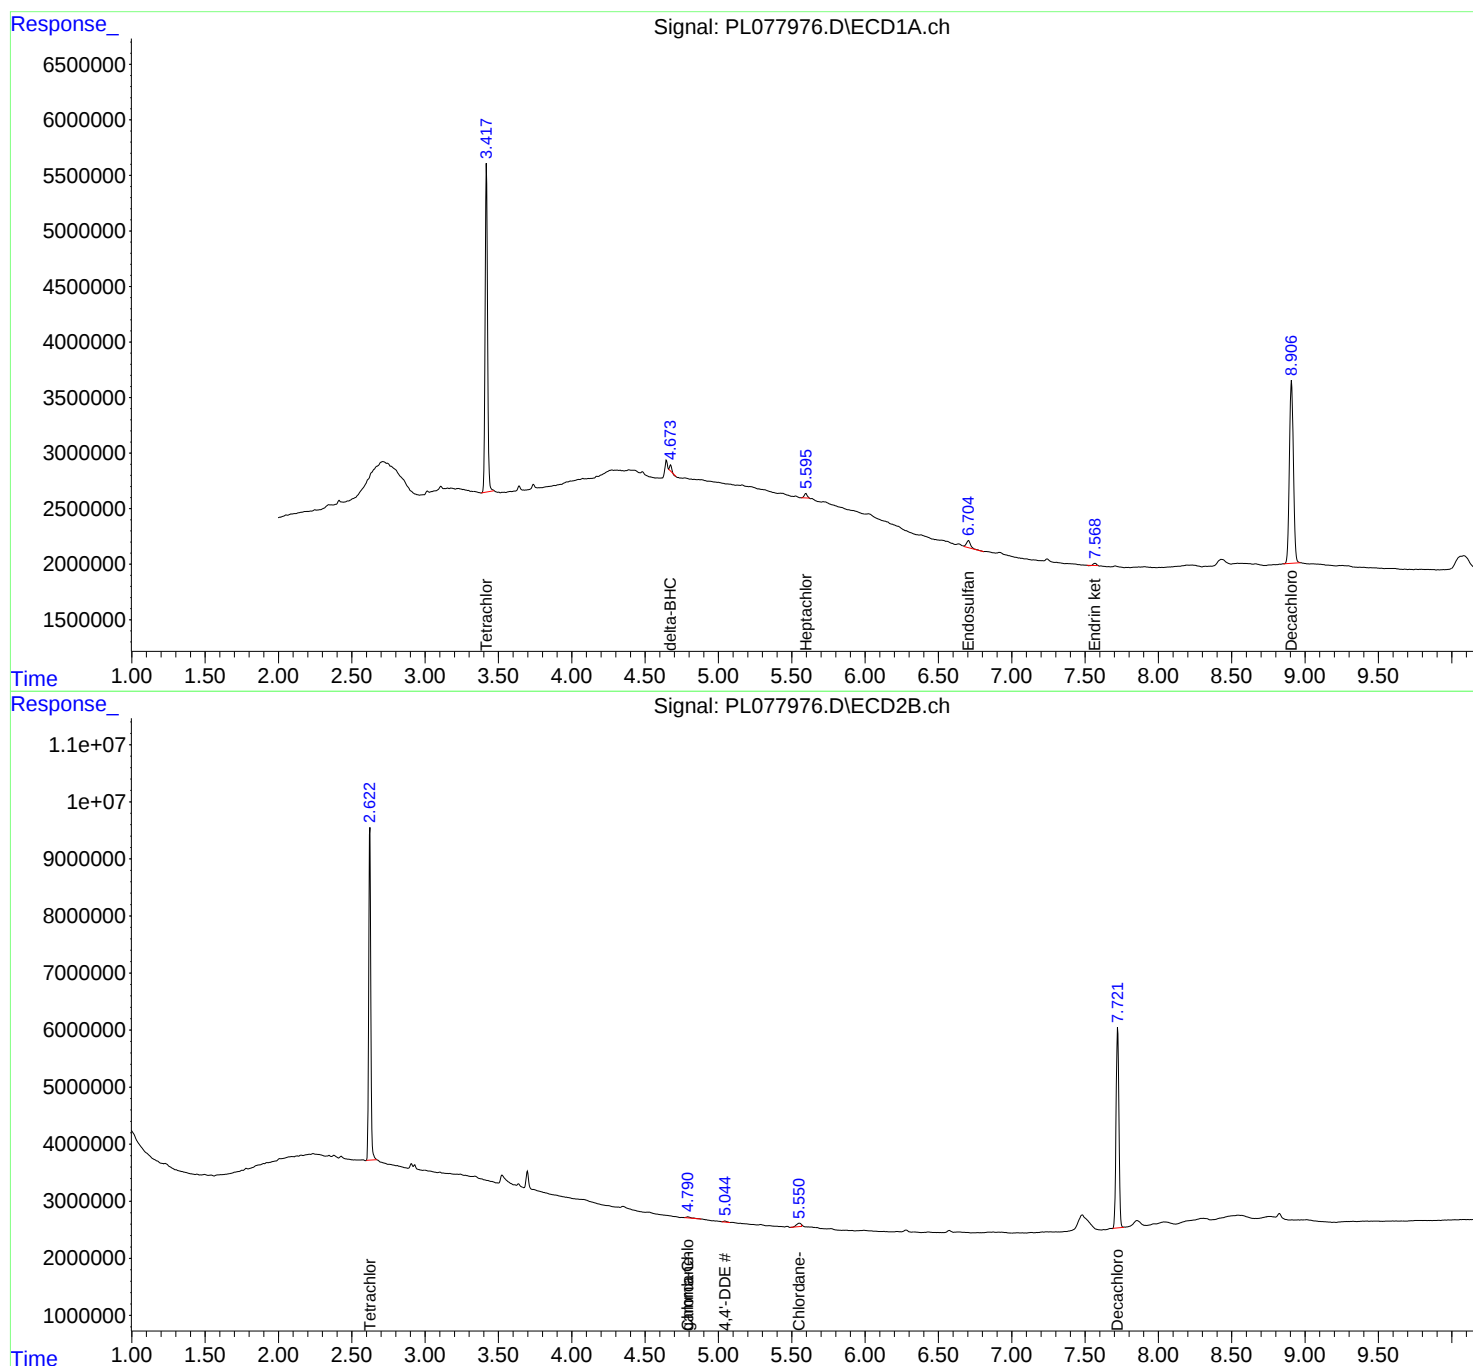


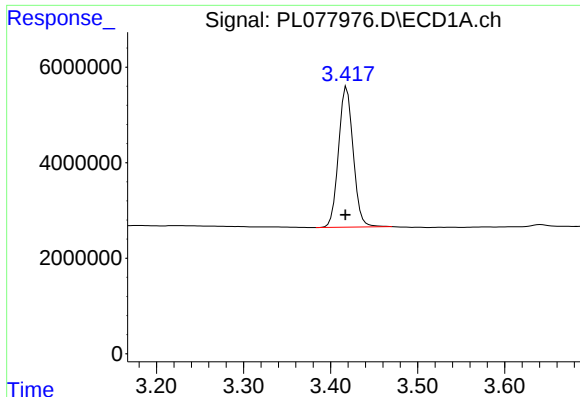

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.002 min
Response: 34439230
Conc: 21.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

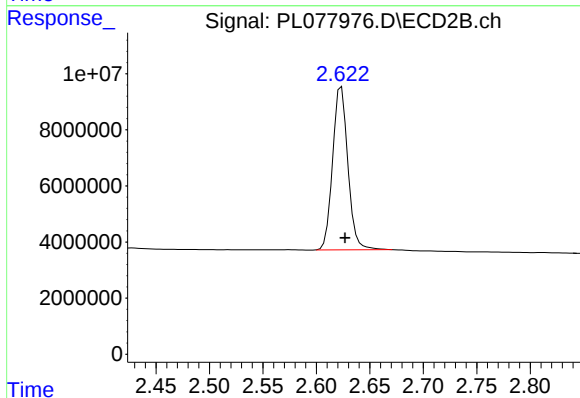


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: -0.004 min
Response: 57878477
Conc: 19.50 ng/ml

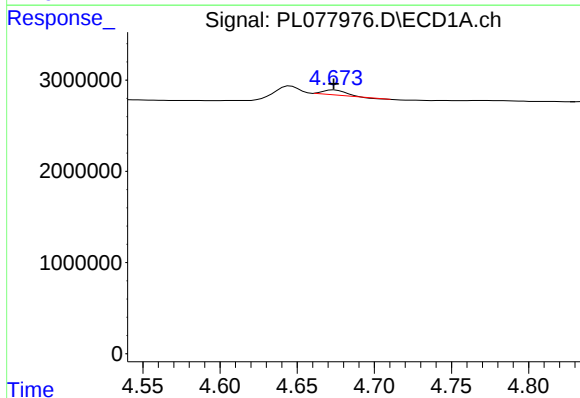


#7 delta-BHC

R.T.: 4.674 min
Delta R.T.: 0.000 min
Response: 461076
Conc: 0.22 ng/ml

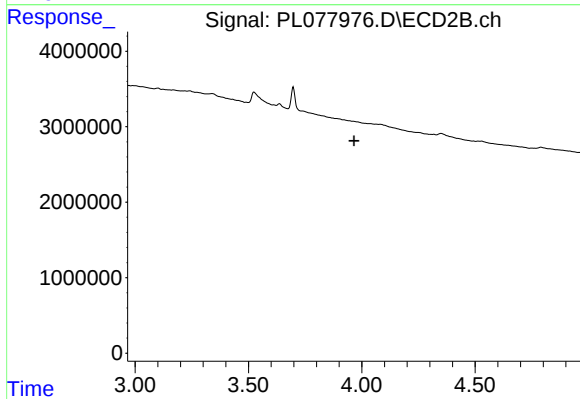

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 3.967 min
Response: 0
Conc: N.D.

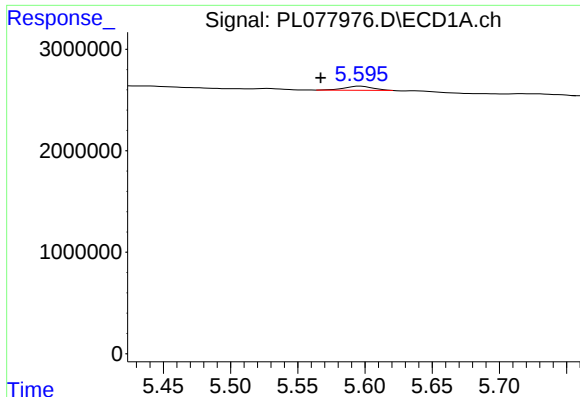

#8 Heptachlor epoxide


R.T.: 5.597 min
Delta R.T.: 0.030 min
Response: 485610
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

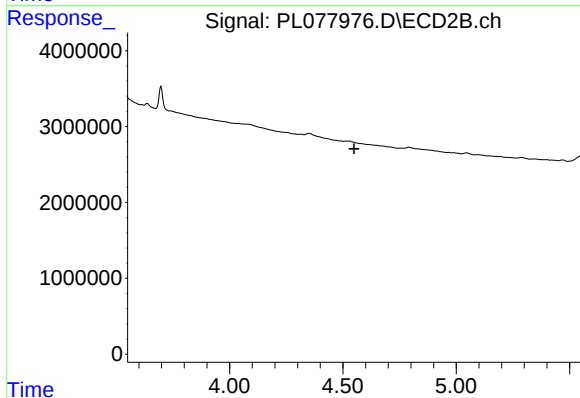


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

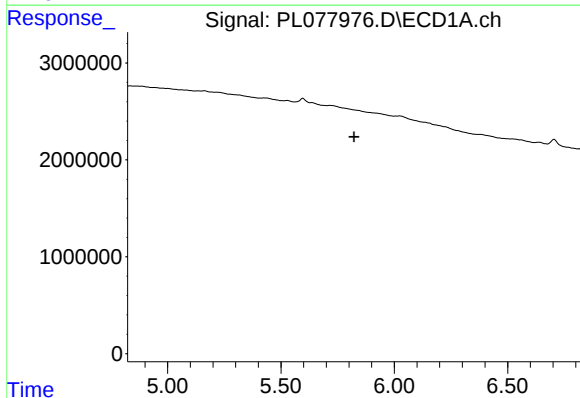


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.823 min
Response: 0
Conc: N.D.

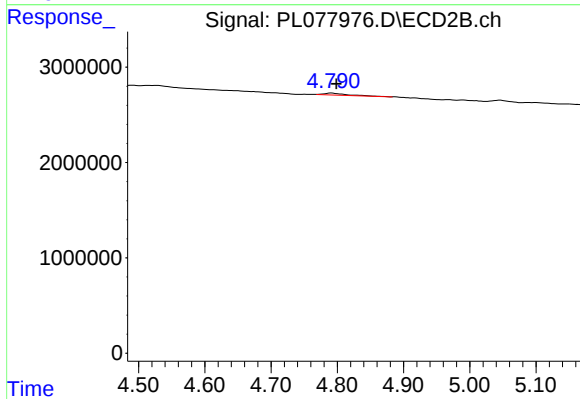

#10 gamma-Chlordane


R.T.: 4.791 min
Delta R.T.: -0.007 min
Response: 465844
Conc: 0.14 ng/ml

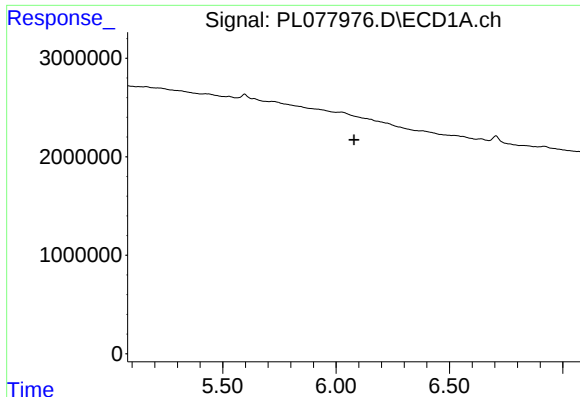

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.080 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

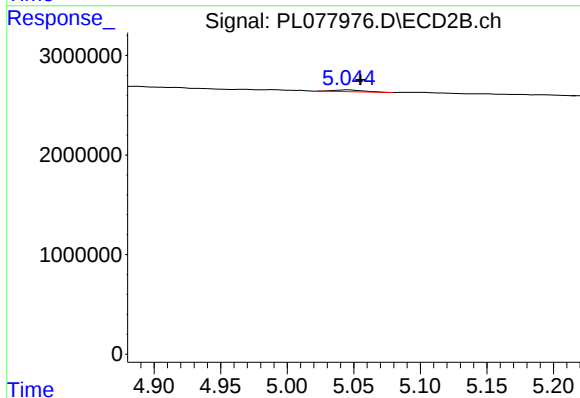


#12 4,4'-DDE

R.T.: 5.046 min
Delta R.T.: -0.009 min
Response: 287164
Conc: 0.09 ng/ml

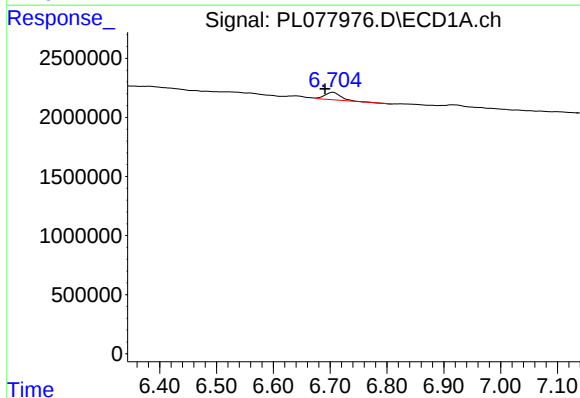


#15 Endosulfan II

R.T.: 6.706 min
Delta R.T.: 0.014 min
Response: 1275745
Conc: 0.92 ng/ml

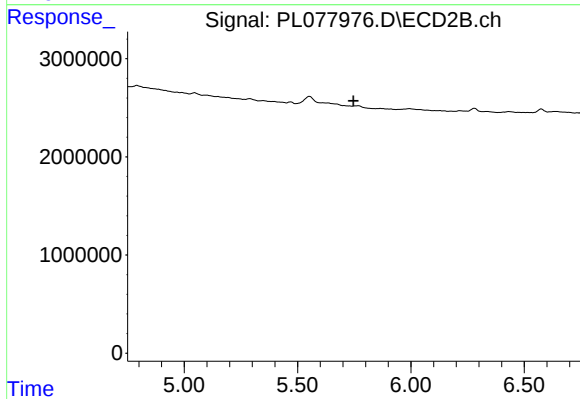

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.747 min
Response: 0
Conc: N.D.

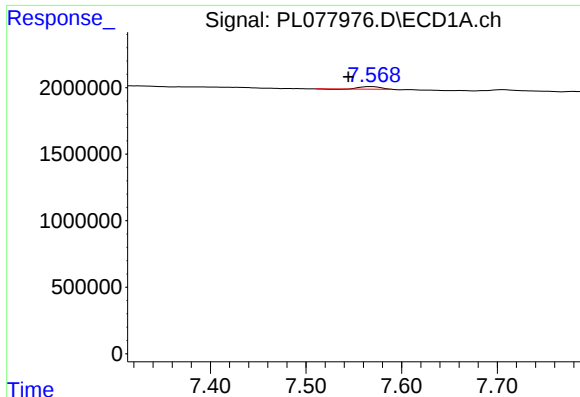

#21 Endrin ketone


R.T.: 7.569 min
Delta R.T.: 0.025 min
Response: 281225
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

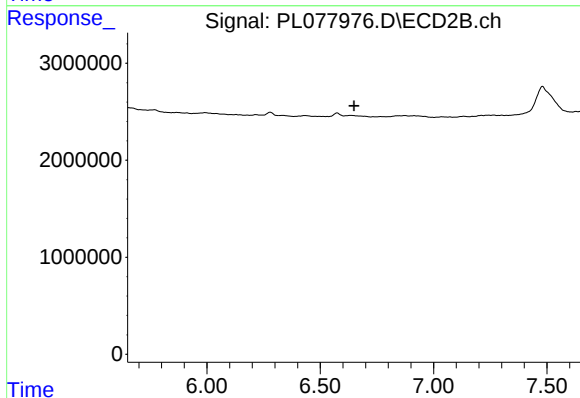


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

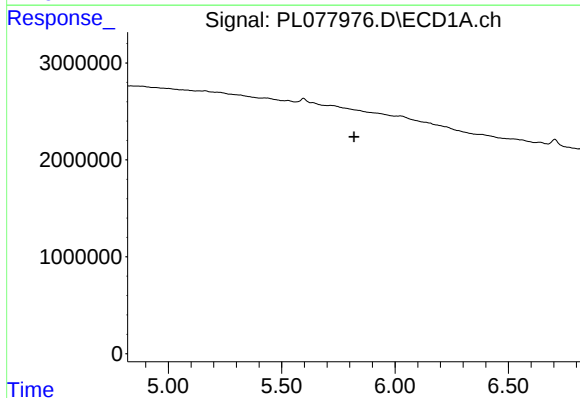


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.820 min
Response: 0
Conc: N.D.

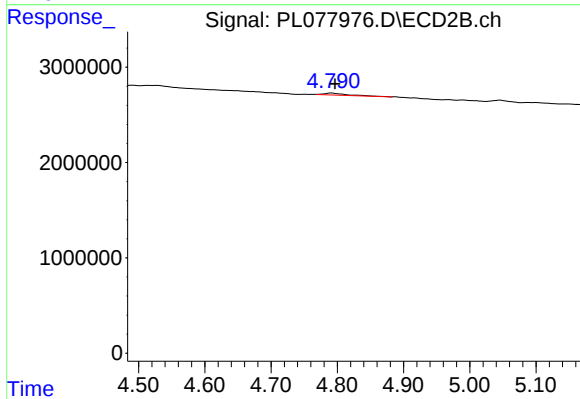

#25 Chlordane-3


R.T.: 4.791 min
Delta R.T.: -0.005 min
Response: 465844
Conc: 1.35 ng/ml

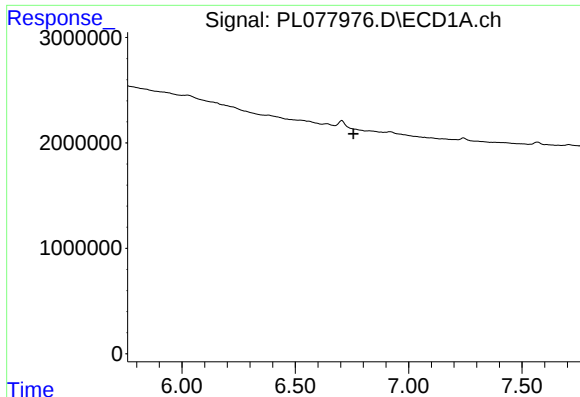

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.757 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

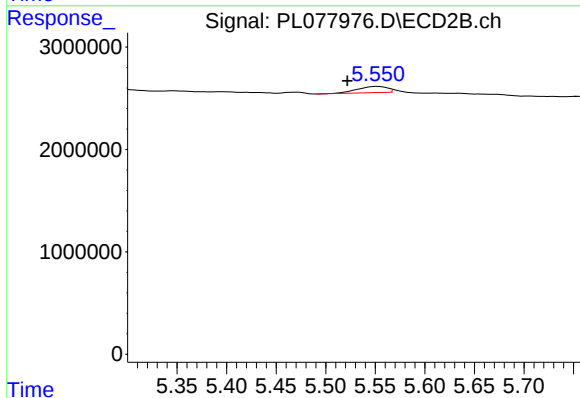


#27 Chlordane-5

R.T.: 5.552 min
Delta R.T.: 0.030 min
Response: 1296122
Conc: 13.77 ng/ml

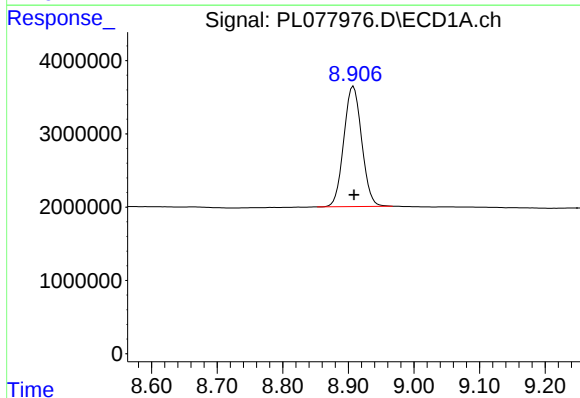

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 31091651
Conc: 24.06 ng/ml

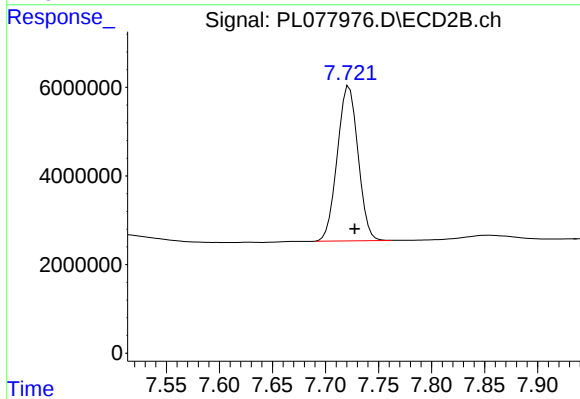

#28 Decachlorobiphenyl

R.T.: 7.722 min
Delta R.T.: -0.005 min
Response: 47575369
Conc: 18.95 ng/ml