

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092922\
 Data File : PL077978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2022 13:57
 Operator : AR\AJ
 Sample : N4862-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-203

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/30/2022
 Supervised By : Ankita Jodhani 09/30/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 23:32:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.419	2.624	14351570	20699446	8.953m	6.972m
28) SA Decachlor...	8.908	7.721	23053012	35871502	17.837	14.290

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092922\
Data File : PL077978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2022 13:57
Operator : AR\AJ
Sample : N4862-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VNJ-203


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/30/2022
Supervised By : Ankita Jodhani 09/30/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 23:32:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

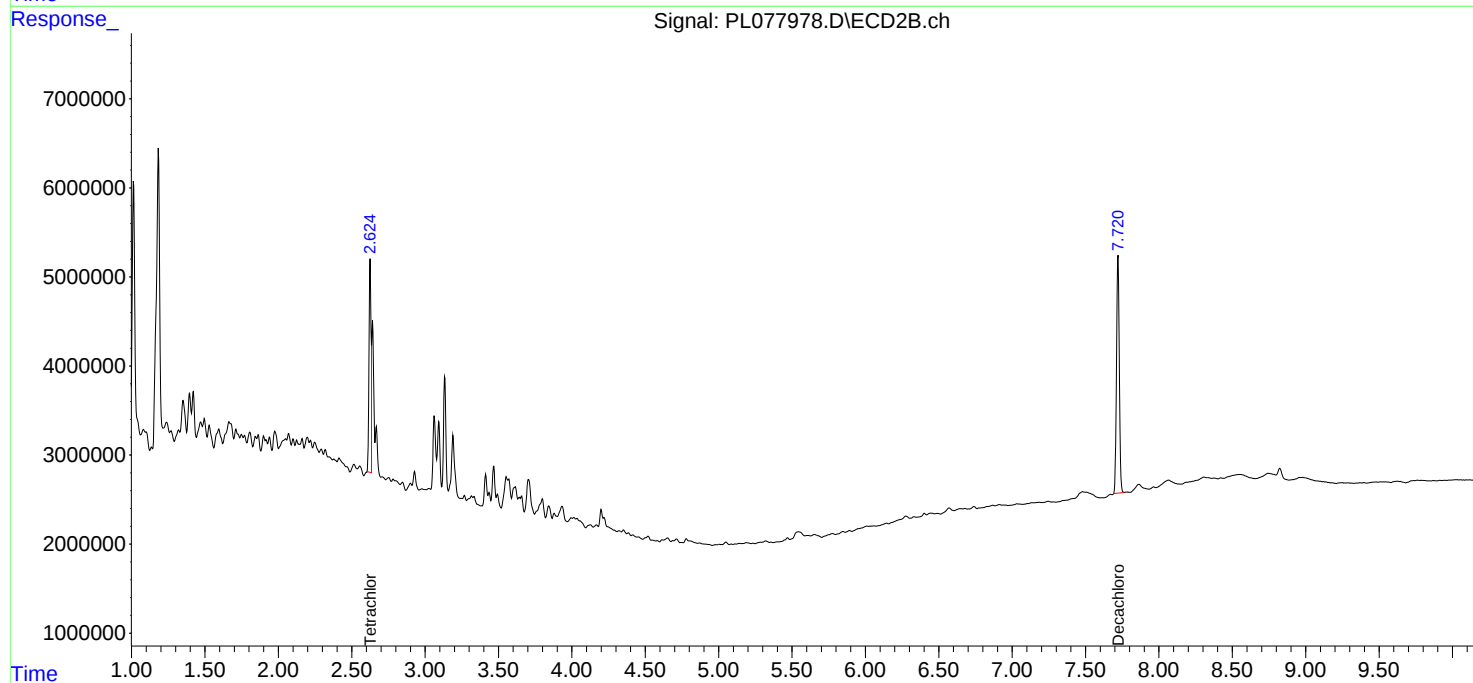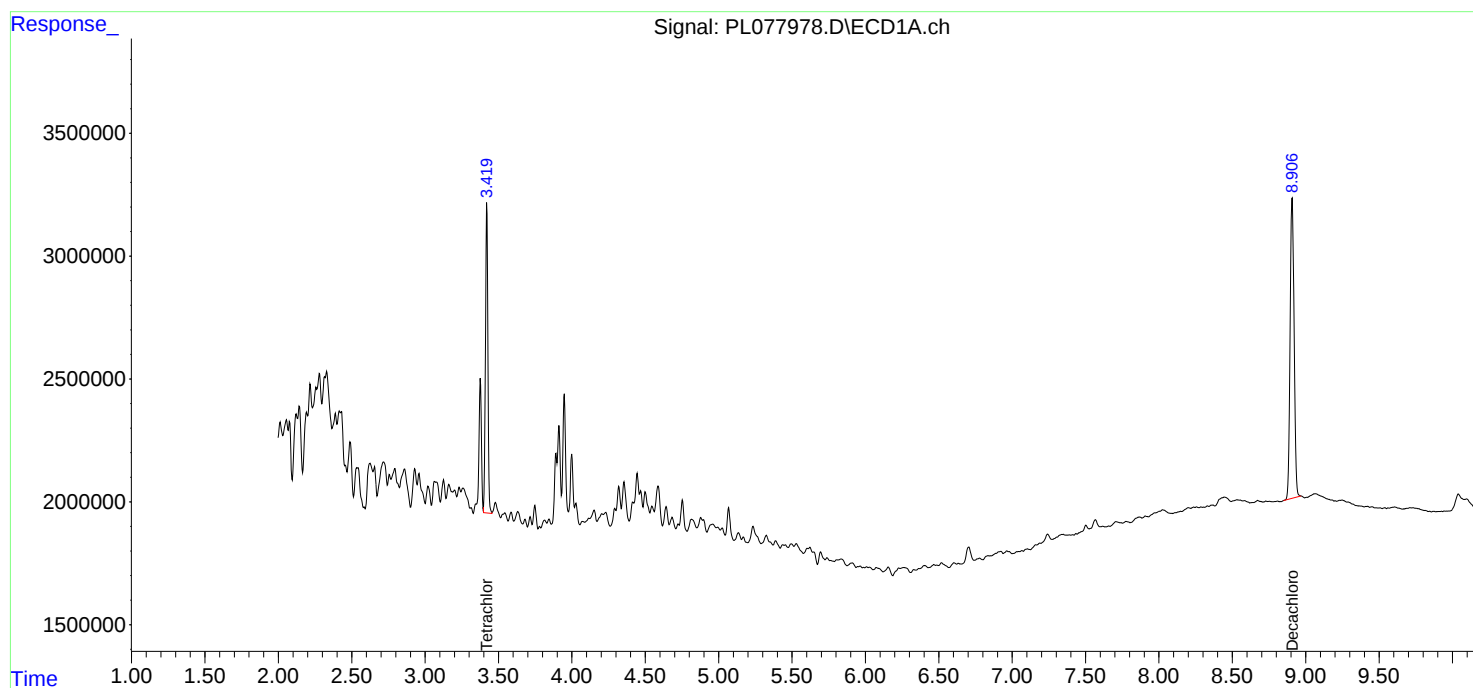

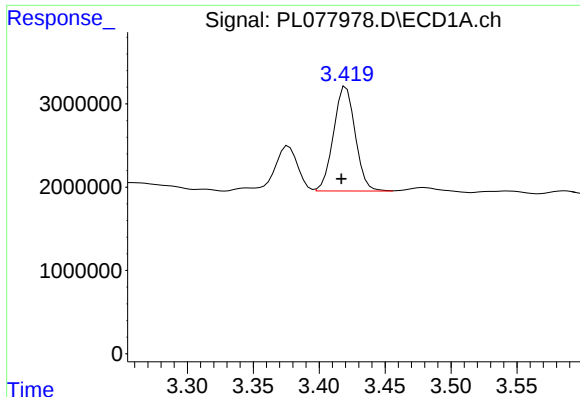


#1 Tetrachloro-m-xylene

R.T.: 3.419 min
Delta R.T.: 0.002 min
Response: 14351570
Conc: 8.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-203


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/30/2022
Supervised By :Ankita Jodhani 09/30/2022

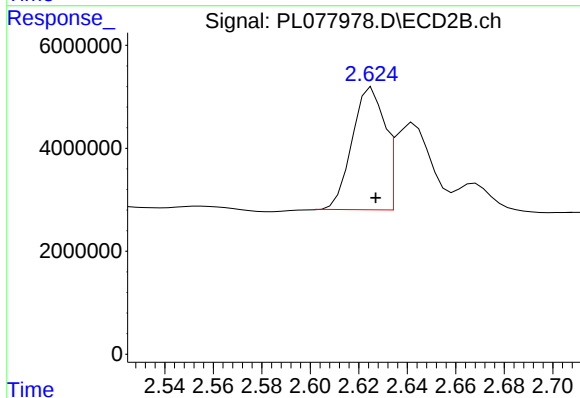


#1 Tetrachloro-m-xylene

R.T.: 2.624 min
Delta R.T.: -0.003 min
Response: 20699446
Conc: 6.97 ng/ml m

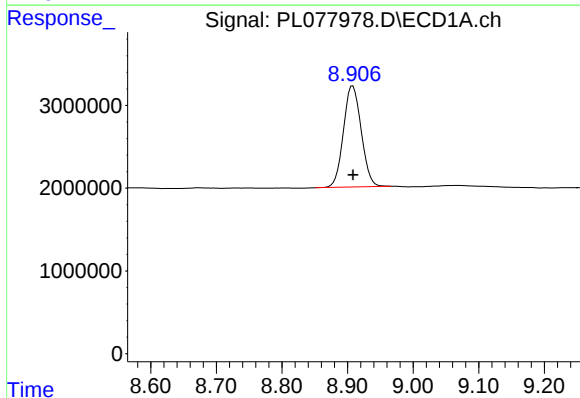

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 23053012
Conc: 17.84 ng/ml

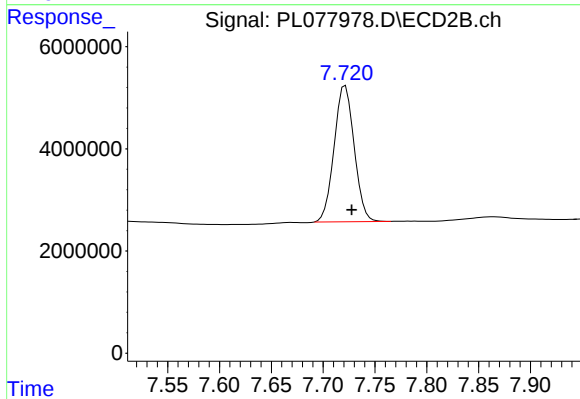

#28 Decachlorobiphenyl

R.T.: 7.721 min
Delta R.T.: -0.006 min
Response: 35871502
Conc: 14.29 ng/ml