

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092922\
 Data File : PL077991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2022 17:24
 Operator : AR\AJ
 Sample : N4875-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/30/2022
 Supervised By :Ankita Jodhani 09/30/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 23:40:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.417	2.646f	8233374	43970353	5.136	14.811m#
2) SA Decachlor...	8.911	7.734	6290048	13839516	4.867m	5.513

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092922\
Data File : PL077991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2022 17:24
Operator : AR\AJ
Sample : N4875-01
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/30/2022
Supervised By : Ankita Jodhani 09/30/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 23:40:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

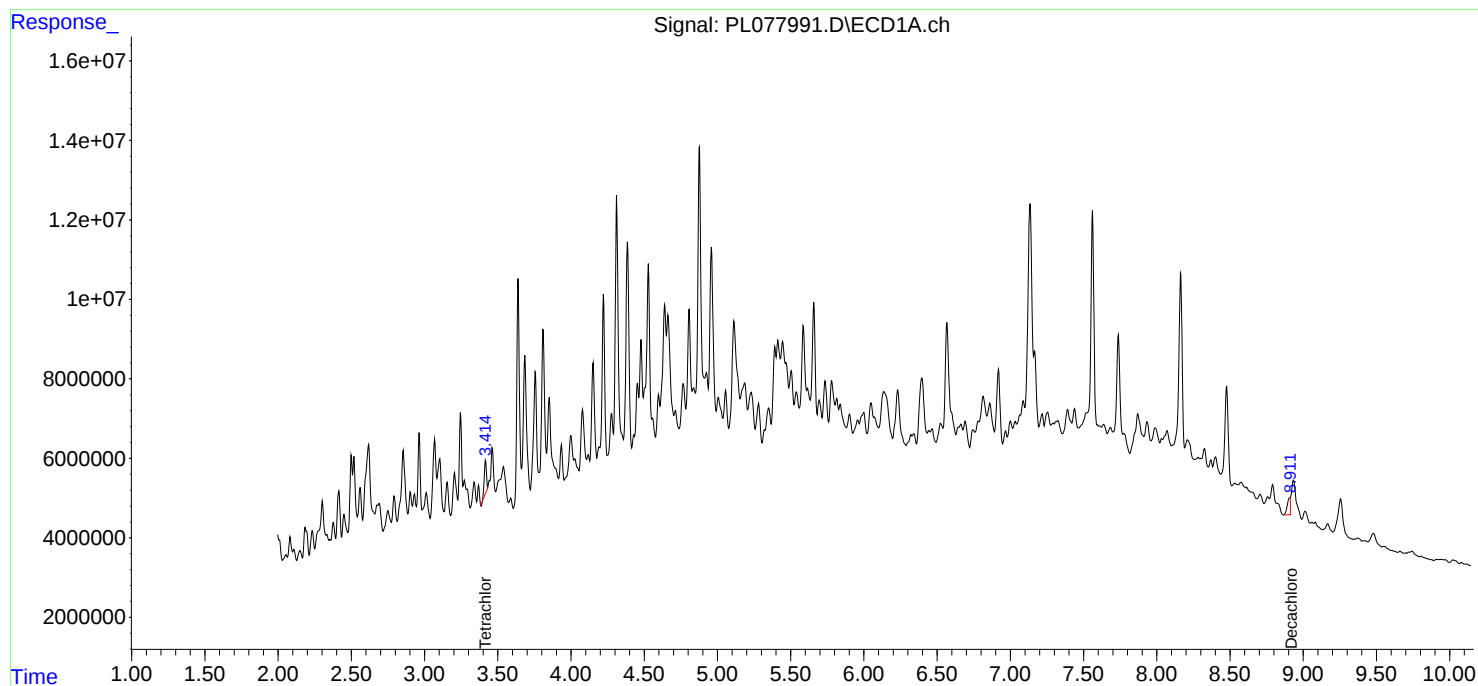

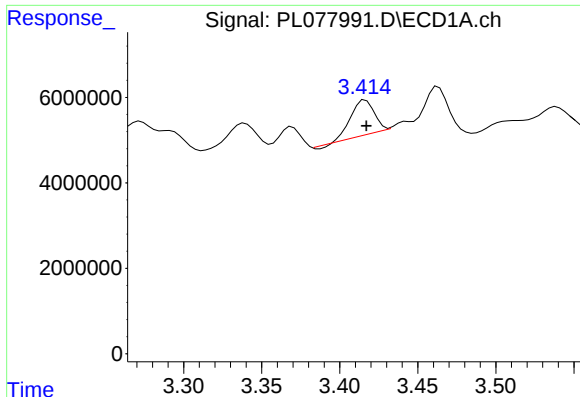


#1 Tetrachloro-m-xylene

R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 8233374
Conc: 5.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/30/2022
Supervised By :Ankita Jodhani 09/30/2022

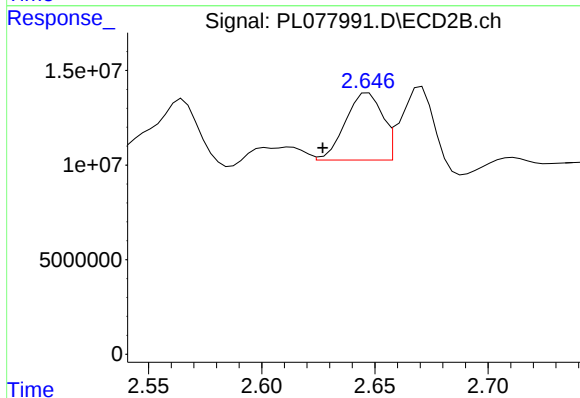


#1 Tetrachloro-m-xylene

R.T.: 2.646 min
Delta R.T.: 0.019 min
Response: 43970353
Conc: 14.81 ng/ml m

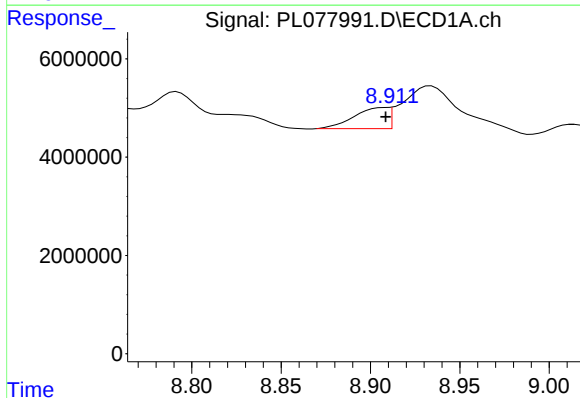

#28 Decachlorobiphenyl

R.T.: 8.911 min
Delta R.T.: 0.002 min
Response: 6290048
Conc: 4.87 ng/ml m

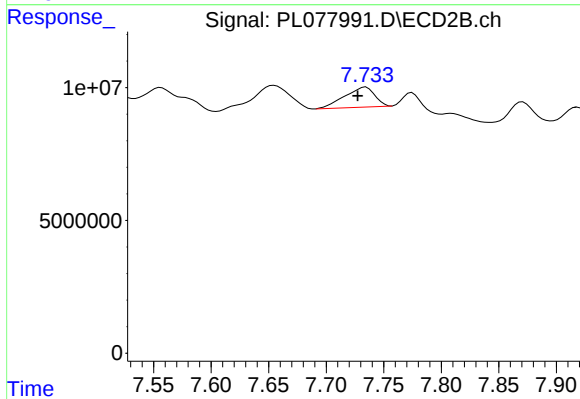

#28 Decachlorobiphenyl

R.T.: 7.734 min
Delta R.T.: 0.007 min
Response: 13839516
Conc: 5.51 ng/ml