

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
 Data File : PL097399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2025 10:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 13:30:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.821	82457499	124.0E6	18.214	18.851
28)	SA Decachlor...	8.999	7.982	62477960	104.4E6	19.094	18.340
Target Compounds							
8)	B Heptachlo...	0.000	4.788	0	4856321	N.D.	0.612 #
10)	B gamma-Chl...	0.000	5.026f	0	9948973	N.D.	1.139 #
18)	B Endrin al...	0.000	6.156f	0	17323966	N.D.	3.246 #
25)	Chlordane-3	0.000	5.026f	0	9948973	N.D.	11.126 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
Data File : PL097399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2025 10:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 13:30:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

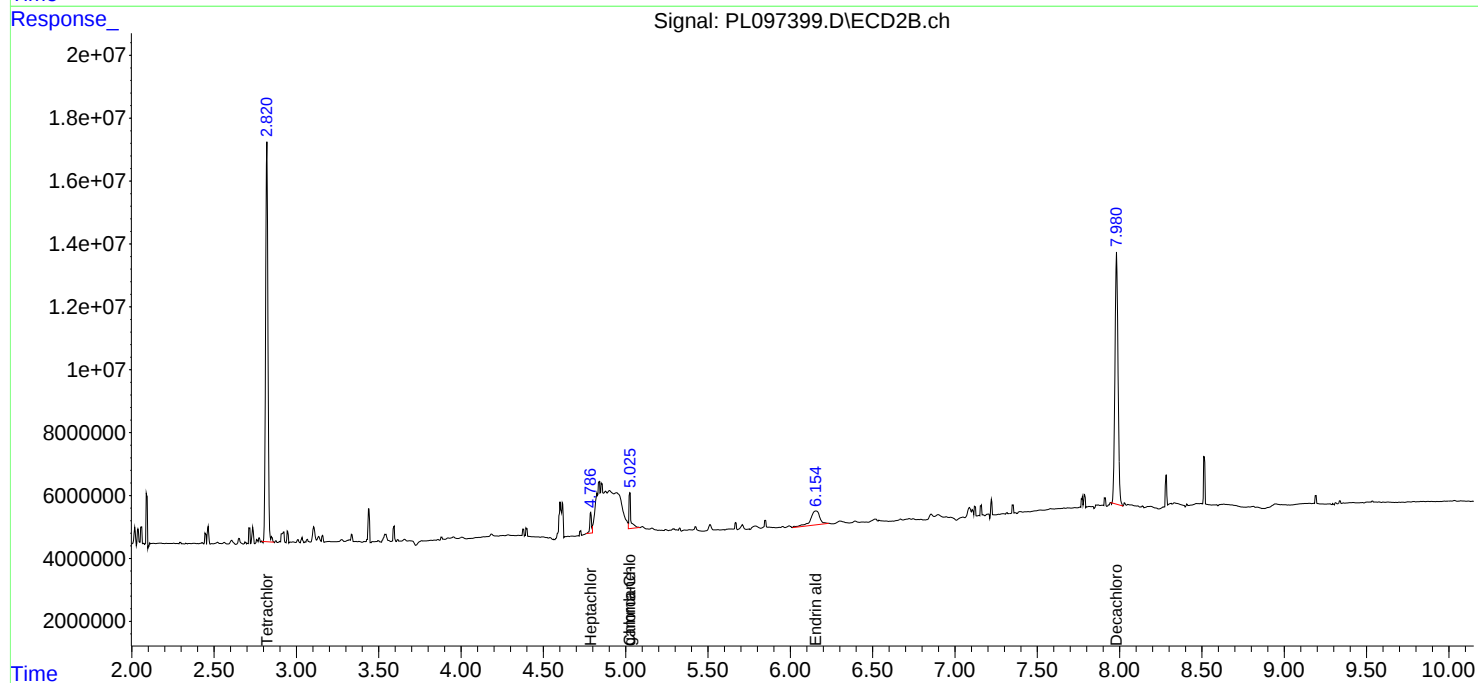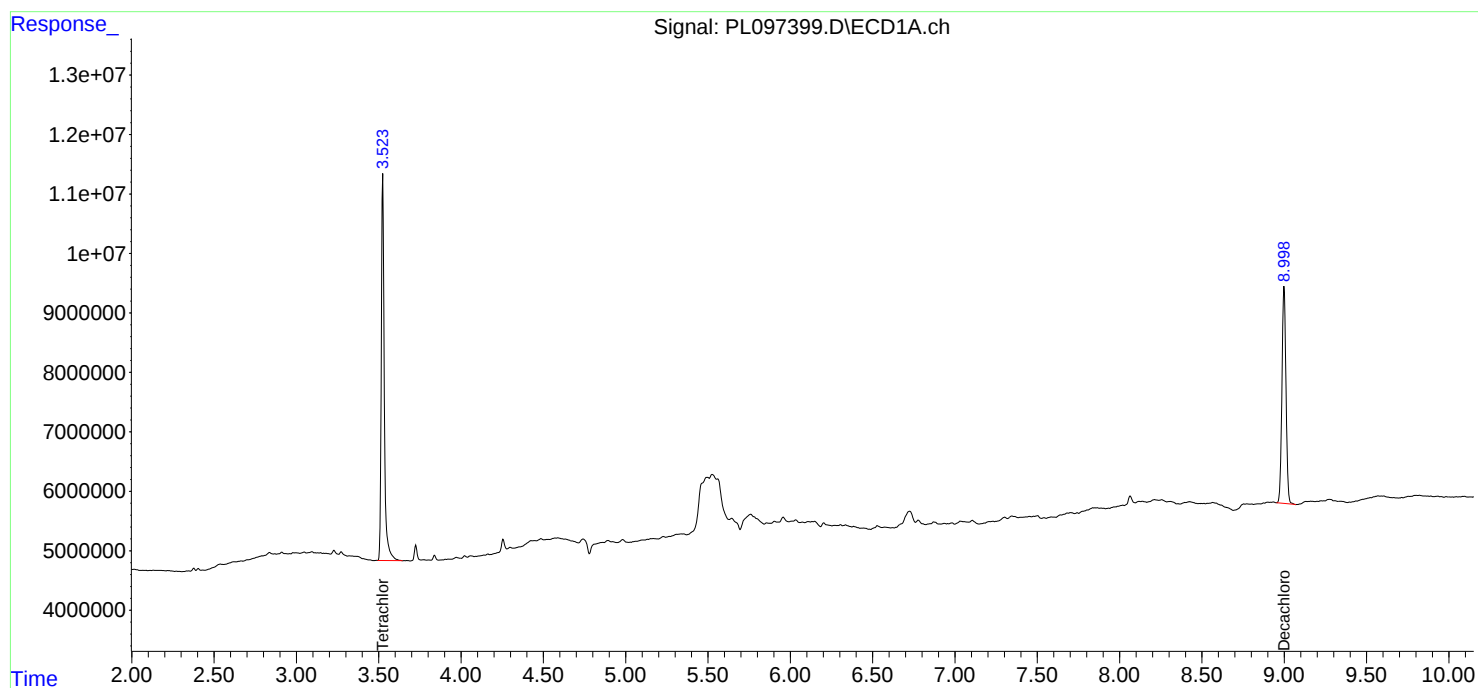


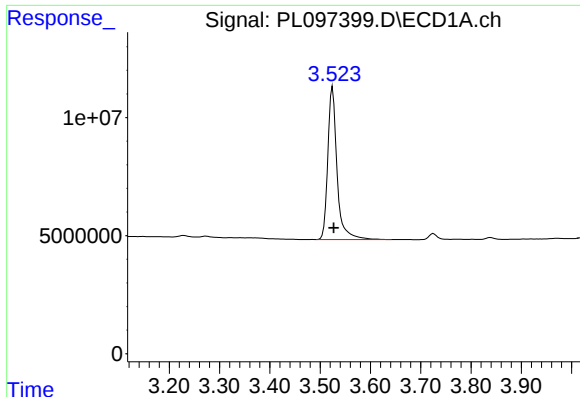

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: -0.002 min
Response: 82457499
Conc: 18.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

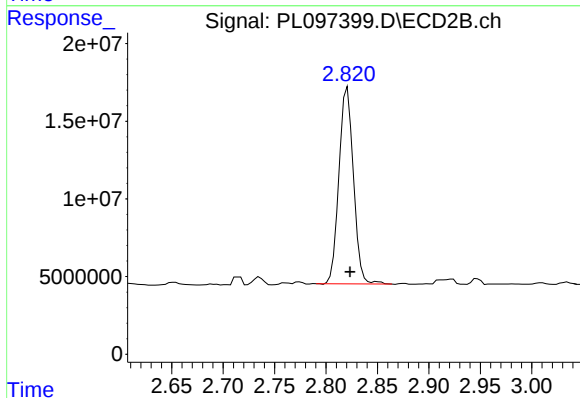


#1 Tetrachloro-m-xylene

R.T.: 2.821 min
Delta R.T.: -0.003 min
Response: 123958574
Conc: 18.85 ng/ml

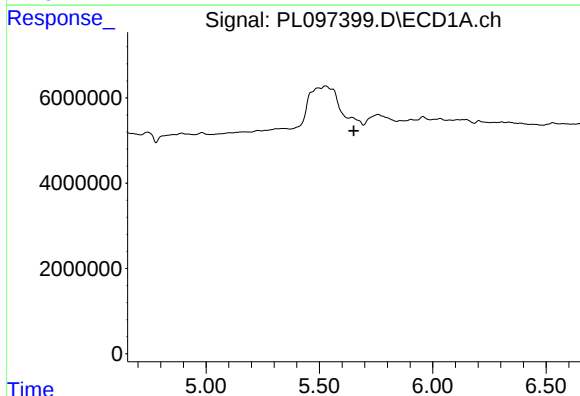


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.652 min
Response: 0
Conc: N.D.

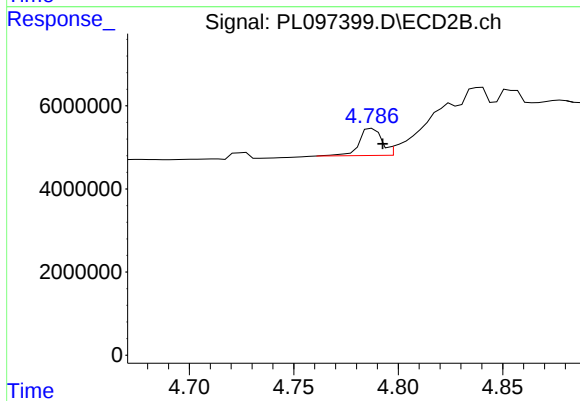

#8 Heptachlor epoxide


R.T.: 4.788 min
Delta R.T.: -0.005 min
Response: 4856321
Conc: 0.61 ng/ml

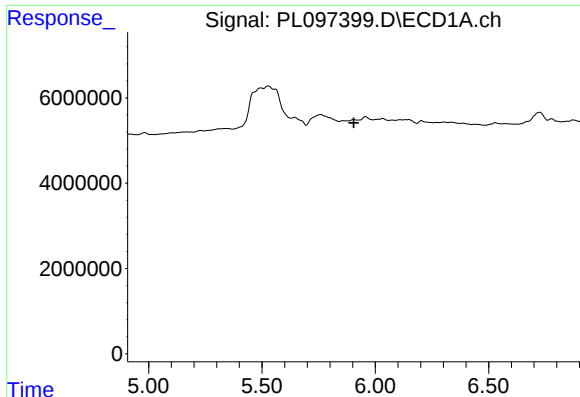

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.905 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

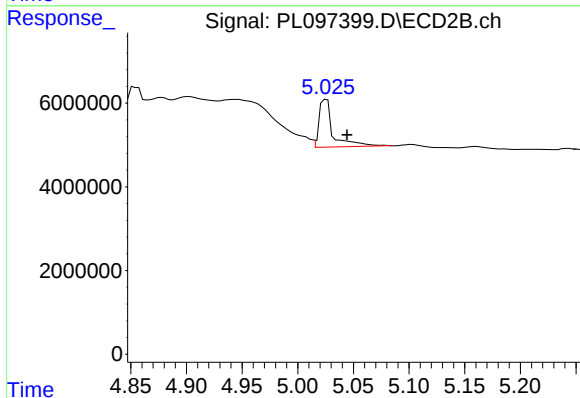


#10 gamma-Chlordane

R.T.: 5.026 min
Delta R.T.: -0.019 min
Response: 9948973
Conc: 1.14 ng/ml

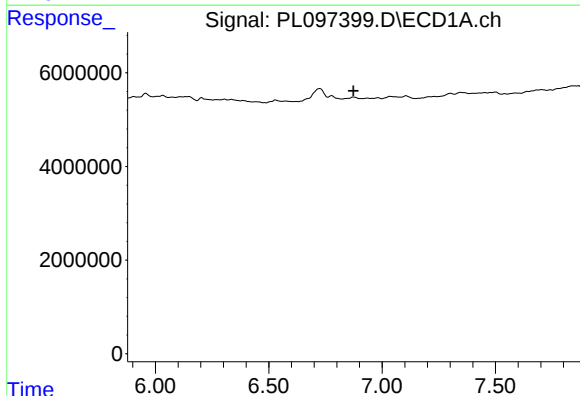


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.874 min
Response: 0
Conc: N.D.

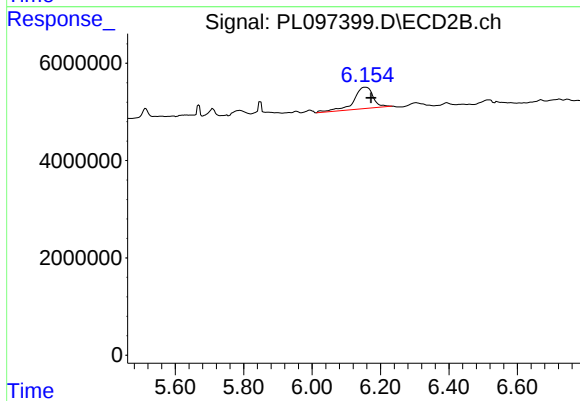

#18 Endrin aldehyde


R.T.: 6.156 min
Delta R.T.: -0.017 min
Response: 17323966
Conc: 3.25 ng/ml

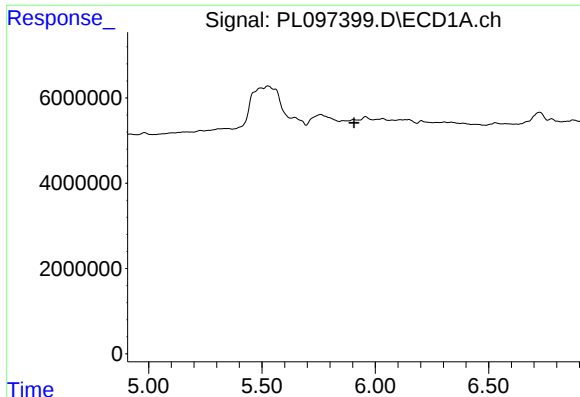

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

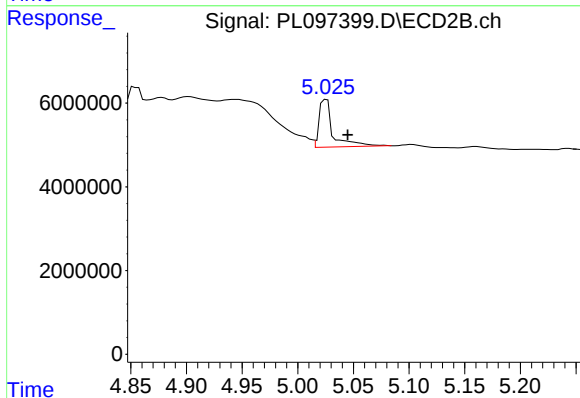


#25 Chlordane-3

R.T.: 5.026 min
Delta R.T.: -0.019 min
Response: 9948973
Conc: 11.13 ng/ml

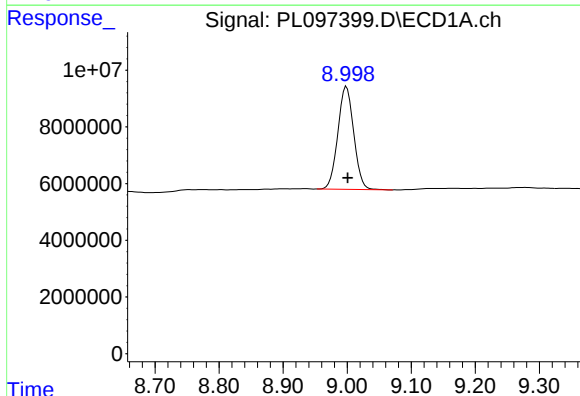

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.002 min
Response: 62477960
Conc: 19.09 ng/ml

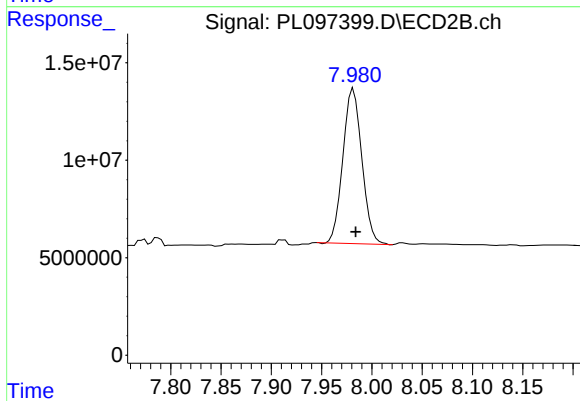

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: -0.002 min
Response: 104383530
Conc: 18.34 ng/ml