

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
 Data File : PL097403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2025 12:46
 Operator : AR\AJ
 Sample : Q3183-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 13:31:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.821	73399234	88627531	16.213	13.478
28)	SA Decachlor...	8.998	7.981	38052773	68885796	11.629	12.103
Target Compounds							
9)	A Endosulfan I	0.000	5.181f	0	6679515	N.D.	0.869 #
10)	B gamma-Chl...	5.902	5.041	8762153	16489663	1.550	1.888
11)	B alpha-Chl...	5.985	5.105	11598370	16544989	2.042	1.993
14)	MA Endrin	0.000	5.708	0	16087062	N.D.	2.142 #
17)	MA 4,4'-DDT	6.976	6.098	6912803	9784633	1.635	1.414
20)	A Methoxychlor	0.000	6.698f	0	3087104	N.D.	0.819 #
23)	Chlordane-1	0.000	3.833	0	5216078	N.D.	20.523 #
25)	Chlordane-3	5.902	5.041	8762153	16489663	10.743	18.440 #
26)	Chlordane-4	5.985	5.105	11598370	16544989	11.596	21.726 #
27)	Chlordane-5	6.826	0.000	6181750	0	36.877	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
Data File : PL097403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2025 12:46
Operator : AR\AJ
Sample : Q3183-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 13:31:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

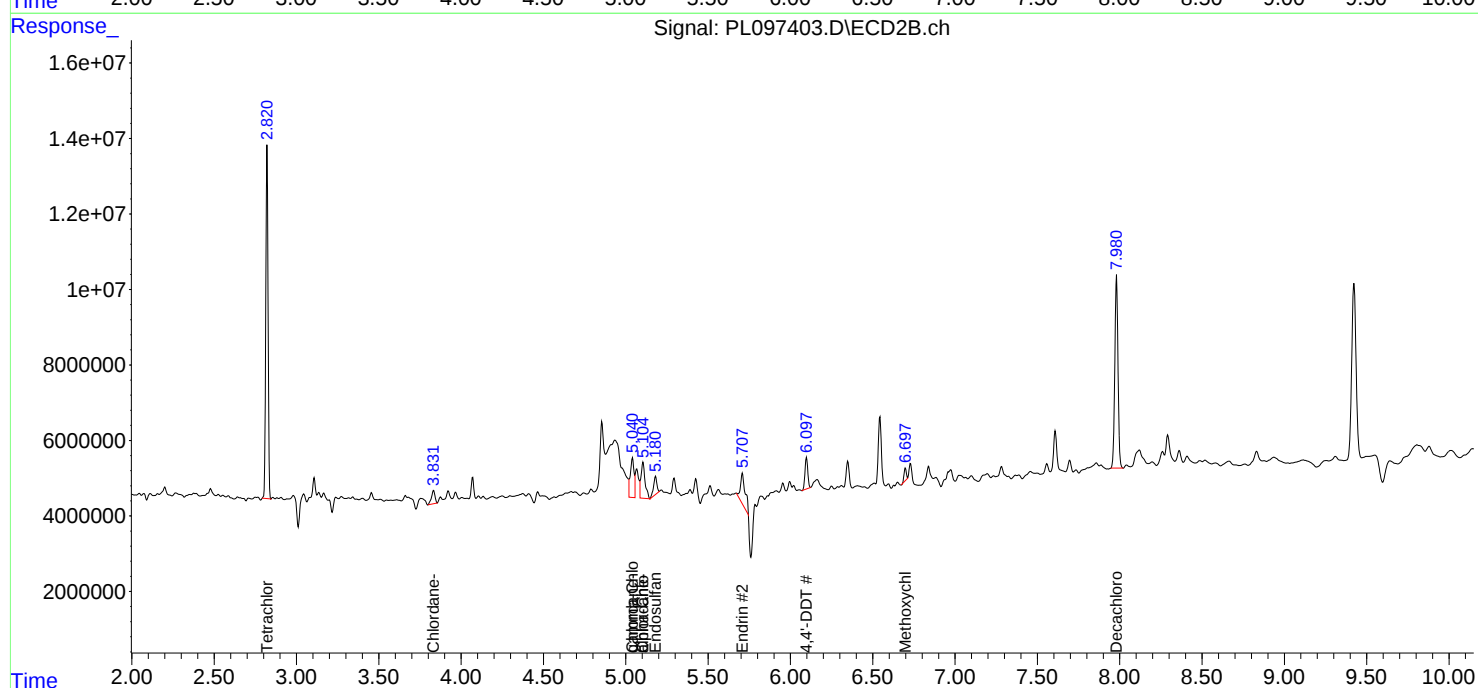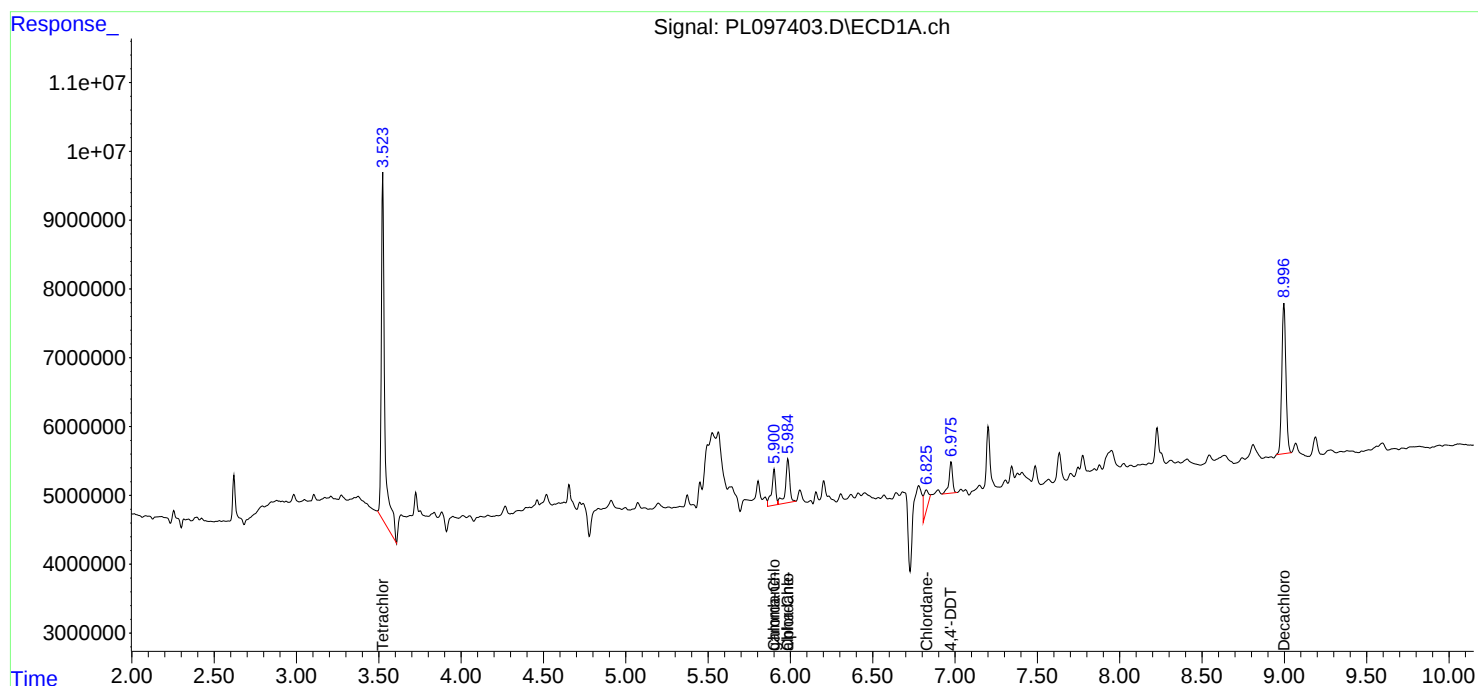


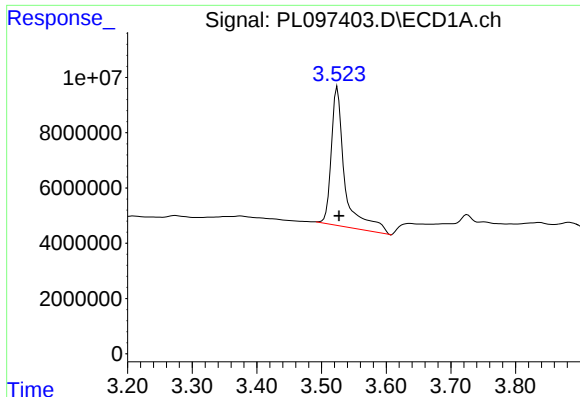

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: -0.002 min
Response: 73399234
Conc: 16.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

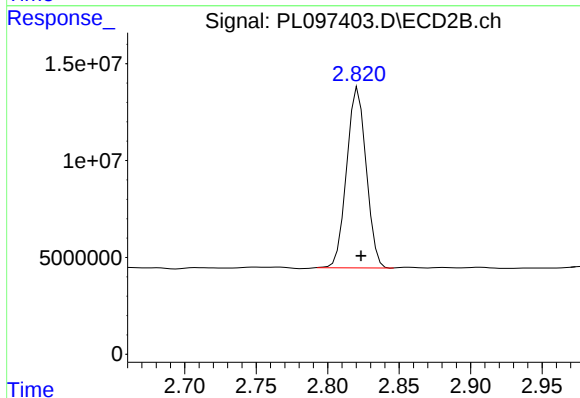


#1 Tetrachloro-m-xylene

R.T.: 2.821 min
Delta R.T.: -0.002 min
Response: 88627531
Conc: 13.48 ng/ml

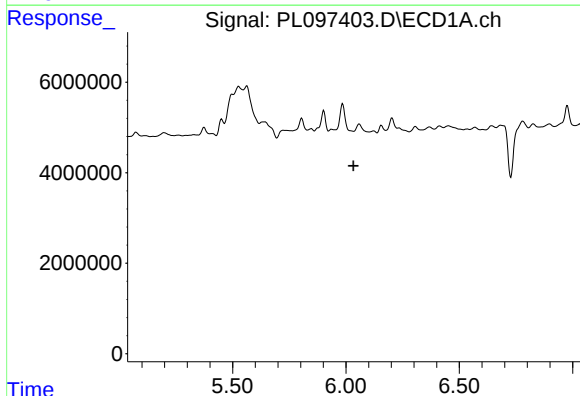


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

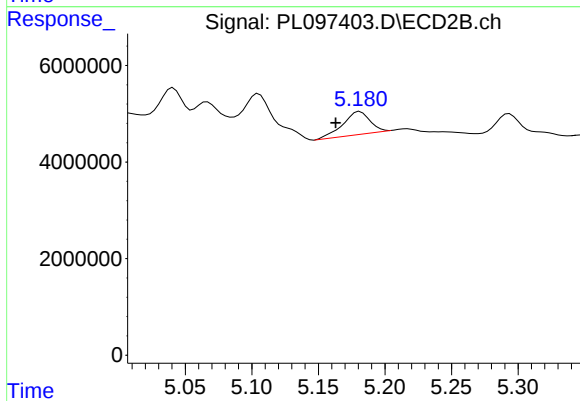

#9 Endosulfan I


R.T.: 5.181 min
Delta R.T.: 0.018 min
Response: 6679515
Conc: 0.87 ng/ml

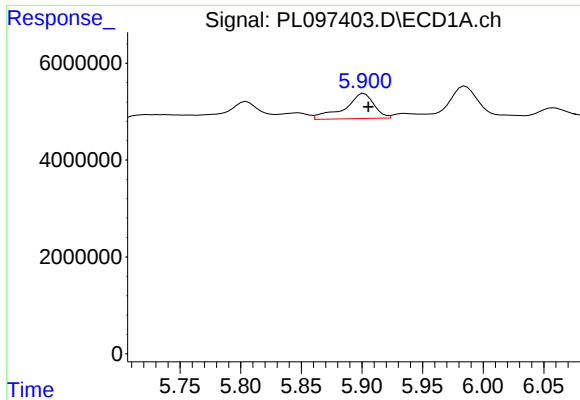

#10 gamma-Chlordane


R.T.: 5.902 min
Delta R.T.: -0.003 min
Response: 8762153
Conc: 1.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

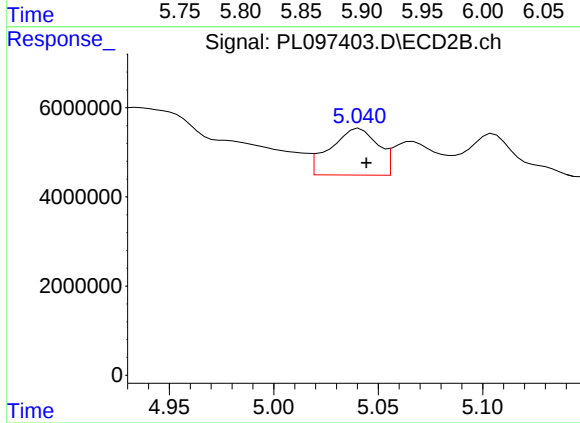


#10 gamma-Chlordane

R.T.: 5.041 min
Delta R.T.: -0.003 min
Response: 16489663
Conc: 1.89 ng/ml

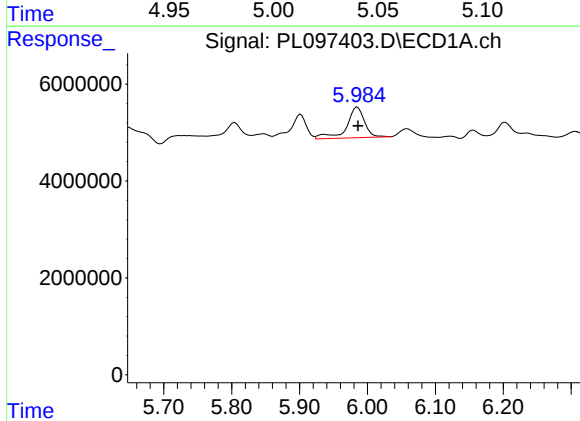


#11 alpha-Chlordane

R.T.: 5.985 min
Delta R.T.: -0.001 min
Response: 11598370
Conc: 2.04 ng/ml

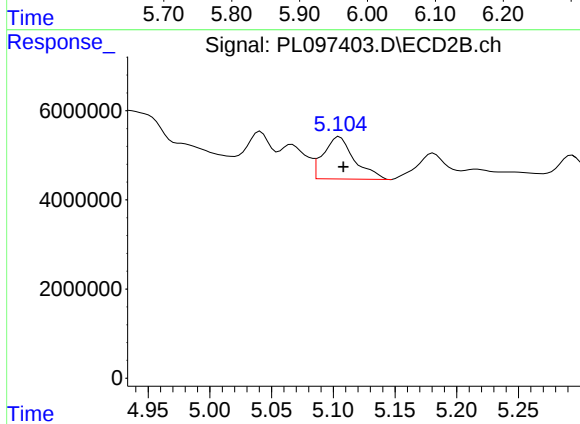

#11 alpha-Chlordane


R.T.: 5.105 min
Delta R.T.: -0.003 min
Response: 16544989
Conc: 1.99 ng/ml

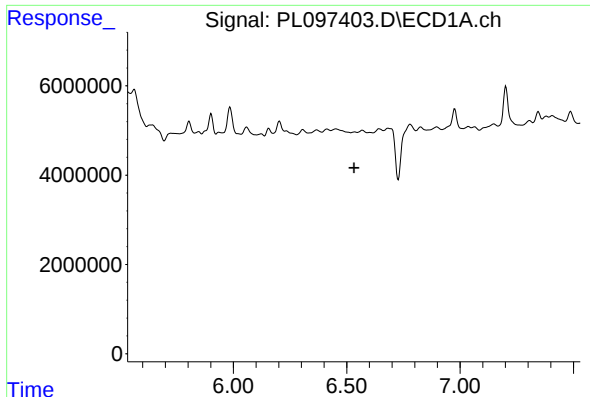

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

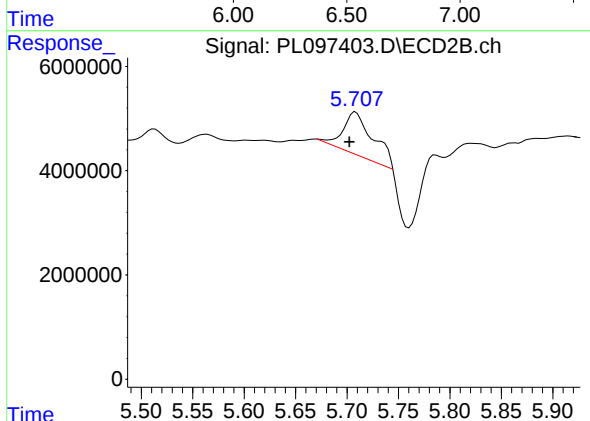


#14 Endrin

R.T.: 5.708 min
Delta R.T.: 0.006 min
Response: 16087062
Conc: 2.14 ng/ml

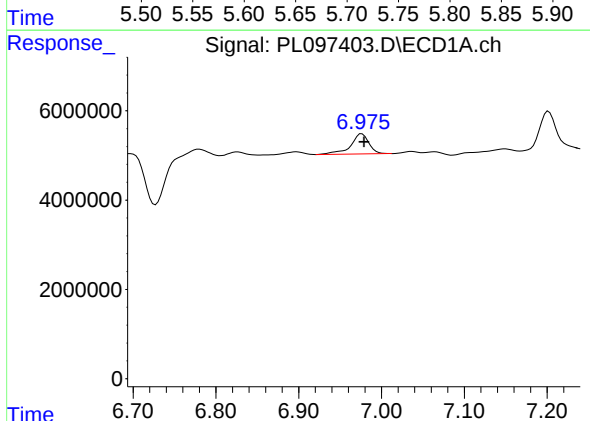


#17 4,4'-DDT

R.T.: 6.976 min
Delta R.T.: -0.003 min
Response: 6912803
Conc: 1.64 ng/ml

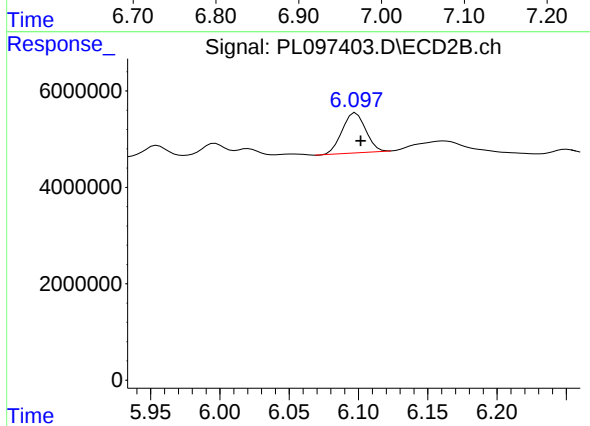

#17 4,4'-DDT


R.T.: 6.098 min
Delta R.T.: -0.003 min
Response: 9784633
Conc: 1.41 ng/ml

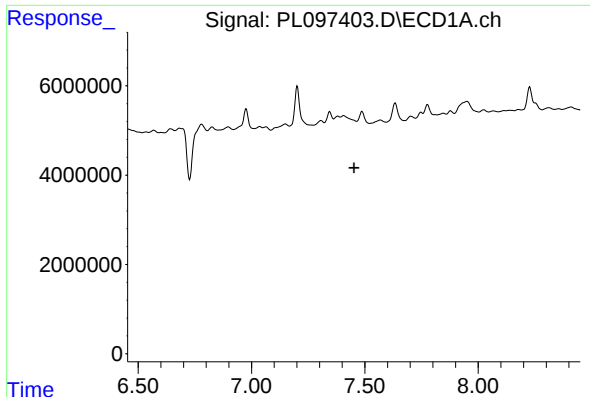

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

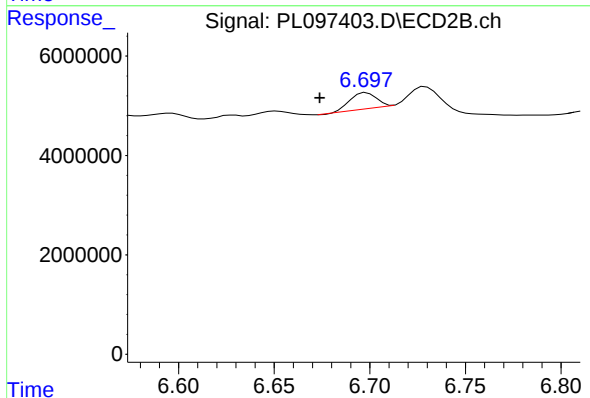


#20 Methoxychlor

R.T.: 6.698 min
Delta R.T.: 0.024 min
Response: 3087104
Conc: 0.82 ng/ml

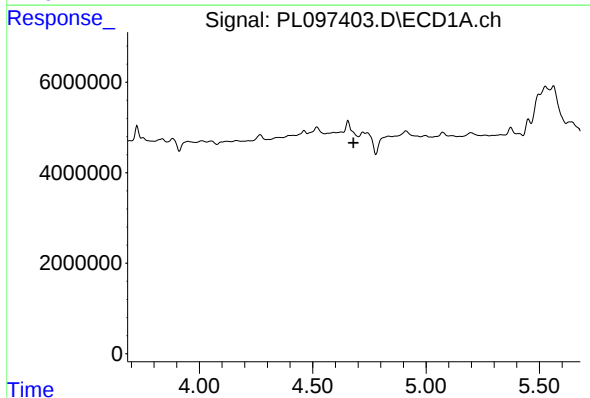


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.680 min
Response: 0
Conc: N.D.

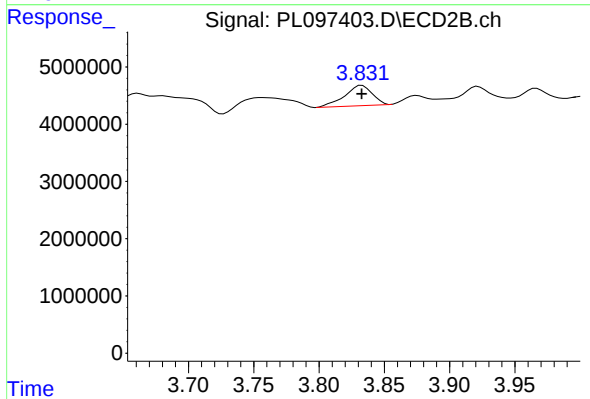

#23 Chlordane-1


R.T.: 3.833 min
Delta R.T.: 0.000 min
Response: 5216078
Conc: 20.52 ng/ml

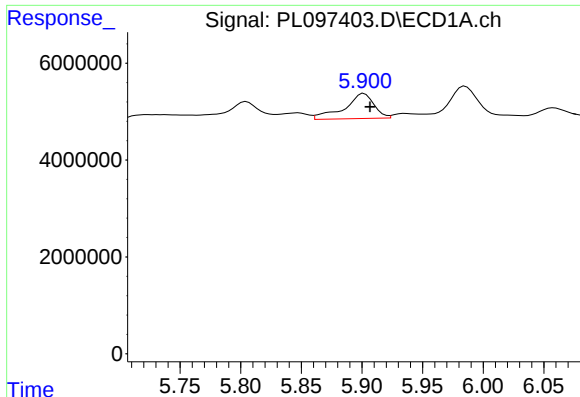

#25 Chlordane-3


R.T.: 5.902 min
Delta R.T.: -0.005 min
Response: 8762153
Conc: 10.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

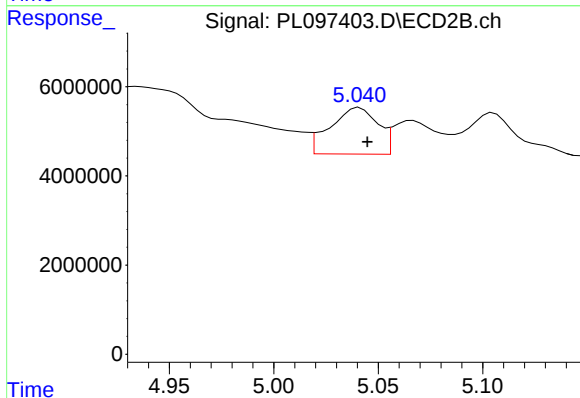


#25 Chlordane-3

R.T.: 5.041 min
Delta R.T.: -0.004 min
Response: 16489663
Conc: 18.44 ng/ml

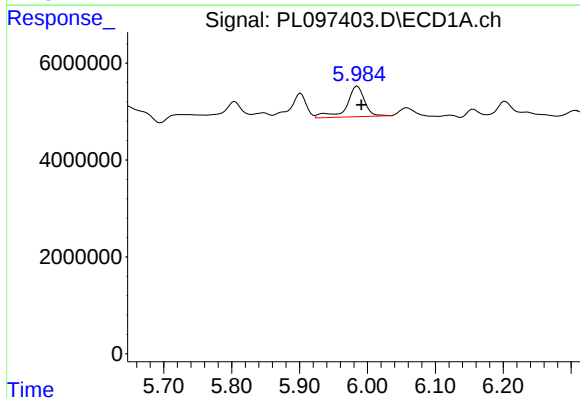


#26 Chlordane-4

R.T.: 5.985 min
Delta R.T.: -0.006 min
Response: 11598370
Conc: 11.60 ng/ml

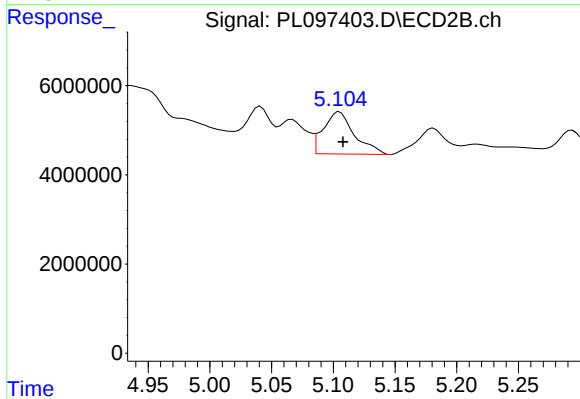

#26 Chlordane-4


R.T.: 5.105 min
Delta R.T.: -0.003 min
Response: 16544989
Conc: 21.73 ng/ml

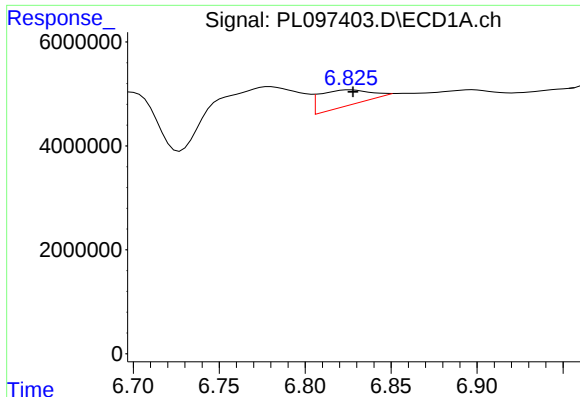

#27 Chlordane-5


R.T.: 6.826 min
Delta R.T.: -0.001 min
Response: 6181750
Conc: 36.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

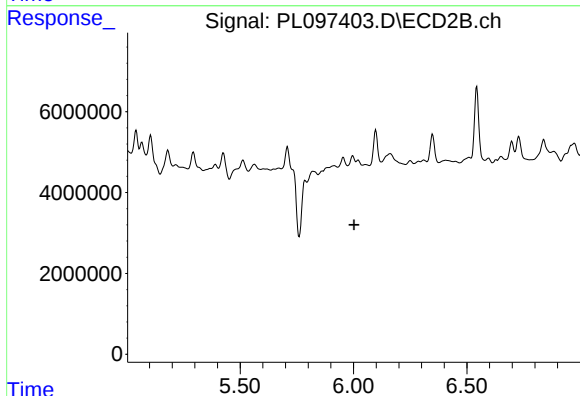


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.002 min
Response: 0
Conc: N.D.

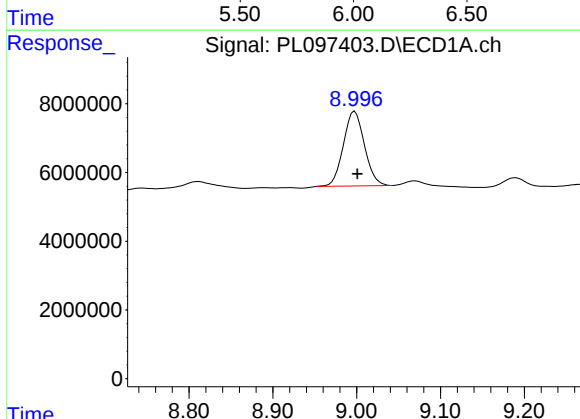

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: -0.003 min
Response: 38052773
Conc: 11.63 ng/ml

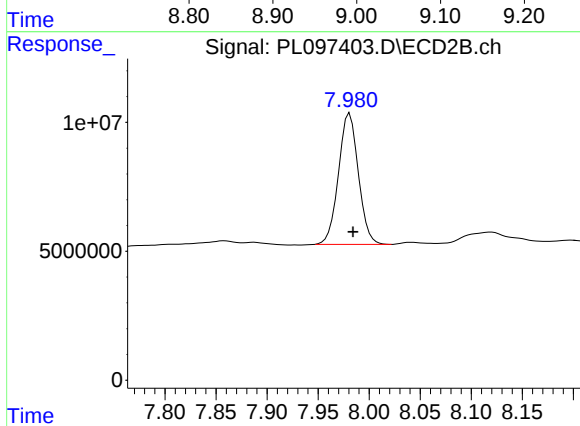

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: -0.003 min
Response: 68885796
Conc: 12.10 ng/ml