

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
 Data File : PL097407.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2025 13:40
 Operator : AR\AJ
 Sample : PB169826BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 14:10:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.526	2.823	83597127	126.8E6	18.466	19.283
28)	SA Decachlor...	8.996	7.981	65844285	83832132	20.122	14.729 #
Target Compounds							
8)	B Heptachlo...	5.642	0.000	10832745	0	1.885	N.D. #
14)	MA Endrin	0.000	5.709	0	24571579	N.D.	3.272 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
Data File : PL097407.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2025 13:40
Operator : AR\AJ
Sample : PB169826BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 14:10:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

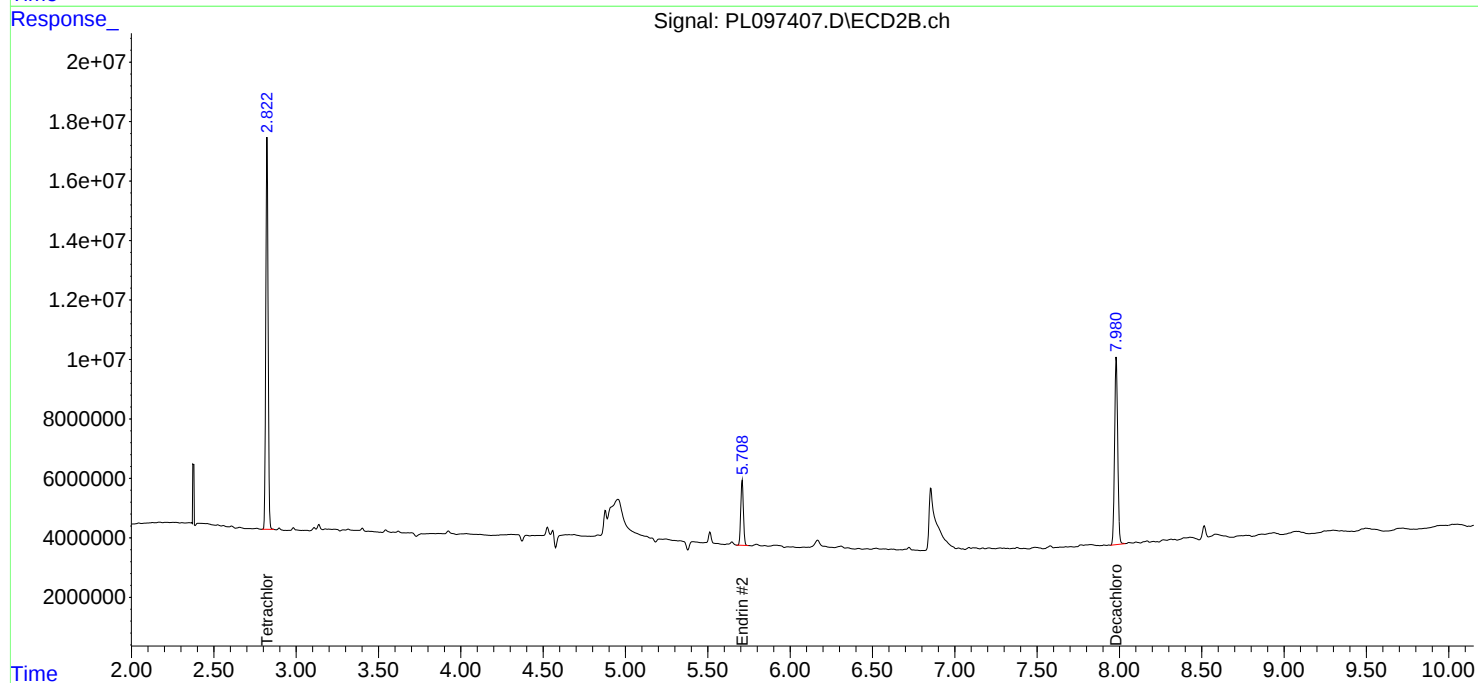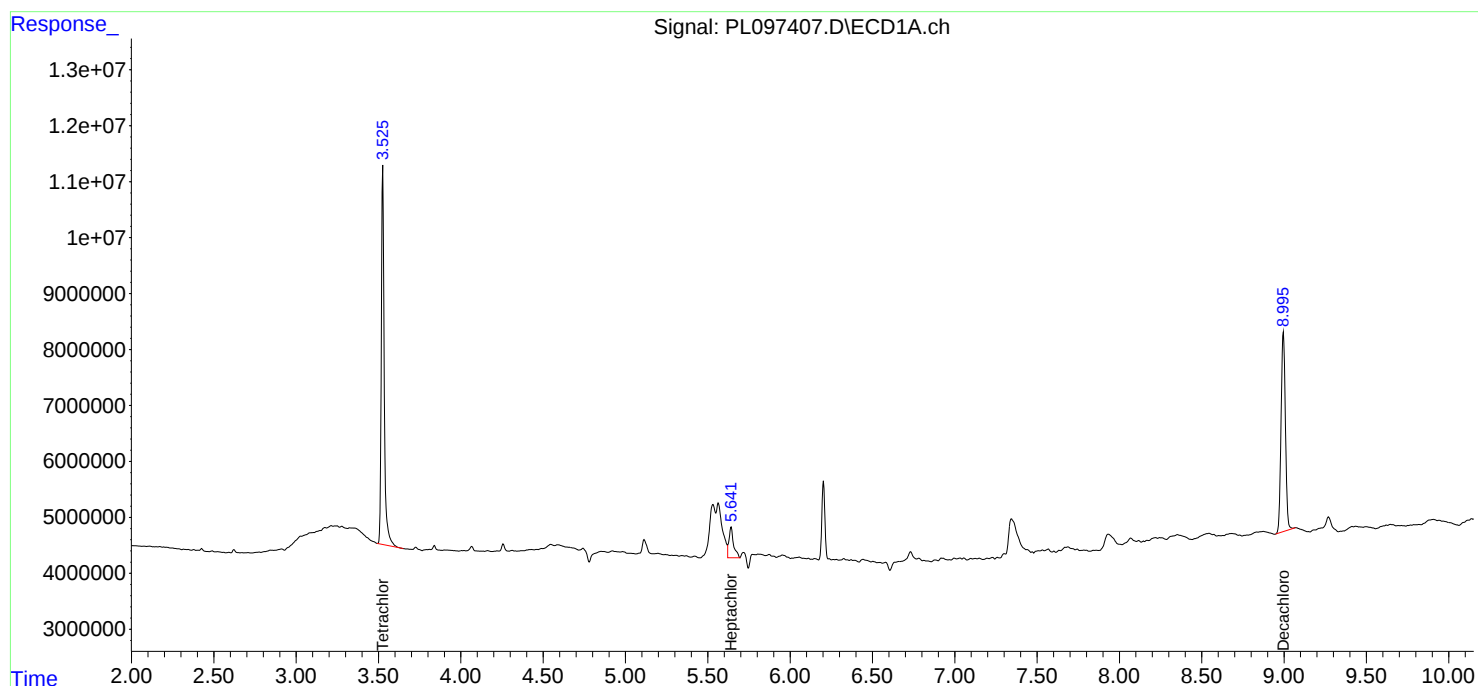


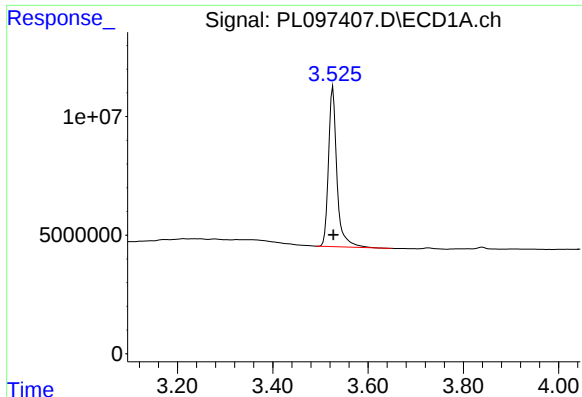

#1 Tetrachloro-m-xylene


R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 83597127
Conc: 18.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

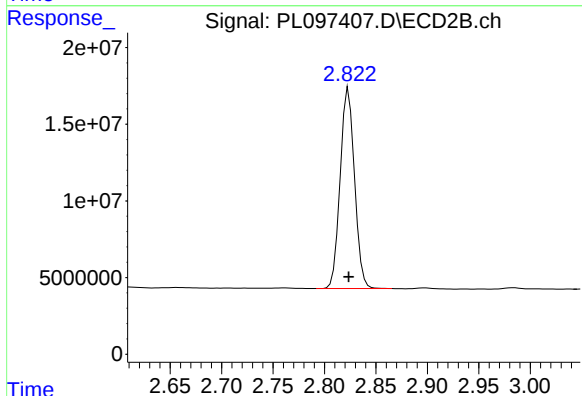


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 126793257
Conc: 19.28 ng/ml

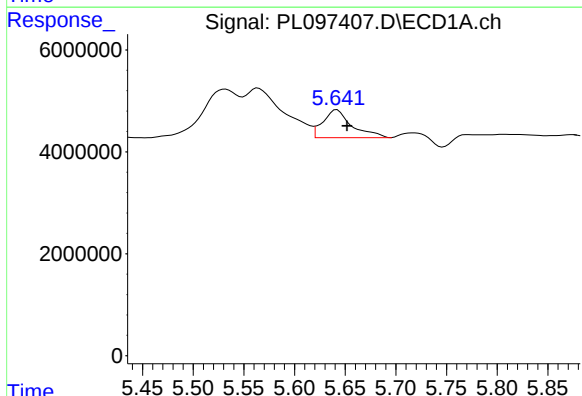


#8 Heptachlor epoxide

R.T.: 5.642 min
Delta R.T.: -0.010 min
Response: 10832745
Conc: 1.88 ng/ml

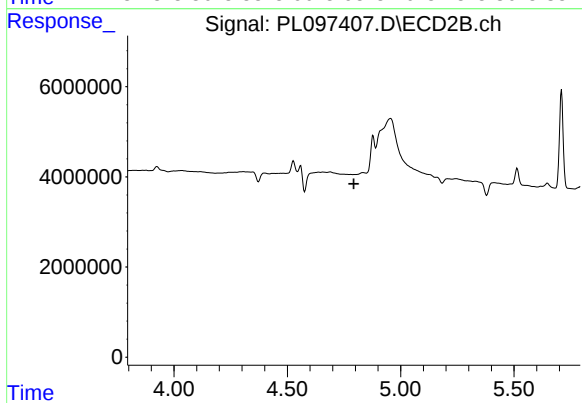

#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.793 min
Response: 0
Conc: N.D.

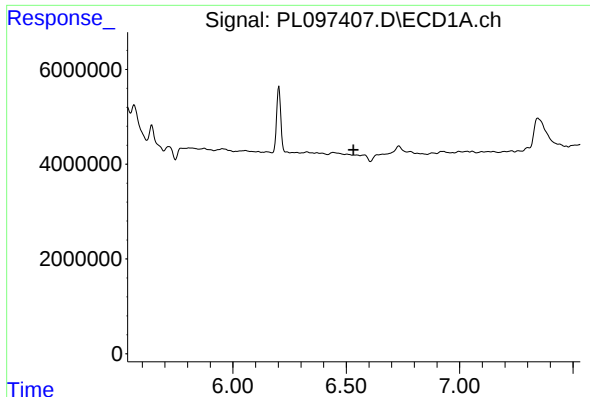

#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#14 Endrin

R.T.: 5.709 min
Delta R.T.: 0.007 min
Response: 24571579
Conc: 3.27 ng/ml

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.005 min
Response: 65844285
Conc: 20.12 ng/ml

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: -0.003 min
Response: 83832132
Conc: 14.73 ng/ml