

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
 Data File : PL097411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2025 17:03
 Operator : AR\AJ
 Sample : Q3170-01 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 02:30:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.823	0	5368026	N.D.	0.816 #
28)	SA Decachlor...	8.996	8.002	6852131	39010220	2.094	6.854 #
Target Compounds							
8)	B Heptachlo...	5.643	0.000	12111863	0	2.108	N.D. #
9)	A Endosulfan I	6.058f	0.000	27078361	0	5.226	N.D. #
13)	MA Dieldrin	0.000	5.428	0	36505229	N.D.	4.464 #
14)	MA Endrin	0.000	5.709	0	47932950	N.D.	6.382 #
15)	B Endosulfa...	6.732	5.997	9106289	25985393	1.851	3.655 #
16)	A 4,4'-DDD	6.648f	0.000	26686044	0	7.078	N.D. #
17)	MA 4,4'-DDT	6.988	0.000	8397634	0	1.987	N.D. #
18)	B Endrin al...	0.000	6.186	0	8062486	N.D.	1.511 #
20)	A Methoxychlor	0.000	6.699f	0	22439020	N.D.	5.953 #
27)	Chlordane-5	6.830	5.997	20693283	25985393	123.444	87.158 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
Data File : PL097411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2025 17:03
Operator : AR\AJ
Sample : Q3170-01 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 02:30:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

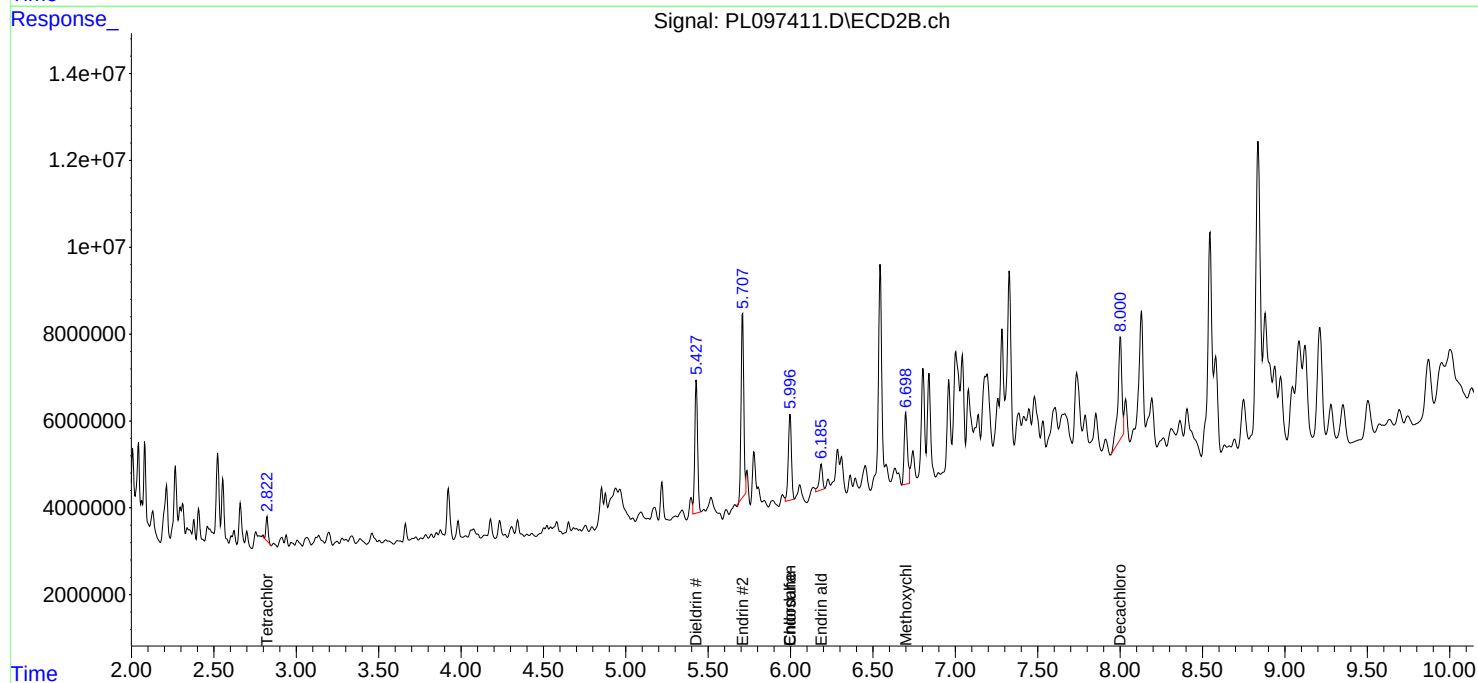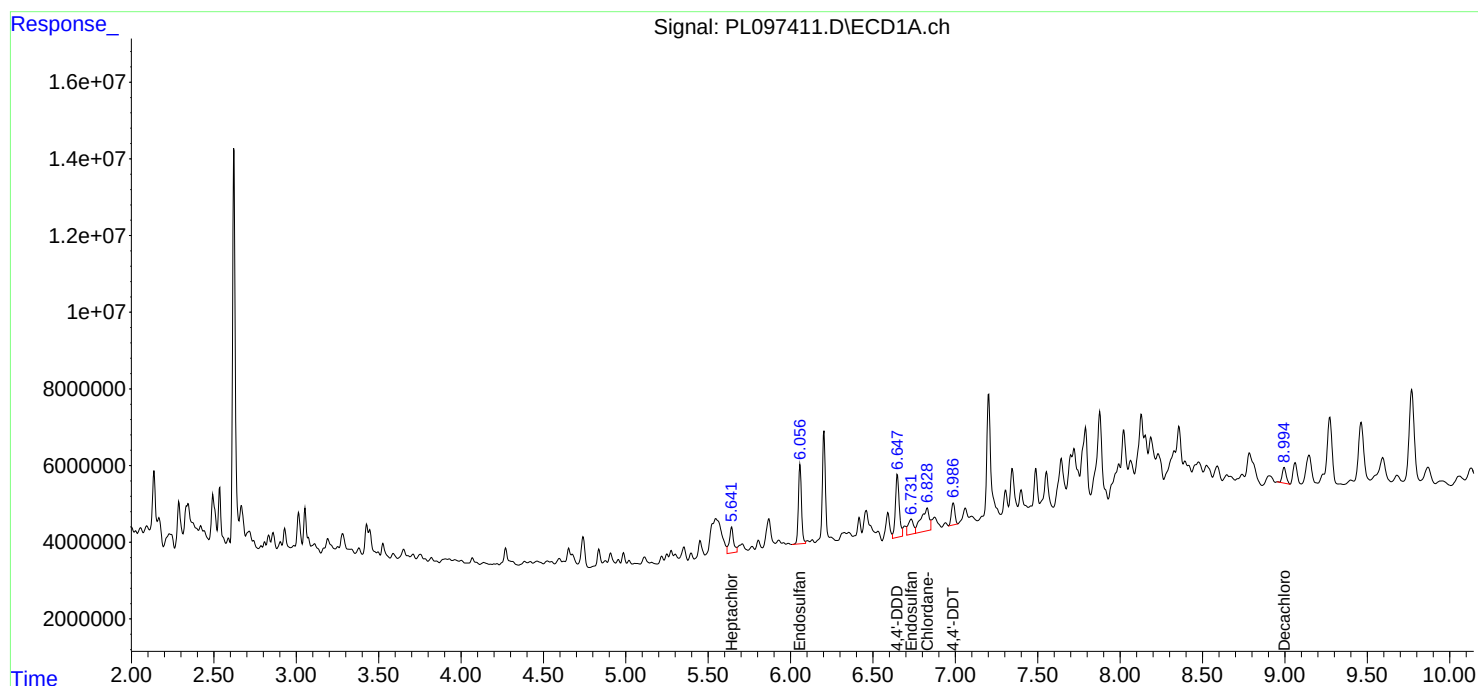


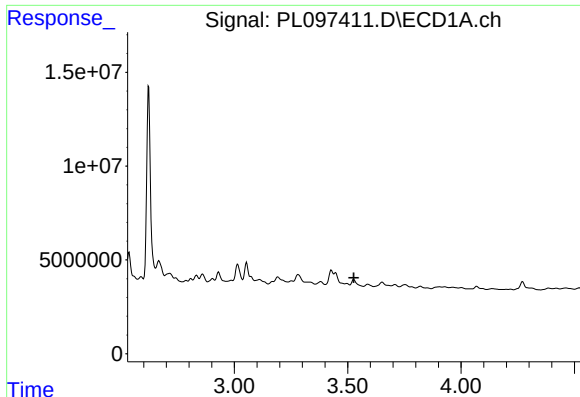

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

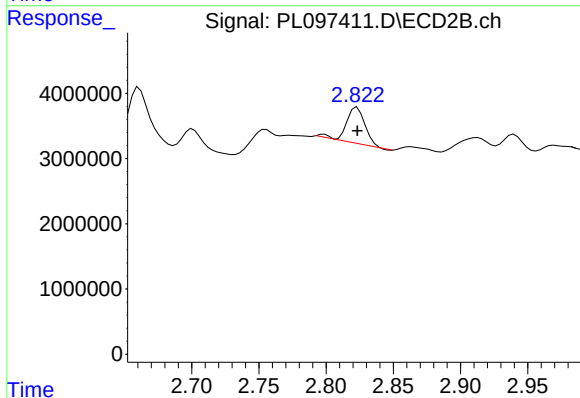


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 5368026
Conc: 0.82 ng/ml

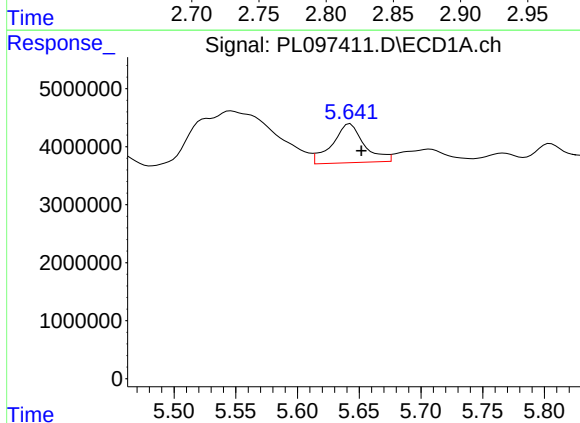


#8 Heptachlor epoxide

R.T.: 5.643 min
Delta R.T.: -0.009 min
Response: 12111863
Conc: 2.11 ng/ml

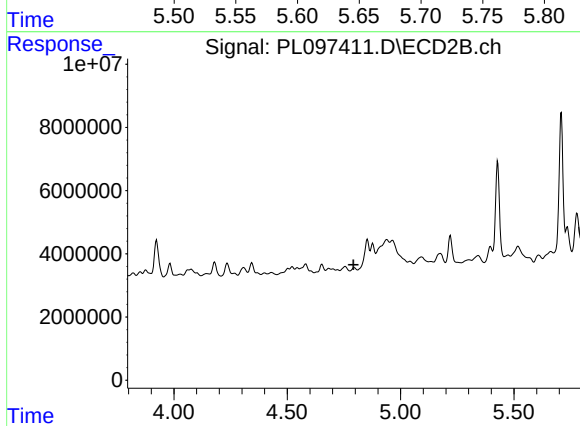

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.793 min
Response: 0
Conc: N.D.

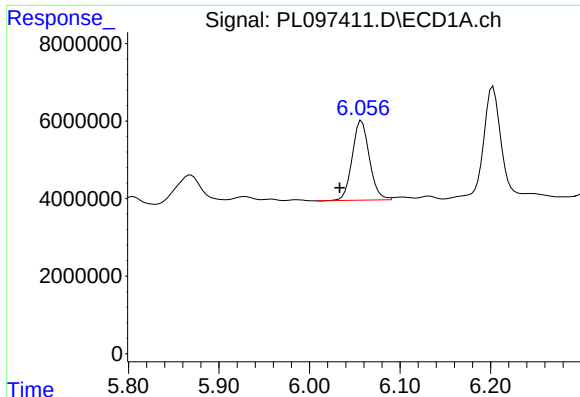

#9 Endosulfan I


R.T.: 6.058 min
Delta R.T.: 0.024 min
Response: 27078361
Conc: 5.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

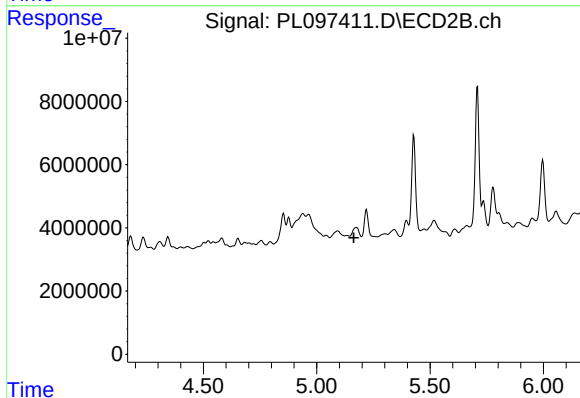


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.163 min
Response: 0
Conc: N.D.

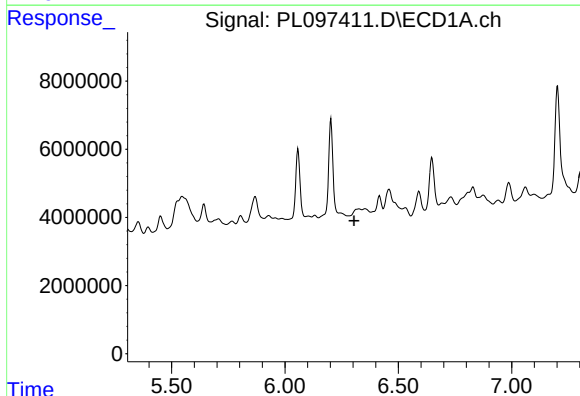


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.306 min
Response: 0
Conc: N.D.

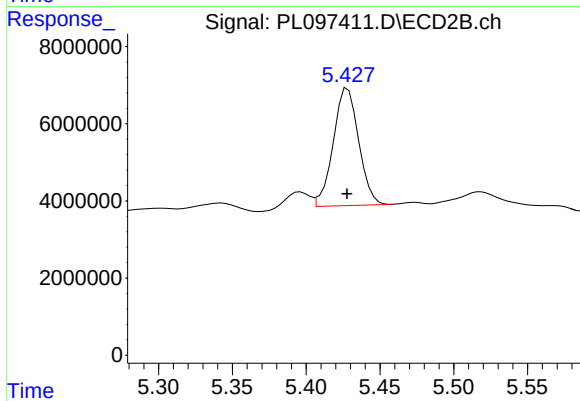

#13 Dieldrin


R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 36505229
Conc: 4.46 ng/ml

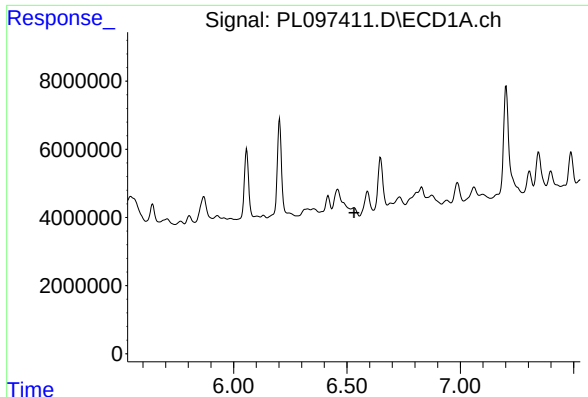

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

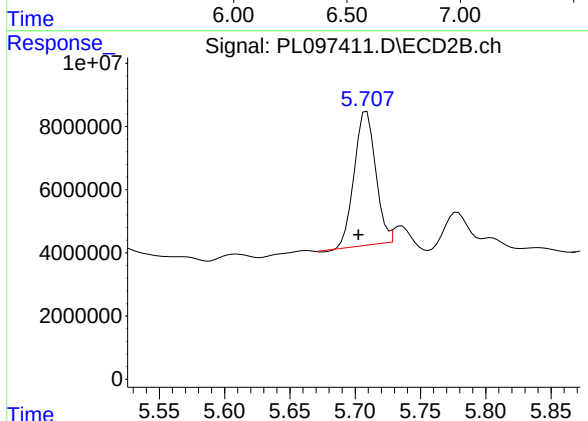


#14 Endrin

R.T.: 5.709 min
Delta R.T.: 0.006 min
Response: 47932950
Conc: 6.38 ng/ml

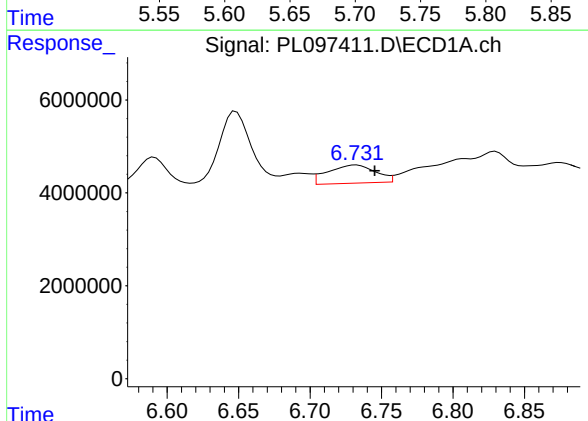


#15 Endosulfan II

R.T.: 6.732 min
Delta R.T.: -0.013 min
Response: 9106289
Conc: 1.85 ng/ml

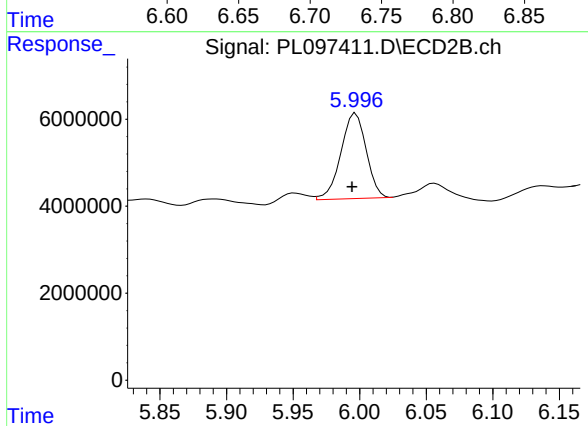

#15 Endosulfan II


R.T.: 5.997 min
Delta R.T.: 0.003 min
Response: 25985393
Conc: 3.66 ng/ml

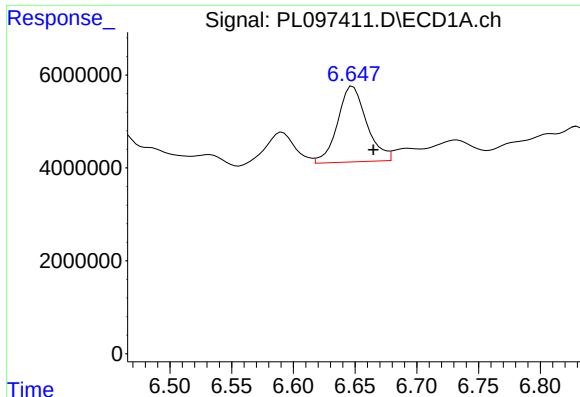

#16 4,4'-DDD


R.T.: 6.648 min
Delta R.T.: -0.017 min
Response: 26686044
Conc: 7.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

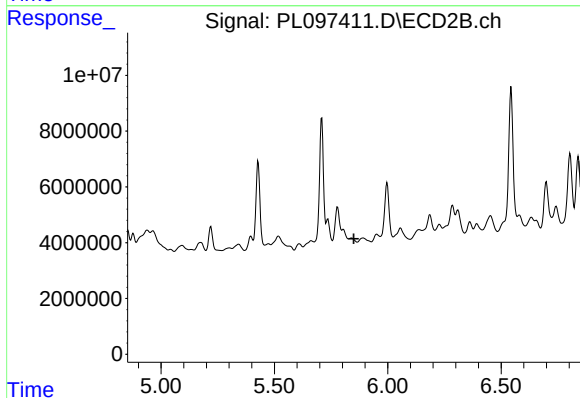


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.850 min
Response: 0
Conc: N.D.

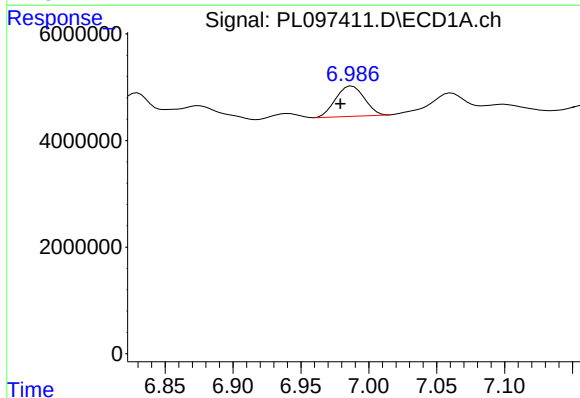


#17 4,4'-DDT

R.T.: 6.988 min
Delta R.T.: 0.009 min
Response: 8397634
Conc: 1.99 ng/ml

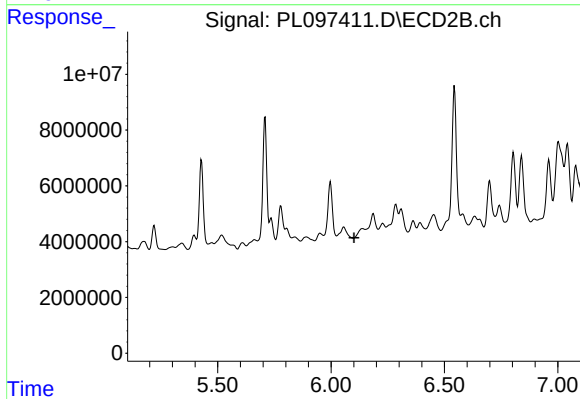

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

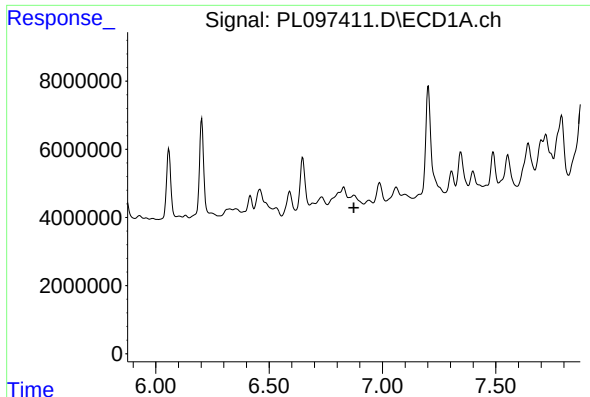

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

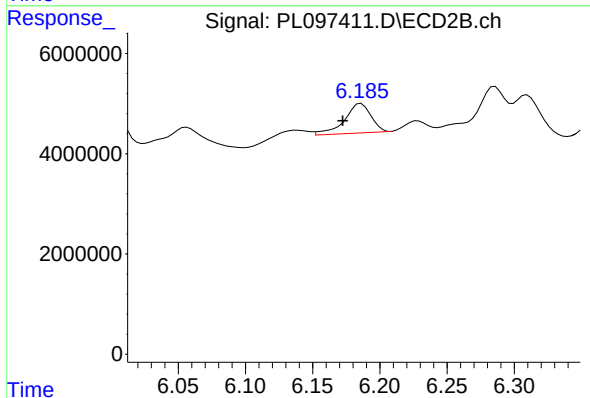


#18 Endrin aldehyde

R.T.: 6.186 min
Delta R.T.: 0.014 min
Response: 8062486
Conc: 1.51 ng/ml

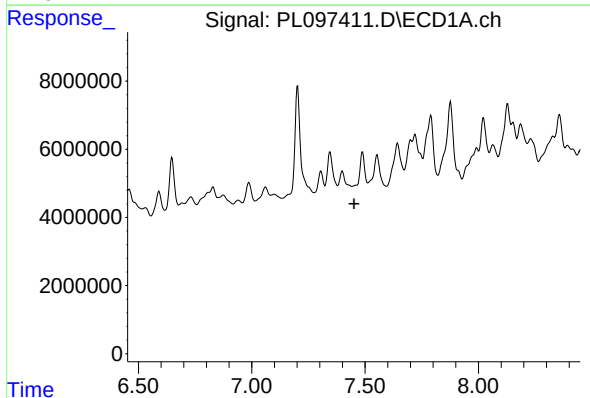


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.452 min
Response: 0
Conc: N.D.

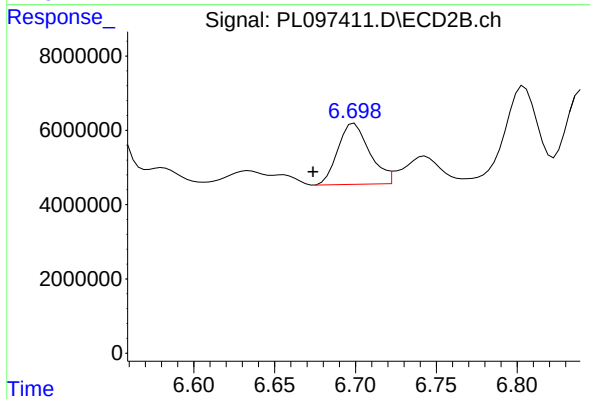

#20 Methoxychlor


R.T.: 6.699 min
Delta R.T.: 0.025 min
Response: 22439020
Conc: 5.95 ng/ml

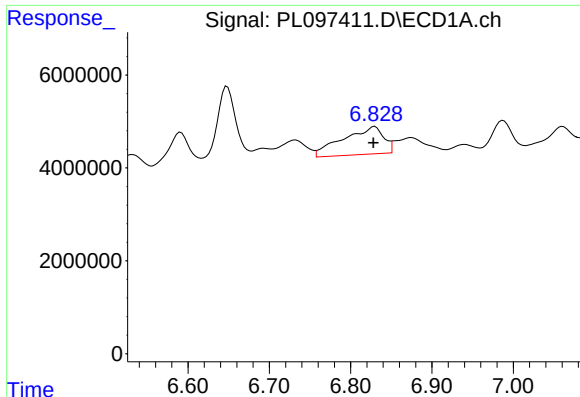

#27 Chlordane-5


R.T.: 6.830 min
Delta R.T.: 0.002 min
Response: 20693283
Conc: 123.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

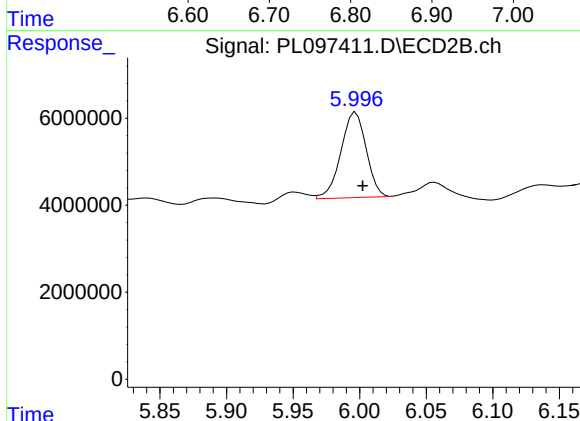


#27 Chlordane-5

R.T.: 5.997 min
Delta R.T.: -0.005 min
Response: 25985393
Conc: 87.16 ng/ml

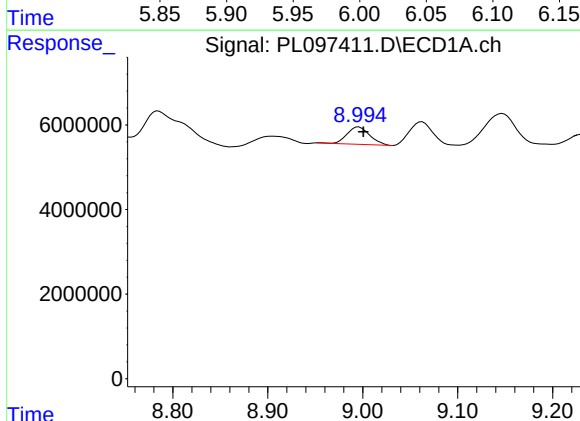

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.005 min
Response: 6852131
Conc: 2.09 ng/ml

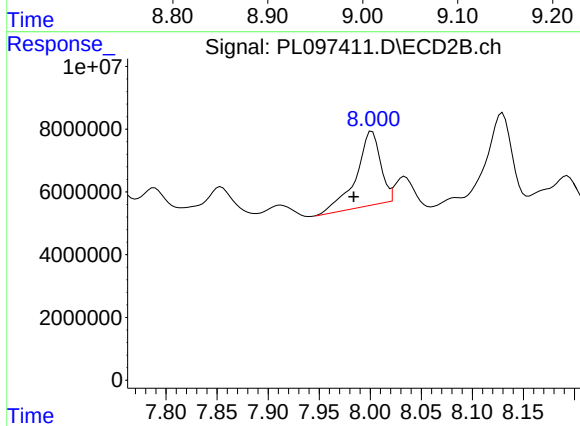

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: 0.018 min
Response: 39010220
Conc: 6.85 ng/ml