

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
 Data File : PL097429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2025 21:08
 Operator : AR\AJ
 Sample : Q3208-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 02:32:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.526	2.824	37919142	55720498	8.376	8.474
28)	SA Decachlor...	8.997	7.981	28133565	45270774	8.598	7.954
Target Compounds							
10)	B gamma-Chl...	5.928f	5.046	32660205	35726088	5.777	4.091 #
11)	B alpha-Chl...	5.990	0.000	24826745	0	4.371	N.D. #
12)	B 4,4'-DDE	6.154	5.296	208.0E6	323.8E6	43.656	42.142
13)	MA Dieldrin	0.000	5.427	0	10595799	N.D.	1.296 #
14)	MA Endrin	0.000	5.711	0	35585349	N.D.	4.738 #
16)	A 4,4'-DDD	6.664	5.847	32632849	27672411	8.655	4.291 #
17)	MA 4,4'-DDT	6.976	6.100	202.5E6	302.1E6	47.905	43.657
19)	B Endosulfa...	0.000	6.395	0	8732925	N.D.	1.275 #
20)	A Methoxychlor	0.000	6.651f	0	5591102	N.D.	1.483 #
21)	B Endrin ke...	7.569f	0.000	17011081	0	4.008	N.D. #
25)	Chlordane-3	5.928f	5.046	32660205	35726088	40.042	39.952
26)	Chlordane-4	5.990	0.000	24826745	0	24.821	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
Data File : PL097429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2025 21:08
Operator : AR\AJ
Sample : Q3208-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 02:32:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

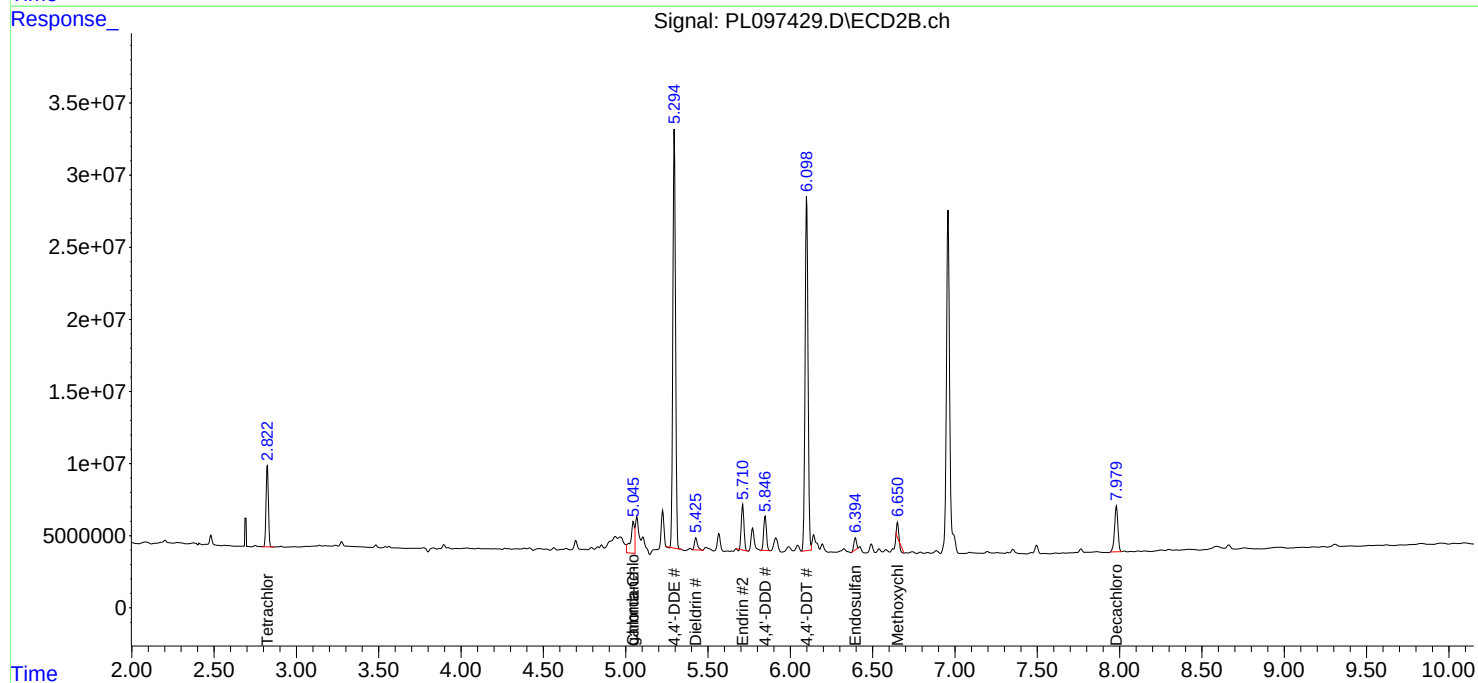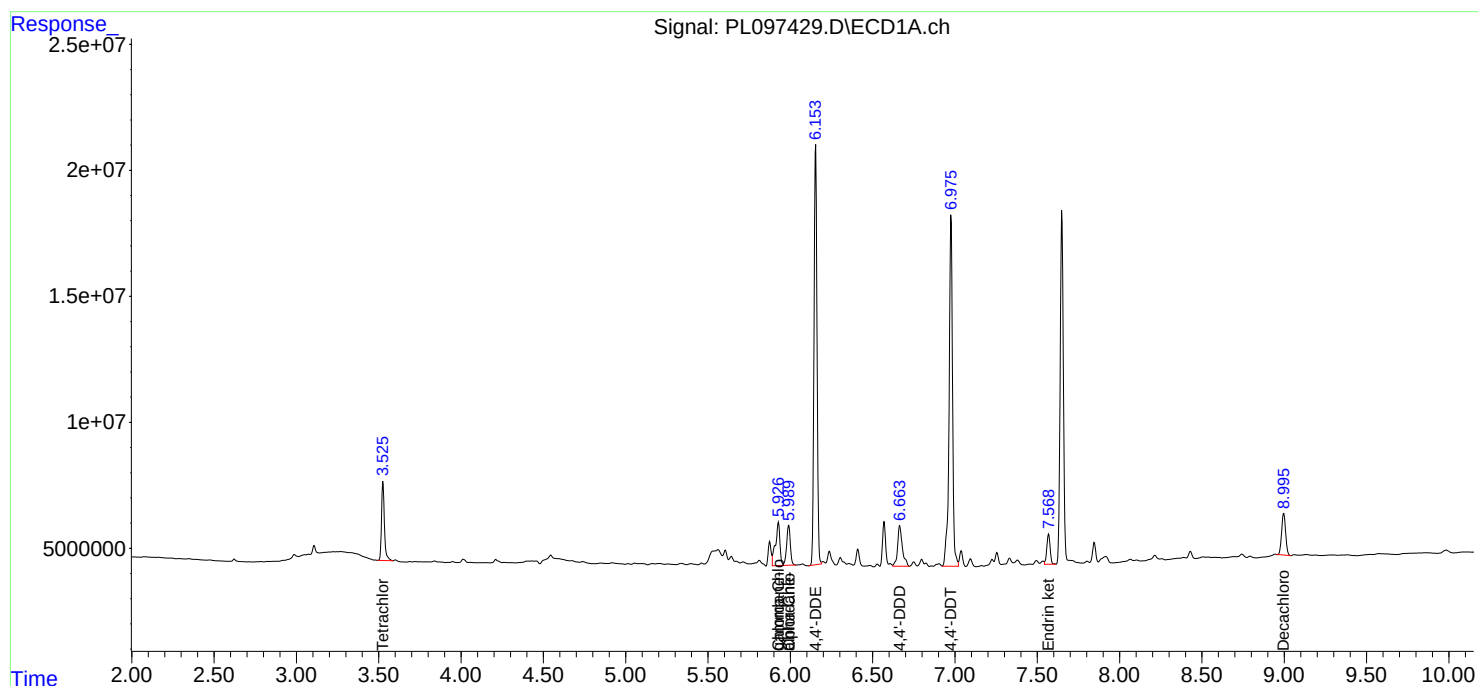


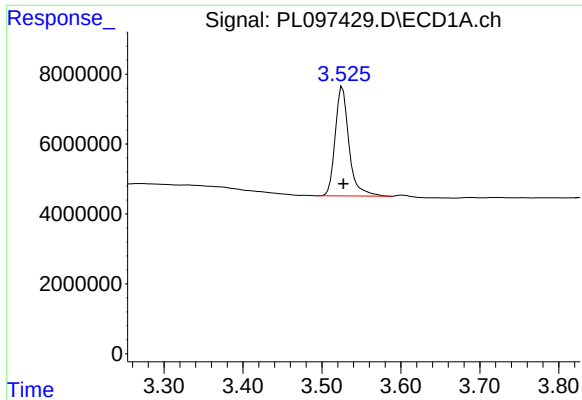

#1 Tetrachloro-m-xylene


R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 37919142
Conc: 8.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

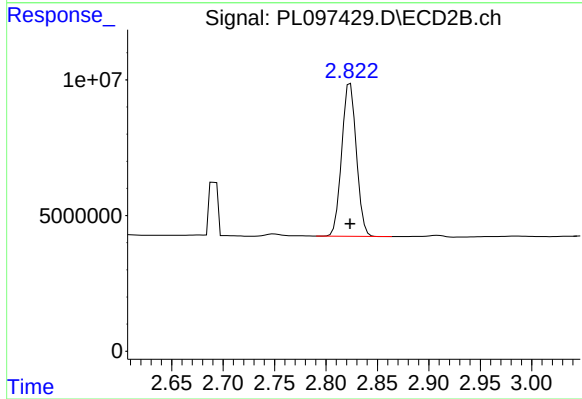


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.000 min
Response: 55720498
Conc: 8.47 ng/ml

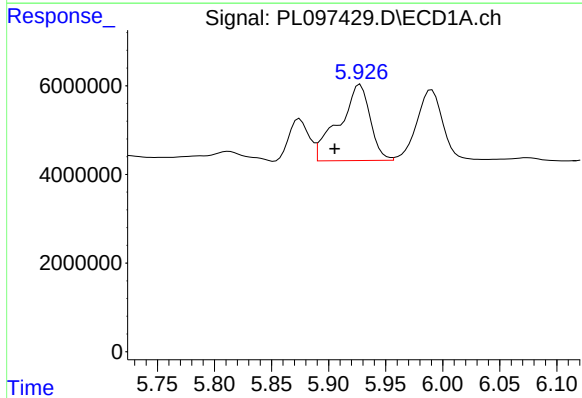


#10 gamma-Chlordane

R.T.: 5.928 min
Delta R.T.: 0.022 min
Response: 32660205
Conc: 5.78 ng/ml

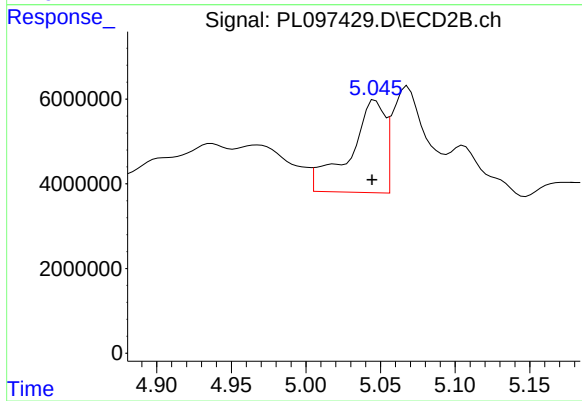

#10 gamma-Chlordane


R.T.: 5.046 min
Delta R.T.: 0.002 min
Response: 35726088
Conc: 4.09 ng/ml

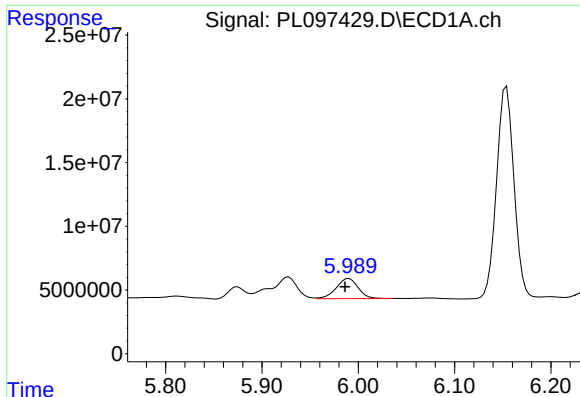

#11 alpha-Chlordane


R.T.: 5.990 min
Delta R.T.: 0.004 min
Response: 24826745
Conc: 4.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

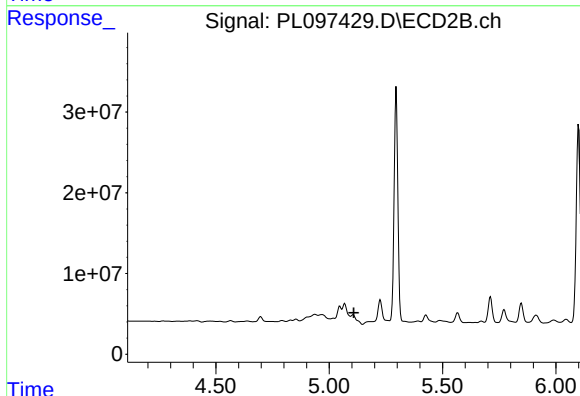


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

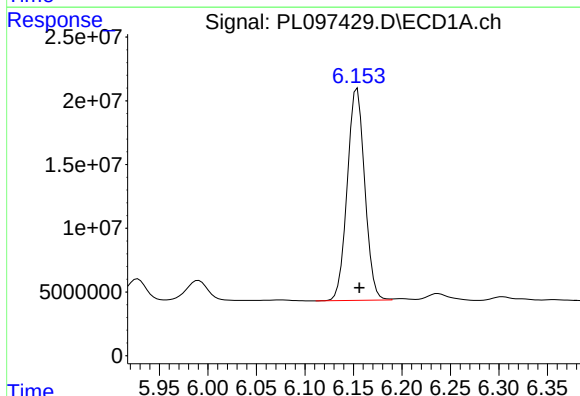


#12 4,4'-DDE

R.T.: 6.154 min
Delta R.T.: -0.002 min
Response: 208009383
Conc: 43.66 ng/ml

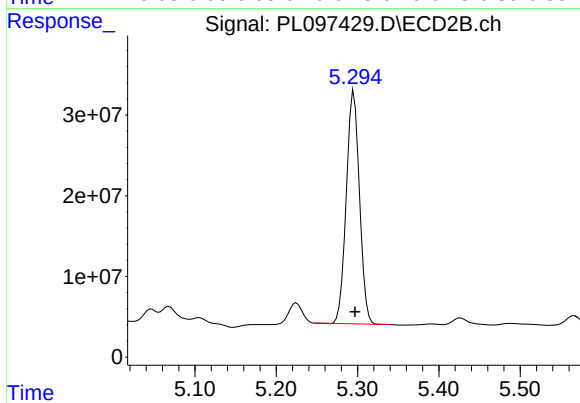

#12 4,4'-DDE


R.T.: 5.296 min
Delta R.T.: -0.001 min
Response: 323849682
Conc: 42.14 ng/ml

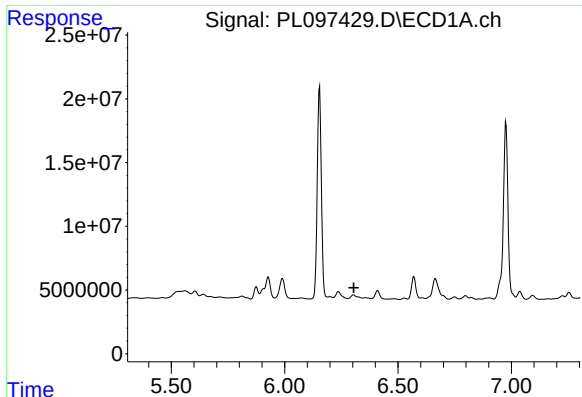

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

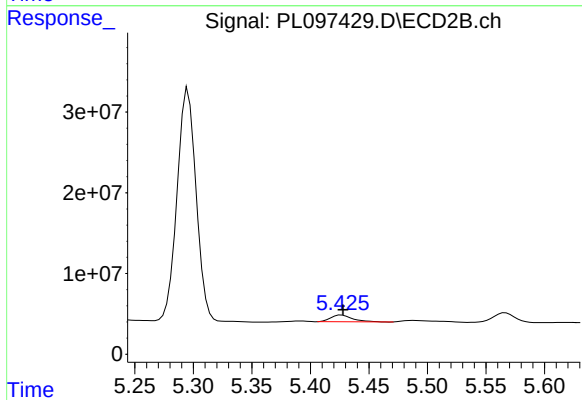


#13 Dieldrin

R.T.: 5.427 min
Delta R.T.: -0.001 min
Response: 10595799
Conc: 1.30 ng/ml

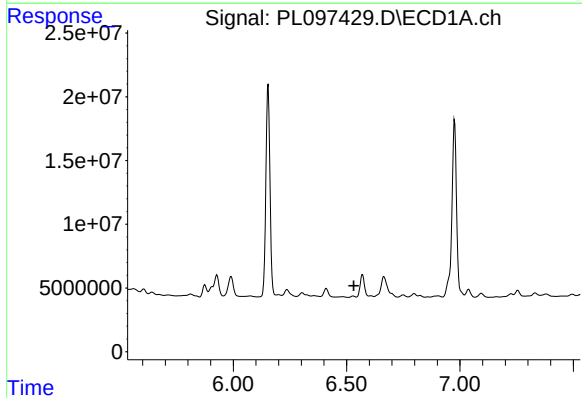


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

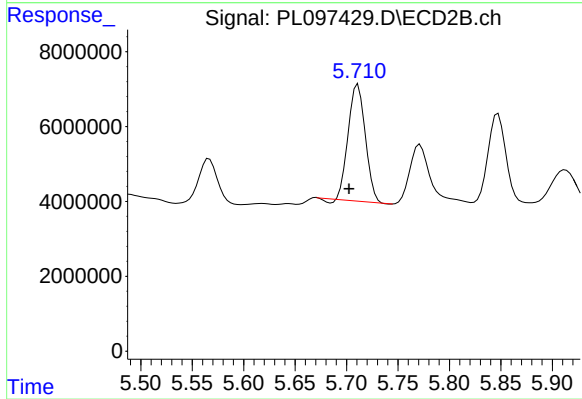

#14 Endrin


R.T.: 5.711 min
Delta R.T.: 0.009 min
Response: 35585349
Conc: 4.74 ng/ml

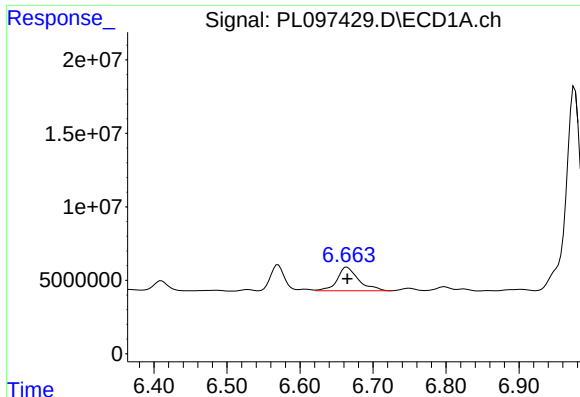

#16 4,4'-DDD


R.T.: 6.664 min
Delta R.T.: 0.000 min
Response: 32632849
Conc: 8.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

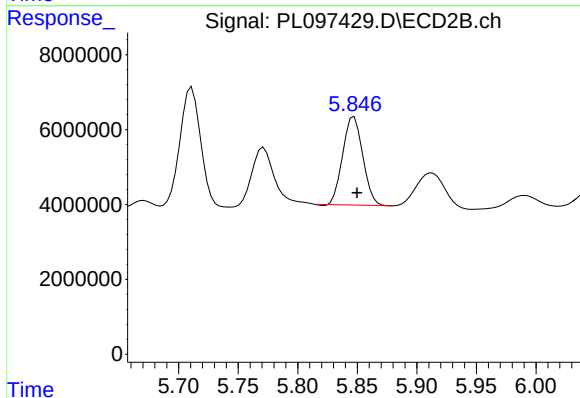


#16 4,4'-DDD

R.T.: 5.847 min
Delta R.T.: -0.002 min
Response: 27672411
Conc: 4.29 ng/ml

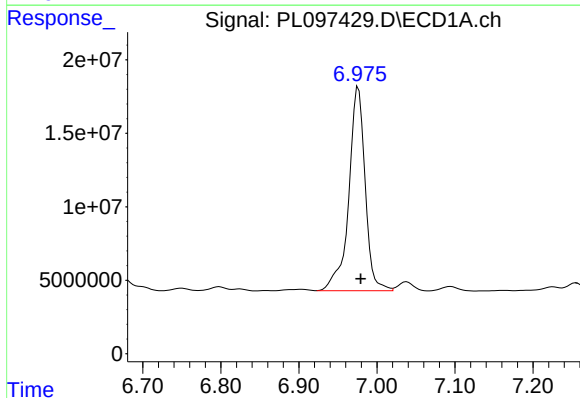


#17 4,4'-DDT

R.T.: 6.976 min
Delta R.T.: -0.003 min
Response: 202504347
Conc: 47.91 ng/ml

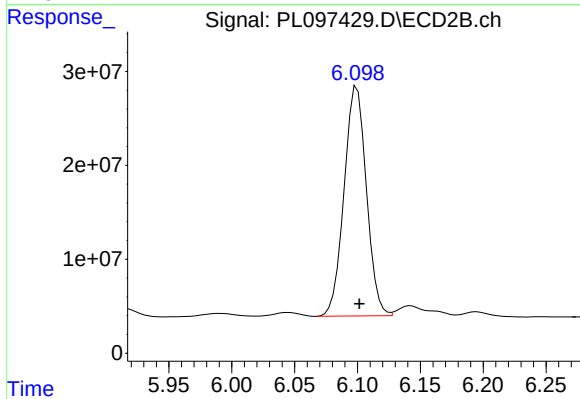

#17 4,4'-DDT


R.T.: 6.100 min
Delta R.T.: -0.002 min
Response: 302129090
Conc: 43.66 ng/ml

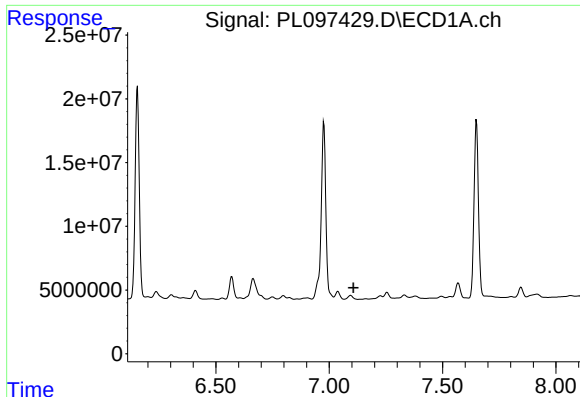

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

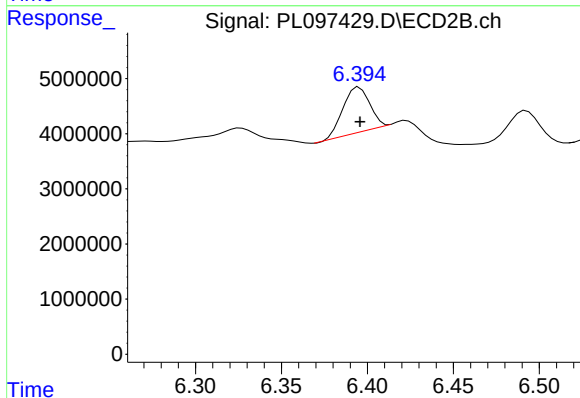


#19 Endosulfan Sulfate

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 8732925
Conc: 1.27 ng/ml

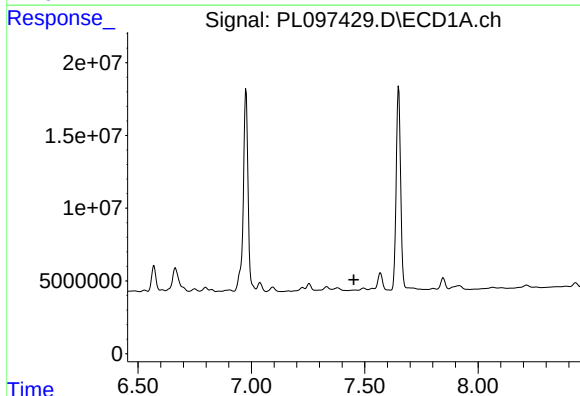


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.452 min
Response: 0
Conc: N.D.

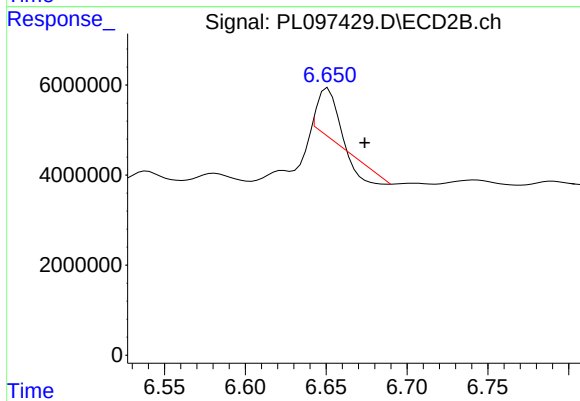

#20 Methoxychlor


R.T.: 6.651 min
Delta R.T.: -0.023 min
Response: 5591102
Conc: 1.48 ng/ml

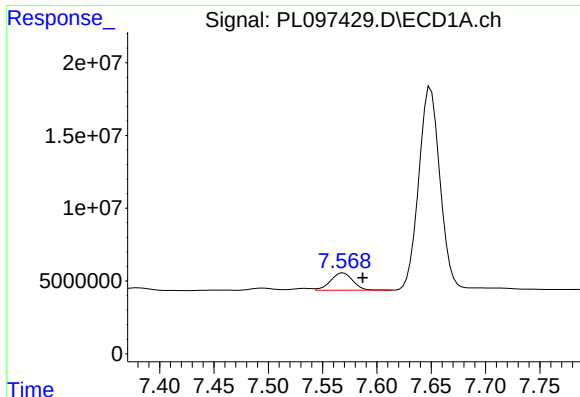

#21 Endrin ketone


R.T.: 7.569 min
Delta R.T.: -0.018 min
Response: 17011081
Conc: 4.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

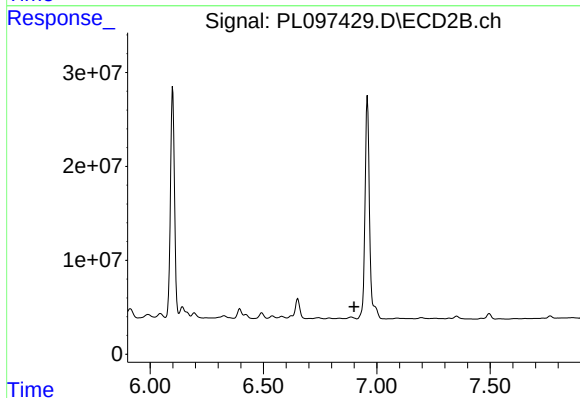


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.900 min
Response: 0
Conc: N.D.

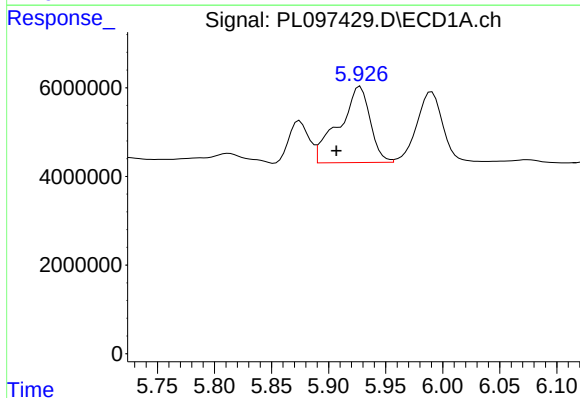


#25 Chlordane-3

R.T.: 5.928 min
Delta R.T.: 0.021 min
Response: 32660205
Conc: 40.04 ng/ml

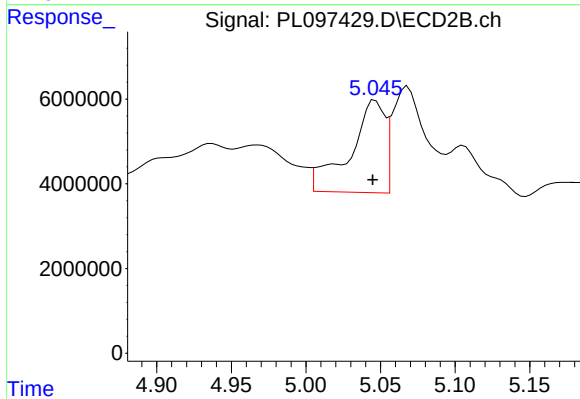

#25 Chlordane-3


R.T.: 5.046 min
Delta R.T.: 0.002 min
Response: 35726088
Conc: 39.95 ng/ml

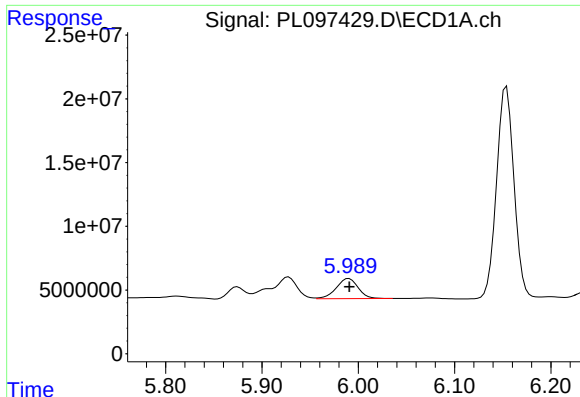

#26 Chlordane-4


R.T.: 5.990 min
Delta R.T.: 0.000 min
Response: 24826745
Conc: 24.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

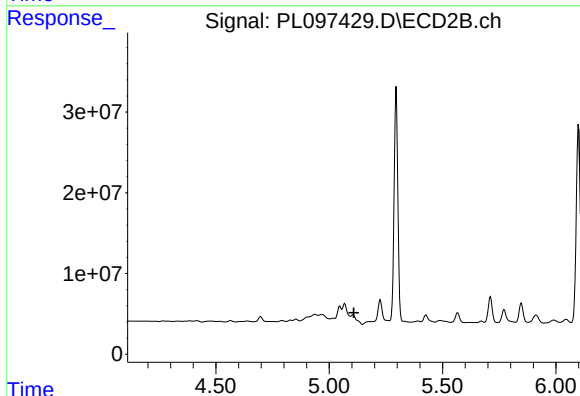


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

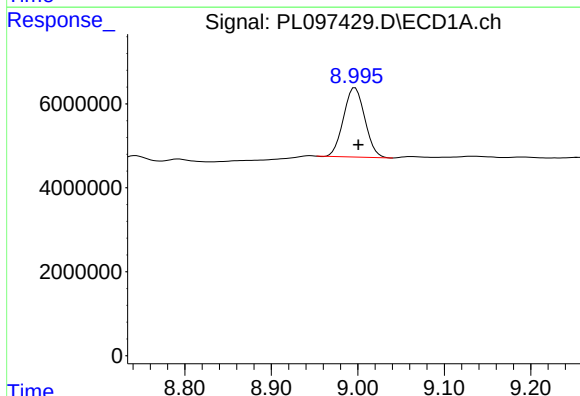

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: -0.004 min
Response: 28133565
Conc: 8.60 ng/ml

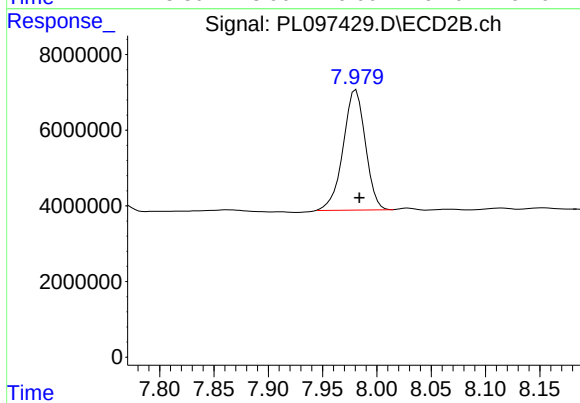

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: -0.003 min
Response: 45270774
Conc: 7.95 ng/ml