

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
 Data File : PL097405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2025 13:13
 Operator : AR\AJ
 Sample : Q3209-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-02-092525

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/30/2025
 Supervised By : mohammad ahmed 10/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 14:09:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.526	2.821	38630290	56965952	8.533	8.663m
28) SA Decachlor...	8.997	7.982	27339900	36557466	8.355	6.423

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092925\
Data File : PL097405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2025 13:13
Operator : AR\AJ
Sample : Q3209-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PL-02-092525


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/30/2025
Supervised By :mohammad ahmed 10/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 14:09:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

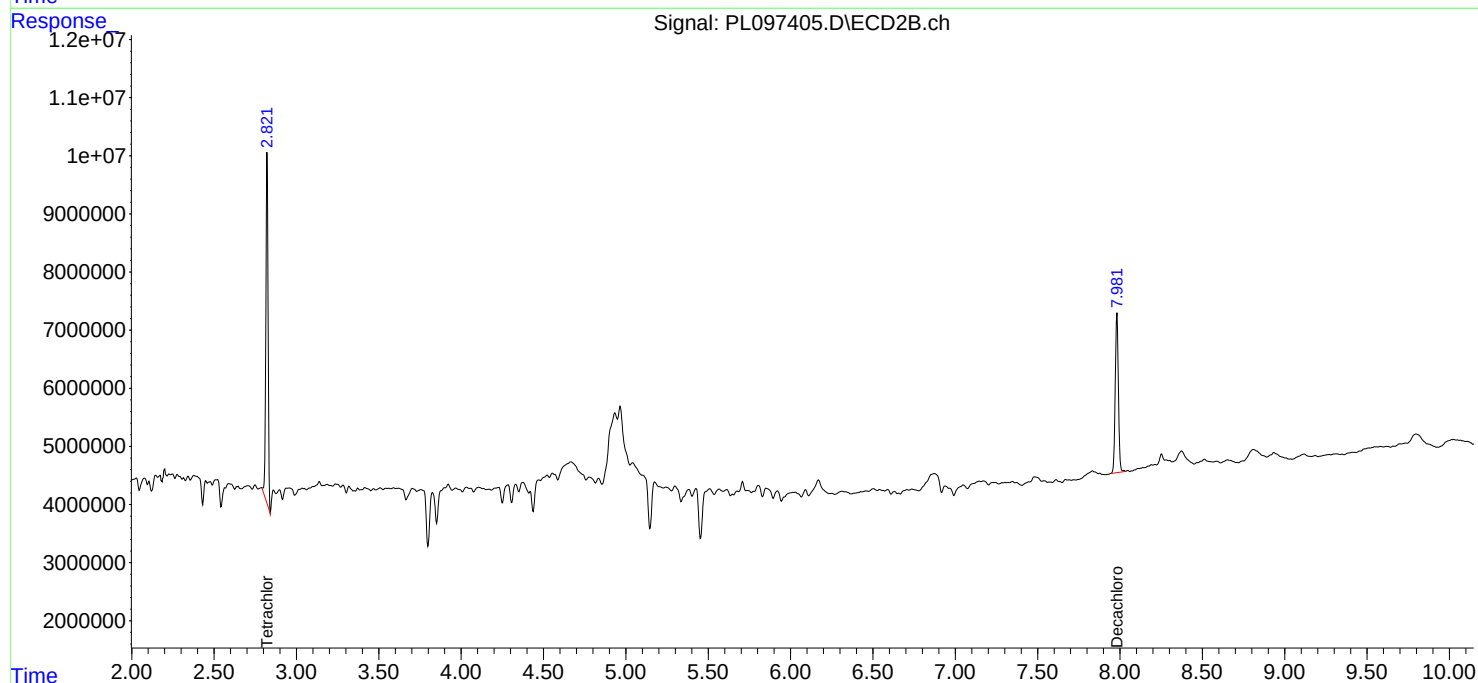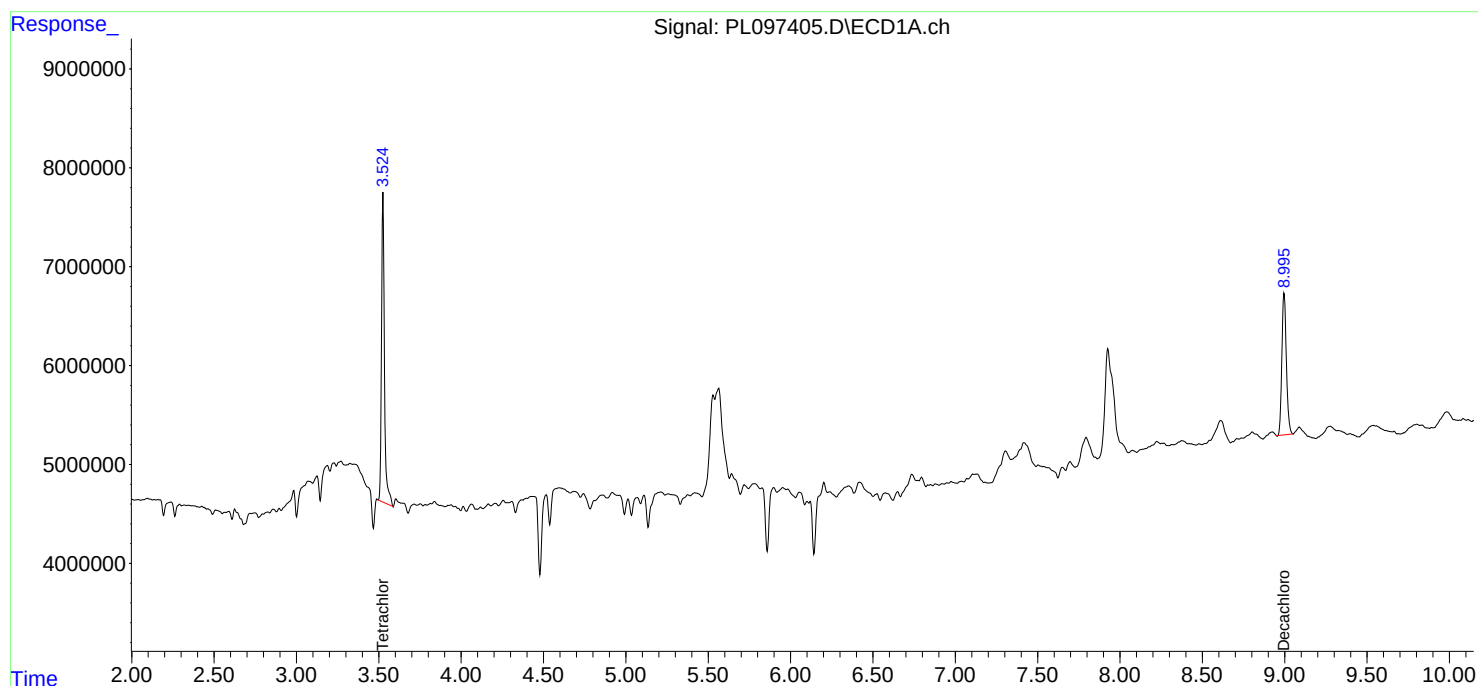

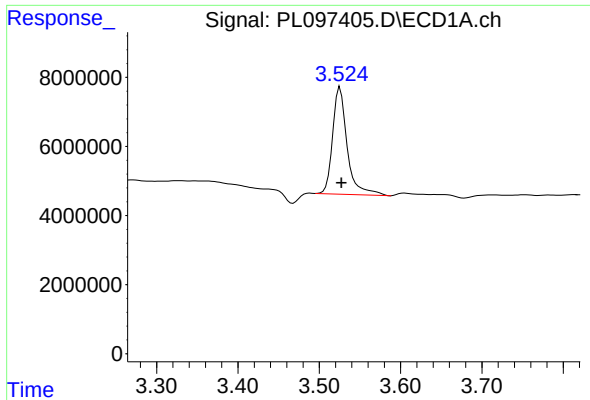


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.001 min
Response: 38630290
Conc: 8.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-092525


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/30/2025
Supervised By :mohammad ahmed 10/01/2025

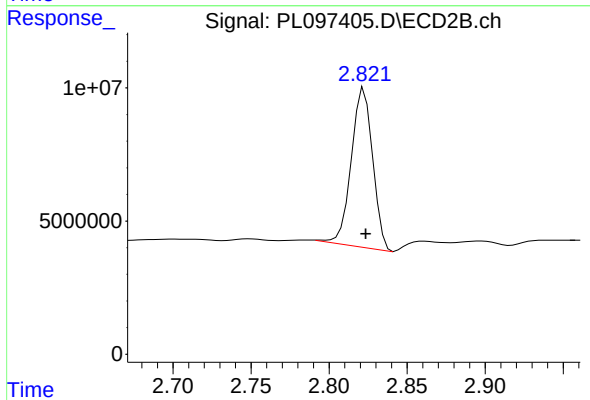


#1 Tetrachloro-m-xylene

R.T.: 2.821 min
Delta R.T.: -0.002 min
Response: 56965952
Conc: 8.66 ng/ml m

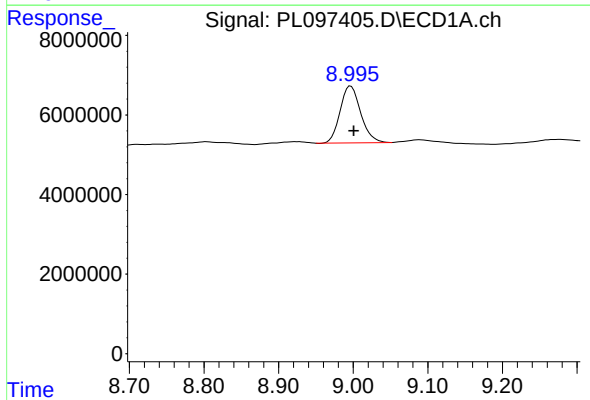

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: -0.004 min
Response: 27339900
Conc: 8.36 ng/ml

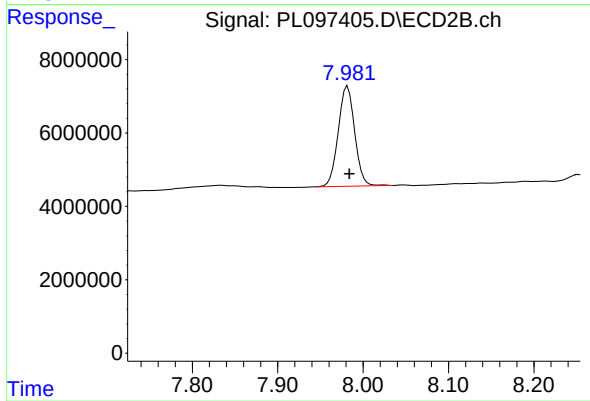

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: -0.002 min
Response: 36557466
Conc: 6.42 ng/ml