

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093019\
 Data File : PL052854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 16:02
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 00:58:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	4.047	224.6E6	59093248	22.585	22.007
28)	SA Decachlor...	8.346	9.124	232.2E6	66737176	23.183	22.748
Target Compounds							
8)	B Heptachlo...	0.000	5.918	0	989043	N.D.	0.295 #
9)	A Endosulfan I	0.000	6.277	0	565460	N.D.	0.181 #
10)	B gamma-Chl...	0.000	6.131f	0	1131212	N.D.	0.334 #
11)	B alpha-Chl...	0.000	6.240	0	401111	N.D.	0.119 #
25)	Chlordane-3	0.000	6.131f	0	1131212	N.D.	2.597 #
26)	Chlordane-4	0.000	6.240	0	401111	N.D.	0.755 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093019\
Data File : PL052854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 16:02
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 00:58:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

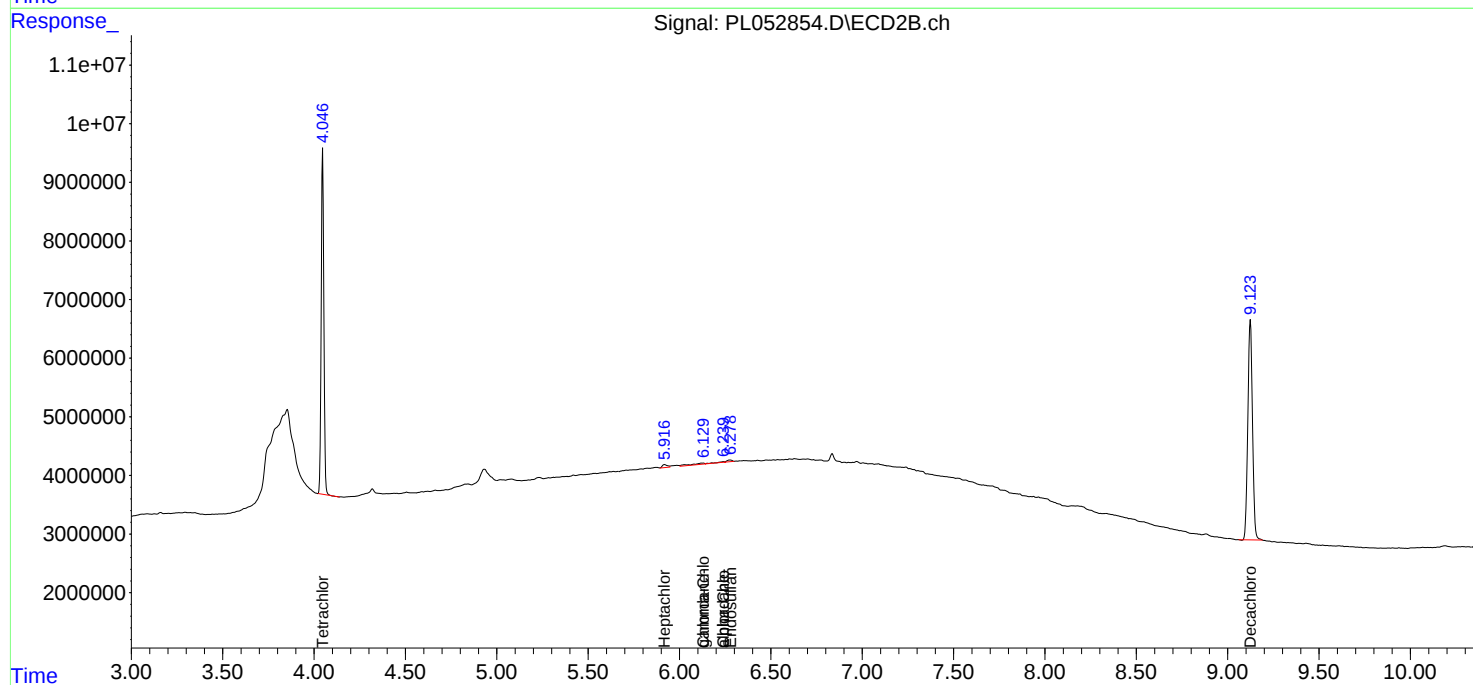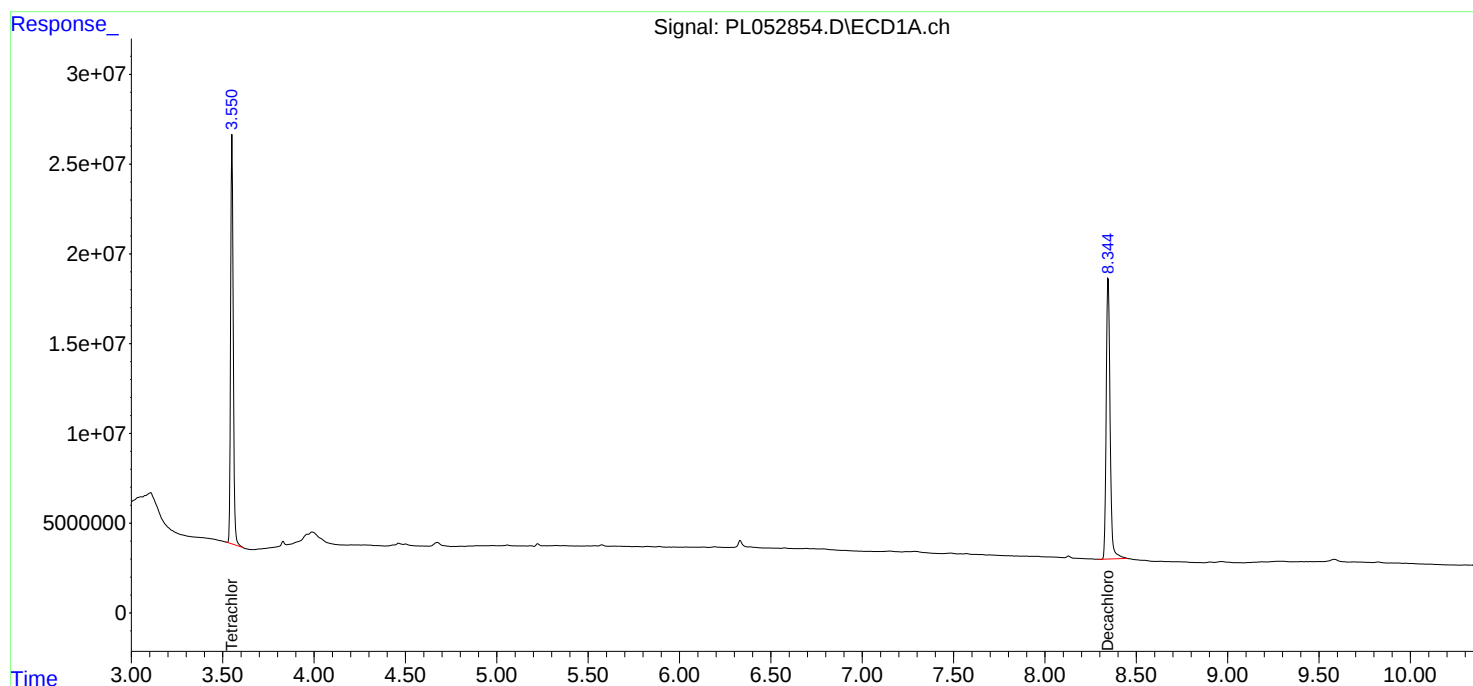


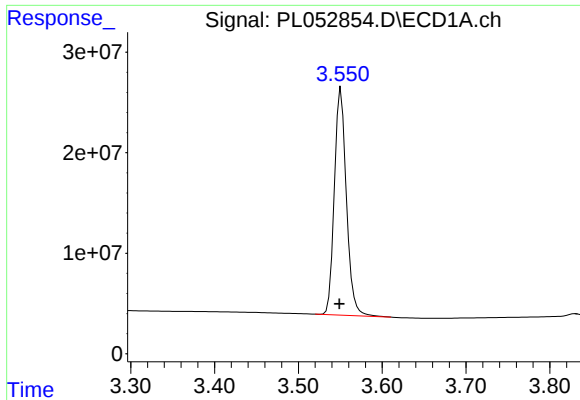

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.002 min
Response: 224643690
Conc: 22.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

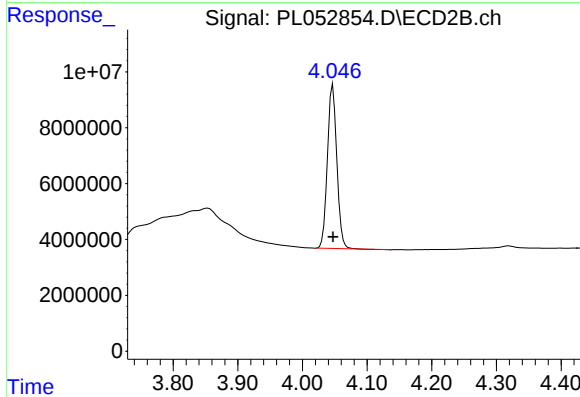


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 59093248
Conc: 22.01 ng/ml

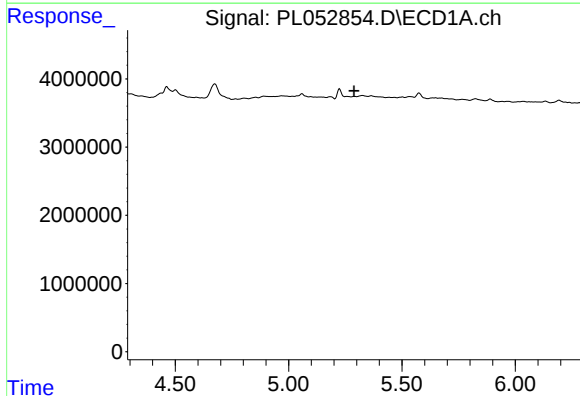


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.289 min
Response: 0
Conc: N.D.

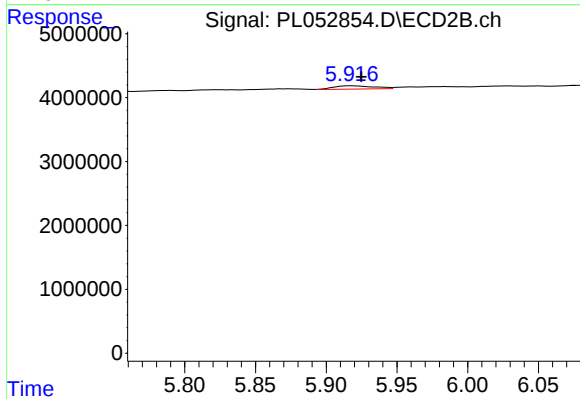

#8 Heptachlor epoxide


R.T.: 5.918 min
Delta R.T.: -0.007 min
Response: 989043
Conc: 0.30 ng/ml

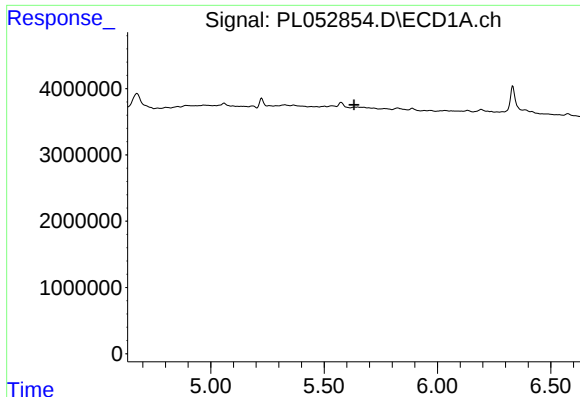

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.632 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

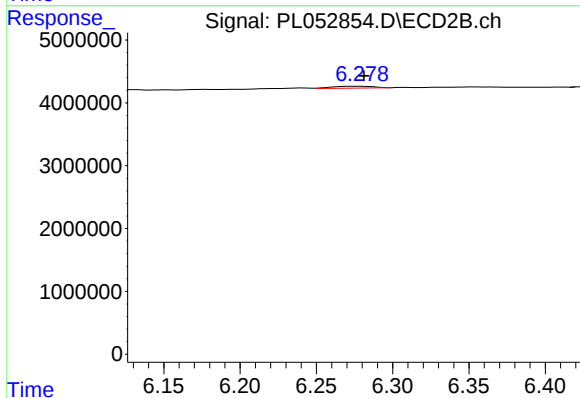


#9 Endosulfan I

R.T.: 6.277 min
Delta R.T.: -0.005 min
Response: 565460
Conc: 0.18 ng/ml

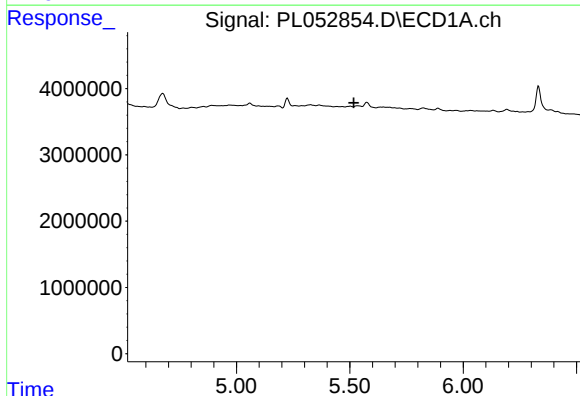


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

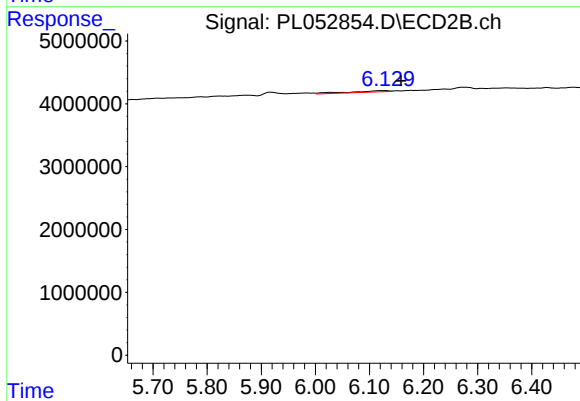

#10 gamma-Chlordane


R.T.: 6.131 min
Delta R.T.: -0.028 min
Response: 1131212
Conc: 0.33 ng/ml

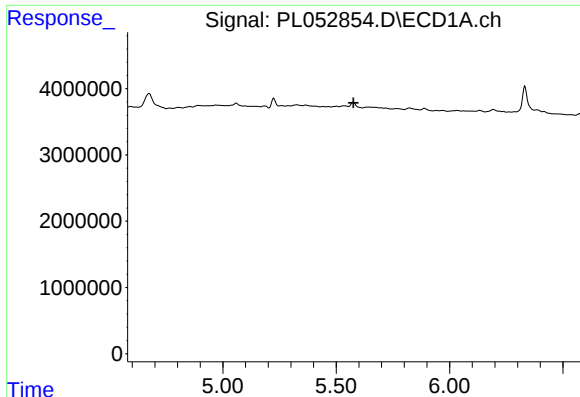

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

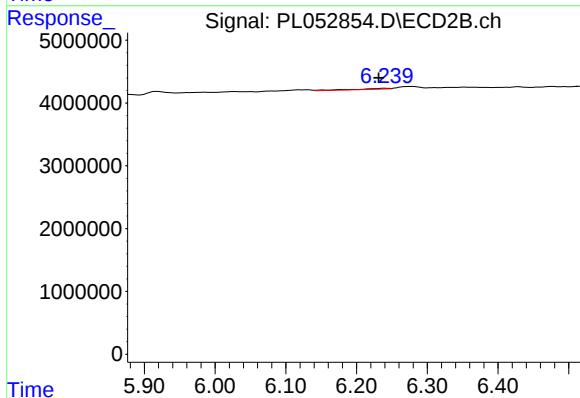


#11 alpha-Chlordane

R.T.: 6.240 min
Delta R.T.: 0.009 min
Response: 401111
Conc: 0.12 ng/ml

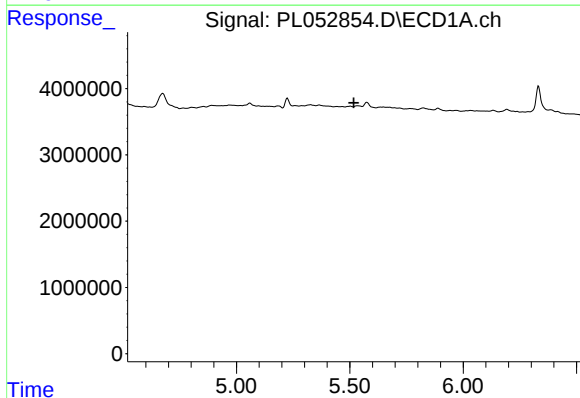


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

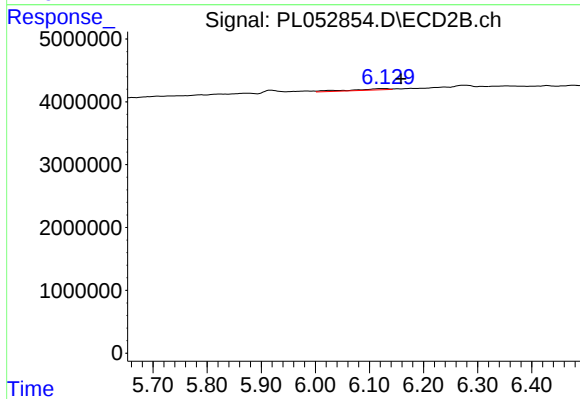

#25 Chlordane-3


R.T.: 6.131 min
Delta R.T.: -0.027 min
Response: 1131212
Conc: 2.60 ng/ml

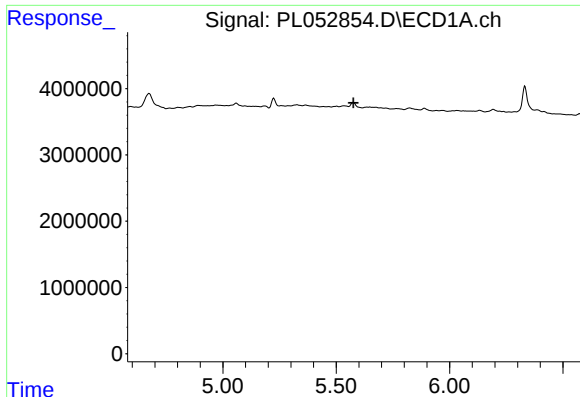

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

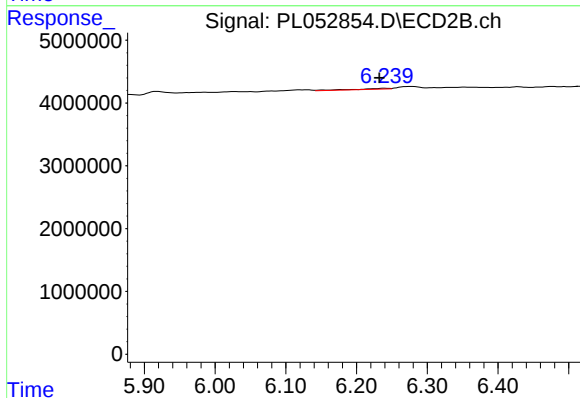


#26 Chlordane-4

R.T.: 6.240 min
Delta R.T.: 0.008 min
Response: 401111
Conc: 0.76 ng/ml

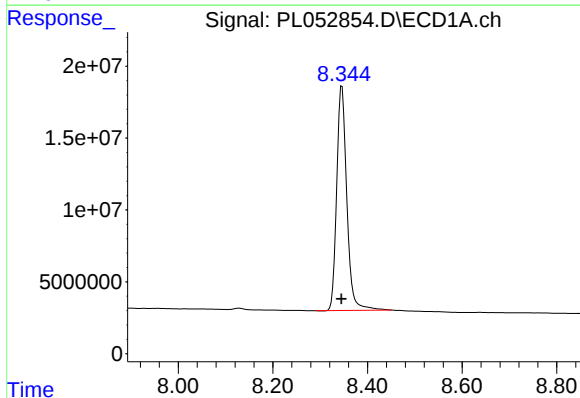

#28 Decachlorobiphenyl

R.T.: 8.346 min
Delta R.T.: 0.000 min
Response: 232199614
Conc: 23.18 ng/ml

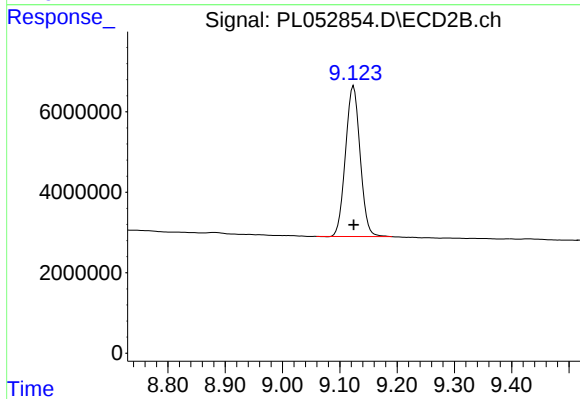

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: 0.000 min
Response: 66737176
Conc: 22.75 ng/ml