

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093019\
 Data File : PL052836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 09:54
 Operator : SG\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 14:15:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	4.047	596.7E6	122.1E6	59.985	45.470
28)	SA Decachlor...	8.350	9.125	473.2E6	133.4E6	47.243	45.458
Target Compounds							
23)	Chlordane-1	4.441	5.045	174.9E6	48177196	503.229	474.981
24)	Chlordane-2	4.948	5.512	194.0E6	53925620	488.436	481.813
25)	Chlordane-3	5.524	6.158	593.7E6	202.4E6	512.414	464.672
26)	Chlordane-4	5.582	6.233	488.5E6	248.7E6	511.816	468.324
27)	Chlordane-5	6.424	7.037	185.3E6	44130984	469.713	500.298



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093019\
Data File : PL052836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 09:54
Operator : SG\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 14:15:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

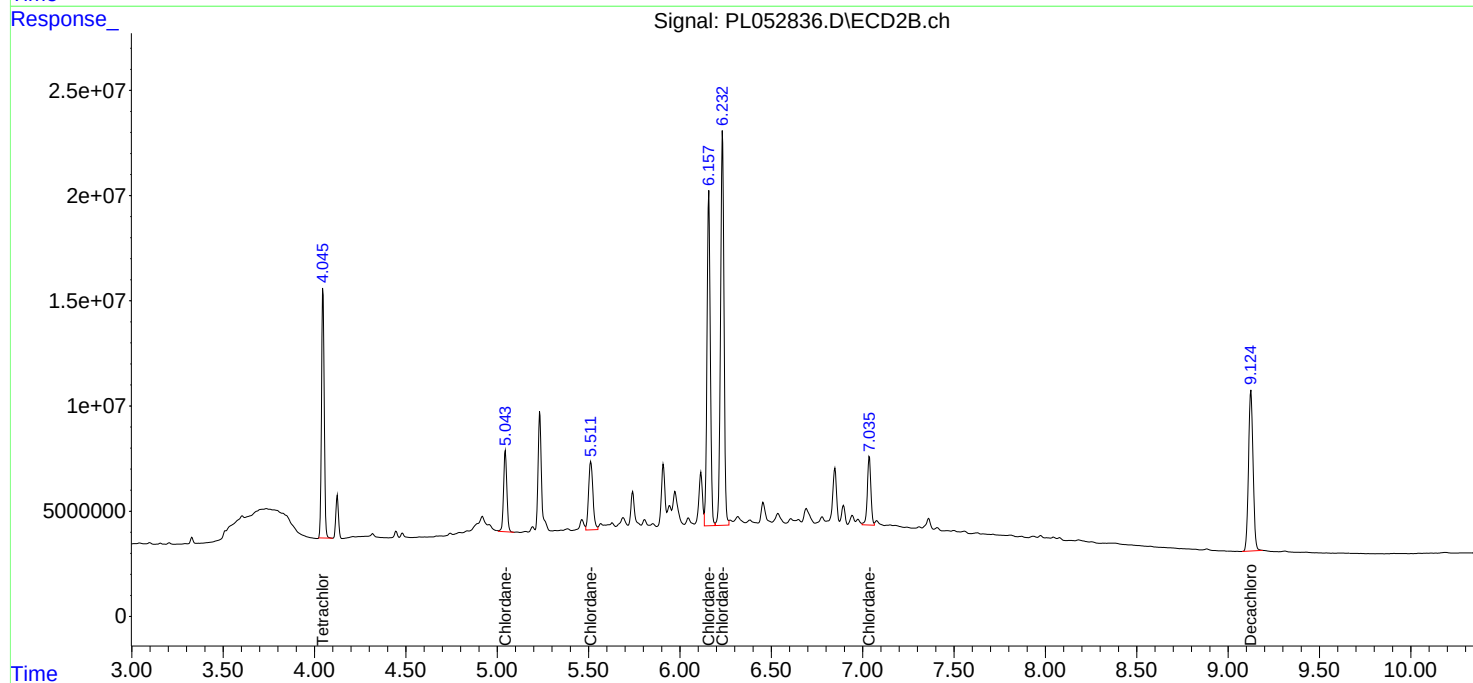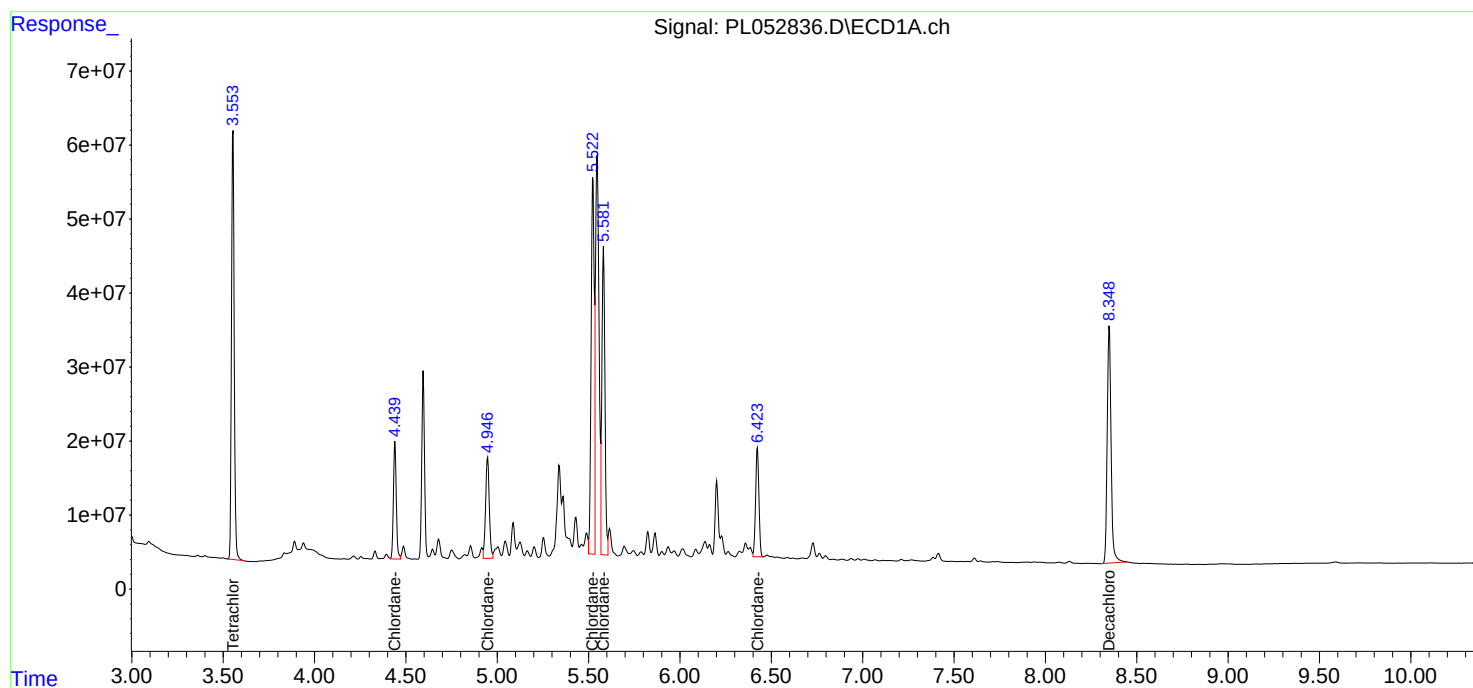


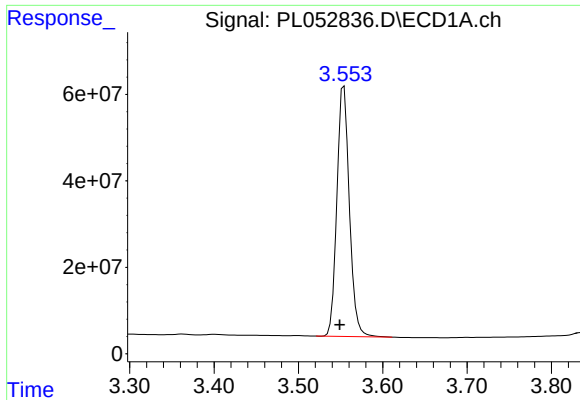

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.005 min
Response: 596654119
Conc: 59.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

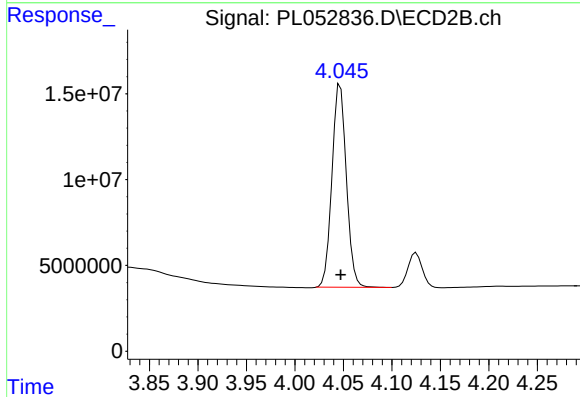


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 122095910
Conc: 45.47 ng/ml

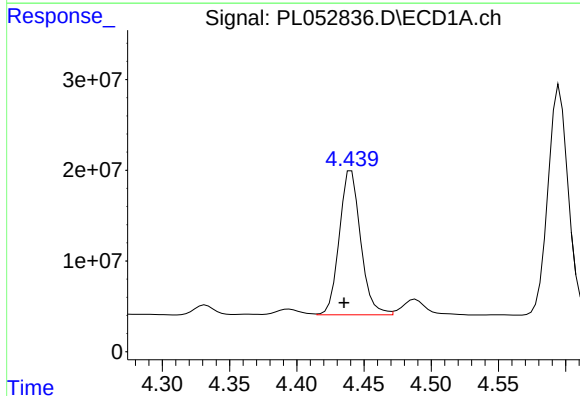


#23 Chlordane-1

R.T.: 4.441 min
Delta R.T.: 0.005 min
Response: 174883022
Conc: 503.23 ng/ml

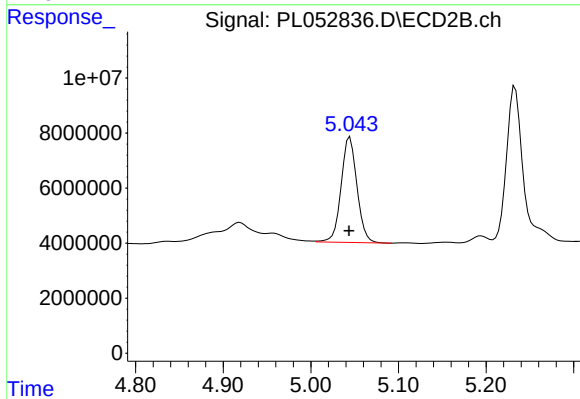

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.001 min
Response: 48177196
Conc: 474.98 ng/ml

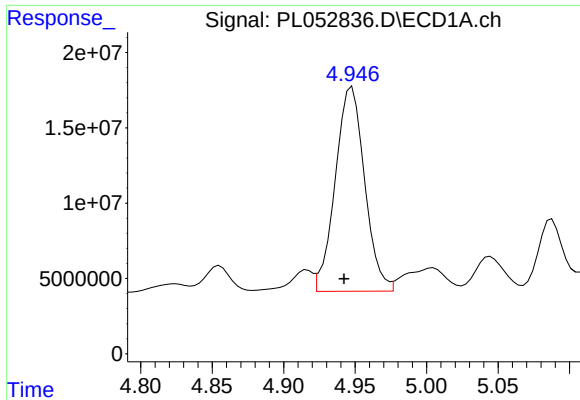

#24 Chlordane-2


R.T.: 4.948 min
Delta R.T.: 0.006 min
Response: 194048909
Conc: 488.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

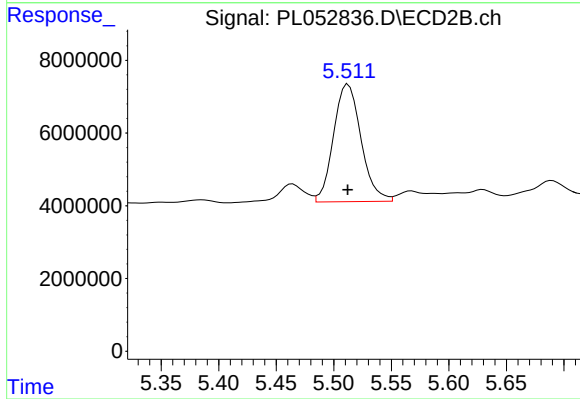


#24 Chlordane-2

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 53925620
Conc: 481.81 ng/ml

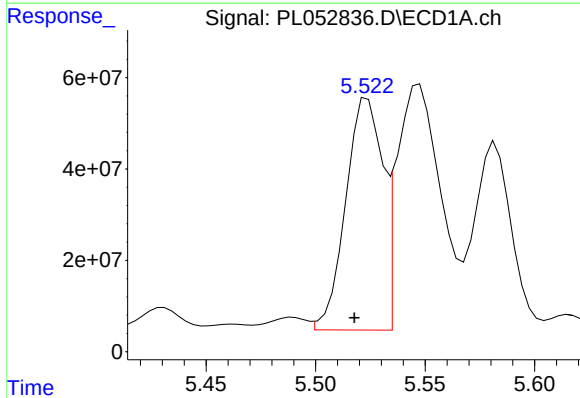


#25 Chlordane-3

R.T.: 5.524 min
Delta R.T.: 0.006 min
Response: 593734118
Conc: 512.41 ng/ml

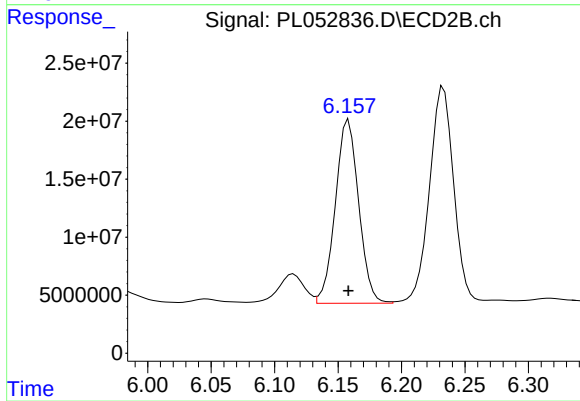

#25 Chlordane-3


R.T.: 6.158 min
Delta R.T.: 0.000 min
Response: 202368947
Conc: 464.67 ng/ml

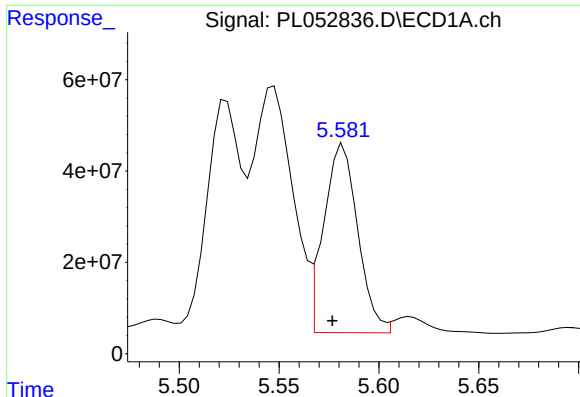

#26 Chlordane-4


R.T.: 5.582 min
Delta R.T.: 0.006 min
Response: 488482919
Conc: 511.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

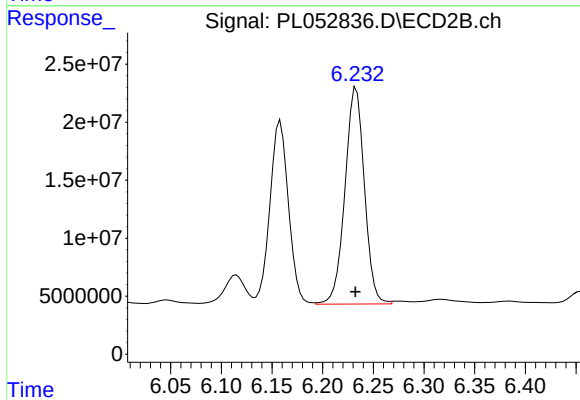


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 248678749
Conc: 468.32 ng/ml

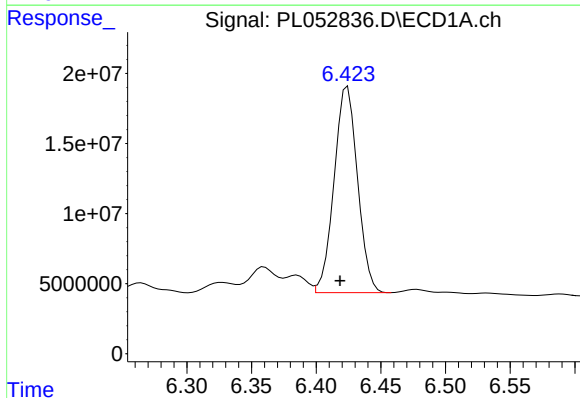


#27 Chlordane-5

R.T.: 6.424 min
Delta R.T.: 0.006 min
Response: 185270827
Conc: 469.71 ng/ml

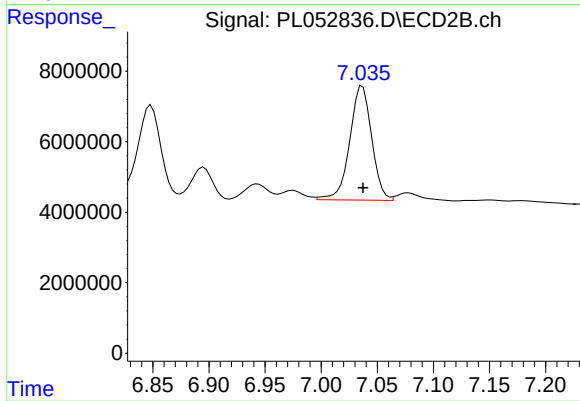

#27 Chlordane-5


R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 44130984
Conc: 500.30 ng/ml

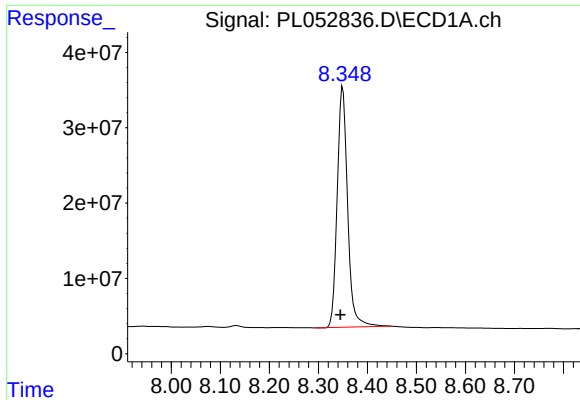

#28 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: 0.005 min
Response: 473191452
Conc: 47.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

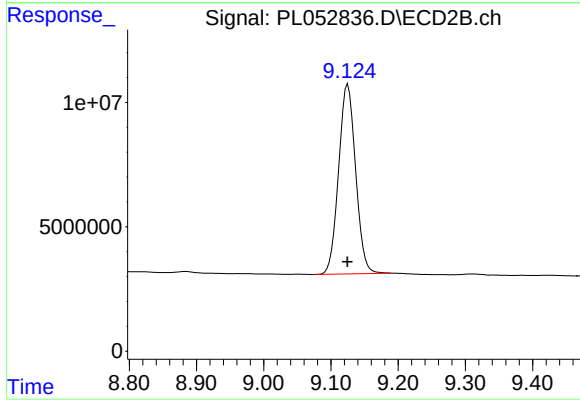

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 133360414
Conc: 45.46 ng/ml