

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093019\
 Data File : PL052842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 11:41
 Operator : SG\AJ
 Sample : K4839-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PT-CHLR-WP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 14:17:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	4.047	332.7E6	56354085	33.448	20.987 #
28)	SA Decachlor...	8.350	9.126	241.3E6	65091191	24.091	22.187
Target Compounds							
23)	Chlordane-1	4.440	5.045	560.7E6	148.0E6	1613.312	1459.241
24)	Chlordane-2	4.946	5.512	571.8E6	158.3E6	1439.243	1414.767
25)	Chlordane-3	5.523	6.158	1777.9E6	563.2E6	1534.432	1293.180
26)	Chlordane-4	5.582	6.233	1535.9E6	660.4E6	1609.261	1243.784
27)	Chlordane-5	6.424	7.037	560.4E6	129.9E6	1420.786	1472.315



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093019\
Data File : PL052842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 11:41
Operator : SG\AJ
Sample : K4839-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 14:17:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

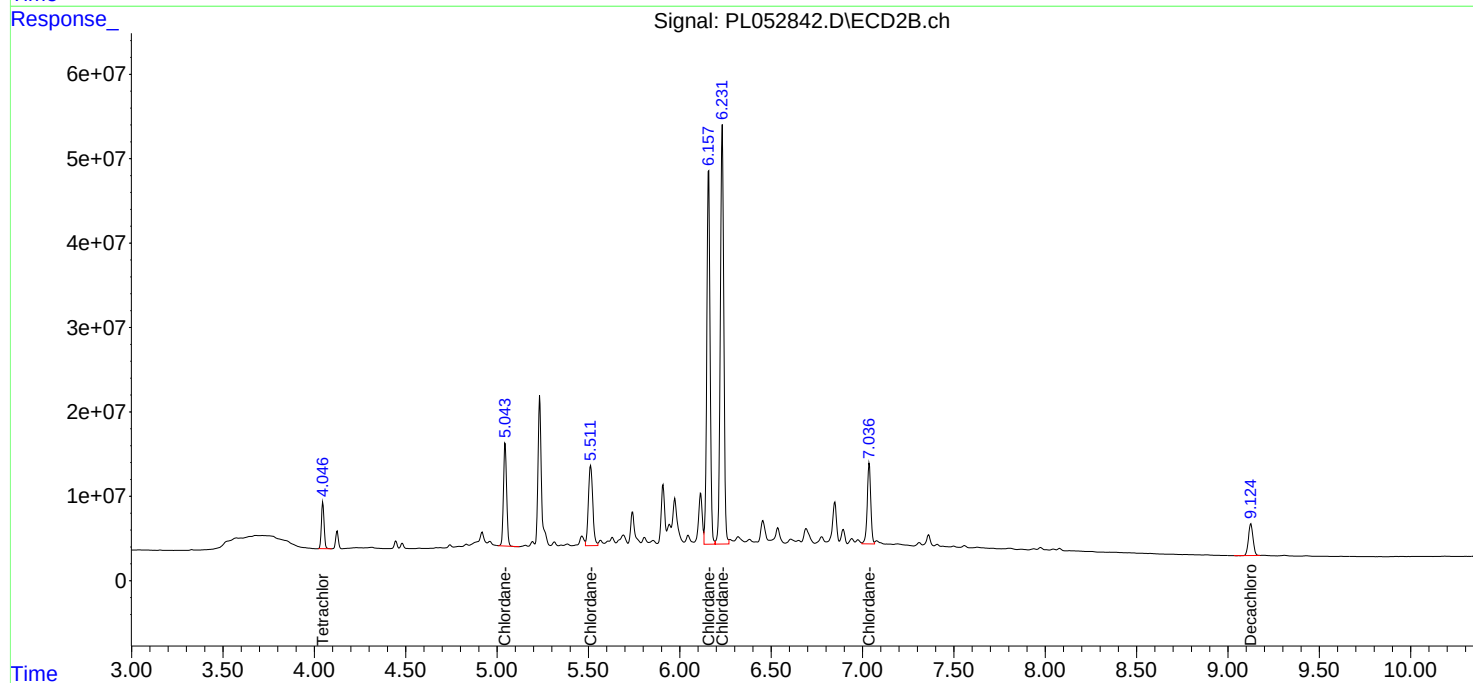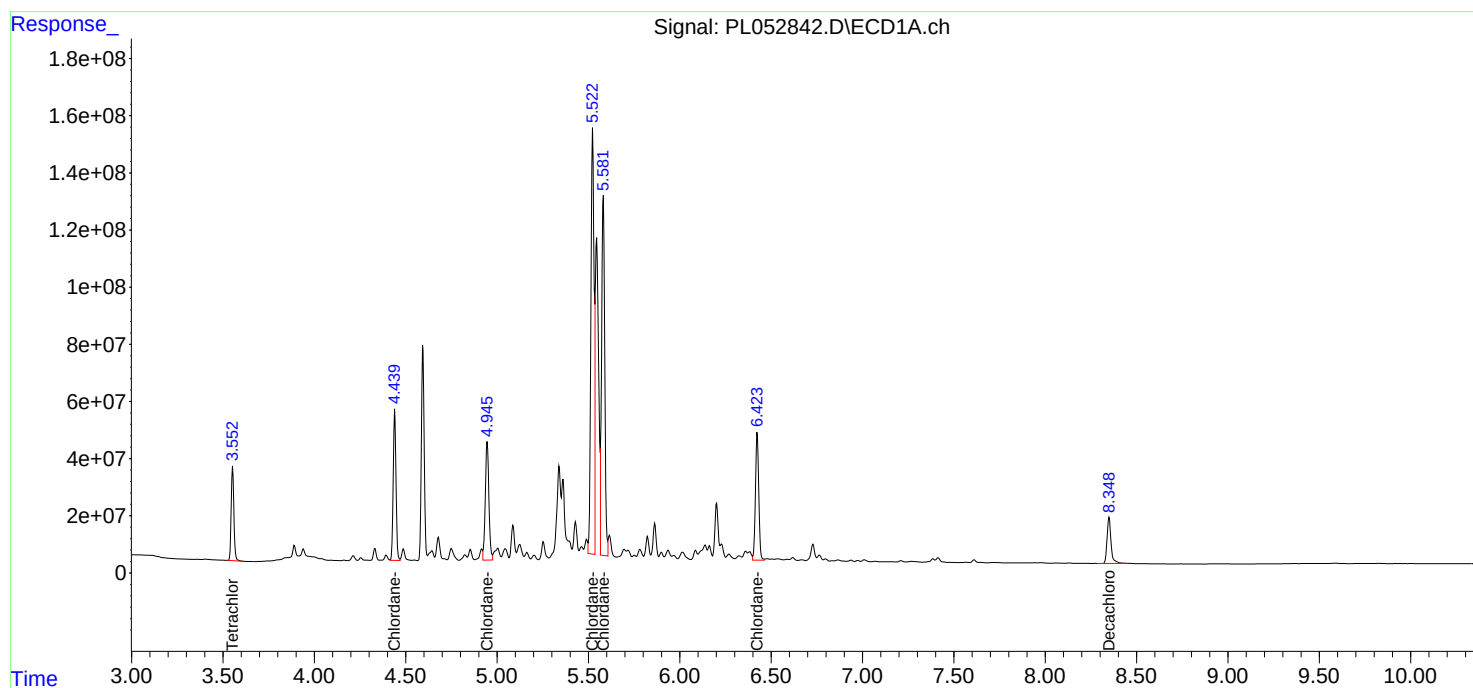


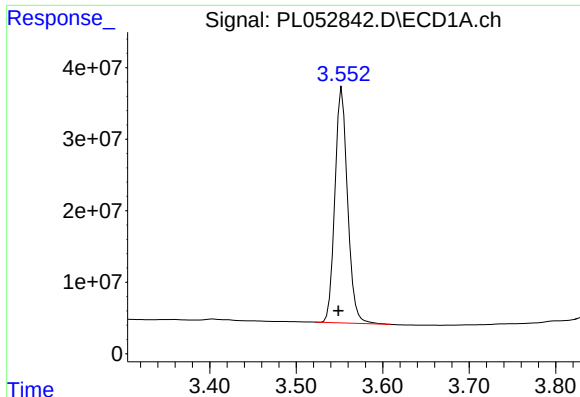

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.004 min
Response: 332701480
Conc: 33.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

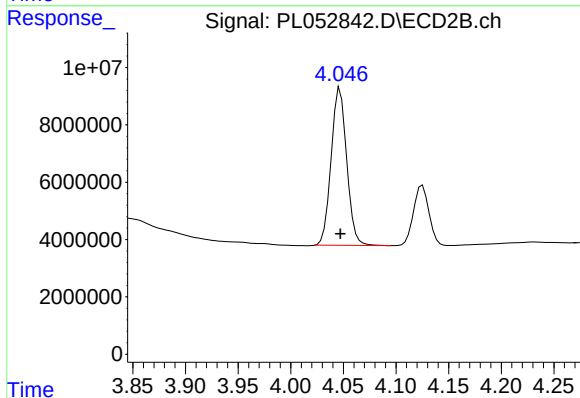


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 56354085
Conc: 20.99 ng/ml

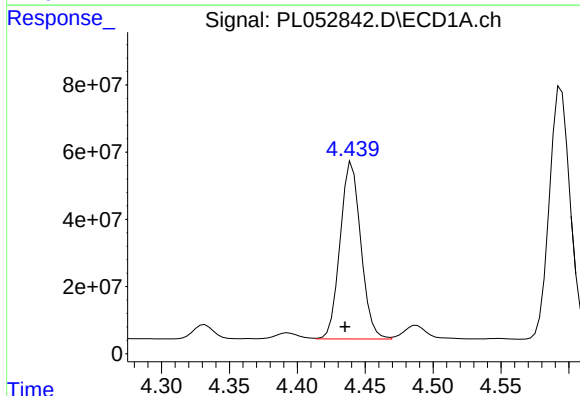


#23 Chlordane-1

R.T.: 4.440 min
Delta R.T.: 0.005 min
Response: 560660987
Conc: 1613.31 ng/ml

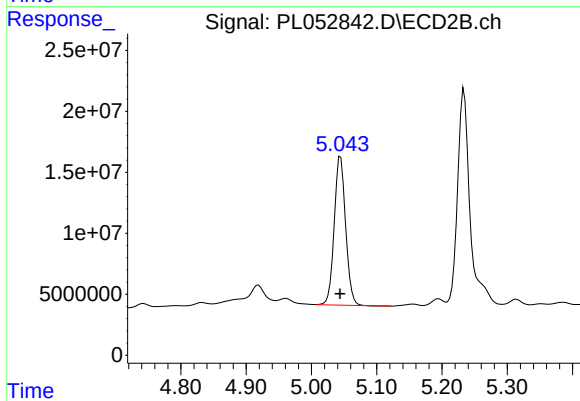

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 148010375
Conc: 1459.24 ng/ml

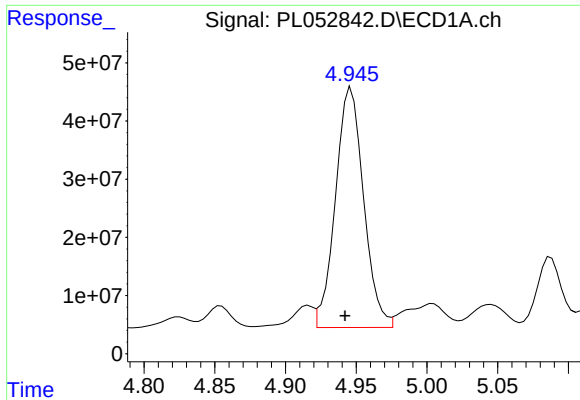

#24 Chlordane-2


R.T.: 4.946 min
Delta R.T.: 0.004 min
Response: 571791927
Conc: 1439.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

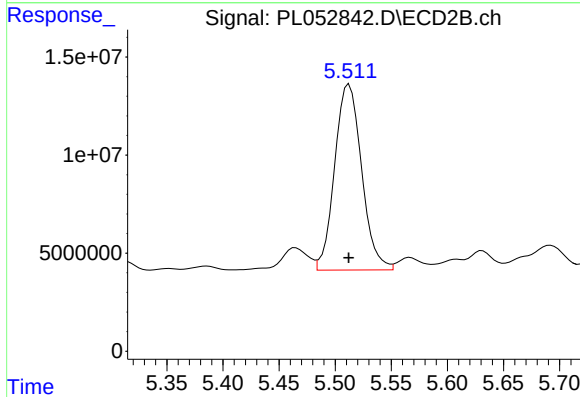


#24 Chlordane-2

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 158343998
Conc: 1414.77 ng/ml

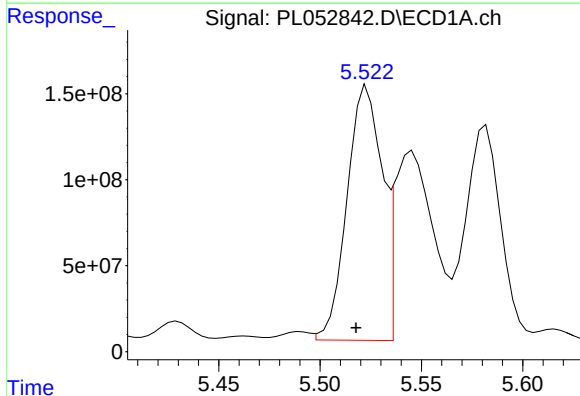


#25 Chlordane-3

R.T.: 5.523 min
Delta R.T.: 0.005 min
Response: 1777944915
Conc: 1534.43 ng/ml

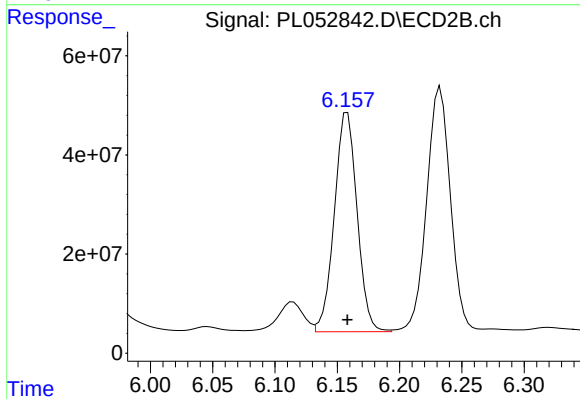

#25 Chlordane-3


R.T.: 6.158 min
Delta R.T.: 0.000 min
Response: 563191912
Conc: 1293.18 ng/ml

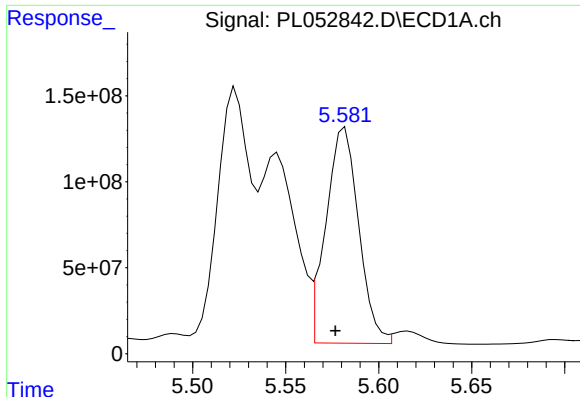

#26 Chlordane-4


R.T.: 5.582 min
Delta R.T.: 0.005 min
Response: 1535896898
Conc: 1609.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

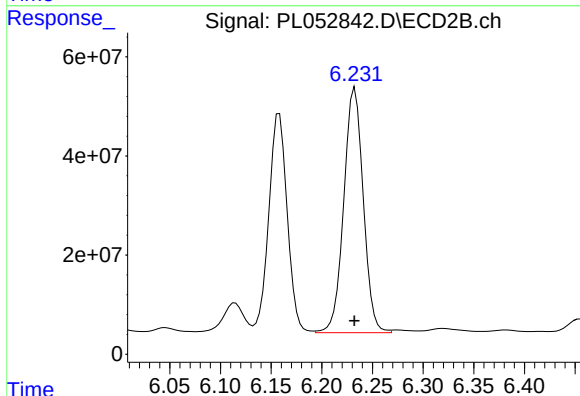


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 660445491
Conc: 1243.78 ng/ml

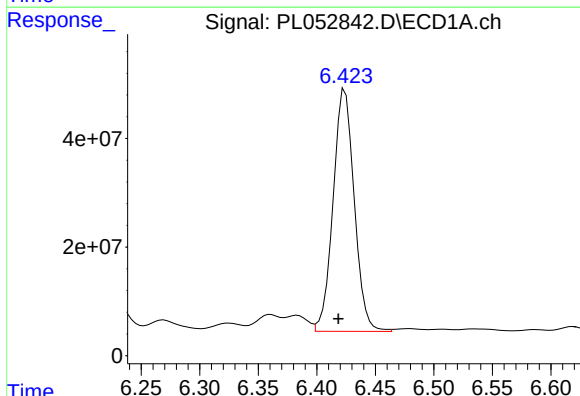


#27 Chlordane-5

R.T.: 6.424 min
Delta R.T.: 0.006 min
Response: 560406582
Conc: 1420.79 ng/ml

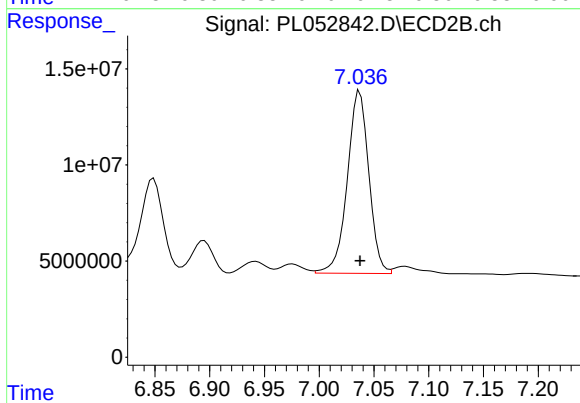

#27 Chlordane-5


R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 129871931
Conc: 1472.31 ng/ml

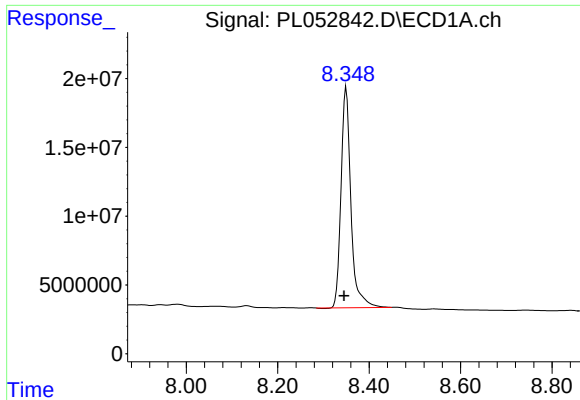

#28 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: 0.005 min
Response: 241294480
Conc: 24.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

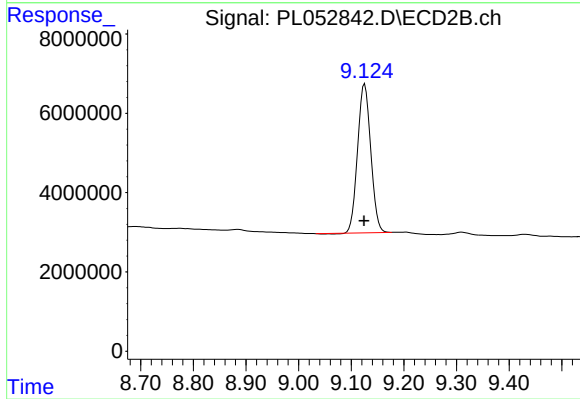

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.001 min
Response: 65091191
Conc: 22.19 ng/ml