

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093019\
 Data File : PL052856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 16:30
 Operator : SG\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 00:59:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	4.047	551.6E6	117.1E6	55.457	43.607
28)	SA Decachlor...	8.344	9.122	448.1E6	128.4E6	44.736	43.782
Target Compounds							
23)	Chlordane-1	4.434	5.044	160.8E6	46927654	462.667	462.662
24)	Chlordane-2	4.941	5.511	182.6E6	52325018	459.720	467.512
25)	Chlordane-3	5.518	6.157	558.7E6	199.4E6	482.172	457.743
26)	Chlordane-4	5.576	6.231	465.3E6	242.2E6	487.550	456.143
27)	Chlordane-5	6.418	7.036	176.1E6	42531623	446.444	482.167



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093019\
Data File : PL052856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 16:30
Operator : SG\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 00:59:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

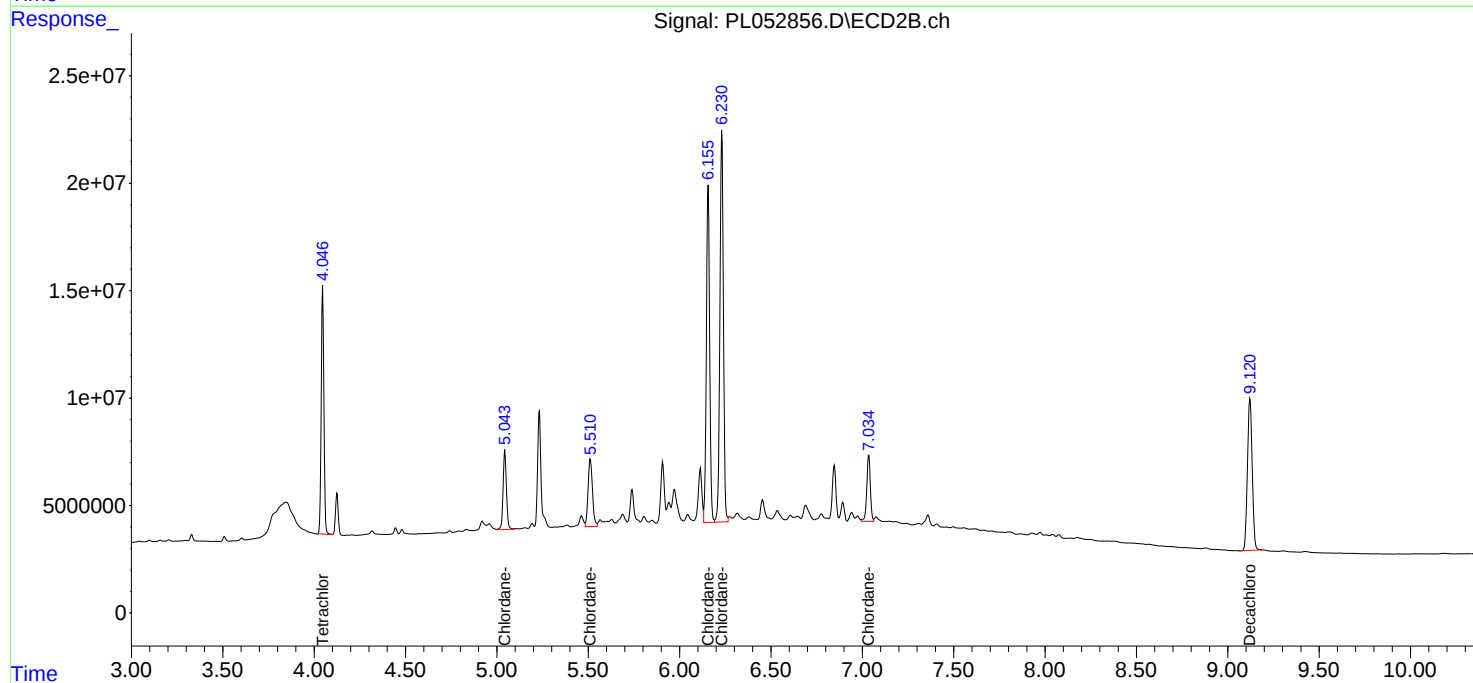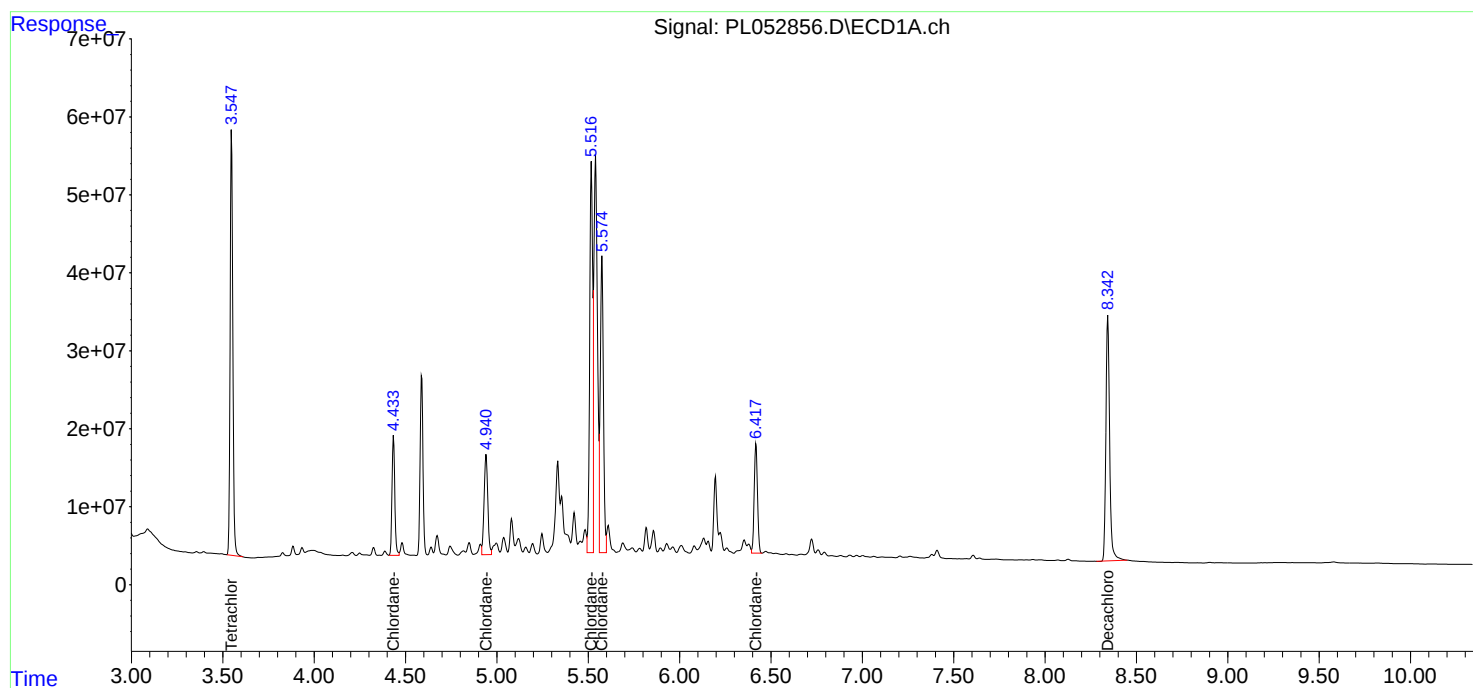


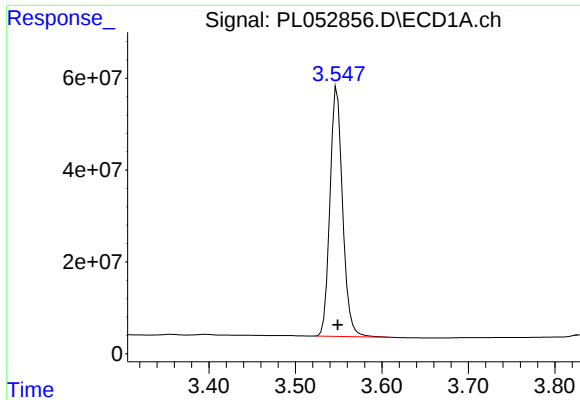

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 551613259
Conc: 55.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

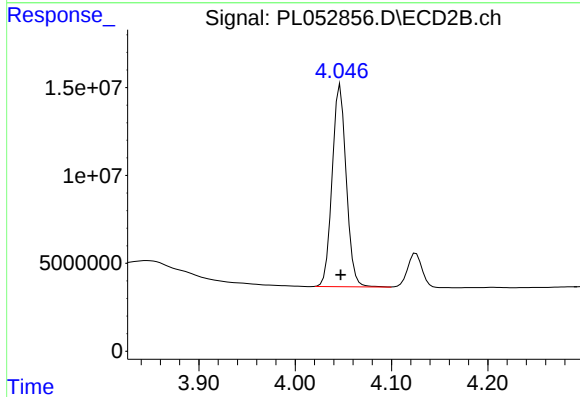


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 117094426
Conc: 43.61 ng/ml

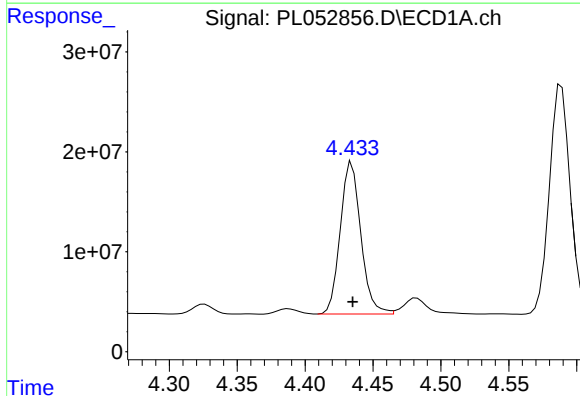


#23 Chlordane-1

R.T.: 4.434 min
Delta R.T.: 0.000 min
Response: 160786660
Conc: 462.67 ng/ml

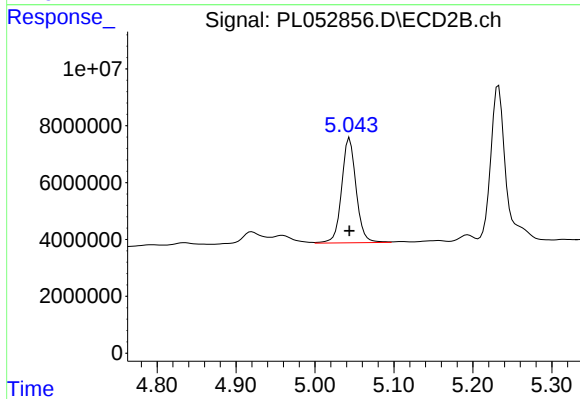

#23 Chlordane-1


R.T.: 5.044 min
Delta R.T.: 0.000 min
Response: 46927654
Conc: 462.66 ng/ml

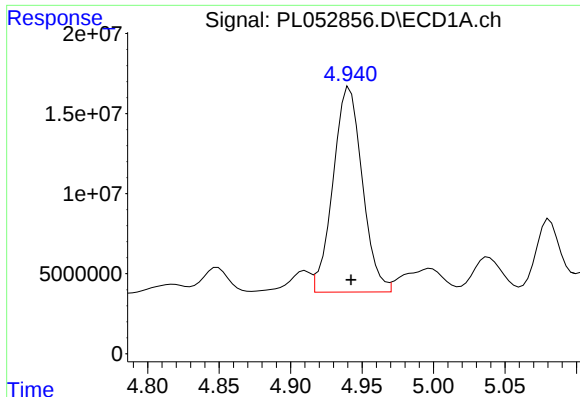

#24 Chlordane-2


R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 182640375
Conc: 459.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

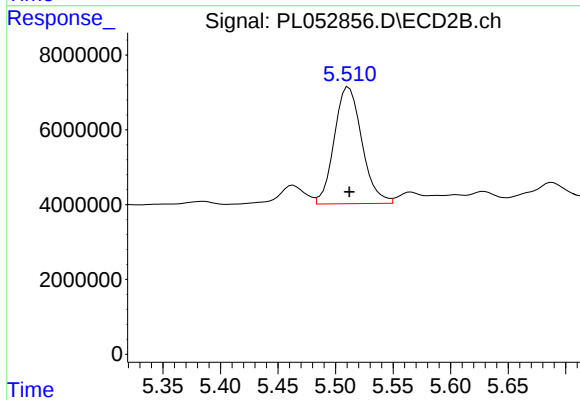


#24 Chlordane-2

R.T.: 5.511 min
Delta R.T.: 0.000 min
Response: 52325018
Conc: 467.51 ng/ml

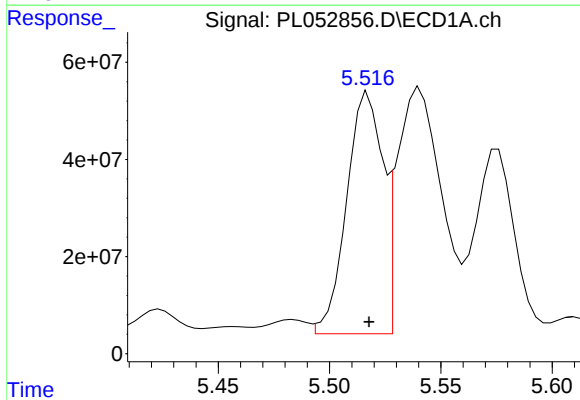


#25 Chlordane-3

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 558692628
Conc: 482.17 ng/ml

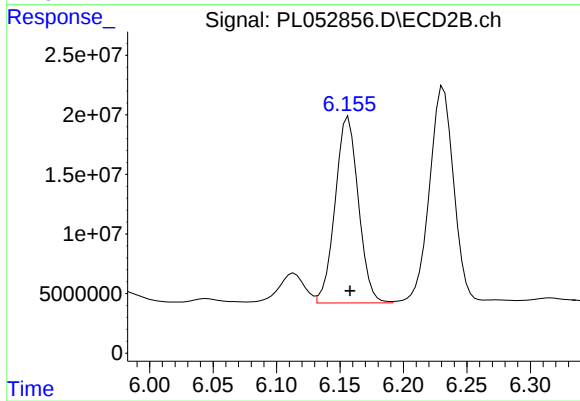

#25 Chlordane-3


R.T.: 6.157 min
Delta R.T.: -0.001 min
Response: 199351234
Conc: 457.74 ng/ml

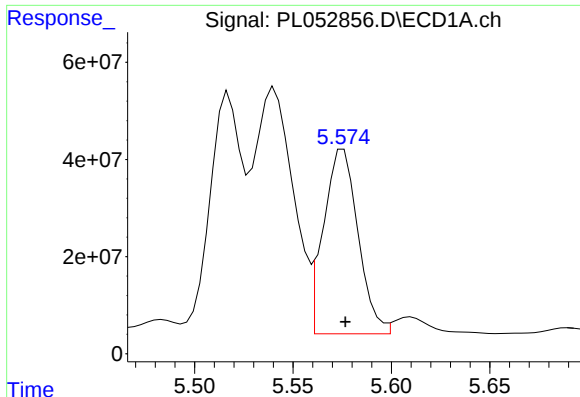

#26 Chlordane-4


R.T.: 5.576 min
Delta R.T.: -0.001 min
Response: 465323067
Conc: 487.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

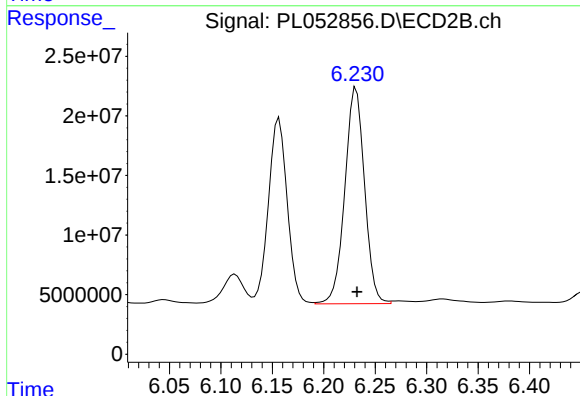


#26 Chlordane-4

R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 242210553
Conc: 456.14 ng/ml

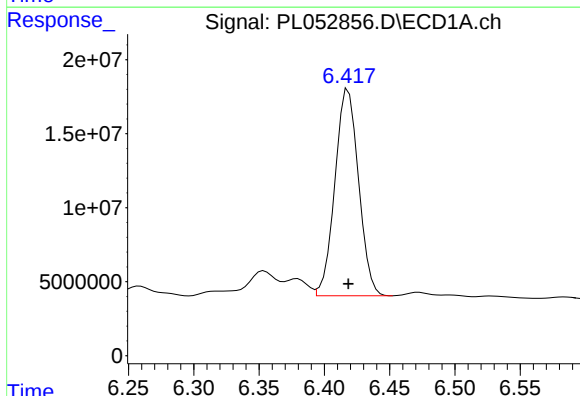


#27 Chlordane-5

R.T.: 6.418 min
Delta R.T.: 0.000 min
Response: 176092958
Conc: 446.44 ng/ml

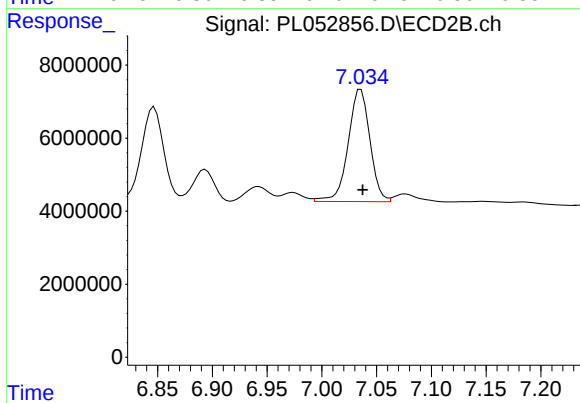

#27 Chlordane-5


R.T.: 7.036 min
Delta R.T.: -0.002 min
Response: 42531623
Conc: 482.17 ng/ml

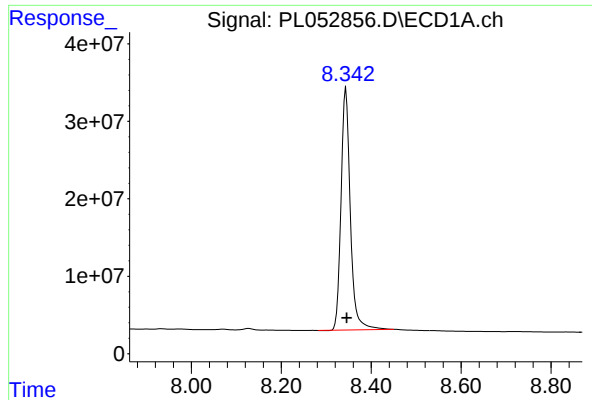

#28 Decachlorobiphenyl

R.T.: 8.344 min
Delta R.T.: -0.001 min
Response: 448079340
Conc: 44.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

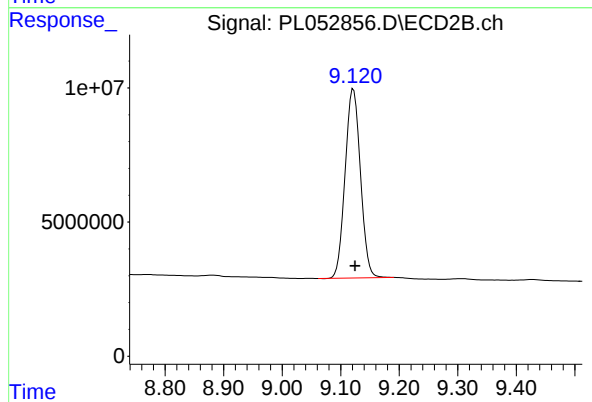

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.003 min
Response: 128443806
Conc: 43.78 ng/ml