

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093022\
 Data File : PL078001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2022 12:40
 Operator : AR\AJ
 Sample : N4877-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/03/2022
 Supervised By :Ankita Jodhani 10/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 23:37:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.419	2.622	40025058	43482590	24.969	14.647m#
28) SA Decachlor...	8.906	7.721	30611934	37101464	23.686	14.780 #
Target Compounds						
12) B 4,4'-DDE	6.078	5.054	7074510	12916032	4.444	3.970

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093022\
Data File : PL078001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2022 12:40
Operator : AR\AJ
Sample : N4877-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2022
Supervised By :Ankita Jodhani 10/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 23:37:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

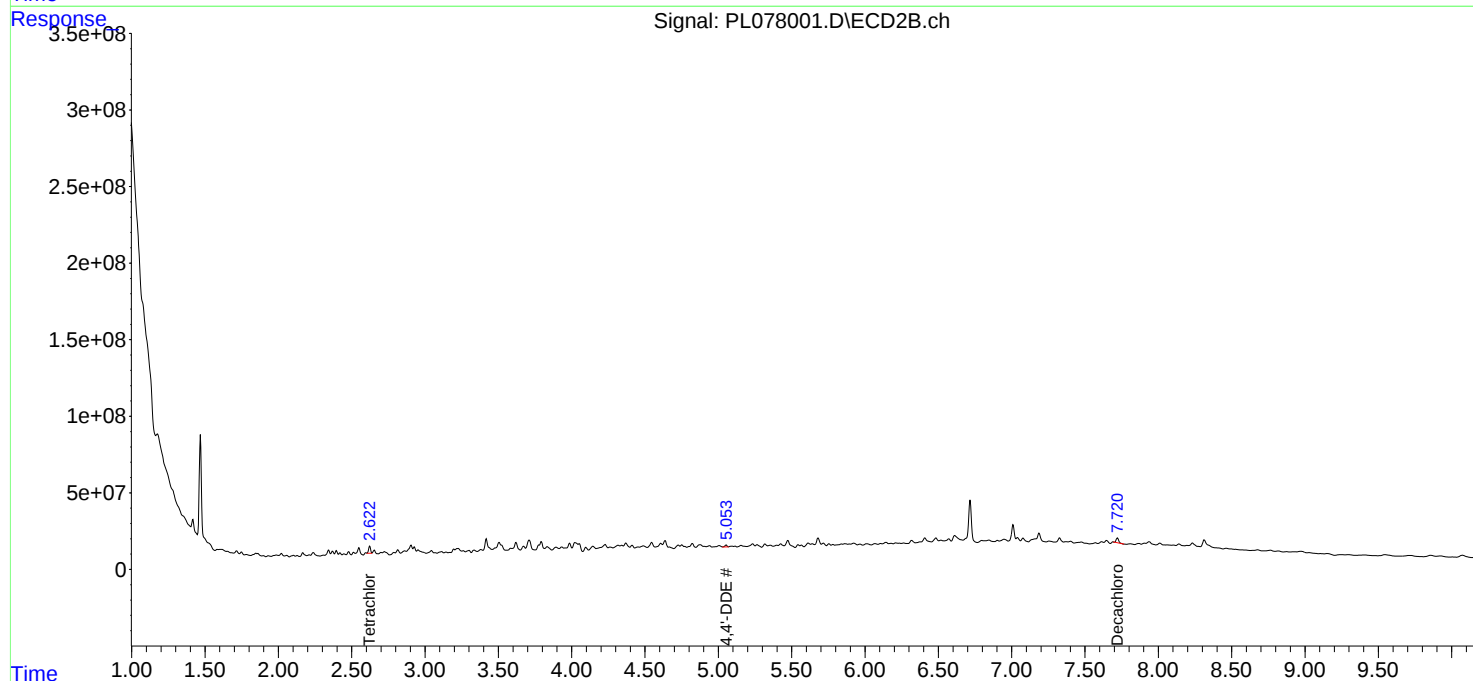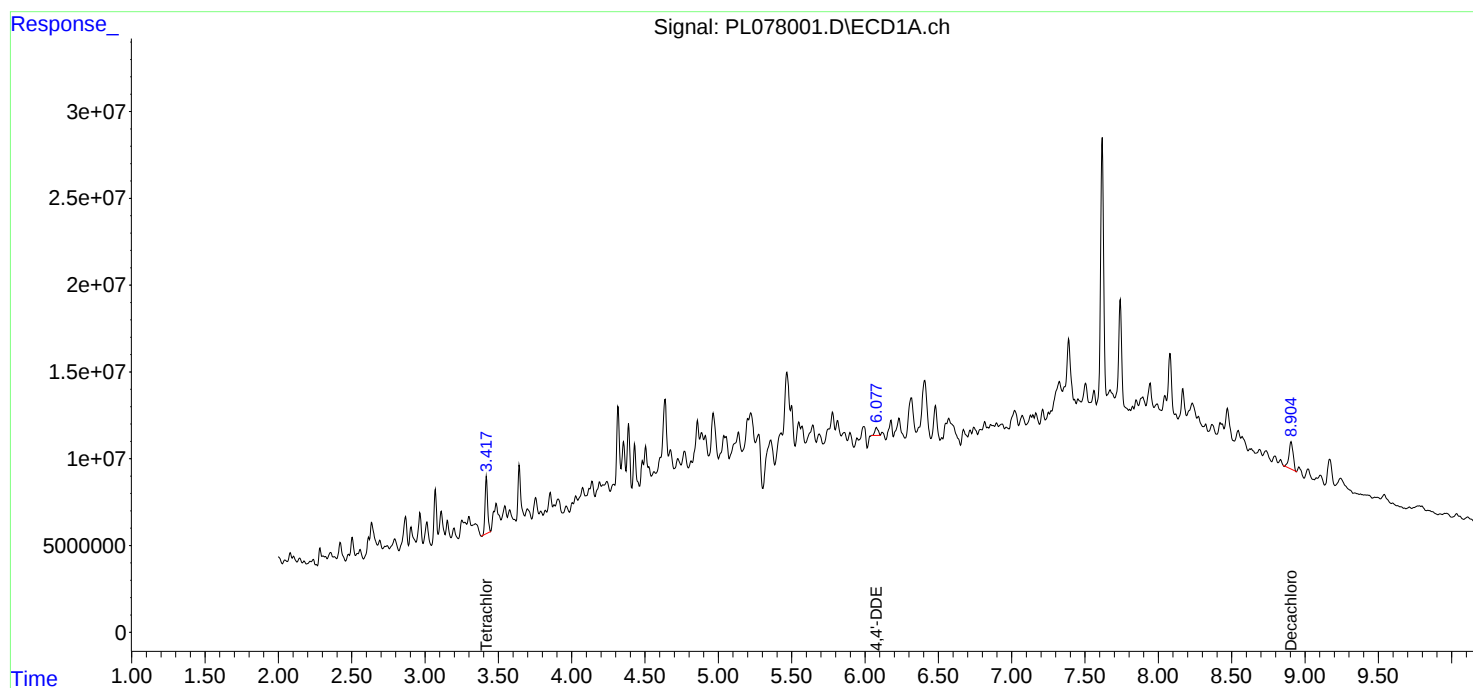

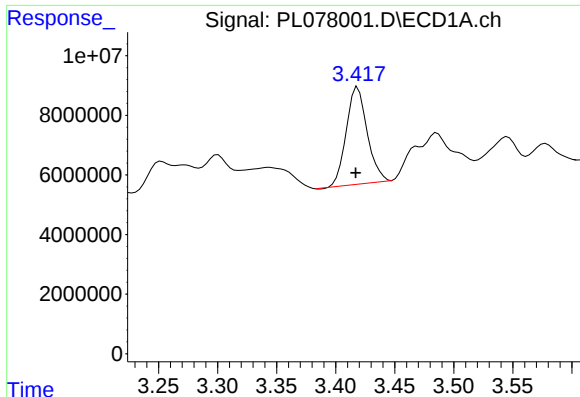


#1 Tetrachloro-m-xylene

R.T.: 3.419 min
Delta R.T.: 0.002 min
Response: 40025058
Conc: 24.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2022
Supervised By :Ankita Jodhani 10/03/2022

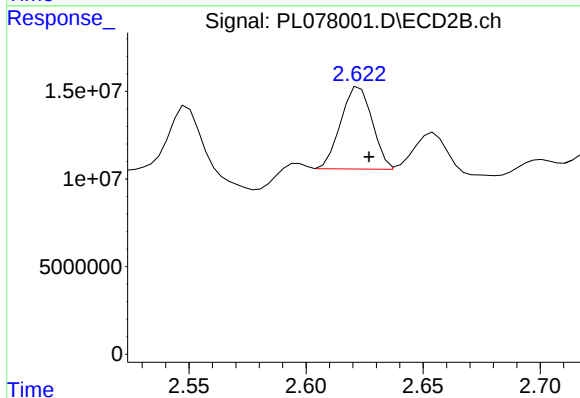


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: -0.005 min
Response: 43482590
Conc: 14.65 ng/ml m

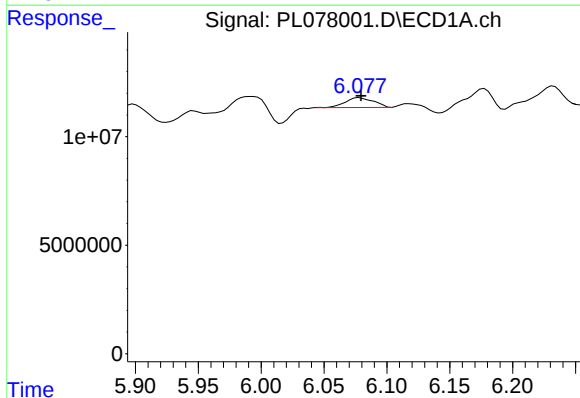


#12 4,4'-DDE

R.T.: 6.078 min
Delta R.T.: -0.001 min
Response: 7074510
Conc: 4.44 ng/ml

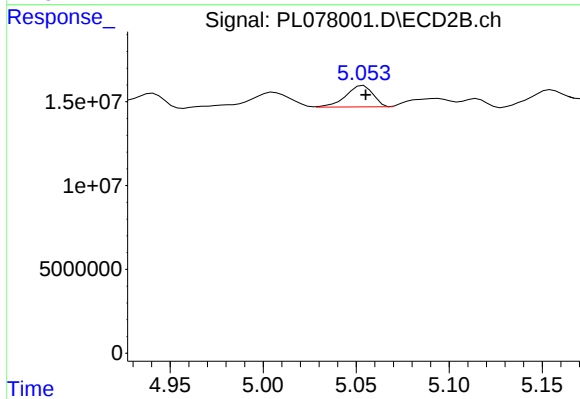

#12 4,4'-DDE

R.T.: 5.054 min
Delta R.T.: -0.001 min
Response: 12916032
Conc: 3.97 ng/ml

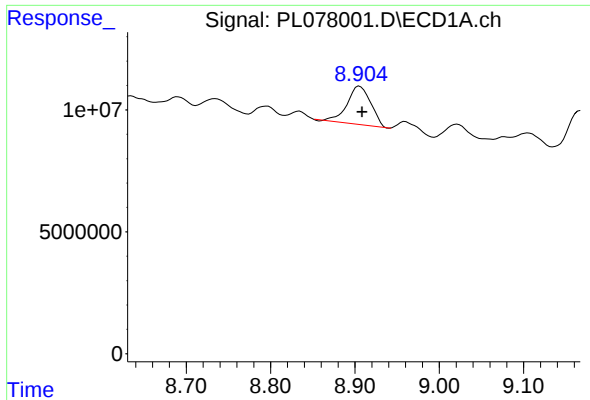


#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: -0.003 min
Response: 30611934
Conc: 23.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2022
Supervised By :Ankita Jodhani 10/03/2022

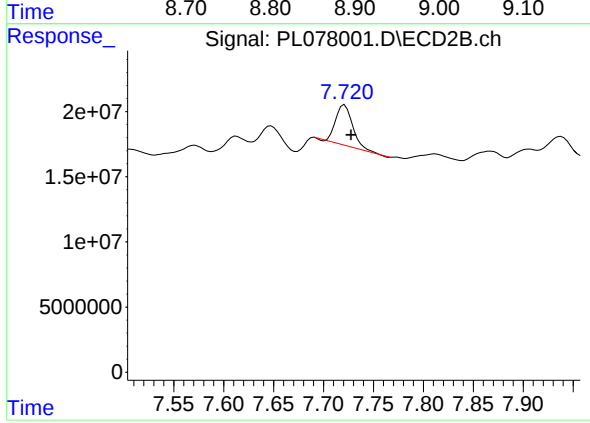

#28 Decachlorobiphenyl

R.T.: 7.721 min
Delta R.T.: -0.006 min
Response: 37101464
Conc: 14.78 ng/ml