

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093022\
 Data File : PL078021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2022 19:13
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 05:56:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.622	81430937	152.5E6	50.799	51.385
28)	SA Decachlor...	8.901	7.718	66725358	105.5E6	51.628	42.035
Target Compounds							
23)	Chlordane-1	4.573	3.599	33472121	50695458	538.412	466.536
24)	Chlordane-2	5.106	4.168	35030716	53446694	525.400	446.171
25)	Chlordane-3	5.818	4.792	134.2E6	158.0E6	544.912	459.379
26)	Chlordane-4	5.896	4.853	160.4E6	165.2E6	539.099	455.197
27)	Chlordane-5	6.755	5.516	25125845	42079866	505.924	447.219



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093022\
Data File : PL078021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2022 19:13
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 05:56:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

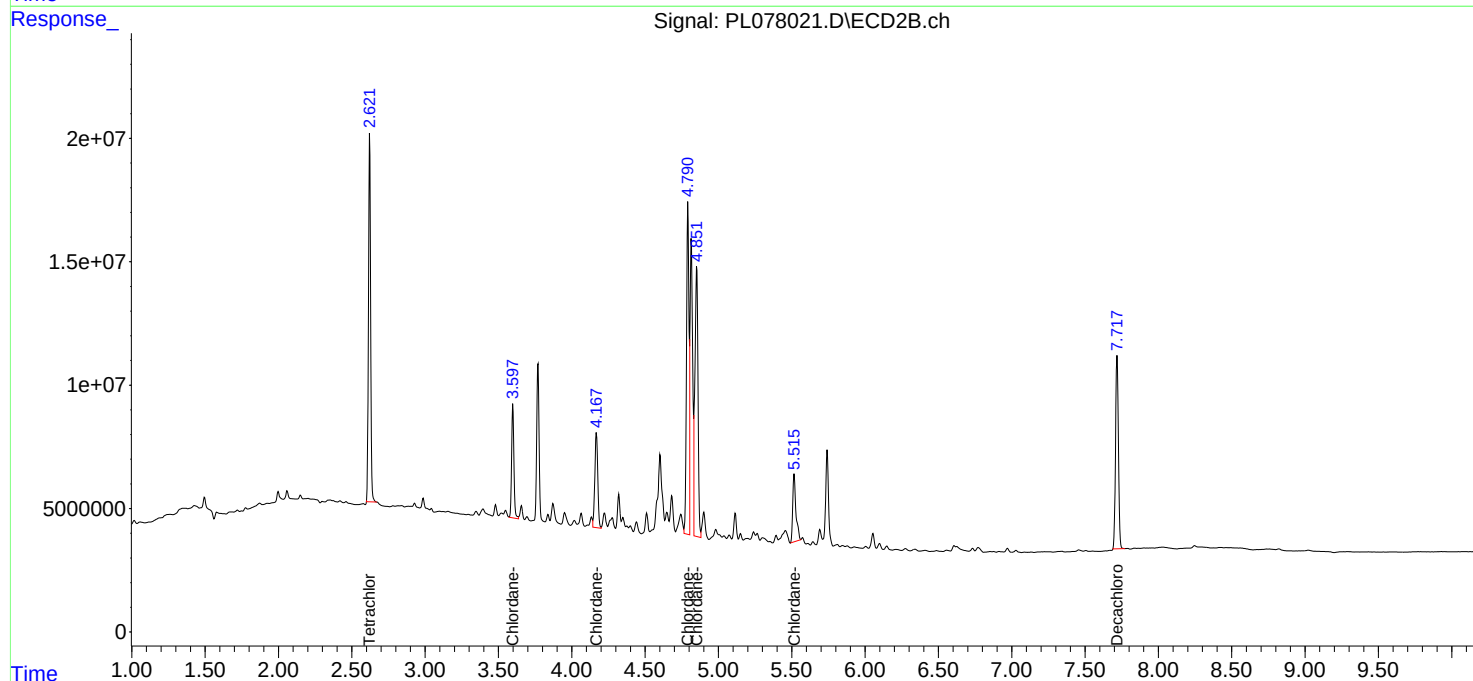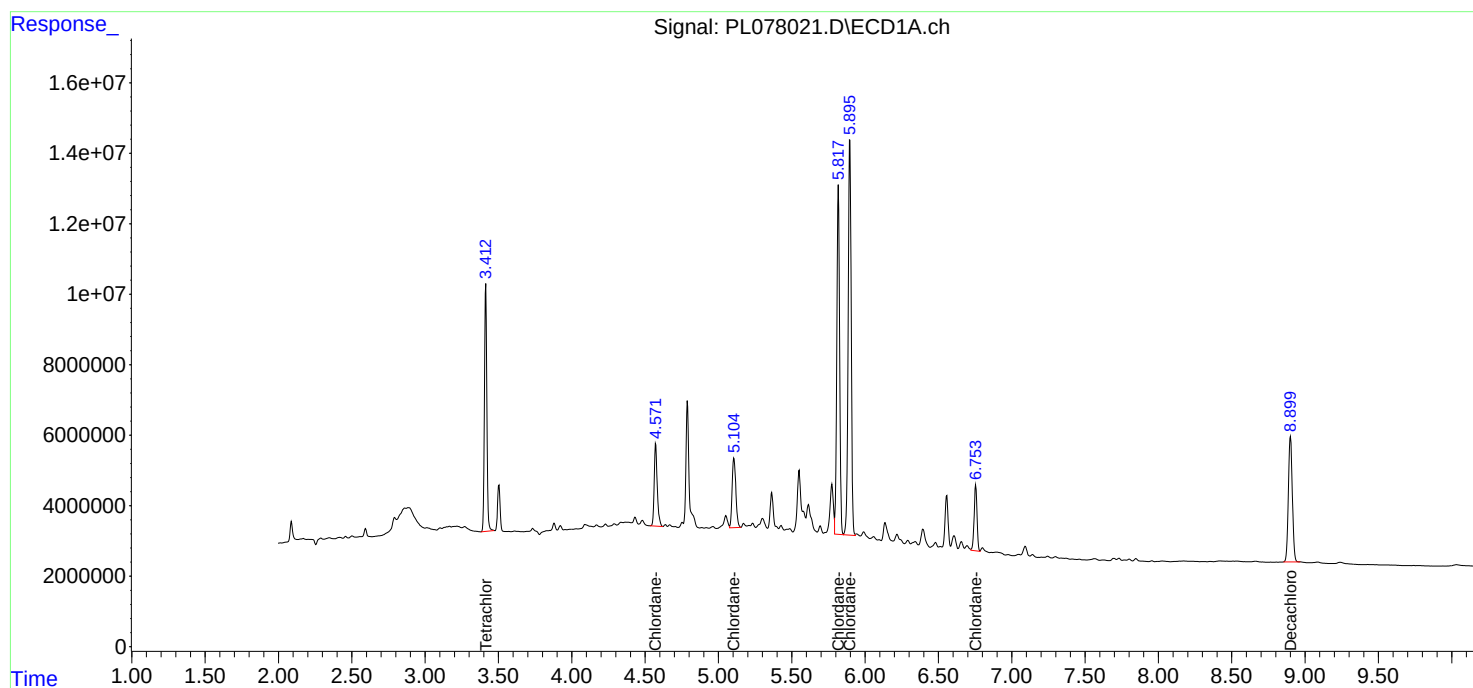


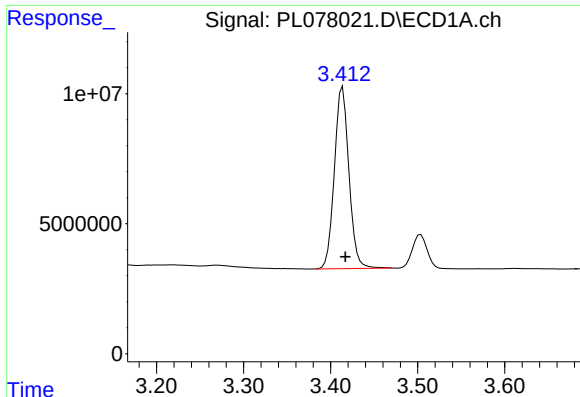

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: -0.003 min
Response: 81430937
Conc: 50.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

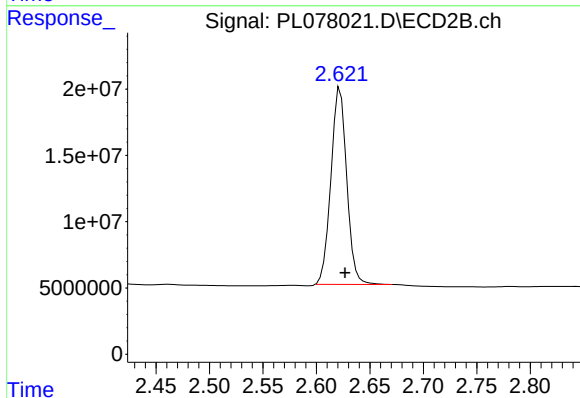


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: -0.005 min
Response: 152548200
Conc: 51.38 ng/ml

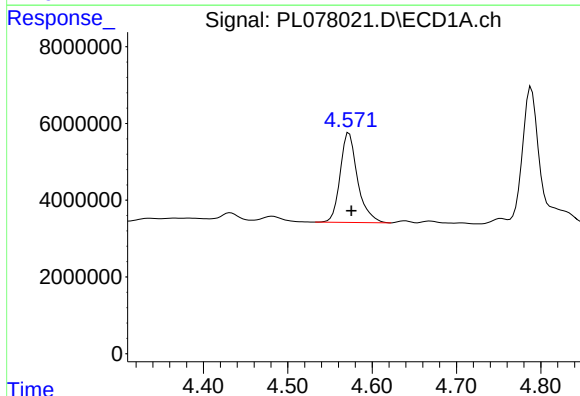


#23 Chlordane-1

R.T.: 4.573 min
Delta R.T.: -0.003 min
Response: 33472121
Conc: 538.41 ng/ml

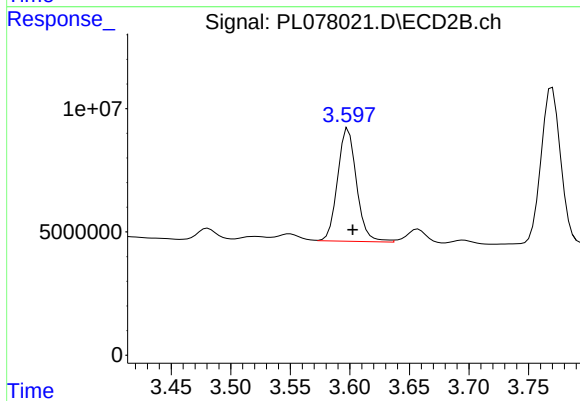

#23 Chlordane-1


R.T.: 3.599 min
Delta R.T.: -0.004 min
Response: 50695458
Conc: 466.54 ng/ml

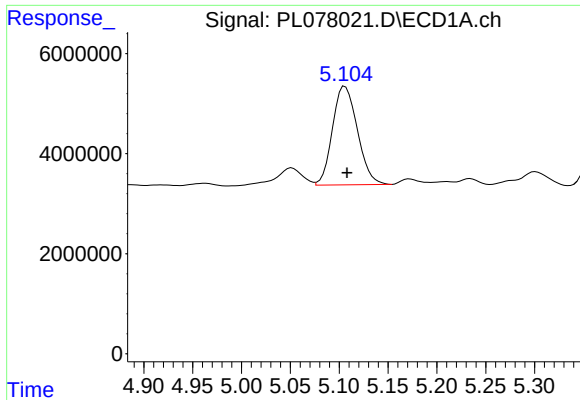

#24 Chlordane-2


R.T.: 5.106 min
Delta R.T.: -0.002 min
Response: 35030716
Conc: 525.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

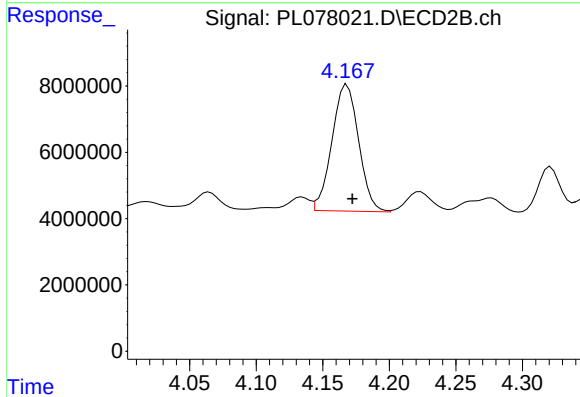


#24 Chlordane-2

R.T.: 4.168 min
Delta R.T.: -0.004 min
Response: 53446694
Conc: 446.17 ng/ml

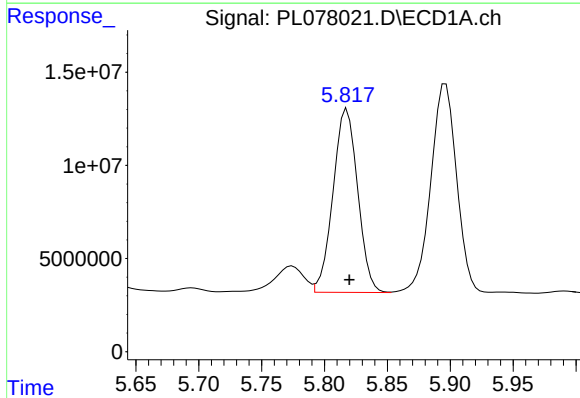


#25 Chlordane-3

R.T.: 5.818 min
Delta R.T.: -0.002 min
Response: 134191263
Conc: 544.91 ng/ml

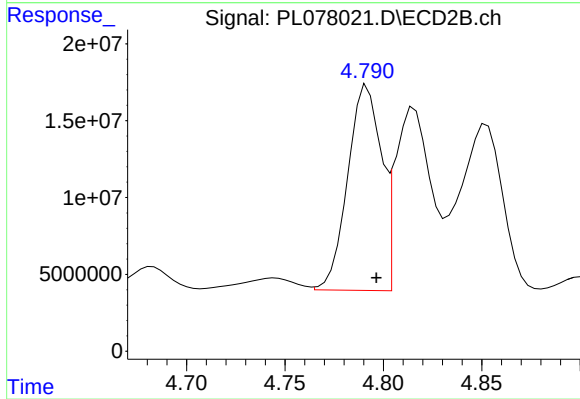

#25 Chlordane-3


R.T.: 4.792 min
Delta R.T.: -0.005 min
Response: 158020688
Conc: 459.38 ng/ml

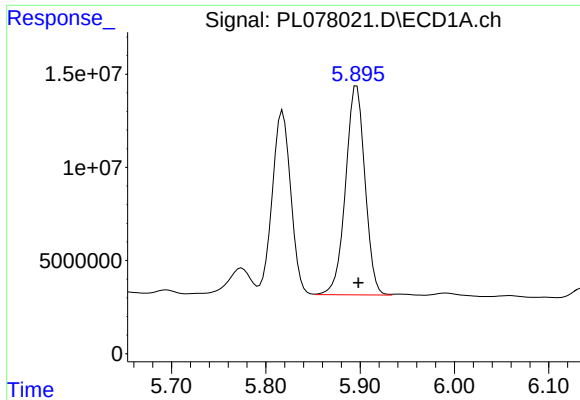

#26 Chlordane-4


R.T.: 5.896 min
Delta R.T.: -0.002 min
Response: 160419643
Conc: 539.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

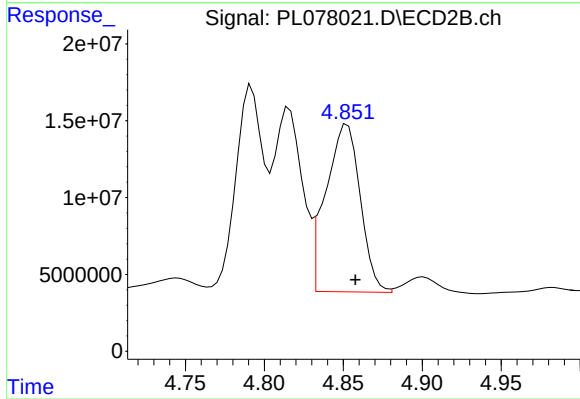


#26 Chlordane-4

R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 165153653
Conc: 455.20 ng/ml

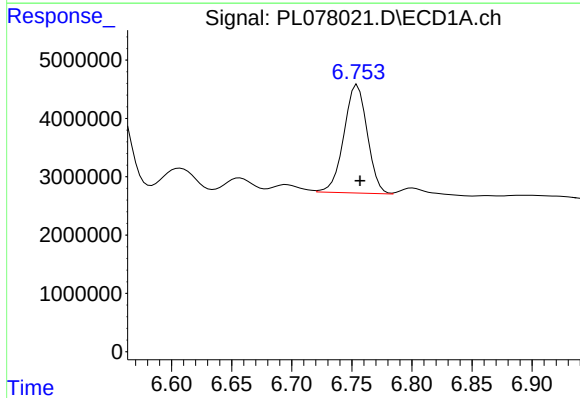


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: -0.002 min
Response: 25125845
Conc: 505.92 ng/ml

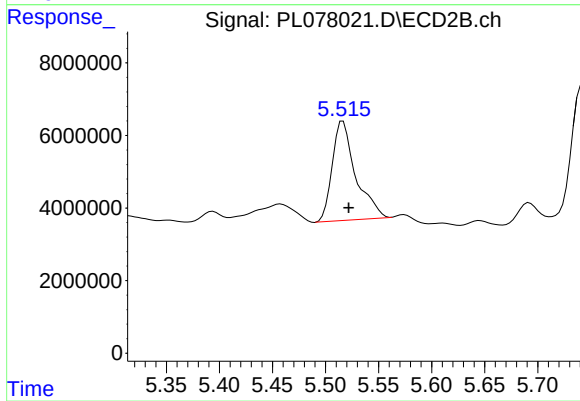

#27 Chlordane-5


R.T.: 5.516 min
Delta R.T.: -0.005 min
Response: 42079866
Conc: 447.22 ng/ml

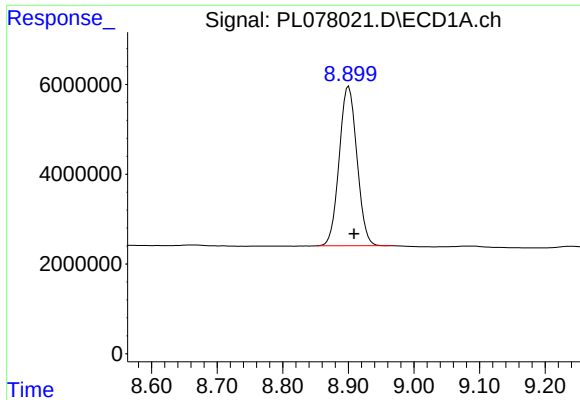

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: -0.008 min
Response: 66725358
Conc: 51.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

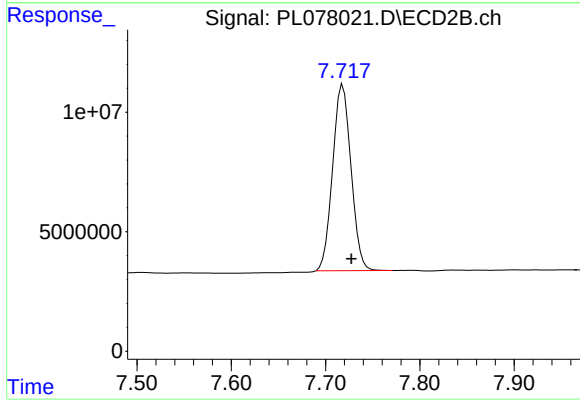

#28 Decachlorobiphenyl

R.T.: 7.718 min
Delta R.T.: -0.009 min
Response: 105517409
Conc: 42.03 ng/ml