

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093025\
 Data File : PL097456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2025 18:32
 Operator : AR\AJ
 Sample : Q3231-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 02:24:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.824	77164273	77311305	17.045	11.757 #
28)	SA Decachlor...	8.999	7.982	30463144	45201378	9.310	7.942
Target Compounds							
3)	MA gamma-BHC...	0.000	3.663	0	8747459	N.D.	0.939 #
9)	A Endosulfan I	6.058f	5.183f	9241907	30584781	1.784	3.981 #
13)	MA Dieldrin	0.000	5.428	0	21016029	N.D.	2.570 #
15)	B Endosulfa...	0.000	5.997	0	7050246	N.D.	0.992 #
20)	A Methoxychlor	0.000	6.699f	0	17515124	N.D.	4.647 #
27)	Chlordane-5	0.000	5.997	0	7050246	N.D.	23.647 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL093025\
Data File : PL097456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2025 18:32
Operator : AR\AJ
Sample : Q3231-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 02:24:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

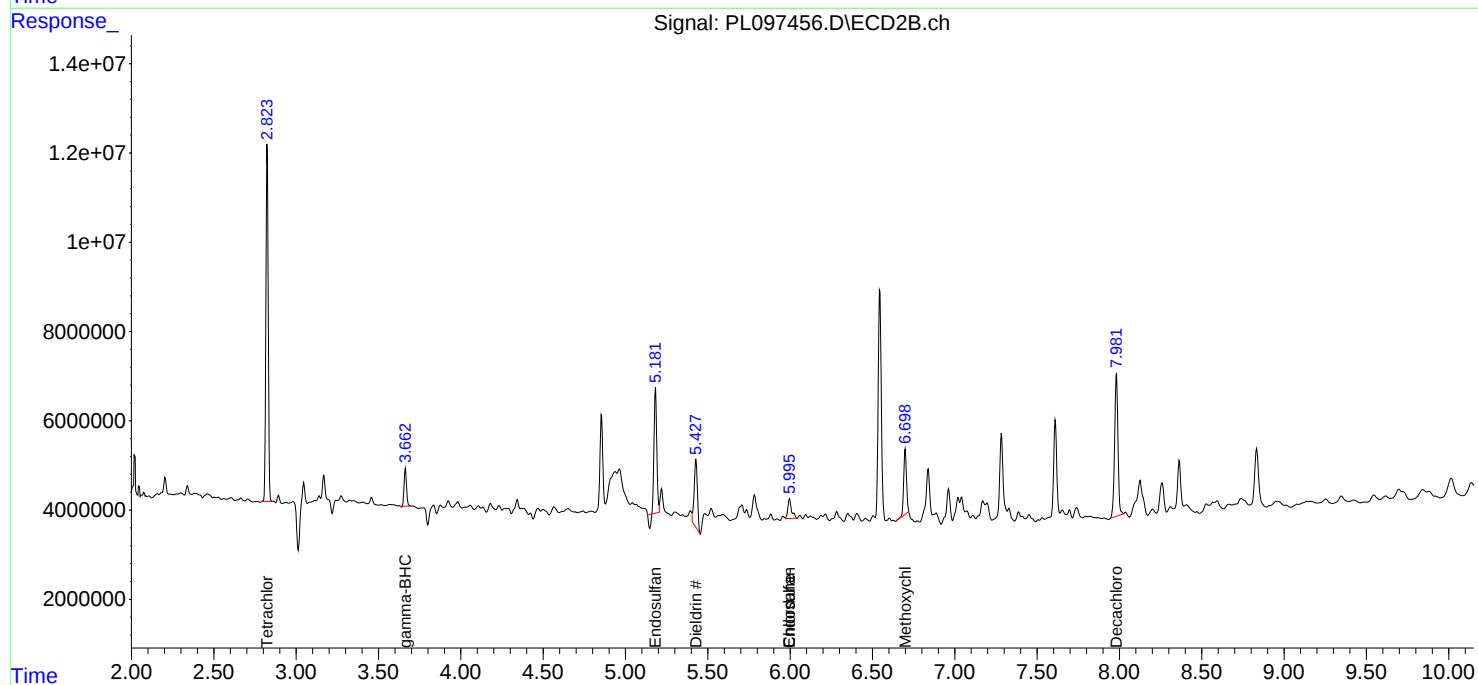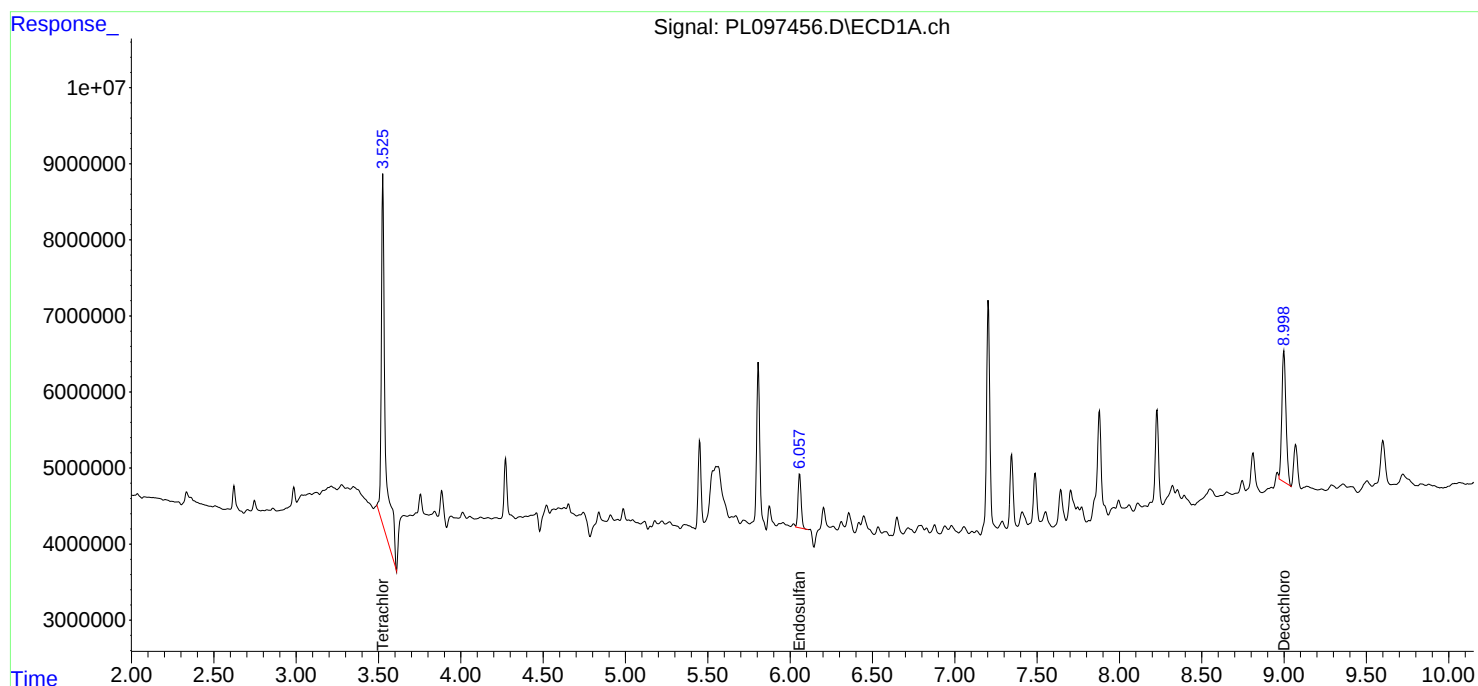


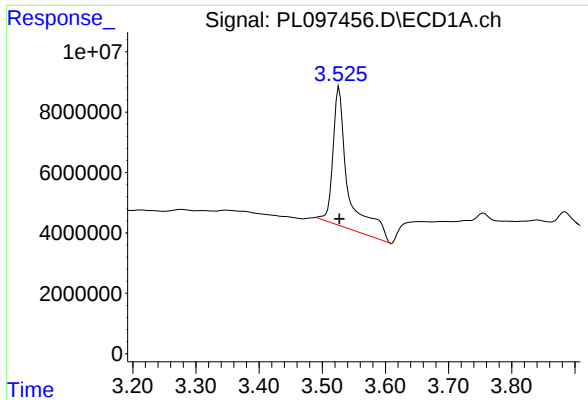

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 77164273
Conc: 17.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

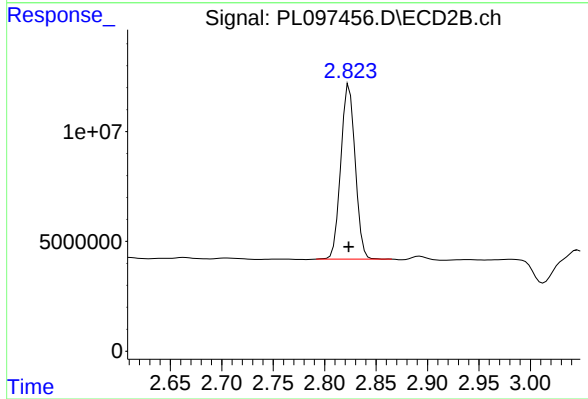


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.000 min
Response: 77311305
Conc: 11.76 ng/ml

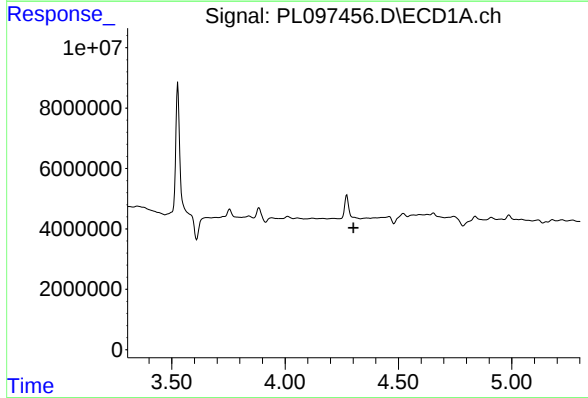


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.302 min
Response: 0
Conc: N.D.

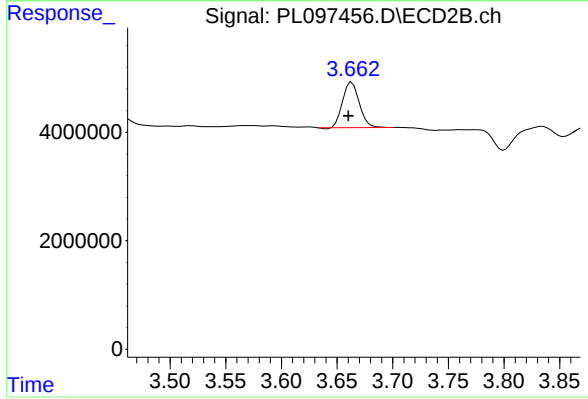

#3 gamma-BHC (Lindane)


R.T.: 3.663 min
Delta R.T.: 0.003 min
Response: 8747459
Conc: 0.94 ng/ml

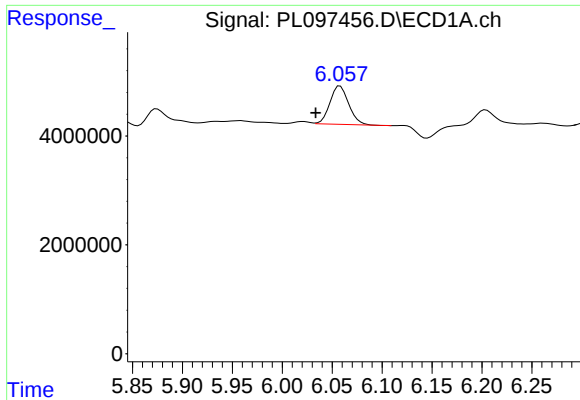

#9 Endosulfan I


R.T.: 6.058 min
Delta R.T.: 0.025 min
Response: 9241907
Conc: 1.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

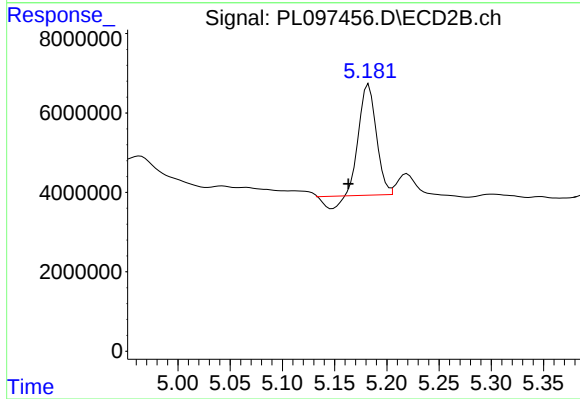


#9 Endosulfan I

R.T.: 5.183 min
Delta R.T.: 0.019 min
Response: 30584781
Conc: 3.98 ng/ml

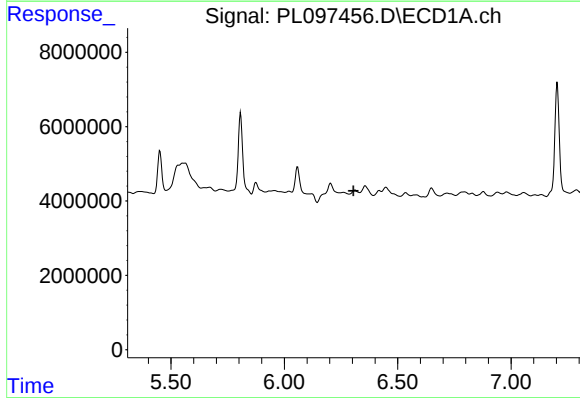


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.306 min
Response: 0
Conc: N.D.

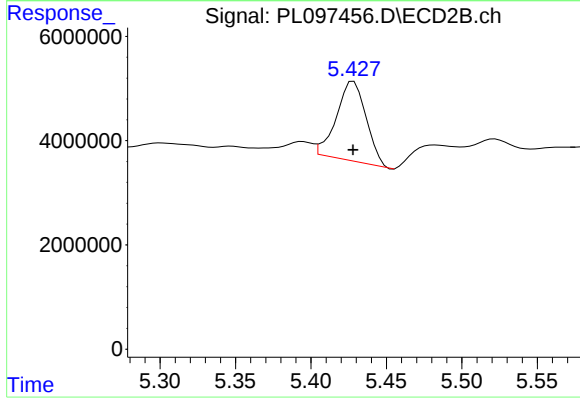

#13 Dieldrin


R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 21016029
Conc: 2.57 ng/ml

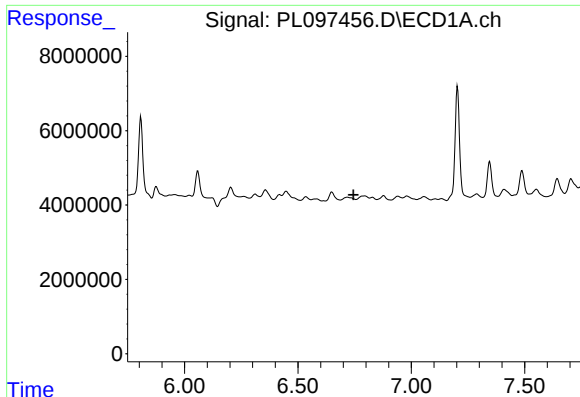

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

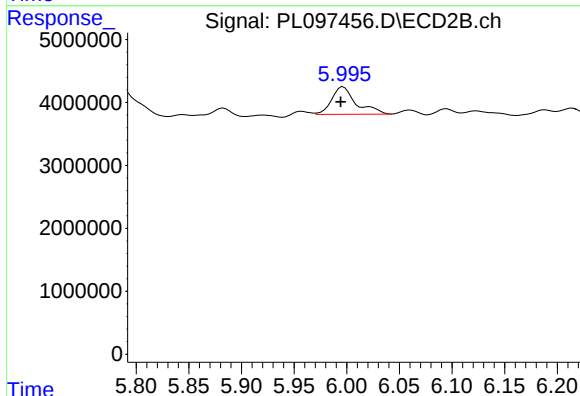


#15 Endosulfan II

R.T.: 5.997 min
Delta R.T.: 0.002 min
Response: 7050246
Conc: 0.99 ng/ml

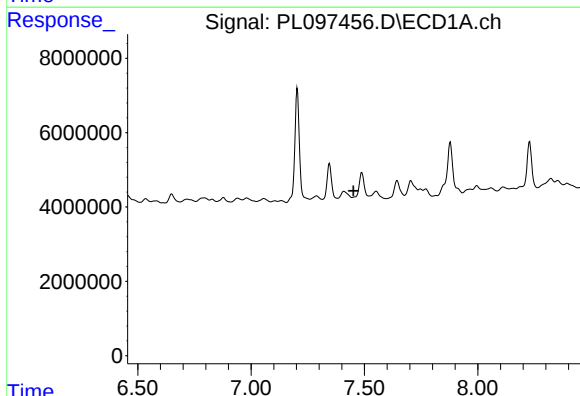


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.452 min
Response: 0
Conc: N.D.

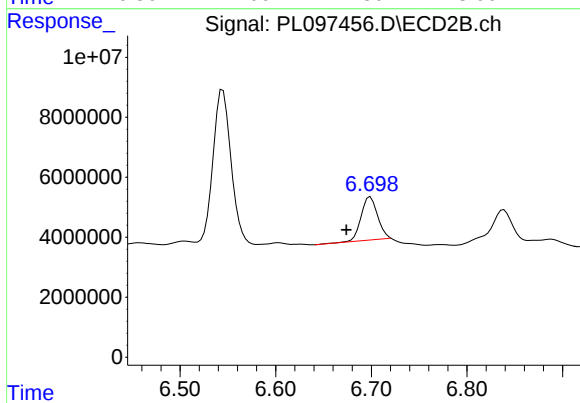

#20 Methoxychlor


R.T.: 6.699 min
Delta R.T.: 0.025 min
Response: 17515124
Conc: 4.65 ng/ml

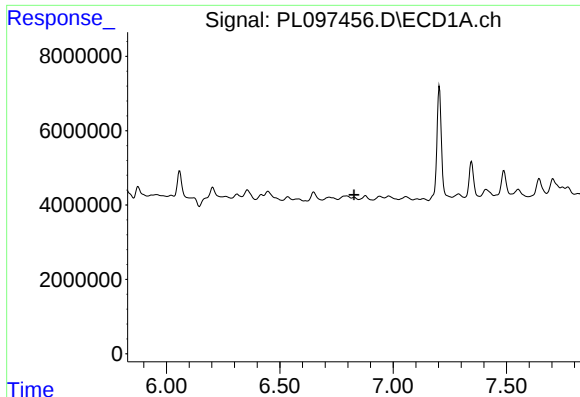

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.828 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

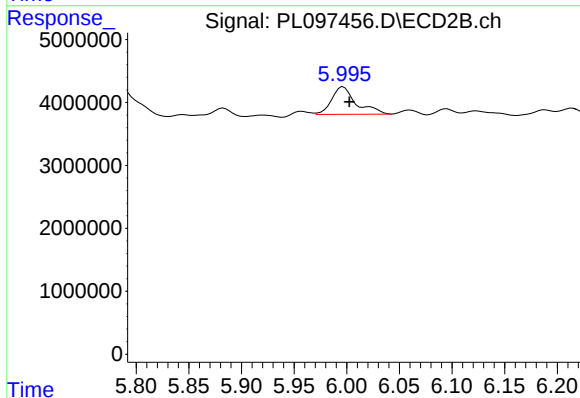


#27 Chlordane-5

R.T.: 5.997 min
Delta R.T.: -0.006 min
Response: 7050246
Conc: 23.65 ng/ml

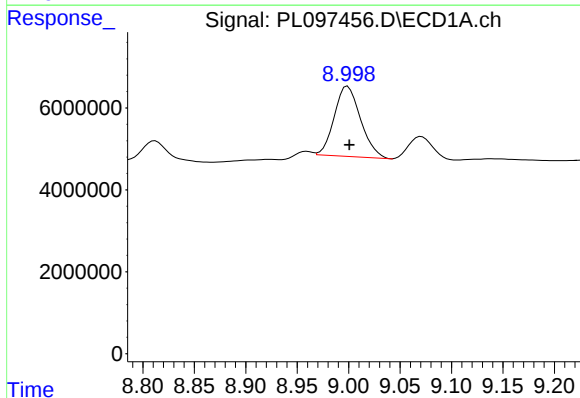

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.002 min
Response: 30463144
Conc: 9.31 ng/ml

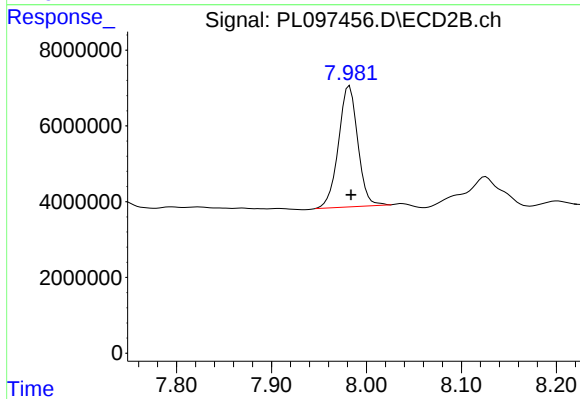

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: -0.002 min
Response: 45201378
Conc: 7.94 ng/ml