

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100119\
 Data File : PL052934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2019 10:49
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 03:43:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6)	B	beta-BHC	0.000	4.919f	0 10790766	N.D. 6.865 #
7)	B	delta-BHC	0.000	5.109	0 1565363	N.D. 0.432 #
8)	B	Heptachlo...	0.000	5.922	0 10959540	N.D. 3.270 #
9)	A	Endosulfan I	0.000	6.280	0 1251667	N.D. 0.400 #
10)	B	gamma-Chl...	0.000	6.160	0 1606656	N.D. 0.475 #
11)	B	alpha-Chl...	0.000	6.232	0 1895283	N.D. 0.563 #
14)	MA	Endrin	0.000	6.756	0 5219892	N.D. 1.880 #
16)	A	4,4'-DDD	0.000	6.876	0 1075387	N.D. 0.438 #
25)		Chlordane-3	0.000	6.160	0 1606656	N.D. 3.689 #
26)		Chlordane-4	0.000	6.232	0 1895283	N.D. 3.569 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100119\
Data File : PL052934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2019 10:49
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 03:43:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

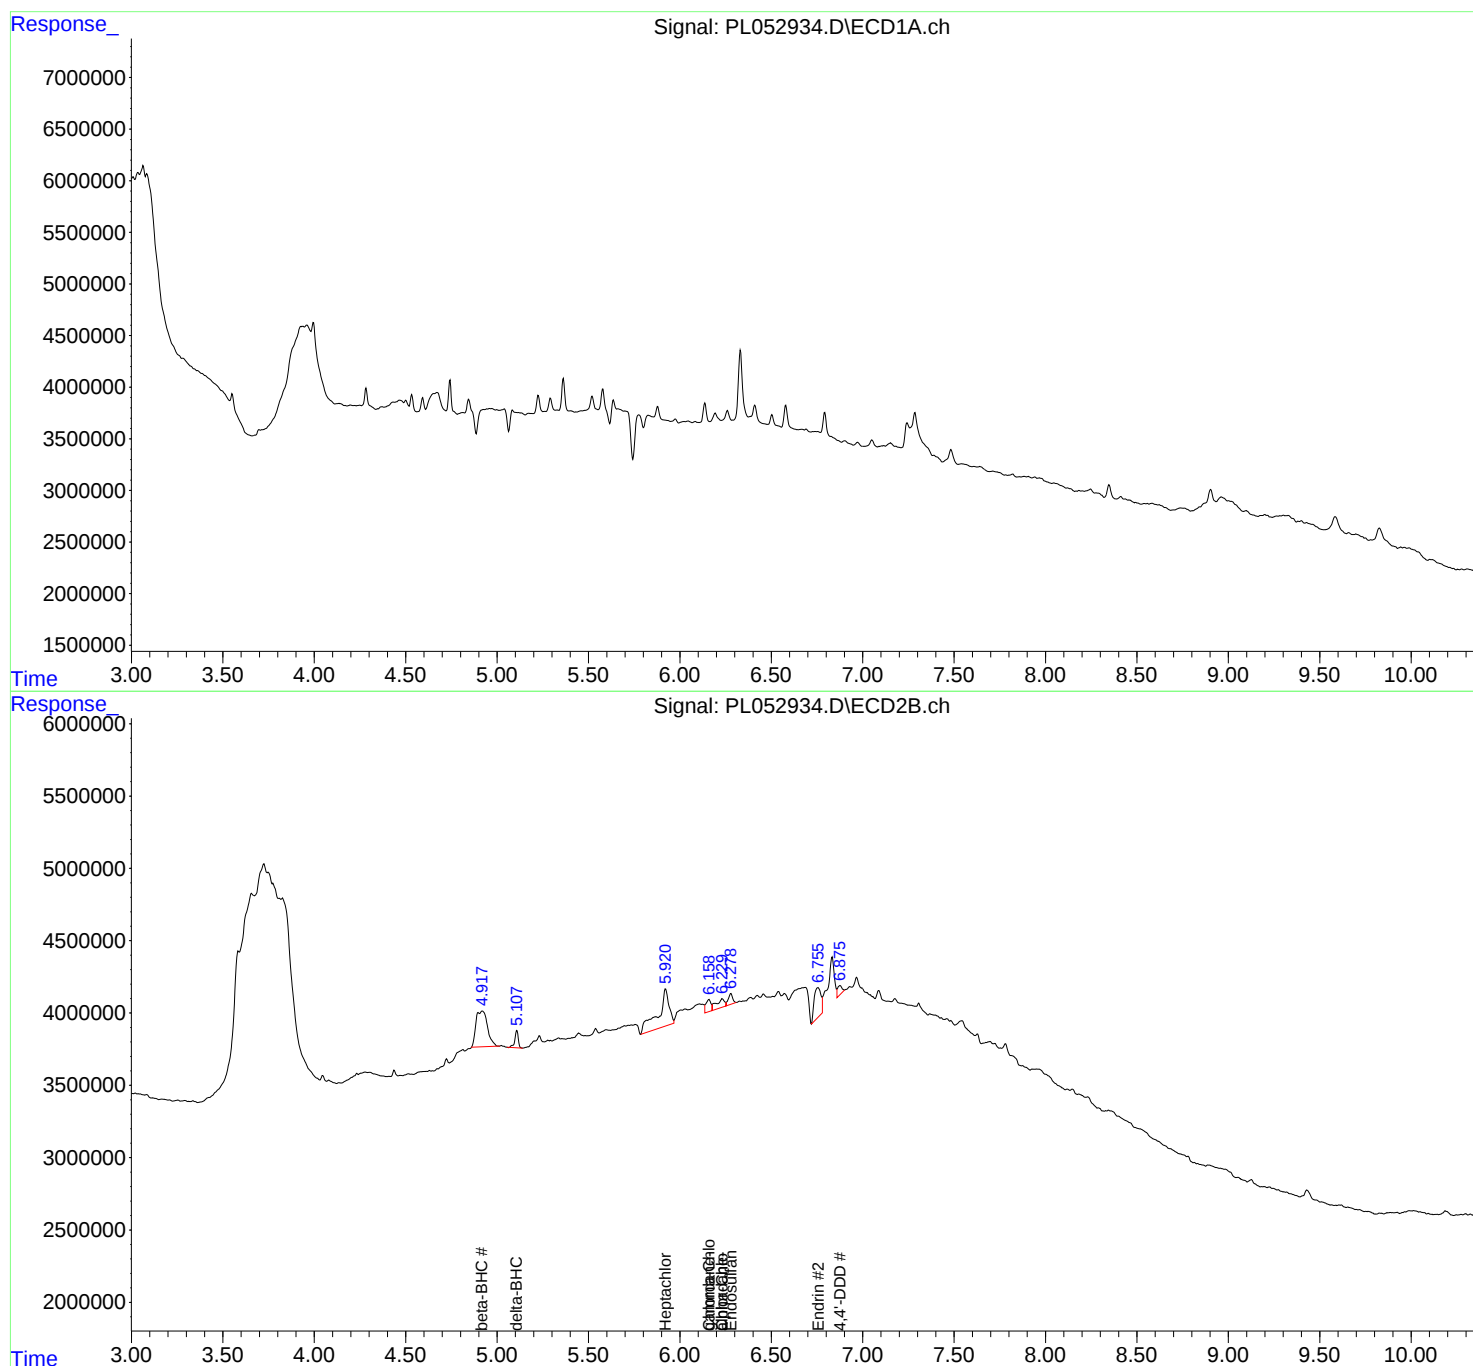


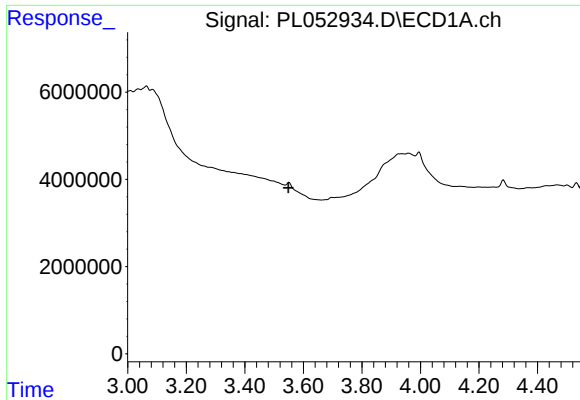

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

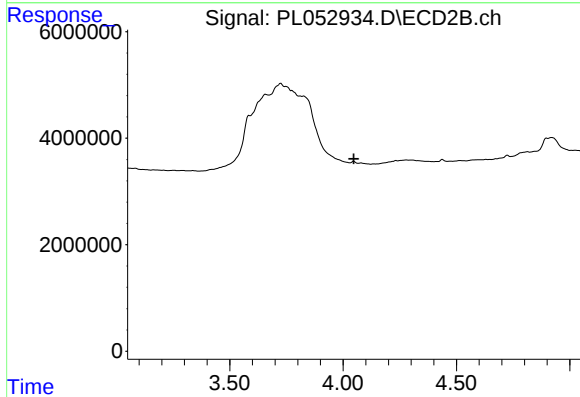


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.047 min
Response: 0
Conc: N.D.

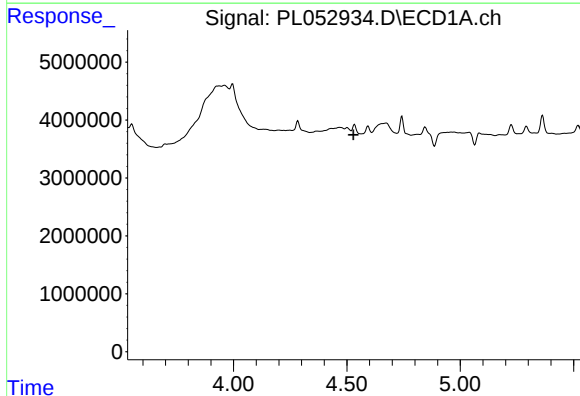


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.530 min
Response: 0
Conc: N.D.

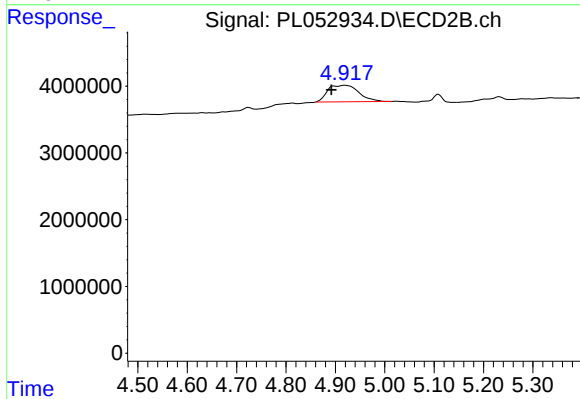

#6 beta-BHC


R.T.: 4.919 min
Delta R.T.: 0.027 min
Response: 10790766
Conc: 6.87 ng/ml

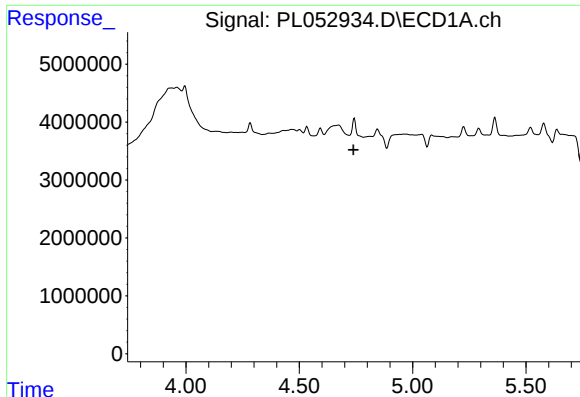

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

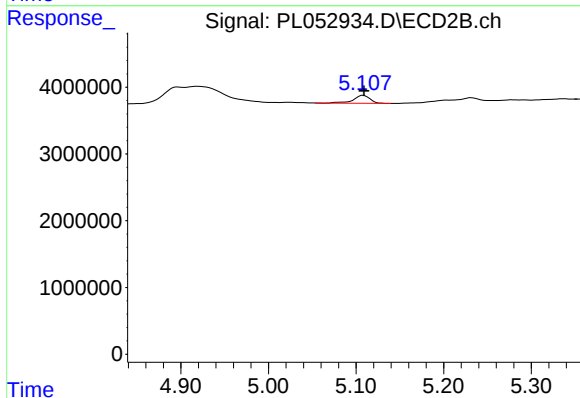


#7 delta-BHC

R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 1565363
Conc: 0.43 ng/ml

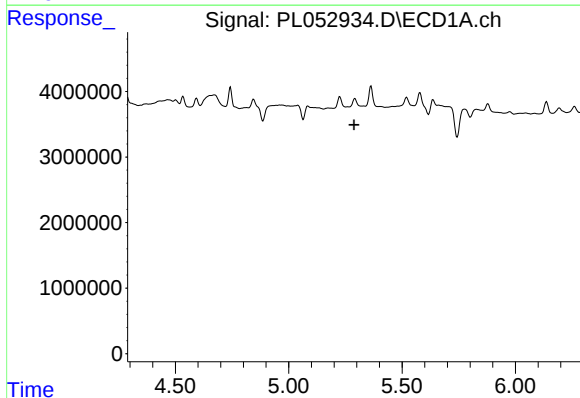


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

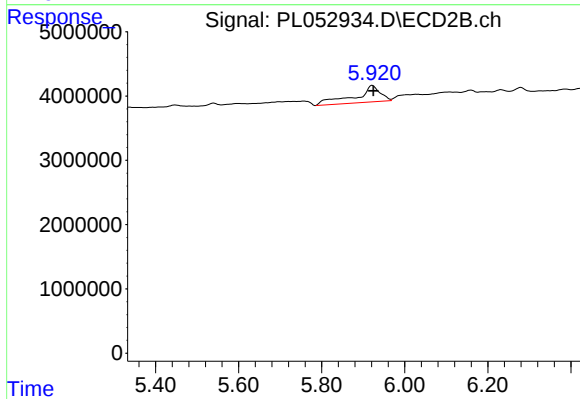

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.003 min
Response: 10959540
Conc: 3.27 ng/ml

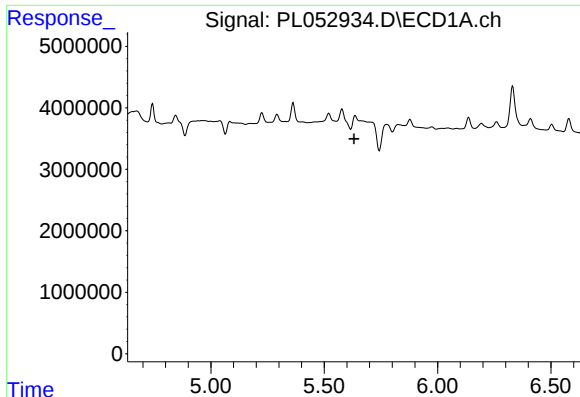

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.632 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

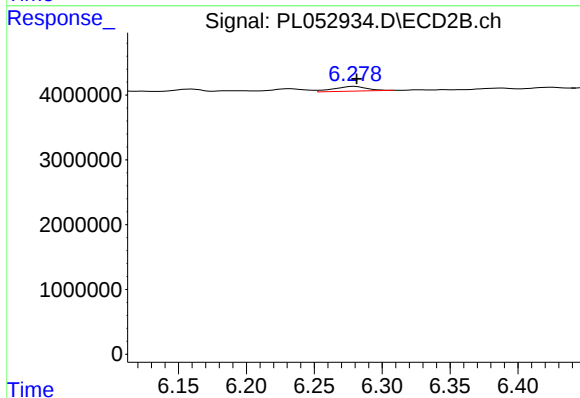


#9 Endosulfan I

R.T.: 6.280 min
Delta R.T.: -0.002 min
Response: 1251667
Conc: 0.40 ng/ml

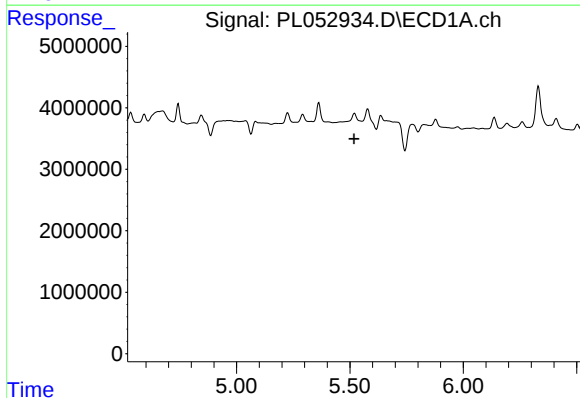


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

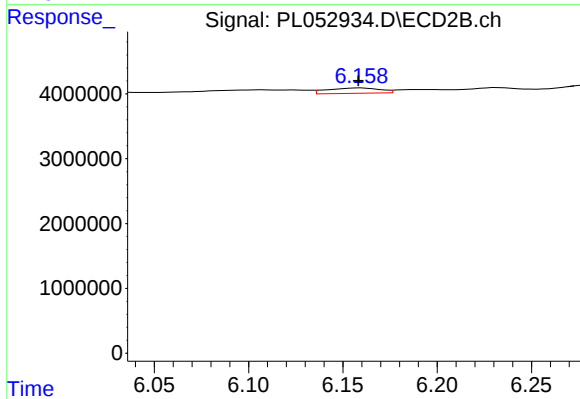

#10 gamma-Chlordane


R.T.: 6.160 min
Delta R.T.: 0.002 min
Response: 1606656
Conc: 0.47 ng/ml

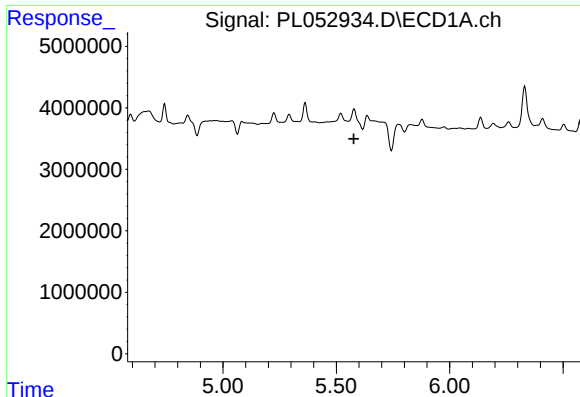

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

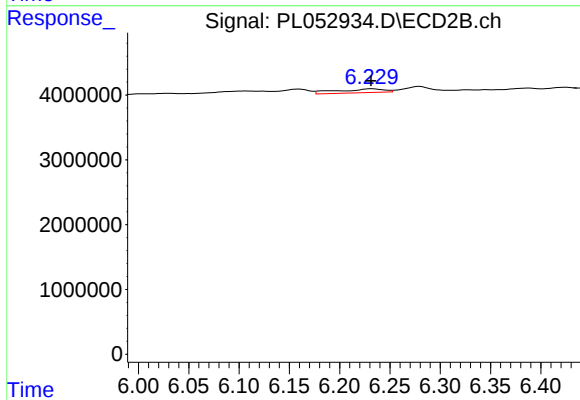


#11 alpha-Chlordane

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 1895283
Conc: 0.56 ng/ml

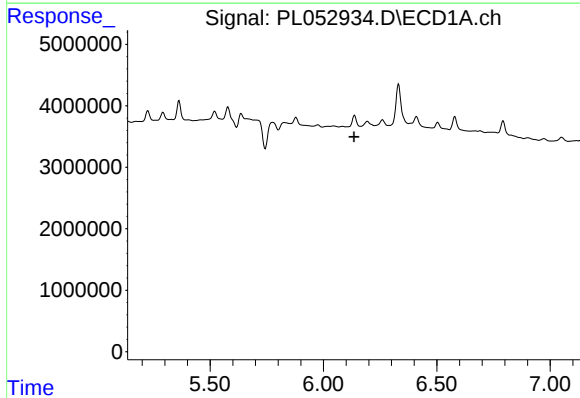


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.135 min
Response: 0
Conc: N.D.

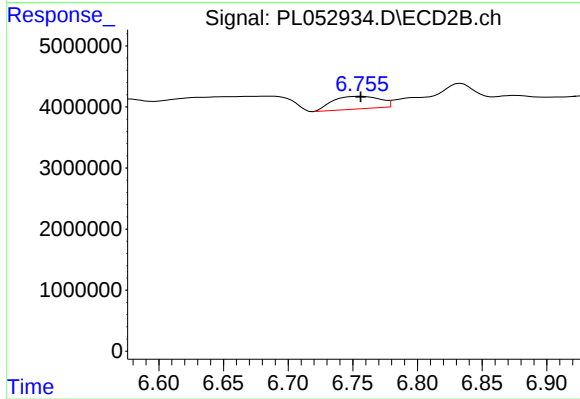

#14 Endrin


R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 5219892
Conc: 1.88 ng/ml

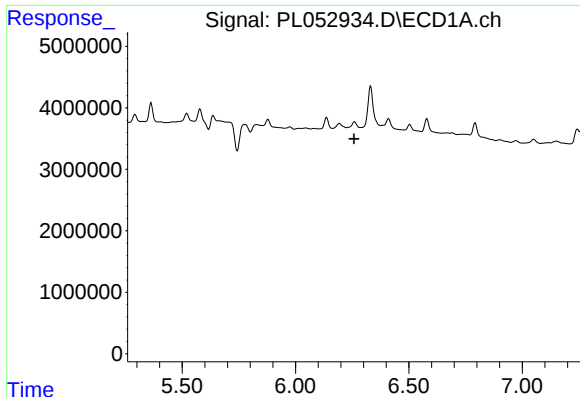

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

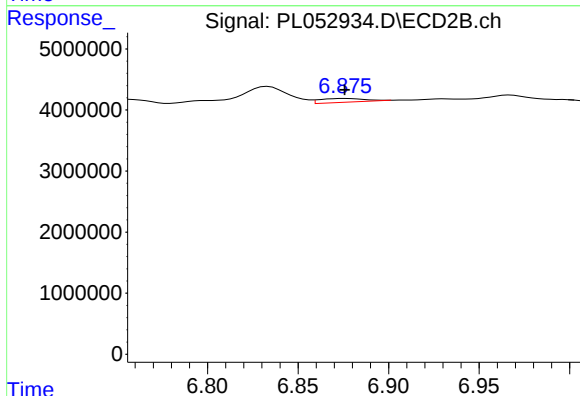


#16 4,4'-DDD

R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 1075387
Conc: 0.44 ng/ml

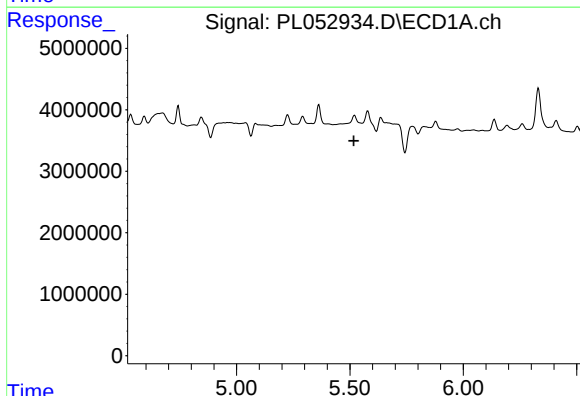


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

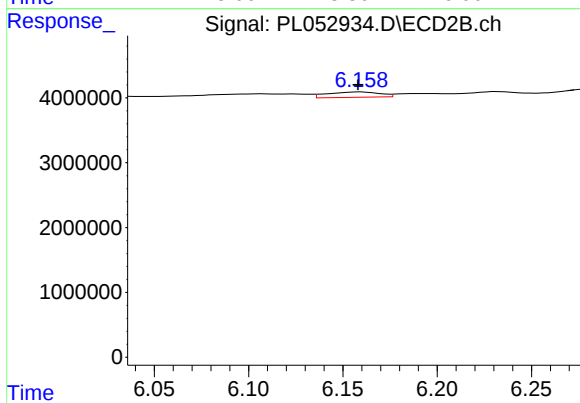

#25 Chlordane-3


R.T.: 6.160 min
Delta R.T.: 0.002 min
Response: 1606656
Conc: 3.69 ng/ml

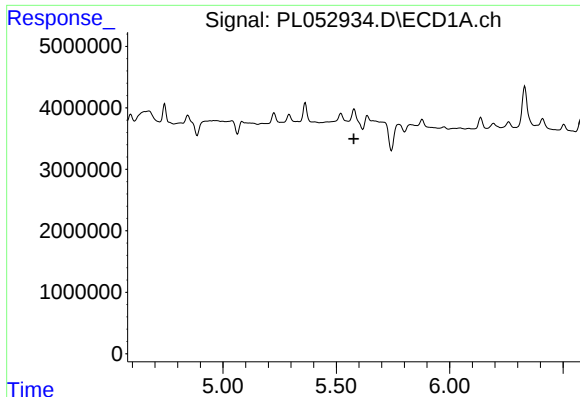

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

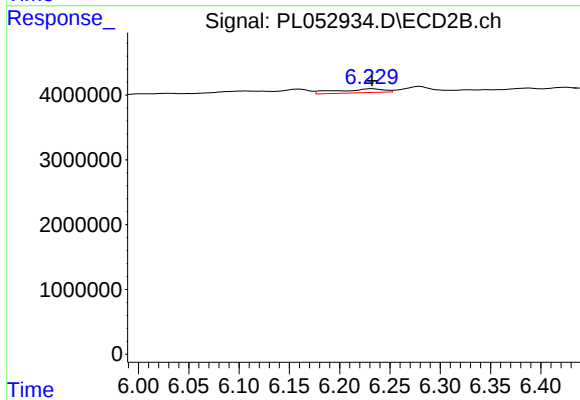


#26 Chlordane-4

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 1895283
Conc: 3.57 ng/ml

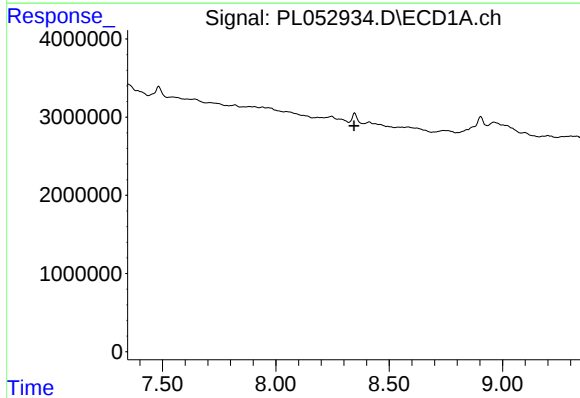

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.345 min
Response: 0
Conc: N.D.

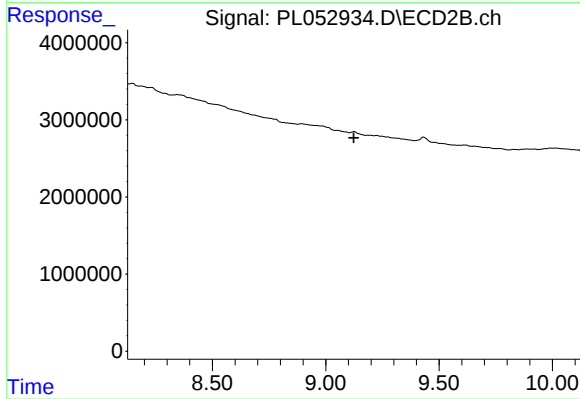

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.124 min
Response: 0
Conc: N.D.