

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100119\
 Data File : PL052967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2019 19:47
 Operator : SG\AJ
 Sample : K5079-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-COMP

Manual Integrations
 APPROVED

Ankita
 10/2/2019 1:19:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 03:49:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	4.047	199.2E6	54746496	20.023	20.388
28)	SA Decachlor...	8.343	9.125	156.4E6	50690975	15.618	17.279
Target Compounds							
10)	B gamma-Chl...	5.514	6.162	7194168	2303533	0.535m	0.681 #
11)	B alpha-Chl...	5.574	6.233	7253357	2860916	0.550m	0.850 #
12)	B 4,4'-DDE	5.738	6.386	4030963	1643867	0.347m	0.503m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100119\
Data File : PL052967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2019 19:47
Operator : SG\AJ
Sample : K5079-01
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1-COMP


Manual Integrations
APPROVED

Ankita
10/2/2019 1:19:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 03:49:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

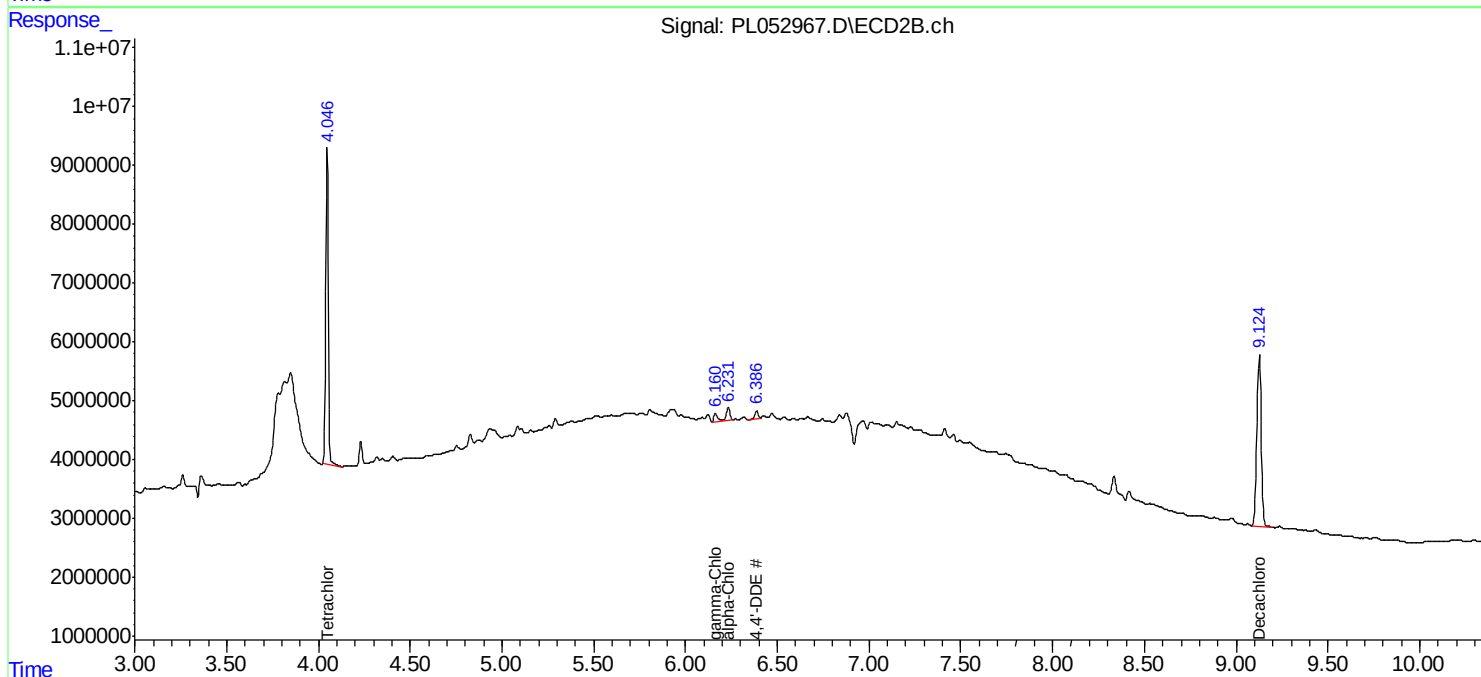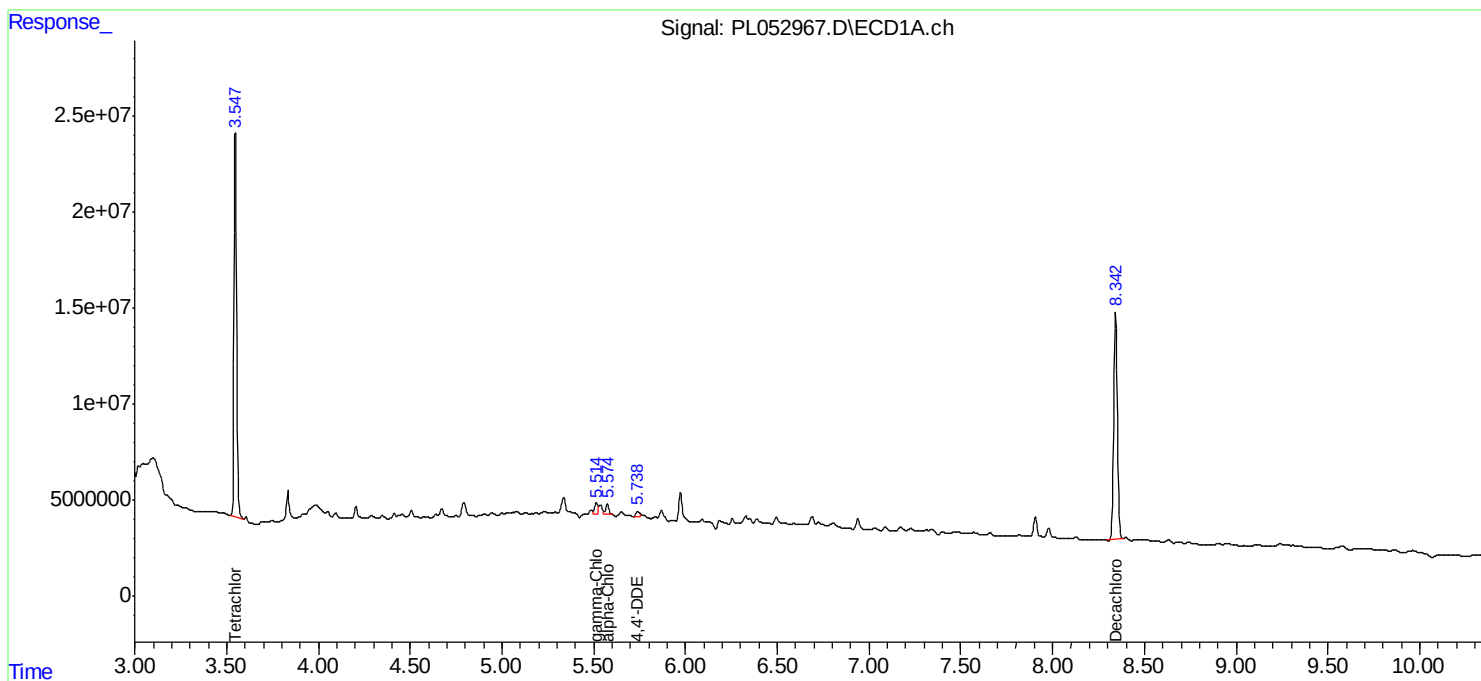

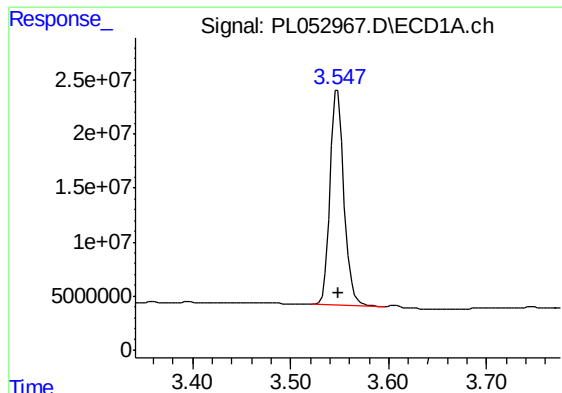


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 199160820
Conc: 20.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP


Manual Integrations
APPROVED

Ankita
10/2/2019 1:19:51 PM

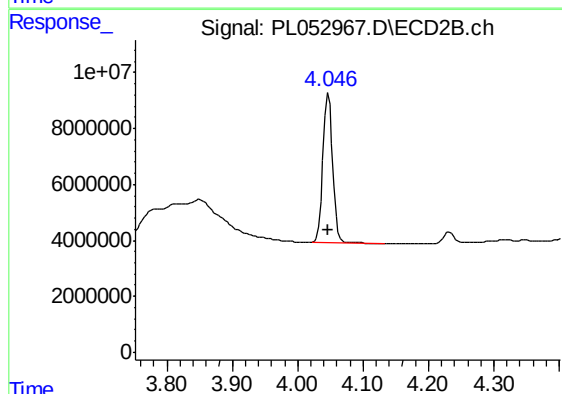


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 54746496
Conc: 20.39 ng/ml

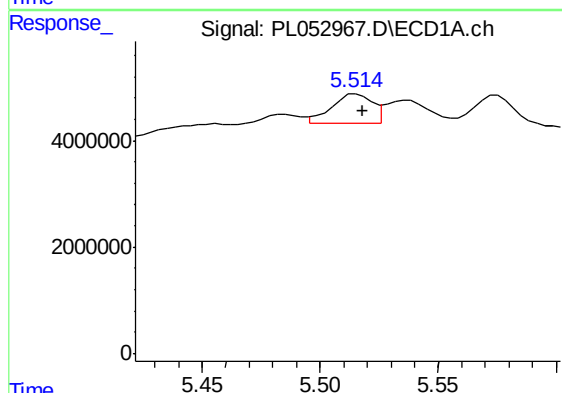


#10 gamma-Chlordane

R.T.: 5.514 min
Delta R.T.: -0.004 min
Response: 7194168
Conc: 0.53 ng/ml m

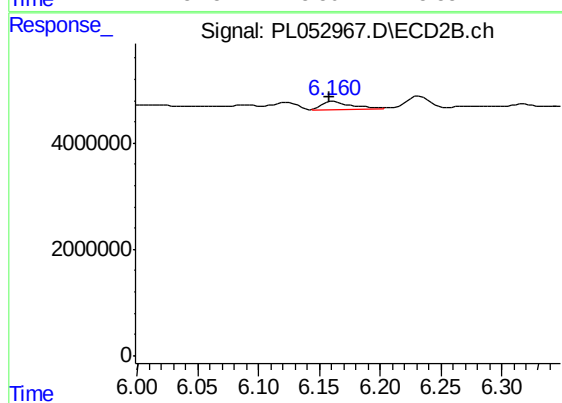

#10 gamma-Chlordane

R.T.: 6.162 min
Delta R.T.: 0.004 min
Response: 2303533
Conc: 0.68 ng/ml

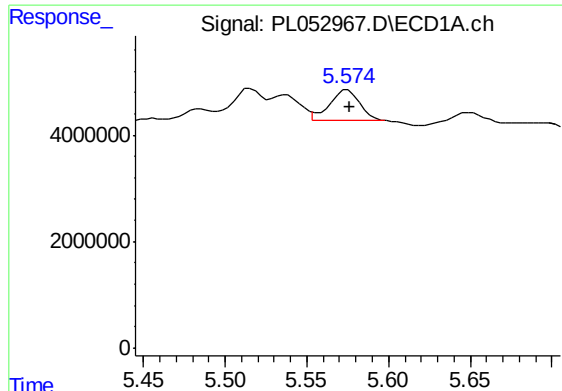


#11 alpha-Chlordane

R.T.: 5.574 min
Delta R.T.: -0.003 min
Response: 7253357
Conc: 0.55 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP


Manual Integrations
APPROVED

Ankita
10/2/2019 1:19:51 PM

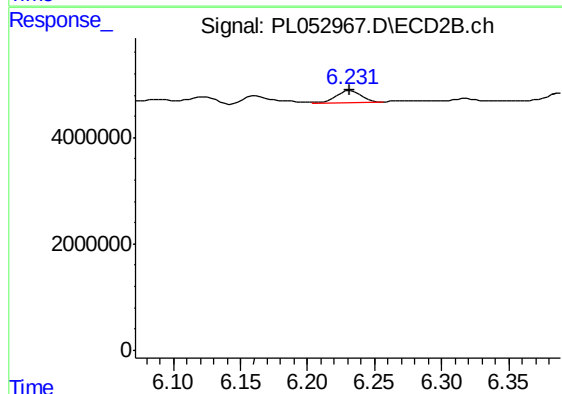


#11 alpha-Chlordane

R.T.: 6.233 min
Delta R.T.: 0.001 min
Response: 2860916
Conc: 0.85 ng/ml

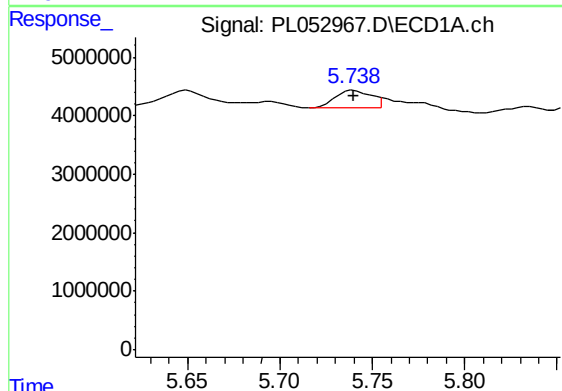


#12 4,4'-DDE

R.T.: 5.738 min
Delta R.T.: -0.002 min
Response: 4030963
Conc: 0.35 ng/ml m

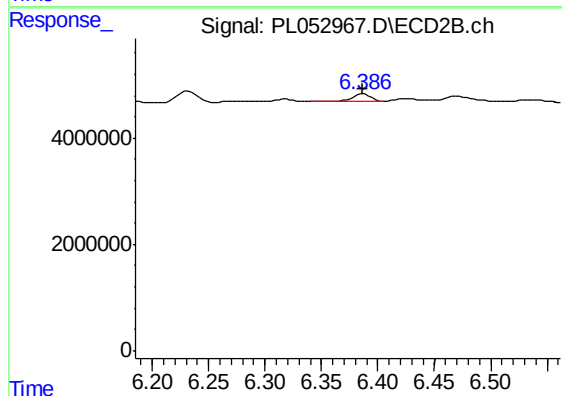

#12 4,4'-DDE

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 1643867
Conc: 0.50 ng/ml m

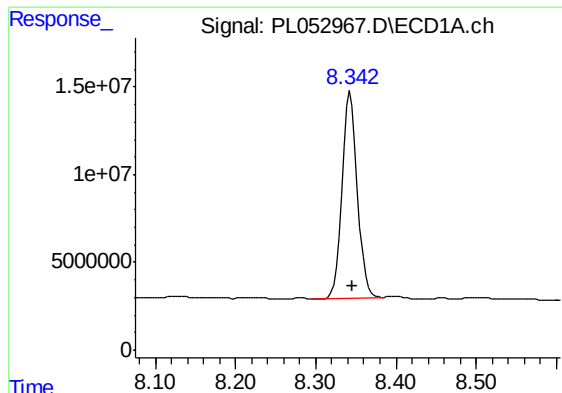


#28 Decachlorobiphenyl

R.T.: 8.343 min
Delta R.T.: -0.002 min
Response: 156435236
Conc: 15.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP

Manual Integrations
APPROVED

Ankita
10/2/2019 1:19:51 PM

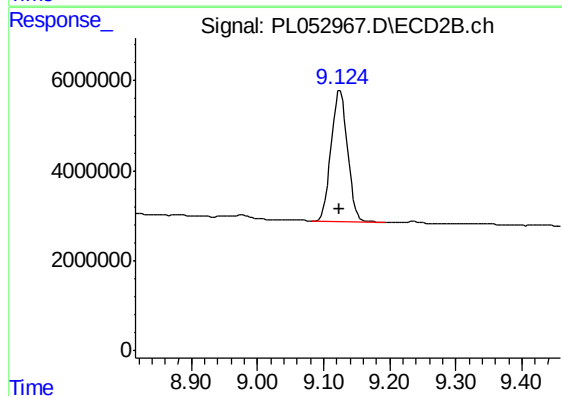

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 50690975
Conc: 17.28 ng/ml