

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100119\
 Data File : PL052972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2019 20:58
 Operator : SG\AJ
 Sample : K5060-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-060

Manual Integrations
 APPROVED

Ankita
 10/2/2019 1:19:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 03:50:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	4.047	173.9E6	49366911	17.485	18.385
28)	SA Decachlor...	8.344	9.126	126.3E6	39061473	12.606	13.315
Target Compounds							
10)	B gamma-Chl...	5.516	6.157	29219778	9792377	2.173m	2.894m#
11)	B alpha-Chl...	5.574	6.232	33991125	16636491	2.577m	4.943m#
13)	MA Dieldrin	5.873	6.539	13661346	1699867	1.058	0.521m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100119\
Data File : PL052972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2019 20:58
Operator : SG\AJ
Sample : K5060-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FK-PS-01-060


Manual Integrations
APPROVED

Ankita
10/2/2019 1:19:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 03:50:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

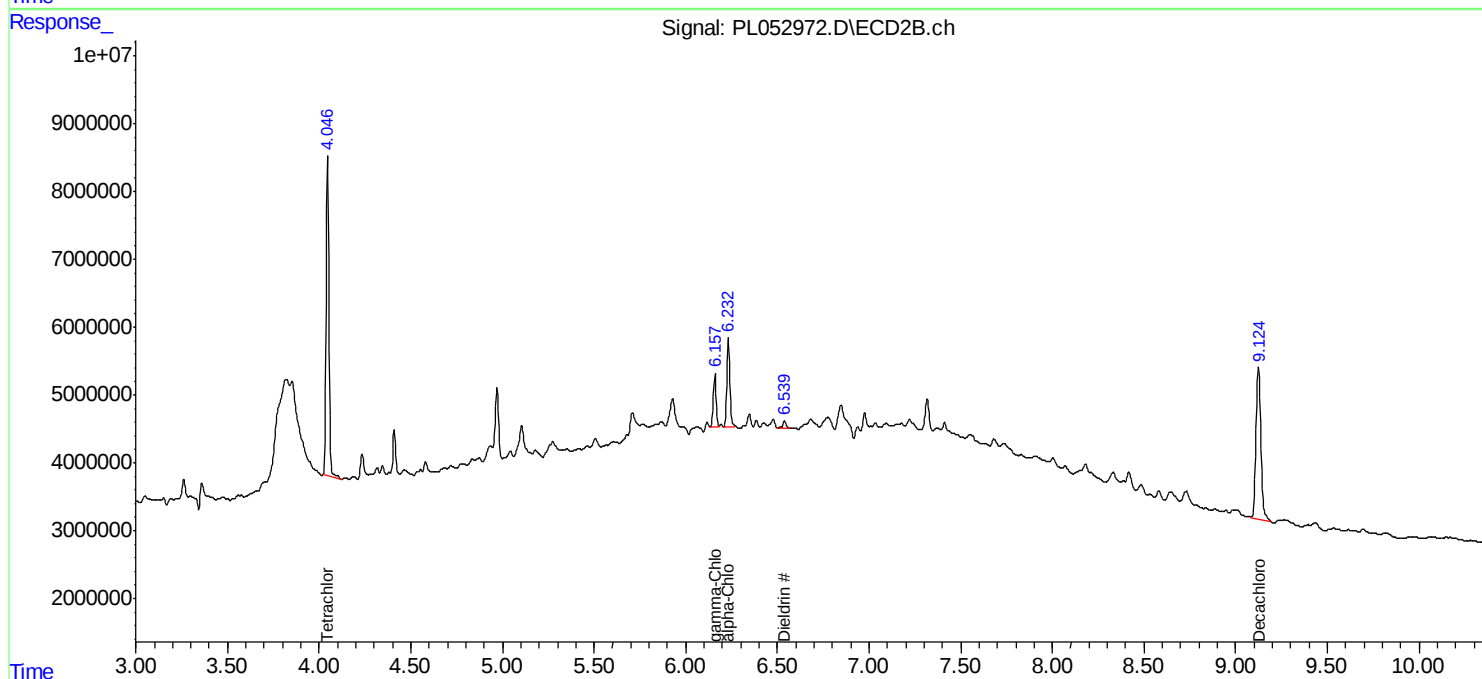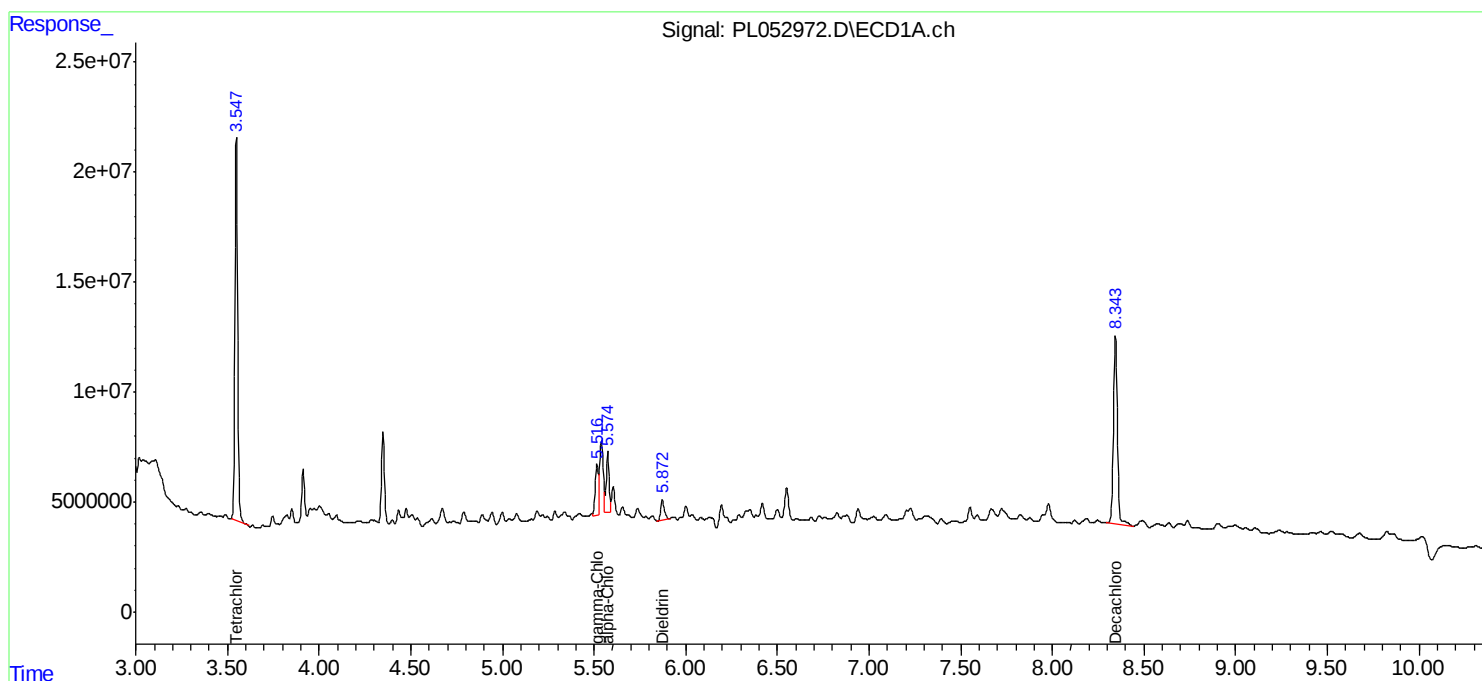

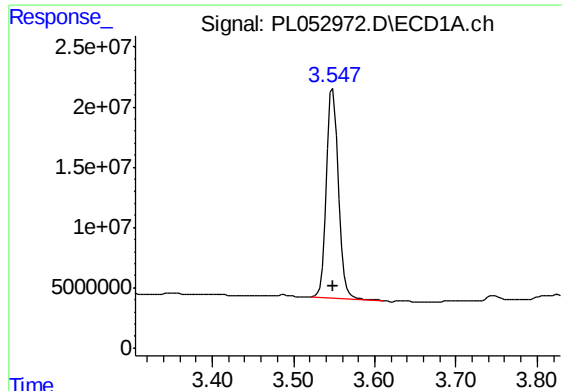


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 173918995
Conc: 17.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-060


Manual Integrations
APPROVED

Ankita
10/2/2019 1:19:54 PM

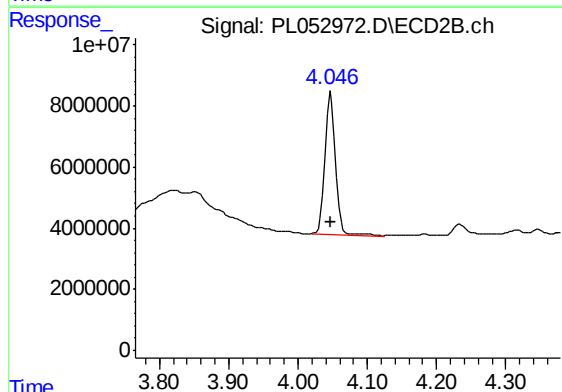


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 49366911
Conc: 18.38 ng/ml

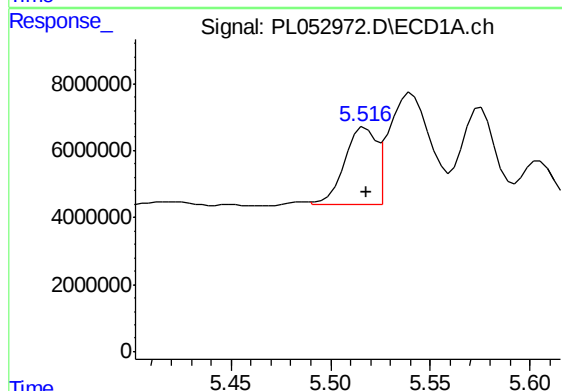


#10 gamma-Chlordane

R.T.: 5.516 min
Delta R.T.: -0.002 min
Response: 29219778
Conc: 2.17 ng/ml m

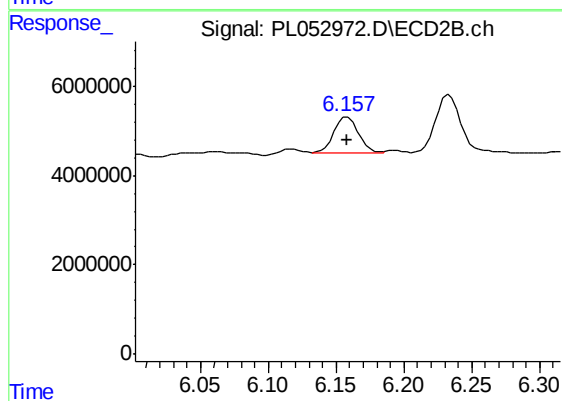

#10 gamma-Chlordane

R.T.: 6.157 min
Delta R.T.: -0.001 min
Response: 9792377
Conc: 2.89 ng/ml m

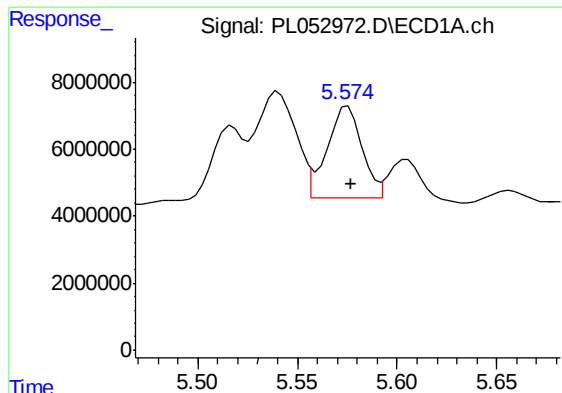


#11 alpha-Chlordane

R.T.: 5.574 min
Delta R.T.: -0.003 min
Response: 33991125
Conc: 2.58 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-060


Manual Integrations
APPROVED

Ankita
10/2/2019 1:19:54 PM

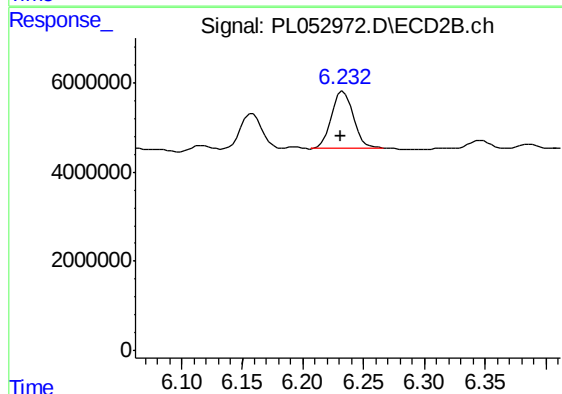


#11 alpha-Chlordane

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 16636491
Conc: 4.94 ng/ml m

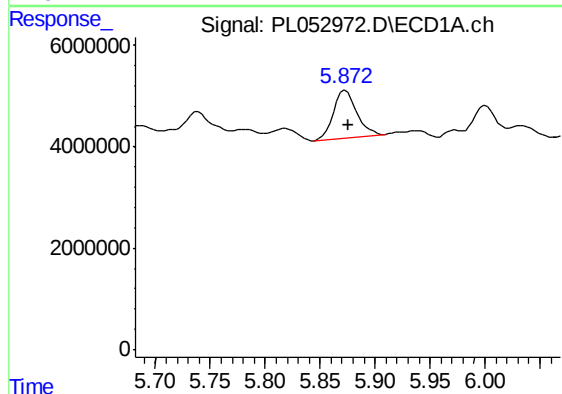


#13 Dieldrin

R.T.: 5.873 min
Delta R.T.: -0.003 min
Response: 13661346
Conc: 1.06 ng/ml

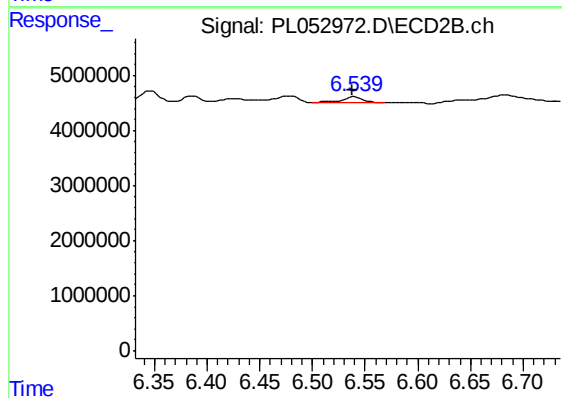

#13 Dieldrin

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 1699867
Conc: 0.52 ng/ml m

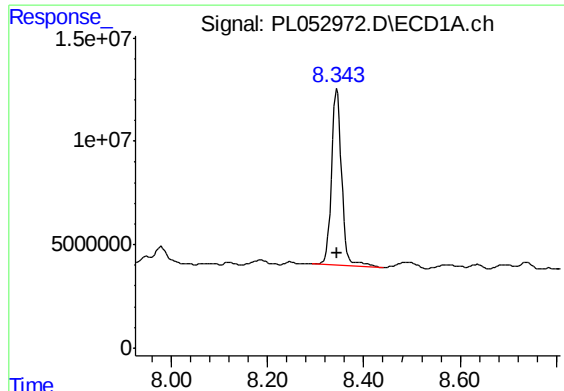


#28 Decachlorobiphenyl

R.T.: 8.344 min
Delta R.T.: 0.000 min
Response: 126258837
Conc: 12.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-060

Manual Integrations
APPROVED

Ankita
10/2/2019 1:19:54 PM

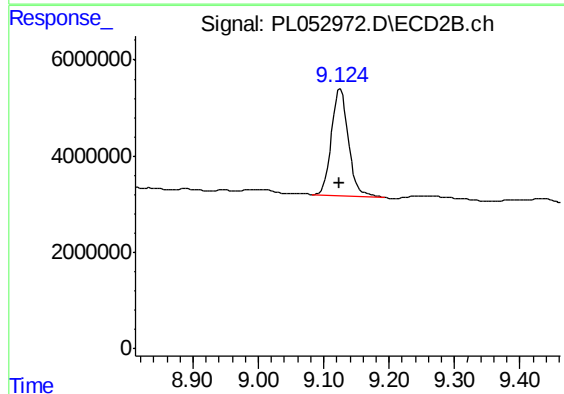

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.001 min
Response: 39061473
Conc: 13.31 ng/ml